

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072320\
 Data File : BM026861.D
 Acq On : 23 Jul 2020 21:11
 Operator : JU/CG
 Sample : L3381-19 2X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 VNJ-225-GRID-B5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070820.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.925	366	372	387	rBV	378246	555544	40.94%	5.042%
2	6.501	634	640	654	rBV	327818	548478	40.42%	4.977%
3	7.278	765	772	781	rBV	390065	582612	42.93%	5.287%
4	8.430	961	968	977	rBV	200903	344507	25.39%	3.126%
5	10.036	1231	1241	1247	rBV	448191	744962	54.89%	6.760%
6	12.548	1662	1668	1678	rVB	466461	667610	49.19%	6.059%
7	12.860	1715	1721	1730	rVB3	10200	18416	1.36%	0.167%
8	13.424	1811	1817	1828	rBV	67808	114841	8.46%	1.042%
9	13.665	1855	1858	1863	rVB2	11510	19370	1.43%	0.176%
10	13.948	1900	1906	1912	rBV2	614684	878087	64.70%	7.969%
11	14.854	2056	2060	2065	rVB2	13702	19322	1.42%	0.175%
12	15.018	2082	2088	2092	rBV	18570	28979	2.14%	0.263%
13	15.459	2158	2163	2171	rBV	372658	525362	38.71%	4.768%
14	15.718	2203	2207	2209	rBV4	18290	21940	1.62%	0.199%
15	16.471	2329	2335	2338	rBV5	8627	17901	1.32%	0.162%
16	16.512	2338	2342	2349	rVV5	23487	50640	3.73%	0.460%
17	16.571	2349	2352	2355	rVB4	15067	19381	1.43%	0.176%
18	16.712	2371	2376	2380	rBV	722936	980892	72.28%	8.902%
19	16.753	2380	2383	2389	rVB	144939	195906	14.44%	1.778%
20	16.848	2395	2399	2404	rVB	41253	58654	4.32%	0.532%
21	17.136	2444	2448	2450	rBV2	13335	18912	1.39%	0.172%
22	17.253	2464	2468	2471	rVB3	14813	18449	1.36%	0.167%
23	17.595	2522	2526	2530	rBV	23328	29204	2.15%	0.265%
24	17.648	2530	2535	2540	rVB3	35305	55767	4.11%	0.506%
25	17.718	2544	2547	2551	rBV2	19204	22515	1.66%	0.204%
26	17.783	2554	2558	2562	rBV3	42592	66656	4.91%	0.605%
27	18.148	2618	2620	2624	rVB5	16870	20941	1.54%	0.190%
28	18.530	2681	2685	2688	rBV2	21220	31933	2.35%	0.290%
29	18.789	2724	2729	2735	rBV	325253	419328	30.90%	3.805%
30	19.153	2784	2791	2795	rBV	309016	478196	35.24%	4.340%
31	19.377	2825	2829	2840	rVB	782833	965267	71.13%	8.760%
32	20.941	3090	3095	3099	rBV2	1014564	1357093	100.00%	12.316%
33	23.006	3442	3446	3451	rVB	759752	1141683	84.13%	10.361%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072320\
Data File : BM026861.D
Acq On : 23 Jul 2020 21:11
Operator : JU/CG
Sample : L3381-19 2X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VNJ-225-GRID-B5

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070820.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION


Sum of corrected areas: 11019348

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072320\
Data File : BM026861.D
Acq On : 23 Jul 2020 21:11
Operator : JU/CG
Sample : L3381-19 2X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VNJ-225-GRID-B5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM070820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

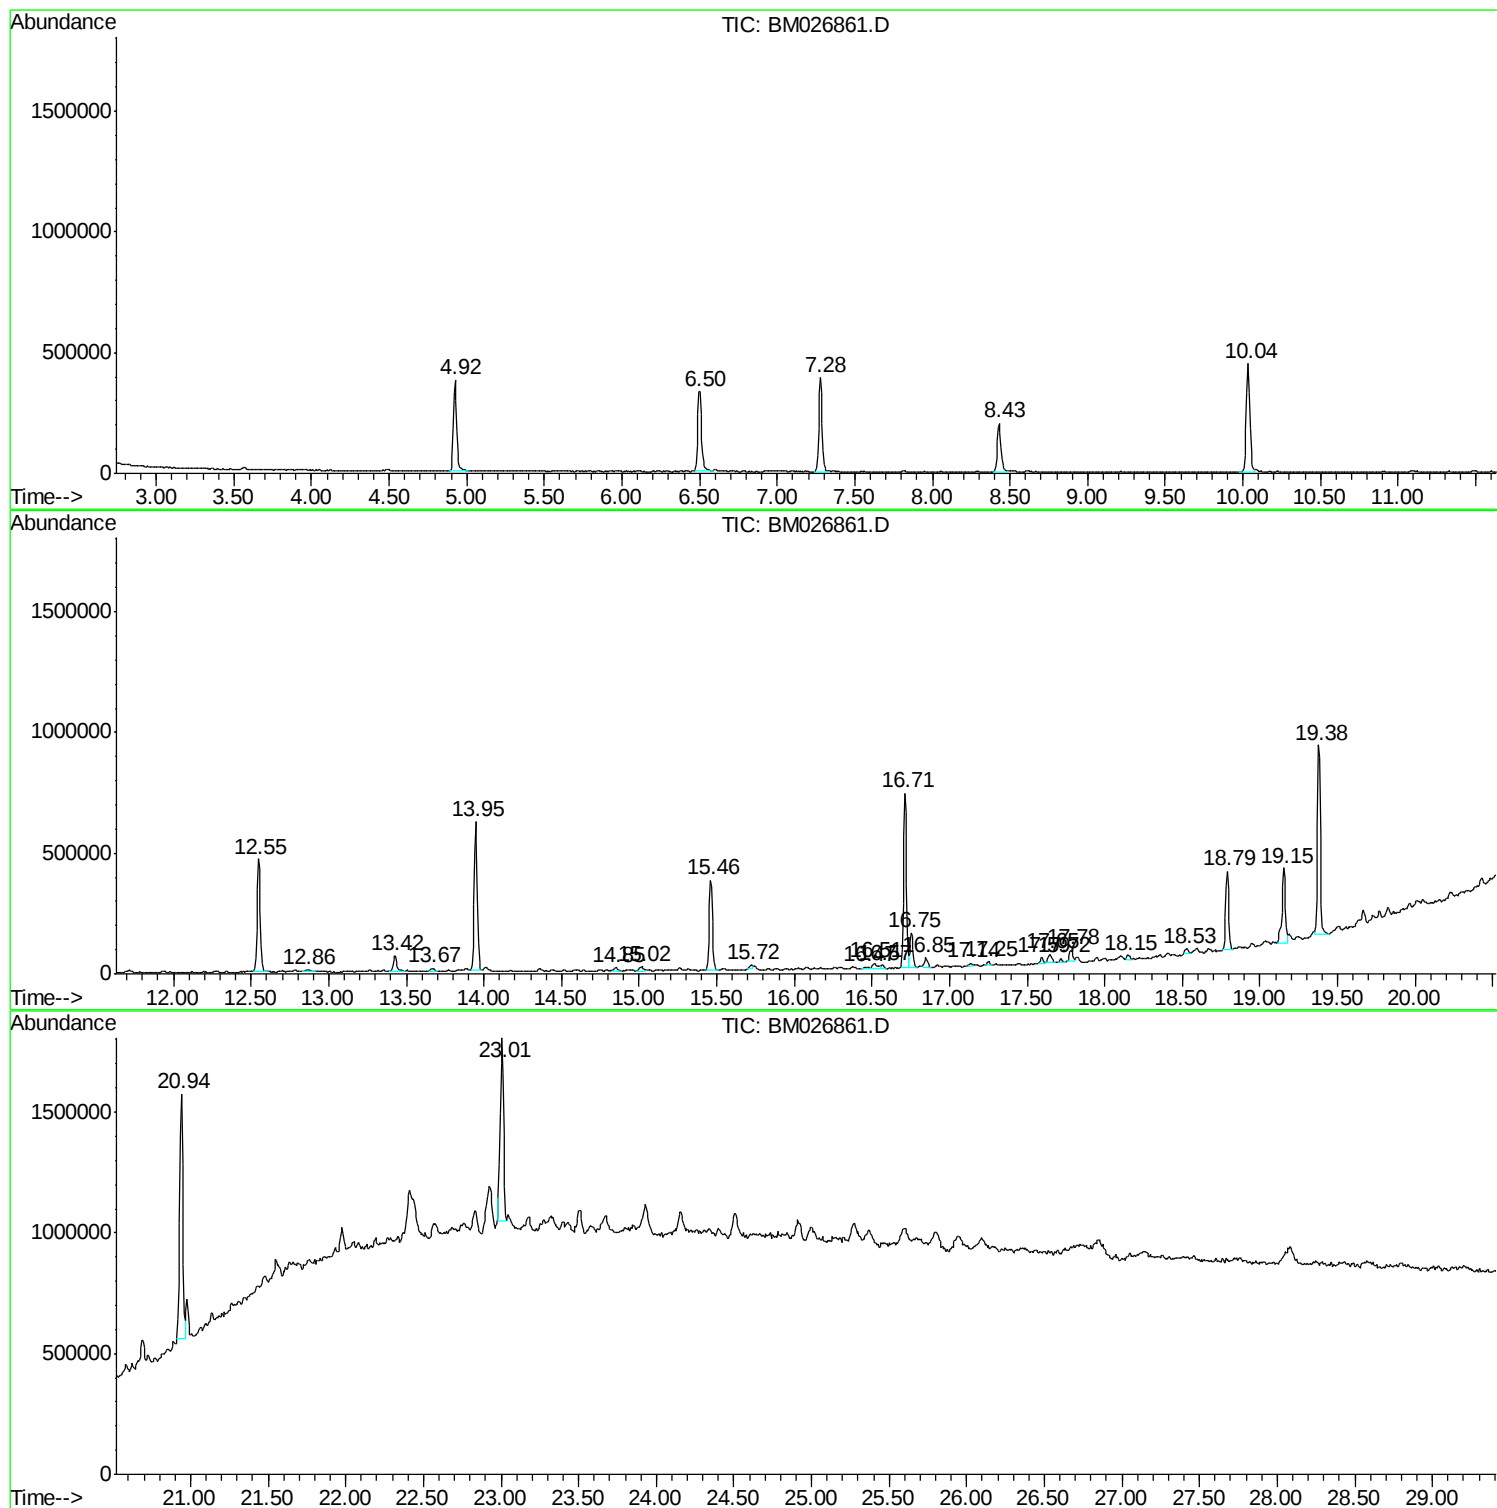

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM072320\
Data File : BM026861.D
Acq On : 23 Jul 2020 21:11
Operator : JU/CG
Sample : L3381-19 2X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VNJ-225-GRID-B5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM072320\
Data File : BM026861.D
Acq On : 23 Jul 2020 21:11
Operator : JU/CG
Sample : L3381-19 2X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VNJ-225-GRID-B5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc