


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM072320\
 Data File : BM026847.D
 Acq On : 23 Jul 2020 11:59
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 22 14:16:10 2020

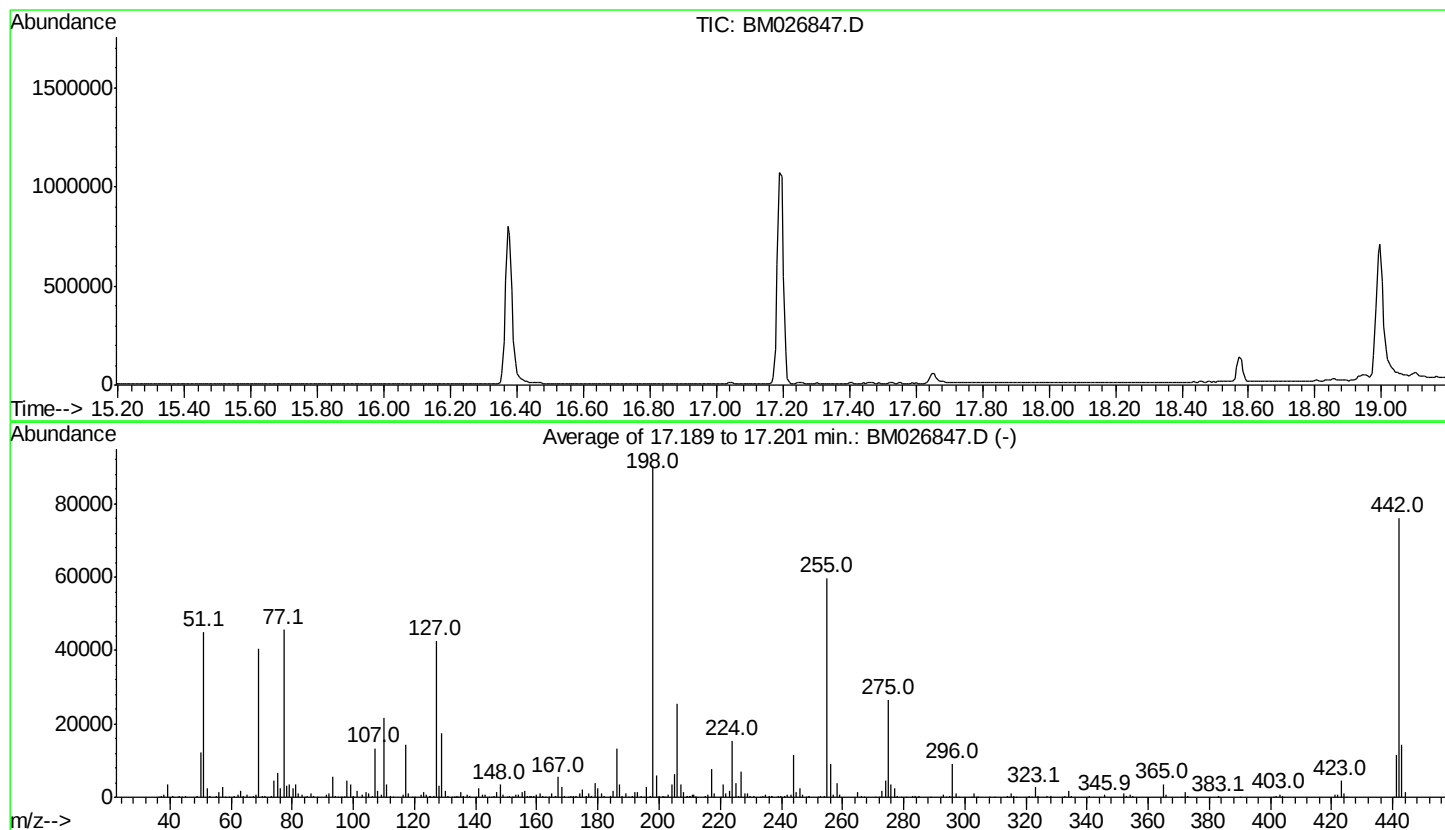

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.9	45154	PASS
68	69	0.00	2	1.8	724	PASS
69	198	0.00	100	44.7	40414	PASS
70	69	0.00	2	0.6	244	PASS
127	198	10	80	47.2	42720	PASS
197	198	0.00	2	0.3	269	PASS
198	198	100	100	100.0	90434	PASS
199	198	5	9	6.7	6048	PASS
275	198	10	60	29.4	26544	PASS
365	198	1	100	3.9	3540	PASS
441	198	0.01	100	12.6	11392	PASS
442	198	50	100	84.3	76192	PASS
443	442	15	24	18.6	14187	PASS