

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072321\
 Data File : BM031135.D
 Acq On : 25 Jul 2021 00:35
 Operator : CG/JU
 Sample : M2973-19
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGED6

Quant Time: Jul 26 02:58:35 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM072221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 26 02:23:23 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.639	152	1197	0.40	ng/ul	0.00
4) Naphthalene-d8	10.401	136	4827	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.262	164	3474	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.006	188	7486	0.40	ng/ul	0.00
17) Chrysene-d12	21.193	240	7790	0.40	ng/ul	0.00
23) Perylene-d12	23.365	264	7816	0.40	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.213	96	6180	4.91	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.993	152	2607	0.31	ng/ul	0.00
18) Fluoranthene-d10	19.035	212	8324	0.35	ng/ul	0.00
Target Compounds						
						Qvalue
15) Phenanthrene	17.051	178	659	0.03	ng/ul#	80
19) Fluoranthene	19.070	202	702	0.02	ng/ul#	49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072321\
Data File : BM031135.D
Acq On : 25 Jul 2021 00:35
Operator : CG/JU
Sample : M2973-19
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGED6

Quant Time: Jul 26 02:58:35 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 26 02:23:23 2021
Response via : Initial Calibration




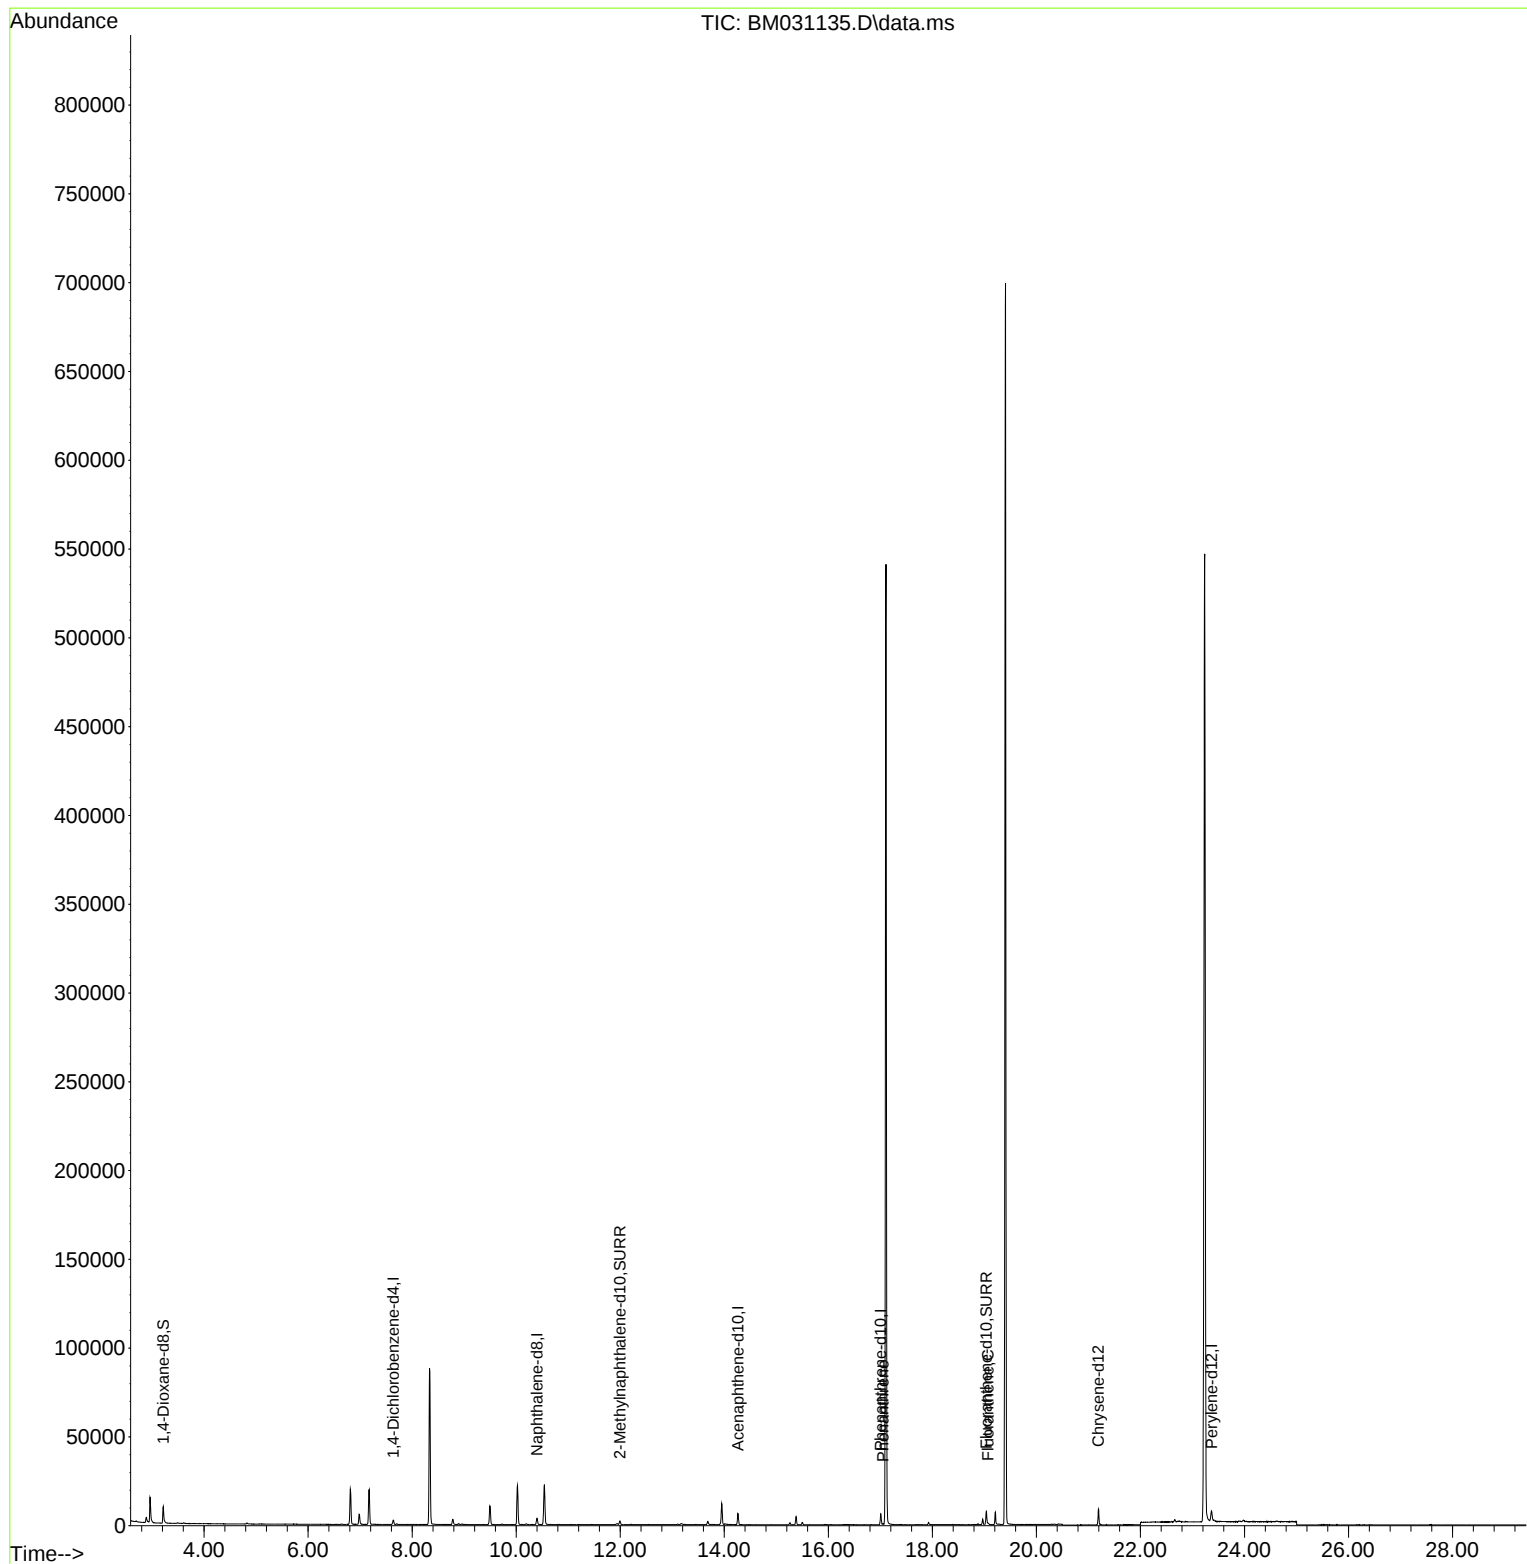


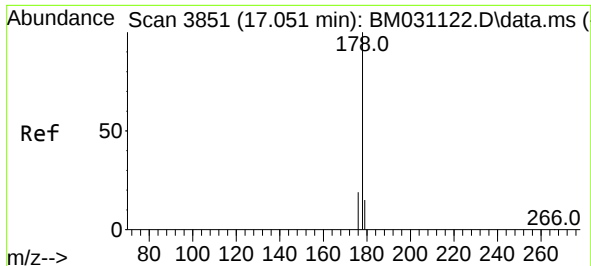

#15
Phenanthrene
Concen: 0.03 ng/ul
RT: 17.051 min Scan# 3851
Delta R.T. -0.003 min
Lab File: BM031135.D
Acq: 25 Jul 2021 00:35

Instrument :
BNA_M
ClientSampleId :
BGED6

Tgt Ion:178 Resp: 659
Ion Ratio Lower Upper
178 100
179 26.2 13.3 19.9#
176 27.1 15.4 23.2#

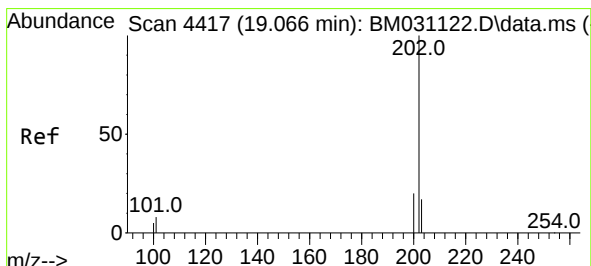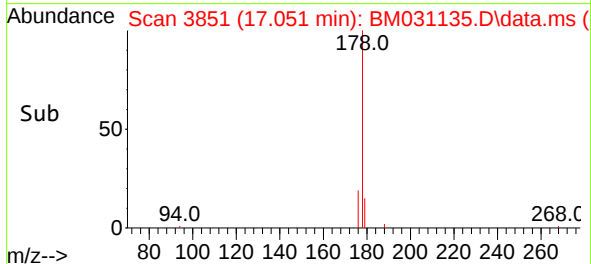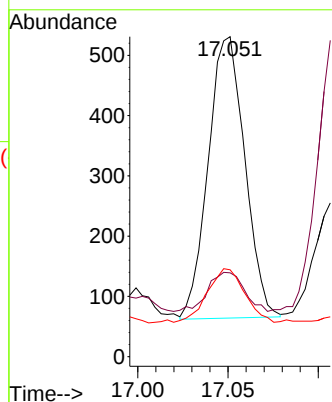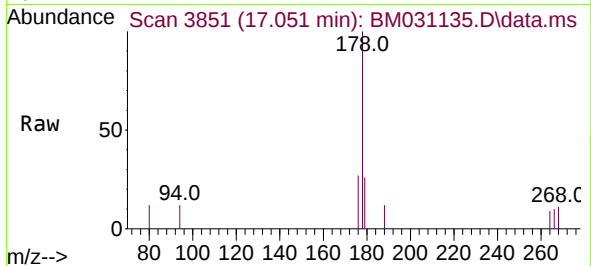

#19
Fluoranthene
Concen: 0.02 ng/ul
RT: 19.070 min Scan# 4418
Delta R.T. 0.000 min
Lab File: BM031135.D
Acq: 25 Jul 2021 00:35

Tgt Ion:202 Resp: 702
Ion Ratio Lower Upper
202 100
101 27.6 6.0 9.0#
100 20.6 4.8 7.2#

