

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072321\
 Data File : BM031143.D
 Acq On : 25 Jul 2021 06:07
 Operator : CG/JU
 Sample : M2973-18
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGED5

Quant Time: Jul 26 03:49:56 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM072221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 26 03:04:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.635	152	1400	0.40	ng/ul	0.00
4) Naphthalene-d8	10.397	136	5640	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.262	164	3872	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.006	188	8316	0.40	ng/ul	# 0.00
17) Chrysene-d12	21.190	240	8036	0.40	ng/ul	0.00
23) Perylene-d12	23.360	264	8073	0.40	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.213	96	6905	4.70	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.989	152	2948	0.30	ng/ul	0.00
18) Fluoranthene-d10	19.035	212	8271	0.34	ng/ul	0.00
Target Compounds						
15) Phenanthrene	17.048	178	694	0.03	ng/ul#	Qvalue 77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072321\
Data File : BM031143.D
Acq On : 25 Jul 2021 06:07
Operator : CG/JU
Sample : M2973-18
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGED5


Quant Time: Jul 26 03:49:56 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 26 03:04:43 2021
Response via : Initial Calibration

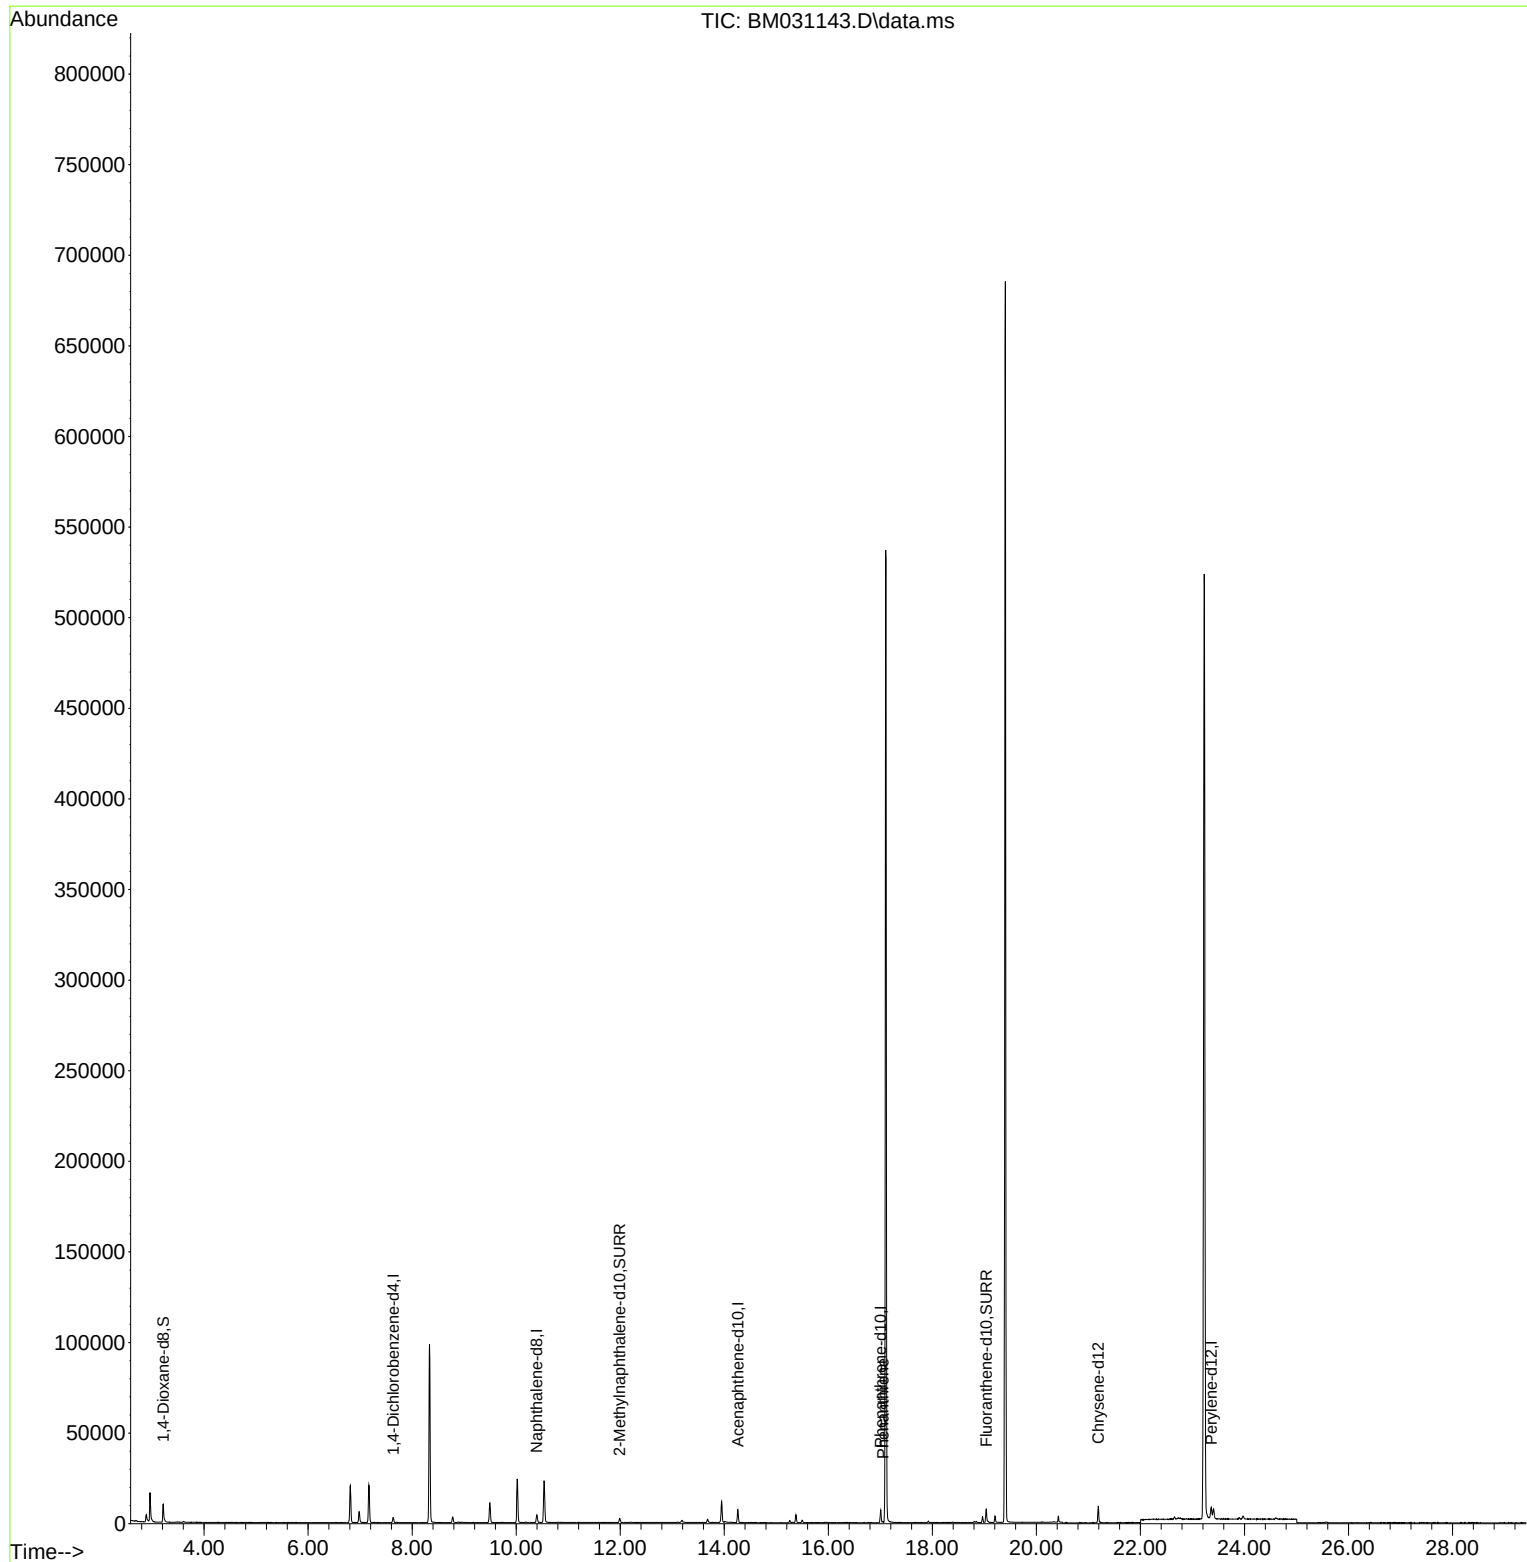

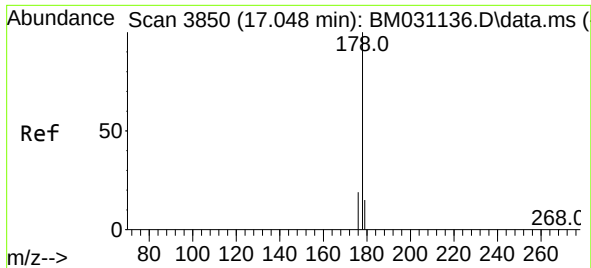

#15
 Phenanthrene
 Concen: 0.03 ng/ul
 RT: 17.048 min Scan# 3850
 Delta R.T. -0.007 min
 Lab File: BM031143.D
 Acq: 25 Jul 2021 06:07

Instrument :
 BNA_M
 ClientSampleId :
 BGED5

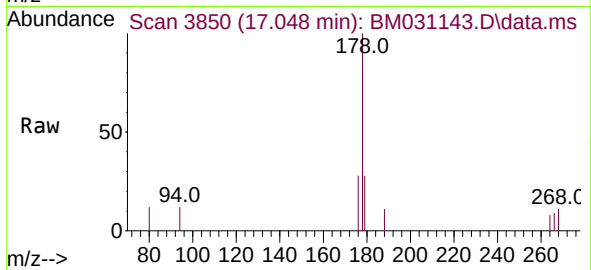

Tgt Ion:	178	Resp:	694
Ion	Ratio	Lower	Upper
178	100		
179	28.4	13.3	19.9#
176	27.8	15.4	23.2#

