

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072321\
 Data File : BM031149.D
 Acq On : 25 Jul 2021 09:46
 Operator : CG/JU
 Sample : M2973-15
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGE20

Quant Time: Jul 26 04:06:12 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM072221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 26 03:04:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.632	152	1349	0.40	ng/ul	-0.01
4) Naphthalene-d8	10.397	136	5424	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.262	164	3790	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.006	188	7967	0.40	ng/ul	0.00
17) Chrysene-d12	21.190	240	7285	0.40	ng/ul	0.00
23) Perylene-d12	23.360	264	7009	0.40	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.213	96	7271	5.13	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.989	152	3006	0.32	ng/ul	0.00
18) Fluoranthene-d10	19.031	212	7568	0.34	ng/ul	-0.01
Target Compounds						
						Qvalue
11) Acenaphthene	14.322	153	783	0.06	ng/ul	97
15) Phenanthrene	17.048	178	548	0.02	ng/ul#	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072321\
Data File : BM031149.D
Acq On : 25 Jul 2021 09:46
Operator : CG/JU
Sample : M2973-15
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGE20

Quant Time: Jul 26 04:06:12 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 26 03:04:43 2021
Response via : Initial Calibration




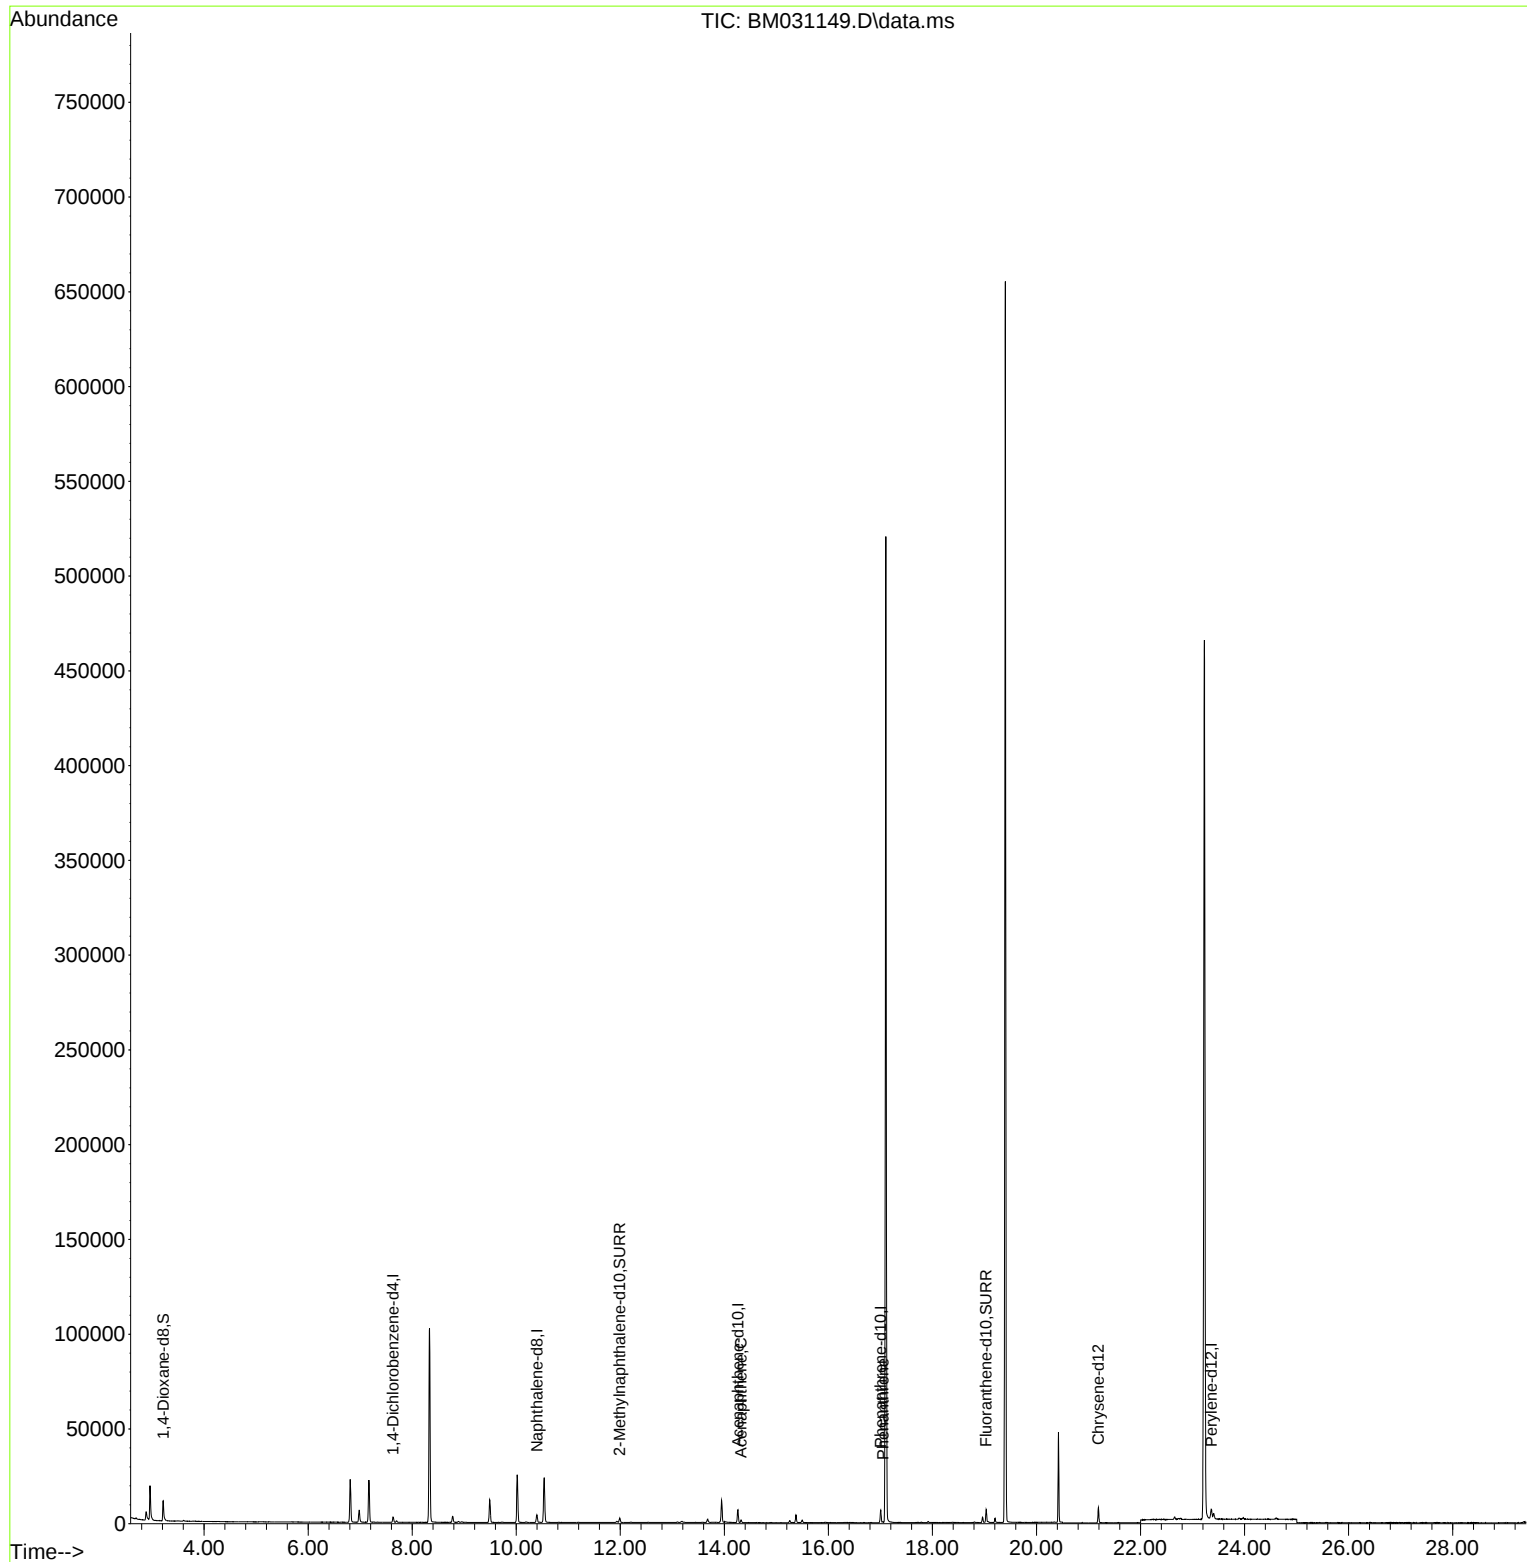


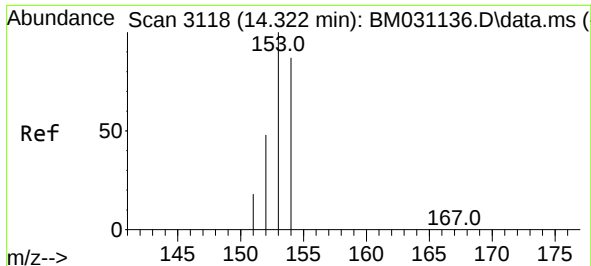

#11
Acenaphthene
Concen: 0.06 ng/ul
RT: 14.322 min Scan# 3118
Delta R.T. -0.008 min
Lab File: BM031149.D
Acq: 25 Jul 2021 09:46

Instrument :
BNA_M
ClientSampled :
BGE20

Tgt Ion:153 Resp: 783
Ion Ratio Lower Upper
153 100
152 50.8 39.4 59.2
154 88.4 68.2 102.4

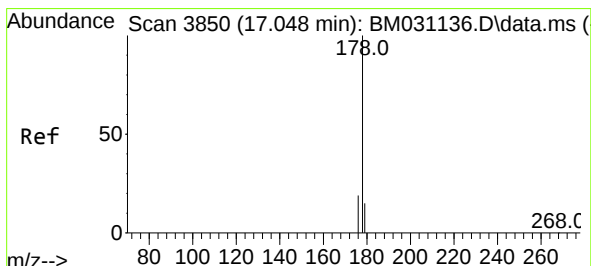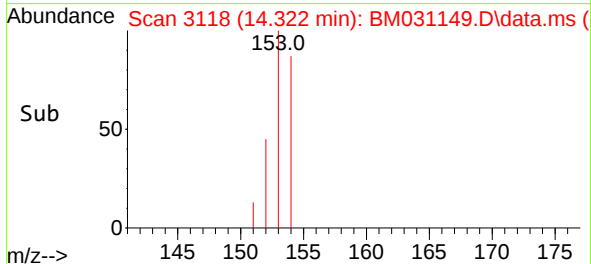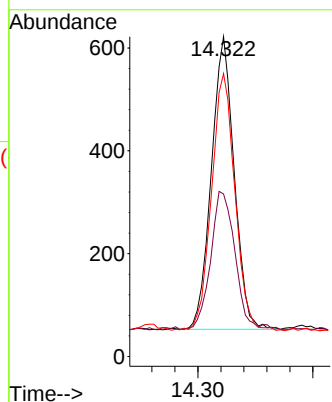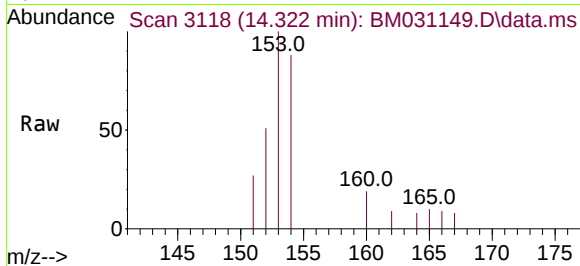

#15
Phenanthrene
Concen: 0.02 ng/ul
RT: 17.048 min Scan# 3850
Delta R.T. -0.007 min
Lab File: BM031149.D
Acq: 25 Jul 2021 09:46

Tgt Ion:178 Resp: 548
Ion Ratio Lower Upper
178 100
179 29.3 13.3 19.9#
176 25.6 15.4 23.2#

