


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM072418\
Data File : BM016054.D
Acq On : 24 Jul 2018 14:12
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jul 23 16:08:38 2018

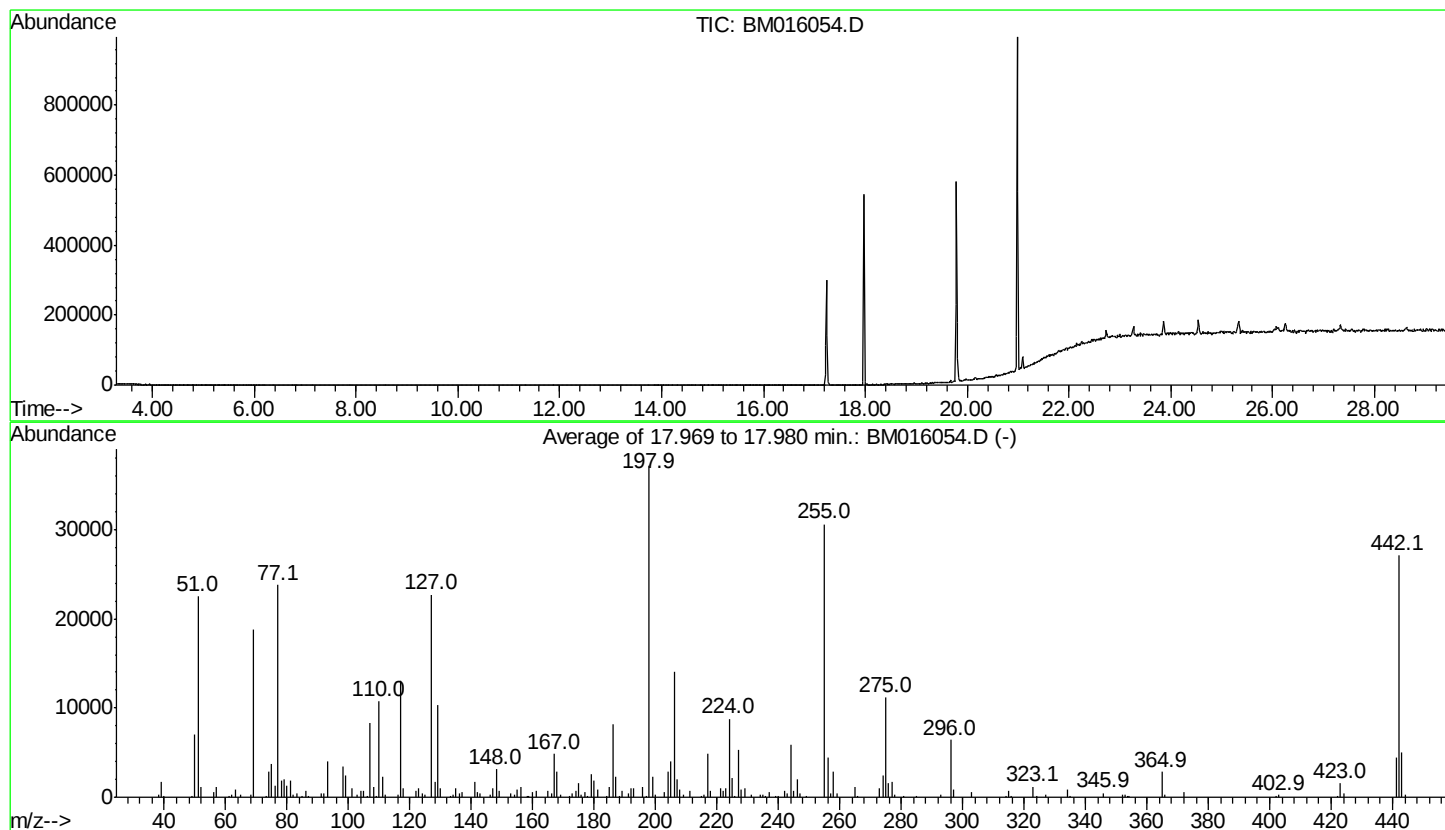

Spectrum Information: Average of 17.969 to 17.980 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.5	22479	PASS
68	69	0.00	2	1.3	236	PASS
69	198	0.00	100	50.4	18736	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	61.1	22698	PASS
197	198	0.00	2	0.3	120	PASS
198	198	100	100	100.0	37176	PASS
199	198	5	9	6.3	2354	PASS
275	198	10	60	29.9	11129	PASS
365	198	1	100	7.5	2804	PASS
441	198	0.01	100	11.9	4407	PASS
442	198	50	100	72.9	27093	PASS
443	442	15	24	18.5	5011	PASS