

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072419\
 Data File : BM021629.D
 Acq On : 24 Jul 2019 17:00
 Operator : HP/JU
 Sample : PB121431BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK31

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072319MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.881	656	662	675	rVB	396364	686813	12.67%	1.864%
2	7.051	686	691	702	rVB	322863	531548	9.81%	1.443%
3	7.240	717	723	739	rVB	434232	760260	14.03%	2.064%
4	7.704	796	802	808	rVB	303156	480339	8.86%	1.304%
5	8.410	916	922	932	rBV	557880	914702	16.88%	2.483%
6	8.869	994	1000	1012	rVB	456931	794585	14.66%	2.157%
7	9.581	1115	1121	1132	rVB	377718	611809	11.29%	1.661%
8	10.110	1205	1211	1230	rBV	545795	1020043	18.82%	2.769%
9	10.486	1268	1275	1282	rVB	456281	770170	14.21%	2.091%
10	10.639	1294	1301	1320	rBV	507849	1042617	19.24%	2.830%
11	12.098	1543	1549	1554	rVB	6393	10396	0.19%	0.028%
12	13.763	1826	1832	1849	rVB	1357851	1891327	34.90%	5.134%
13	14.039	1872	1879	1892	rBV	1545446	2188829	40.39%	5.942%
14	14.345	1925	1931	1939	rBV	856351	1219788	22.51%	3.311%
15	14.574	1964	1970	1991	rBV	302810	692538	12.78%	1.880%
16	15.345	2094	2101	2112	rBV	2098530	2893354	53.39%	7.854%
17	15.480	2119	2124	2138	rBV	390580	611460	11.28%	1.660%
18	15.586	2138	2142	2147	rVB3	18459	23594	0.44%	0.064%
19	16.127	2229	2234	2238	rBV4	5362	6463	0.12%	0.018%
20	17.098	2393	2399	2407	rBV2	1184938	1625782	30.00%	4.413%
21	17.198	2409	2416	2432	rVV	2343017	3351035	61.84%	9.097%
22	19.133	2741	2745	2749	rBV3	19843	28486	0.53%	0.077%
23	19.386	2784	2788	2792	rBV	17833	23281	0.43%	0.063%
24	19.498	2801	2807	2816	rBV	3374491	4372666	80.69%	11.870%
25	21.292	3107	3112	3120	rBV	1696317	2295866	42.37%	6.232%
26	23.397	3464	3470	3481	rVB	2903804	5418993	100.00%	14.710%
27	23.544	3489	3495	3507	rVB	1312436	2571932	47.46%	6.982%


Sum of corrected areas: 36838676

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072419\
Data File : BM021629.D
Acq On : 24 Jul 2019 17:00
Operator : HP/JU
Sample : PB121431BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK31

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072319MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

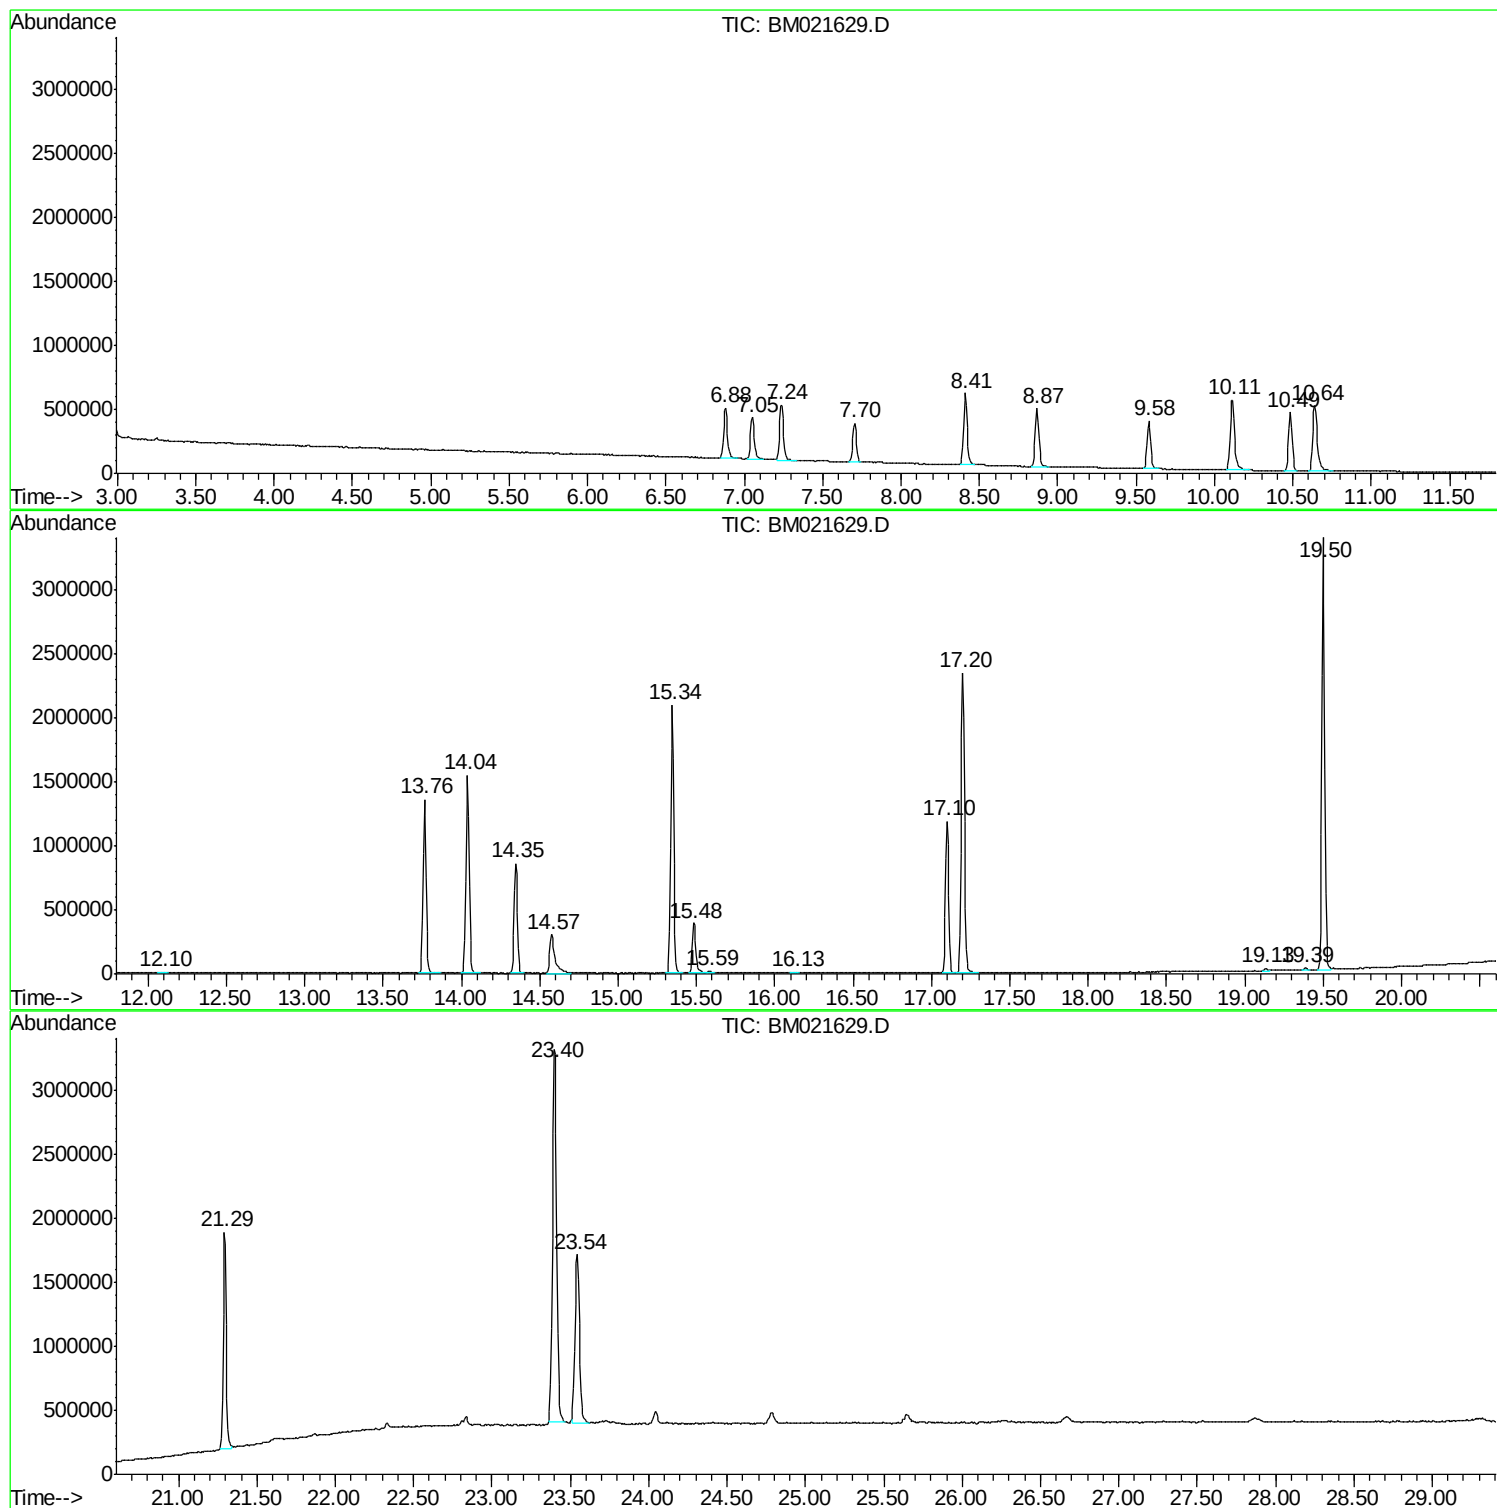

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM072419\
Data File : BM021629.D
Acq On : 24 Jul 2019 17:00
Operator : HP/JU
Sample : PB121431BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK31

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072319MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM072419\
Data File : BM021629.D
Acq On : 24 Jul 2019 17:00
Operator : HP/JU
Sample : PB121431BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK31

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072319MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc