

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072423\
 Data File : BM041095.D
 Acq On : 25 Jul 2023 03:31
 Operator : MA/JU
 Sample : 03534-08
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4720

Quant Time: Jul 25 04:03:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 25 00:13:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.832	152	3611	0.400	ng/ul	0.00
4) Naphthalene-d8	10.636	136	11953	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.490	164	5939	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.248	188	11724	0.400	ng/ul	0.00
17) Chrysene-d12	21.451	240	9961	0.400	ng/ul	0.00
23) Perylene-d12	23.830	264	12680	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.250	96	23662	4.248	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.242	152	4892	0.287	ng/ul	0.00
18) Fluoranthene-d10	19.283	212	8671	0.320	ng/ul	0.00
Target Compounds						
					Qvalue	
24) Benzo(b)fluoranthene	23.108	252	1236	0.024	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072423\
Data File : BM041095.D
Acq On : 25 Jul 2023 03:31
Operator : MA/JU
Sample : 03534-08
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4720

Quant Time: Jul 25 04:03:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 00:13:11 2023
Response via : Initial Calibration

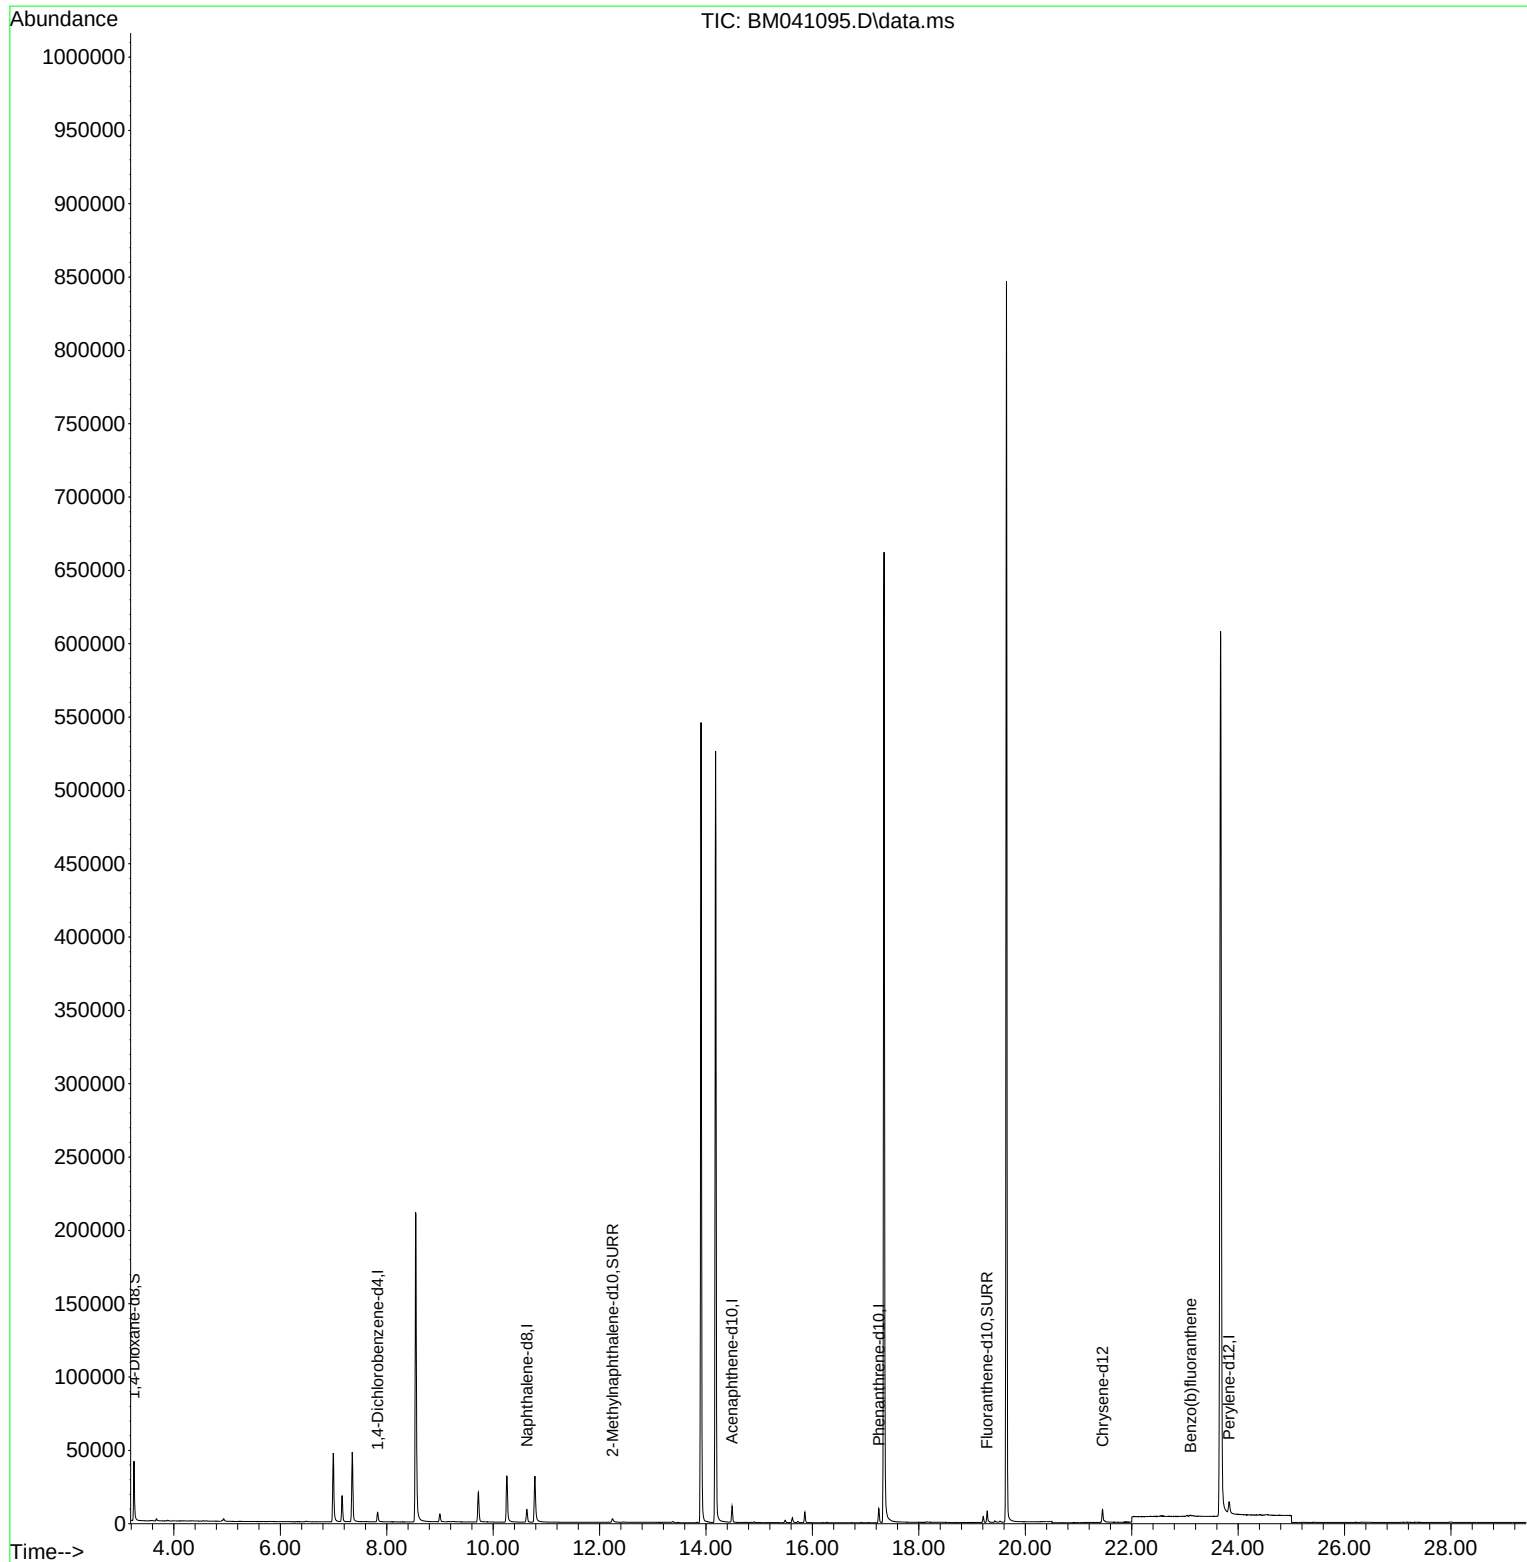

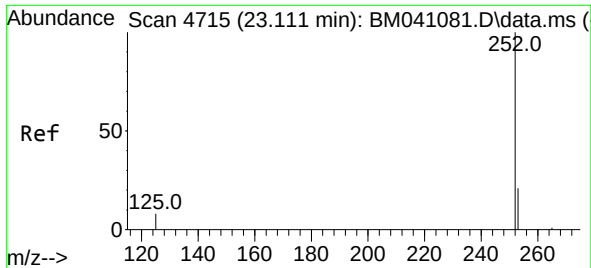

#24

Benzo(b)fluoranthene

Concen: 0.024 ng/ul

RT: 23.108 min Scan# 41

Delta R.T. -0.009 min

Lab File: BM041095.D


Acq: 25 Jul 2023 03:31

Instrument :

BNA_M

ClientSampleId :

A4720

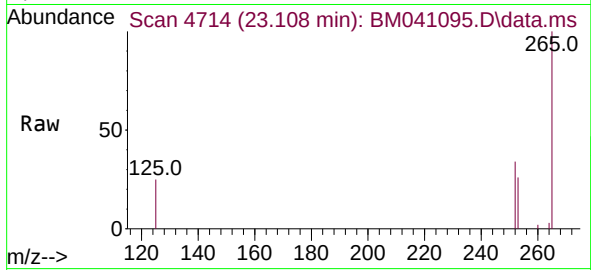

Tgt Ion:252 Resp: 1236

Ion Ratio Lower Upper

252 100

253 77.5 0.0 57.6#

125 74.3 0.0 33.6#

