

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072519\
 Data File : BM021653.D
 Acq On : 26 Jul 2019 01:18
 Operator : HP/JU
 Sample : PB121603BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jul 26 01:51:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 24 01:21:49 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	105176	20.00	ng/ul	0.00
18) Naphthalene-d8	10.48	136	501832	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.35	164	377601	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.10	188	904262	20.00	ng/ul	0.00
77) Chrysene-d12	21.29	240	1059002	20.00	ng/ul	0.00
85) Perylene-d12	23.53	264	1099770	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.25	96	12195	6.32	ng/uL	0.00
5) Phenol-d5	6.88	99	313795	35.18	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	186798	36.10	ng/ul	0.00
9) 2-Chlorophenol-d4	7.23	132	261987	37.45	ng/ul	0.00
13) 4-Methylphenol-d8	8.40	113	288360	37.84	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	148307	39.93	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	170033	42.67	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.10	165	331107	37.26	ng/ul	0.00
29) 4-Chloroaniline-d4	10.63	131	439590	51.00	ng/ul	0.00
43) Dimethylphthalate-d6	13.76	166	1212607	37.48	ng/ul	0.00
46) Acenaphthylene-d8	14.03	160	1367892	34.76	ng/ul	0.00
51) 4-Nitrophenol-d4	14.57	143	170871	30.79	ng/ul	0.00
57) Fluorene-d10	15.34	176	1066177	36.52	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.48	200	138637	24.48	ng/ul	0.00
70) Anthracene-d10	17.20	188	1884965	42.37	ng/ul	0.00
78) Pyrene-d10	19.49	212	2327565	45.04	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.39	264	2514291	42.82	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
15) N-Nitroso-di-n-propylamine	8.40	70	7356	1.307	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072519\
Data File : BM021653.D
Acq On : 26 Jul 2019 01:18
Operator : HP/JU
Sample : PB121603BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jul 26 01:51:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 24 01:21:49 2019
Response via : Initial Calibration

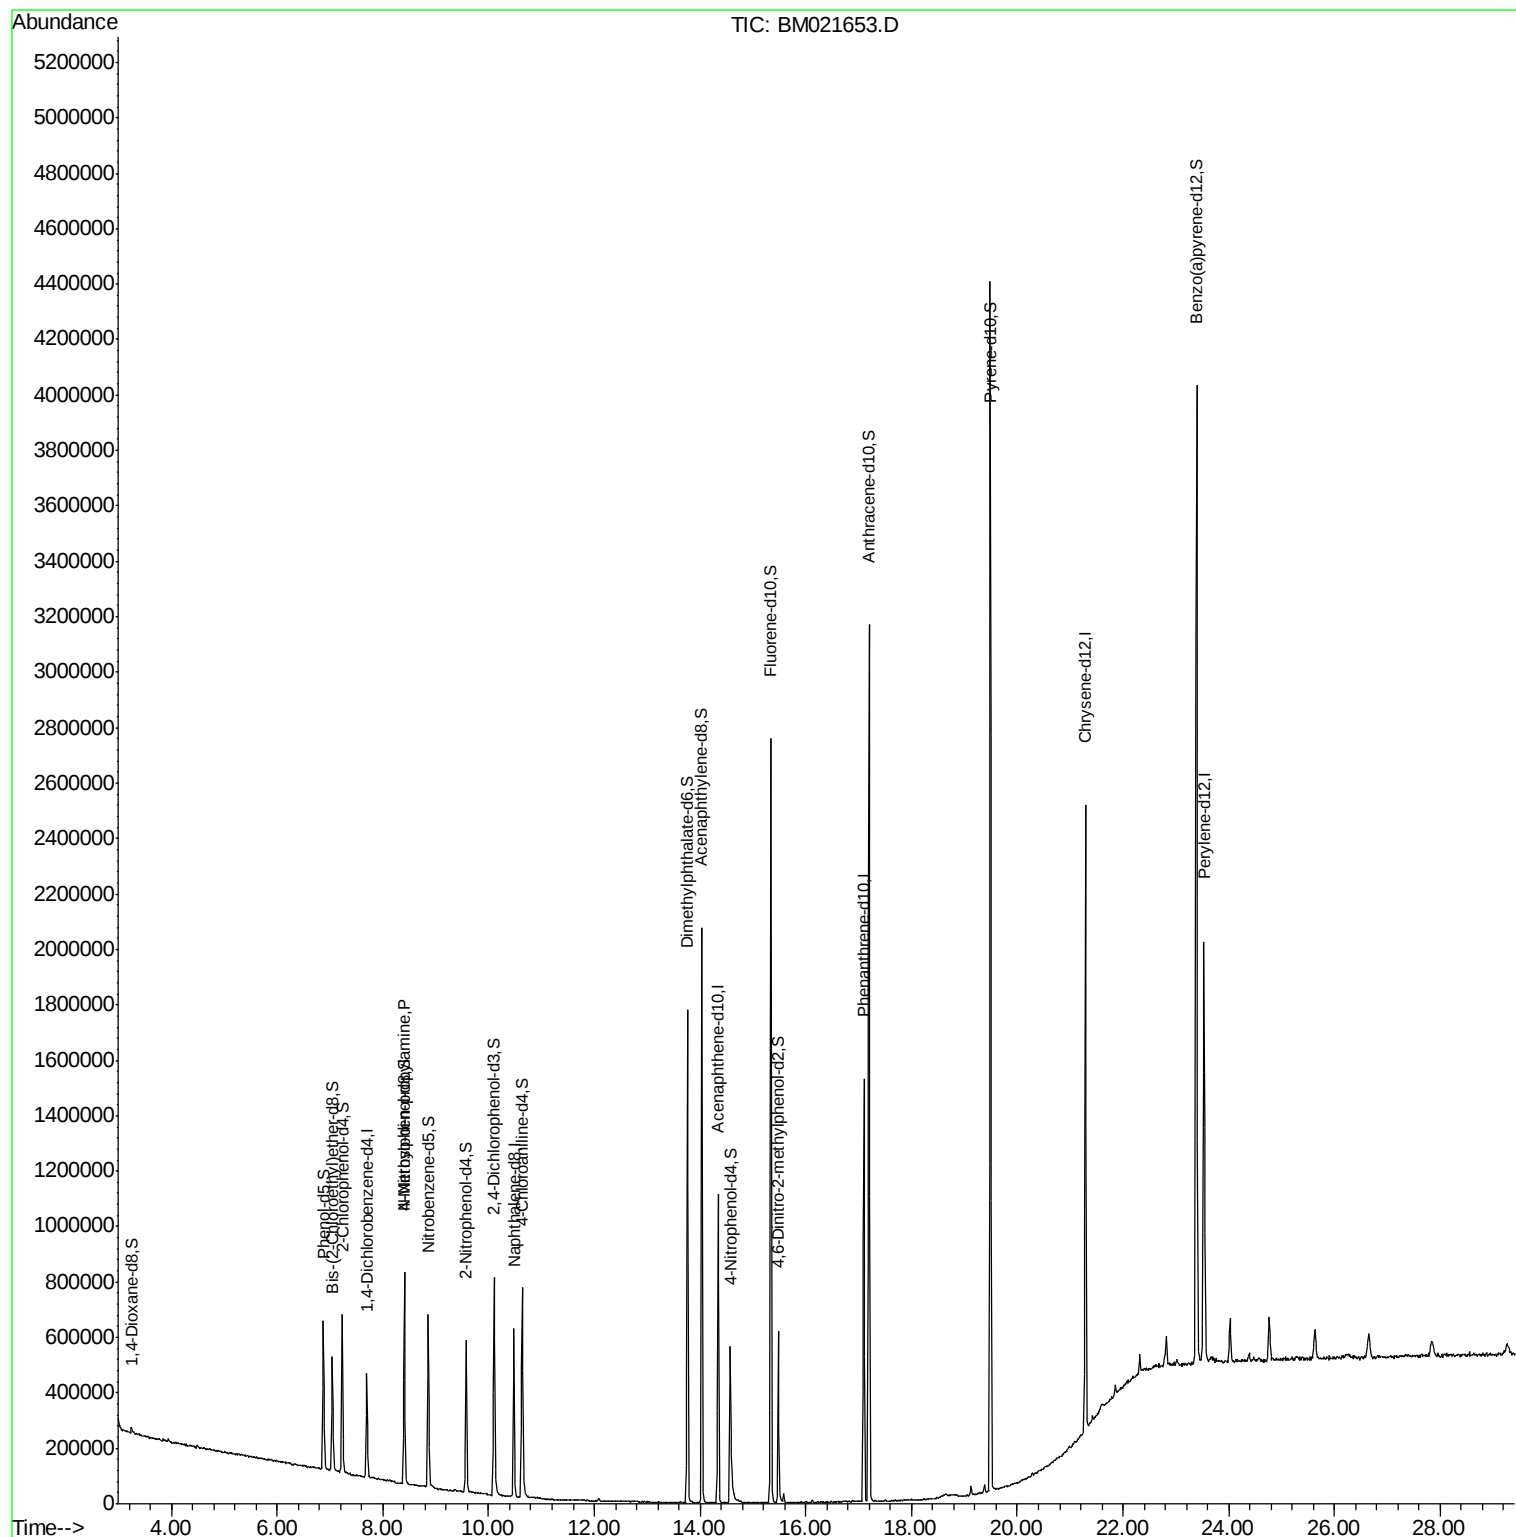

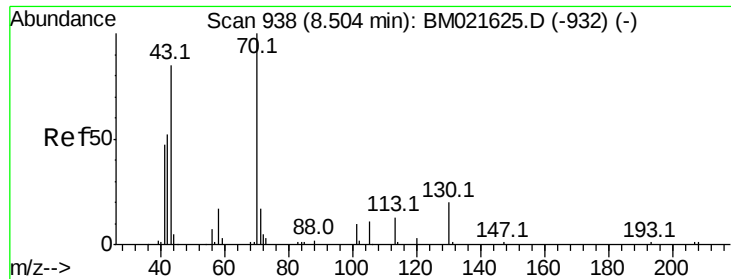

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.307 ng/ul
 RT: 8.40 min Scan# 921
 Delta R.T. -0.11 min
 Lab File: BM021653.D
 Acq: 26 Jul 2019 01:18

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion: 70 Resp: 7356
 Ion Ratio Lower Upper
 70 100
 42 360.3 42.2 63.2#
 101 0.0 7.6 11.4#
 130 0.0 16.7 25.1#

