

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072519\
 Data File : BM021667.D
 Acq On : 26 Jul 2019 10:23
 Operator : HP/JU
 Sample : K3893-20
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEP24

Quant Time: Jul 26 11:26:04 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 24 01:21:49 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	115570	20.00	ng/ul	0.00
18) Naphthalene-d8	10.47	136	536215	20.00	ng/ul	-0.01
35) Acenaphthene-d10	14.34	164	389883	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.09	188	933799	20.00	ng/ul	0.00
77) Chrysene-d12	21.29	240	1081447	20.00	ng/ul	0.00
85) Perylene-d12	23.53	264	1092330	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.25	96	12113	5.71	ng/uL	0.00
5) Phenol-d5	6.88	99	253598	25.87	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	155522	27.35	ng/ul	0.00
9) 2-Chlorophenol-d4	7.23	132	212460	27.64	ng/ul	0.00
13) 4-Methylphenol-d8	8.40	113	231273	27.62	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	117113	29.51	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	131616	30.91	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.10	165	269381	28.37	ng/ul	0.00
29) 4-Chloroaniline-d4	10.63	131	346685	37.64	ng/ul	0.00
43) Dimethylphthalate-d6	13.76	166	915311	27.40	ng/ul	0.00
46) Acenaphthylene-d8	14.03	160	1073205	26.41	ng/ul	0.00
51) 4-Nitrophenol-d4	14.57	143	87629	15.29	ng/ul	0.00
57) Fluorene-d10	15.34	176	832105	27.61	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.48	200	67863	11.60	ng/ul	0.00
70) Anthracene-d10	17.19	188	1392207	30.30	ng/ul	0.00
78) Pyrene-d10	19.49	212	1734194	32.86	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.39	264	1756637	30.12	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.80	163	232353	7.245	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072519\
Data File : BM021667.D
Acq On : 26 Jul 2019 10:23
Operator : HP/JU
Sample : K3893-20
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEP24

Quant Time: Jul 26 11:26:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 24 01:21:49 2019
Response via : Initial Calibration

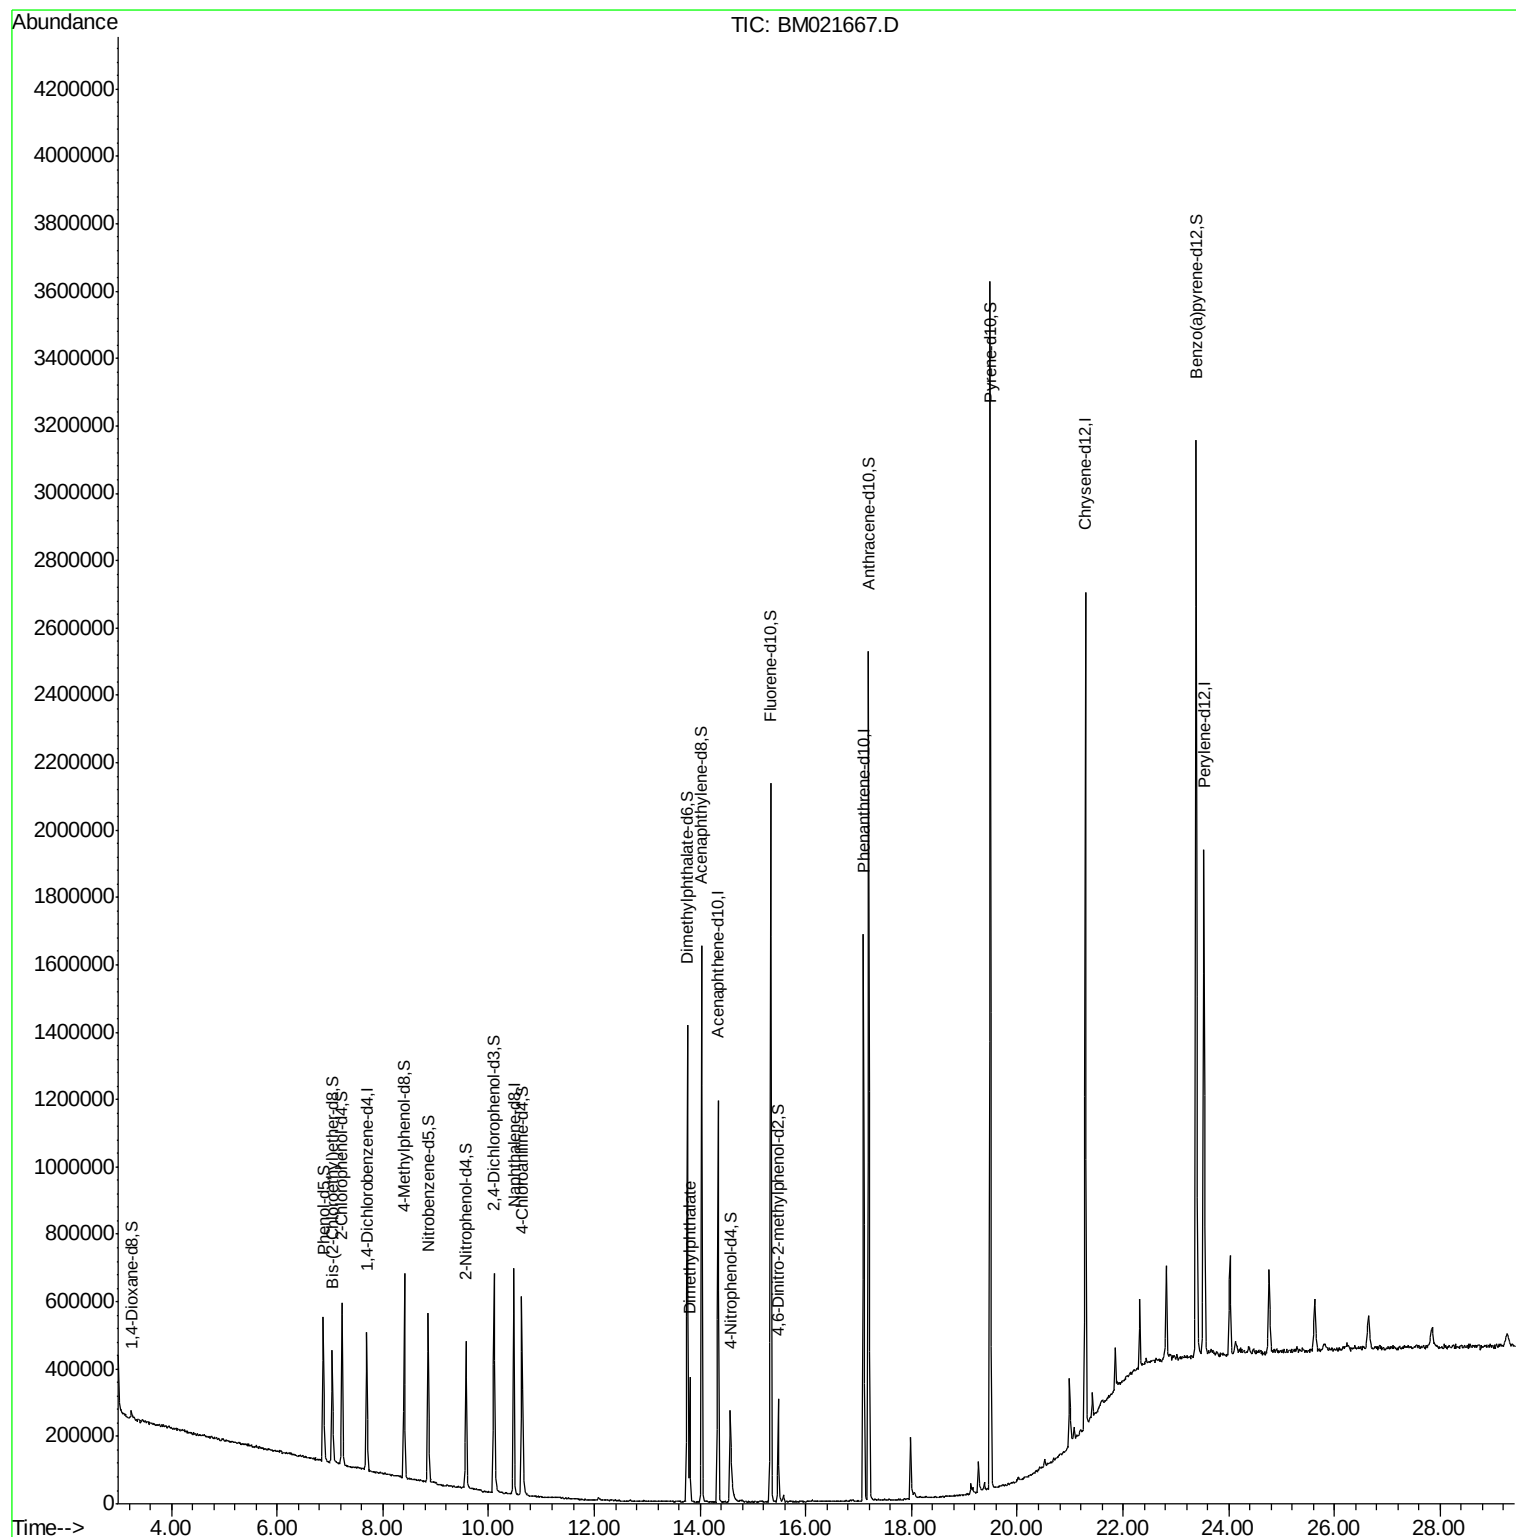

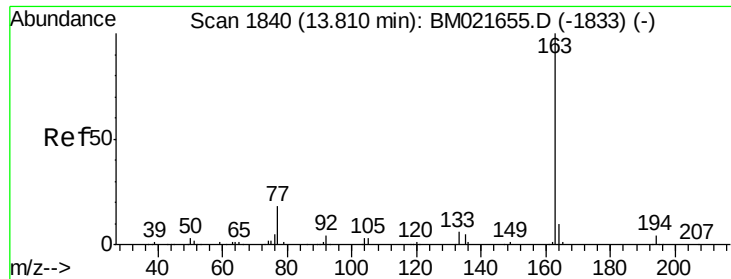

#44

Dimethylphthalate

Concen: 7.245 ng/ul

RT: 13.80 min Scan# 1839

Delta R.T. -0.01 min

Lab File: BM021667.D

Acq: 26 Jul 2019 10:23

Instrument :

BNA_M

ClientSampleId :

BEP24


Tot Ion:163 Resp: 232353

Ion Ratio Lower Upper

163 100

194 4.4 3.2 4.8

164 10.1 8.2 12.4

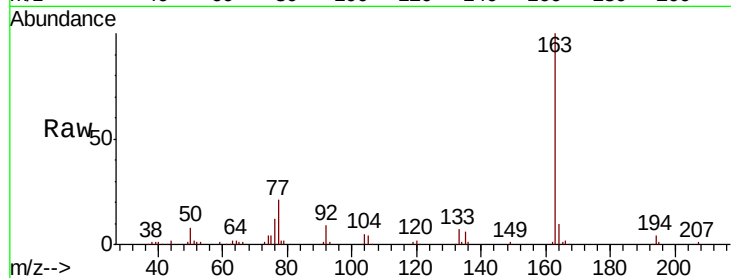

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

