


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM072621\
Data File : BM031181.D
Acq On : 27 Jul 2021 03:03
Operator : CG/JU
Sample : PB137860BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK860

Manual Integrations
APPROVED

mohammad
7/27/2021 12:09:50 PM

Quant Time: Jul 27 07:12:15 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 22 01:52:16 2021
Response via : Initial Calibration

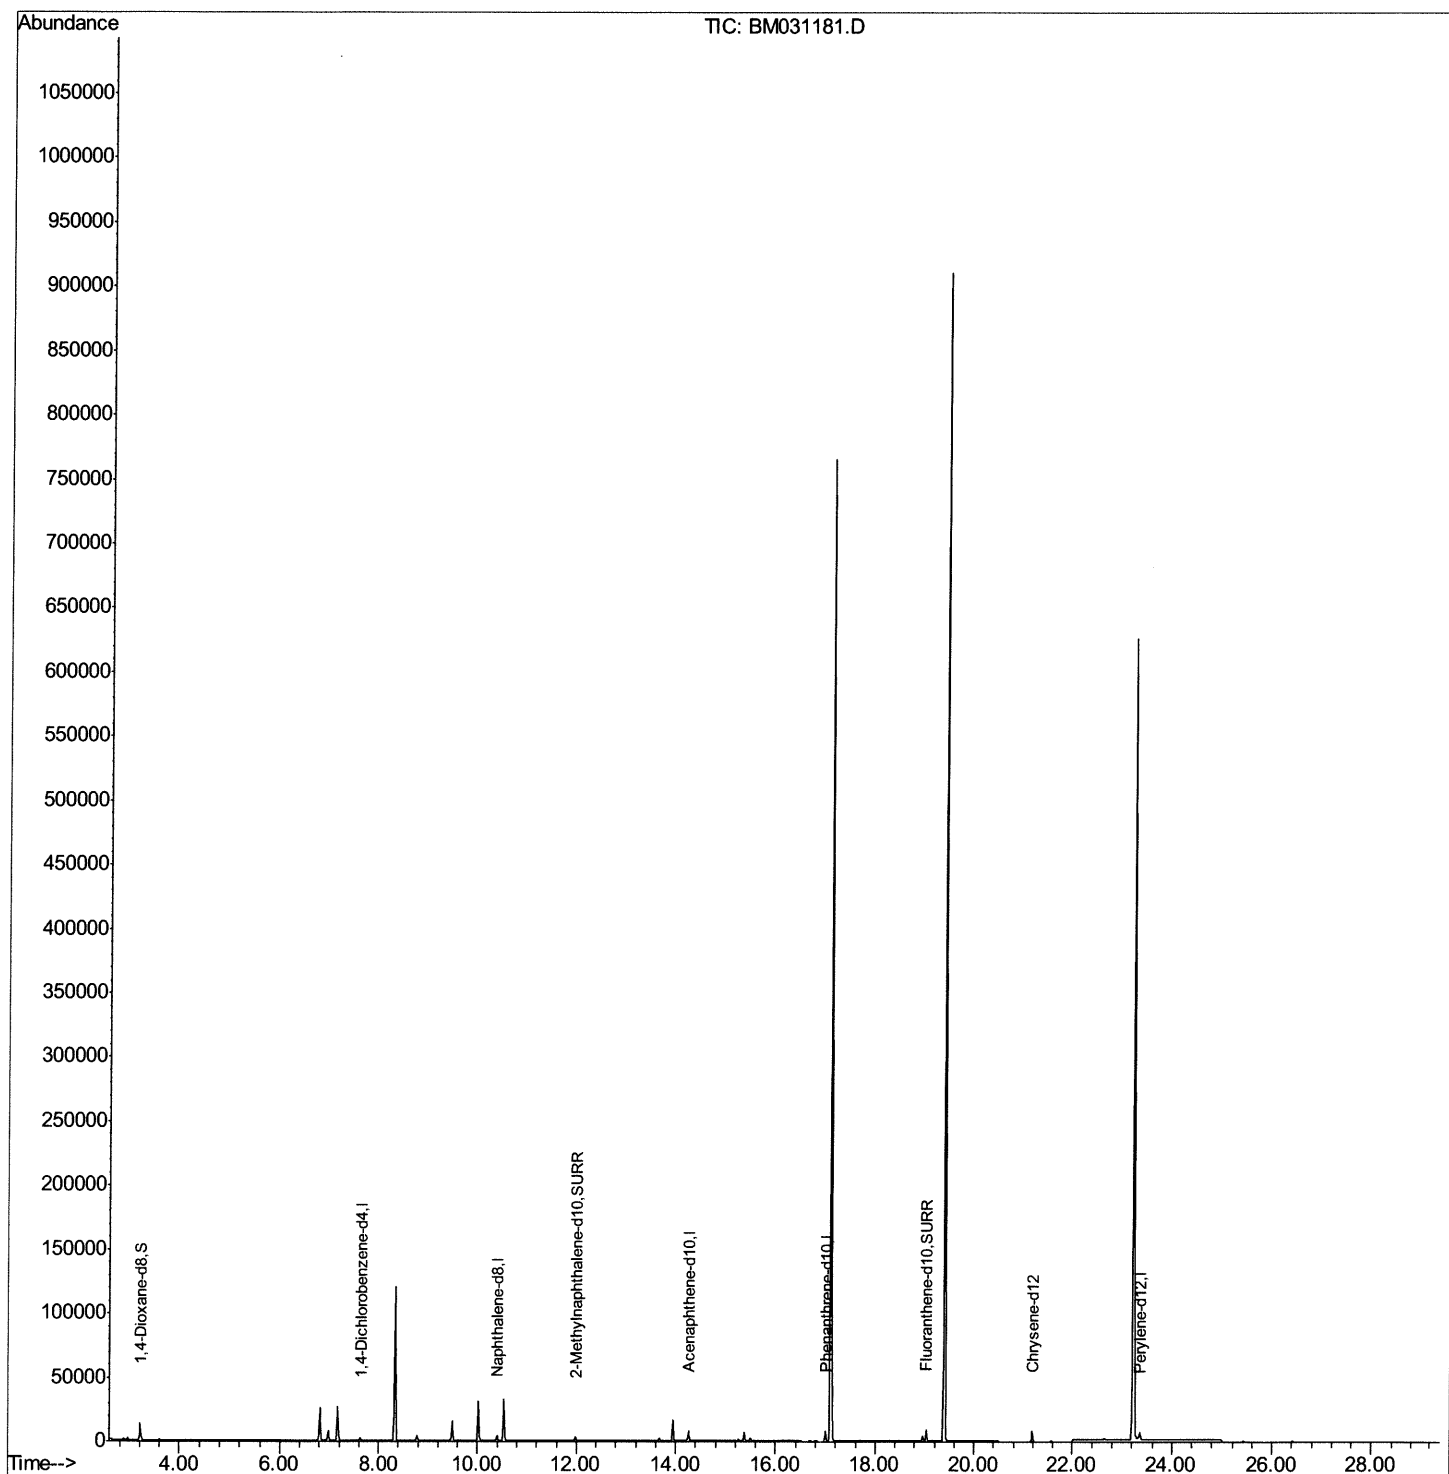

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM072621\
Data File : BM031181.D
Acq On : 27 Jul 2021 03:03
Operator : CG/JU
Sample : PB137860BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK860

Manual Integrations
APPROVED

mohammad
7/27/2021 12:09:50 PM

Quant Time: Jul 27 06:23:17 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 22 01:52:16 2021
Response via : Initial Calibration

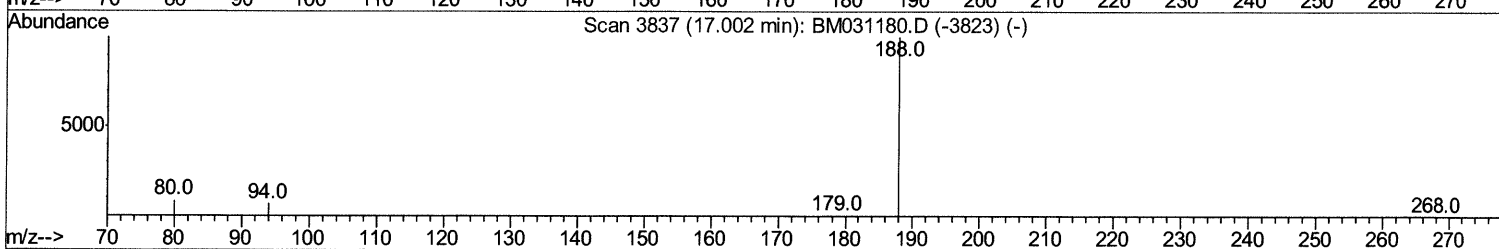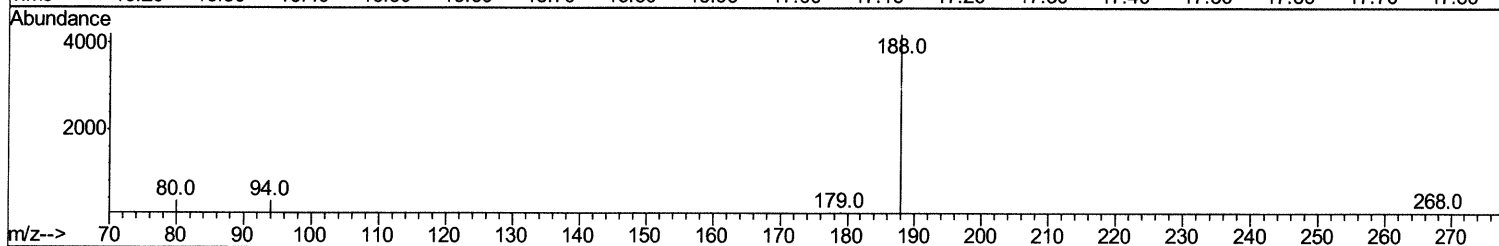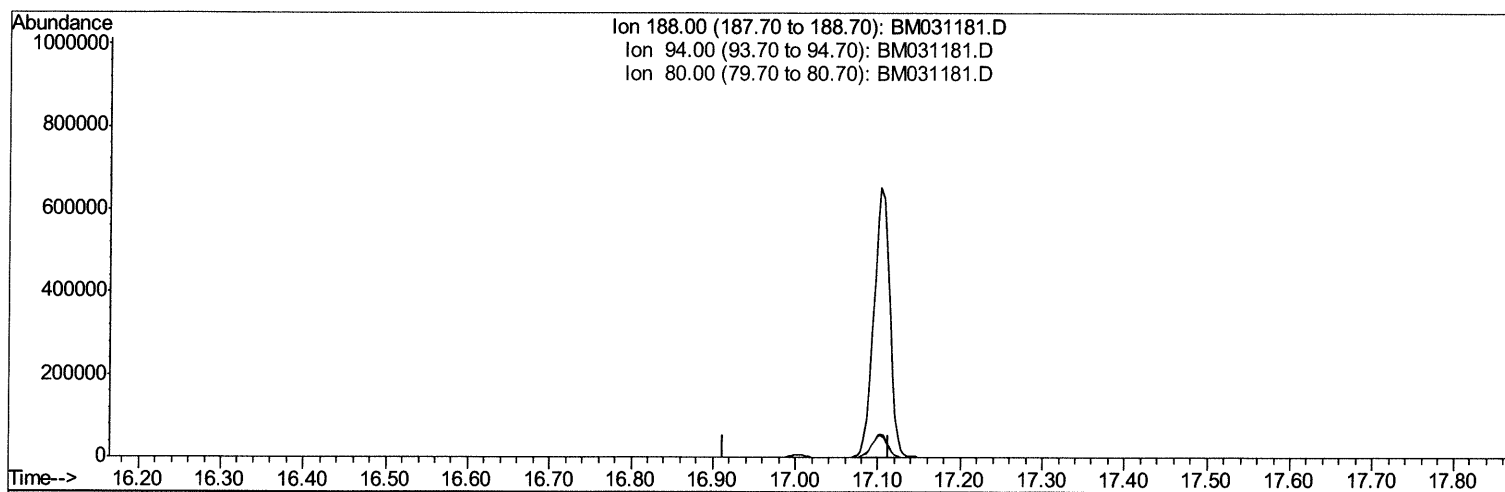

TIC: BM031181.D

(13) Phenanthrene-d10 (I)

17.013min (-17.013) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	7.90	0.00#
80.00	8.20	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM072621\
 Data File : BM031181.D
 Acq On : 27 Jul 2021 03:03
 Operator : CG/JU
 Sample : PB137860BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK860

Manual Integrations
 APPROVED

mohammad
 7/27/2021 12:09:50 PM

Quant Time: Jul 27 06:23:17 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM072221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 22 01:52:16 2021
 Response via : Initial Calibration

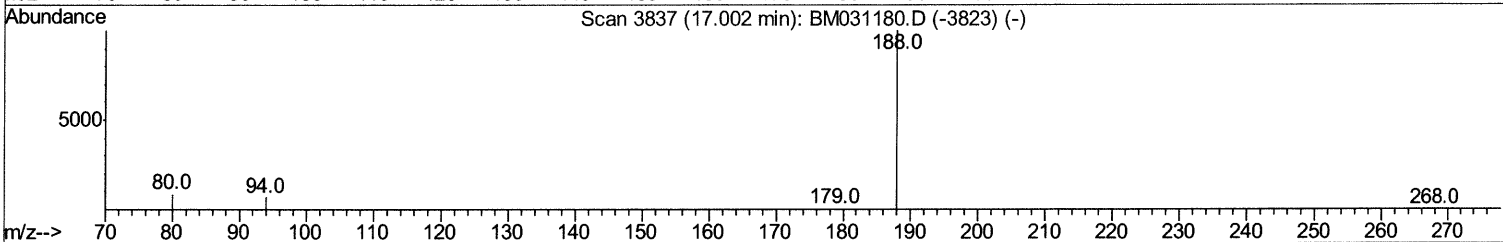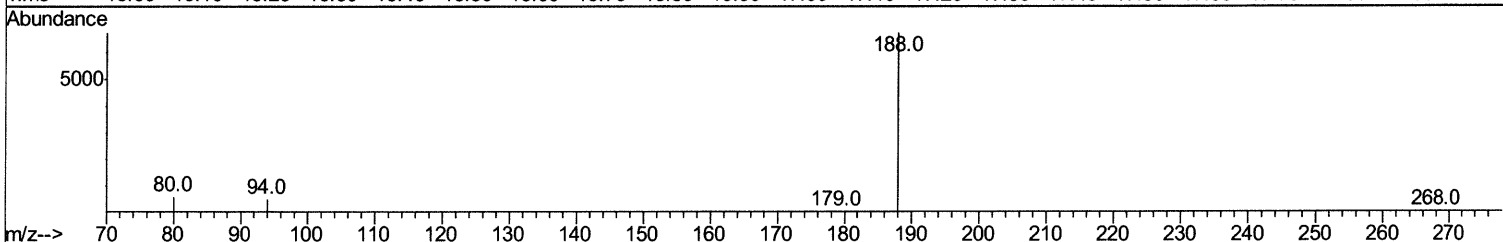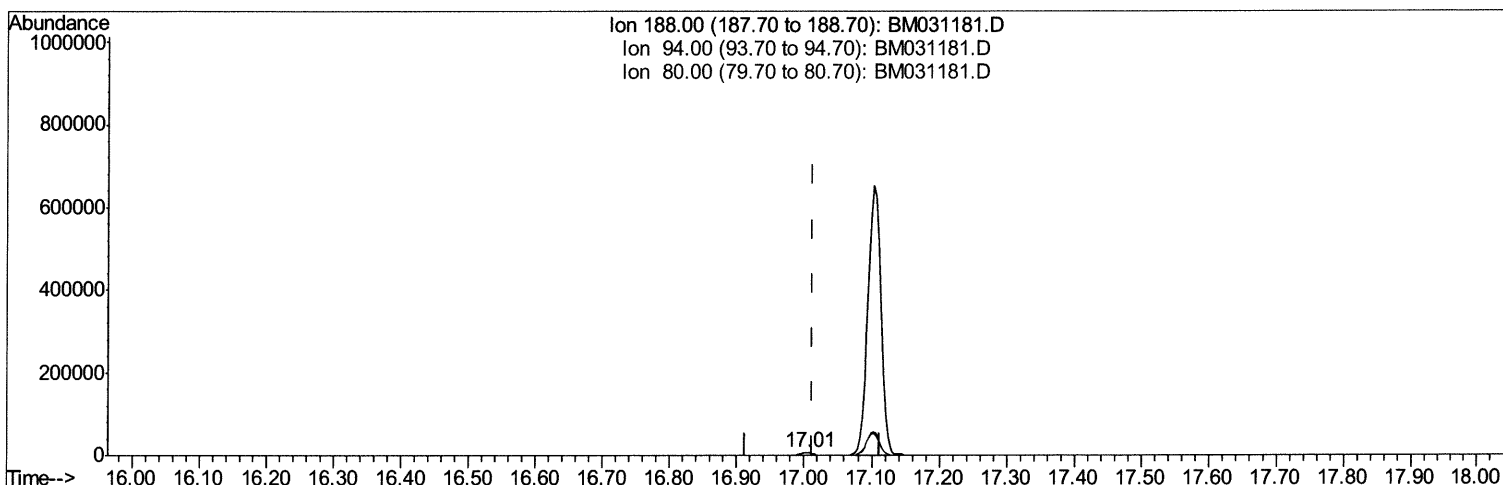

TIC: BM031181.D

(13) Phenanthrene-d10 (I)

17.006min (-0.007) 0.40ng/ul m

response 9167

Ion	Exp%	Act%
188.00	100	100
94.00	7.90	7.59
80.00	8.20	8.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM072621\
Data File : BM031181.D
Acq On : 27 Jul 2021 03:03
Operator : CG/JU
Sample : PB137860BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK860

Manual Integrations
APPROVED

mohammad
7/27/2021 12:09:50 PM

Quant Time: Jul 27 07:12:15 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 22 01:52:16 2021
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	1360	0.40	ng/ul	-0.01
4) Naphthalene-d8	10.40	136	5700	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.26	164	4406	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.01	188	9167m	0.40	ng/ul	0.00
17) Chrysene-d12	21.19	240	7539	0.40	ng/ul	-0.01
23) Perylene-d12	23.36	264	7342	0.40	ng/ul	-0.01

ju 7/29/21

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.21	96	8760	6.13	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.99	152	3641	0.36	ng/ul	0.00
18) Fluoranthene-d10	19.03	212	9990	0.43	ng/ul	-0.01

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed