


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM072621\
Data File : BM031191.D
Acq On : 27 Jul 2021 09:10
Operator : CG/JU
Sample : M3123-01
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0060

Manual Integrations
APPROVED

mohammad
7/27/2021 12:10:17 PM

Quant Time: Jul 27 10:20:51 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 22 01:52:16 2021
Response via : Initial Calibration

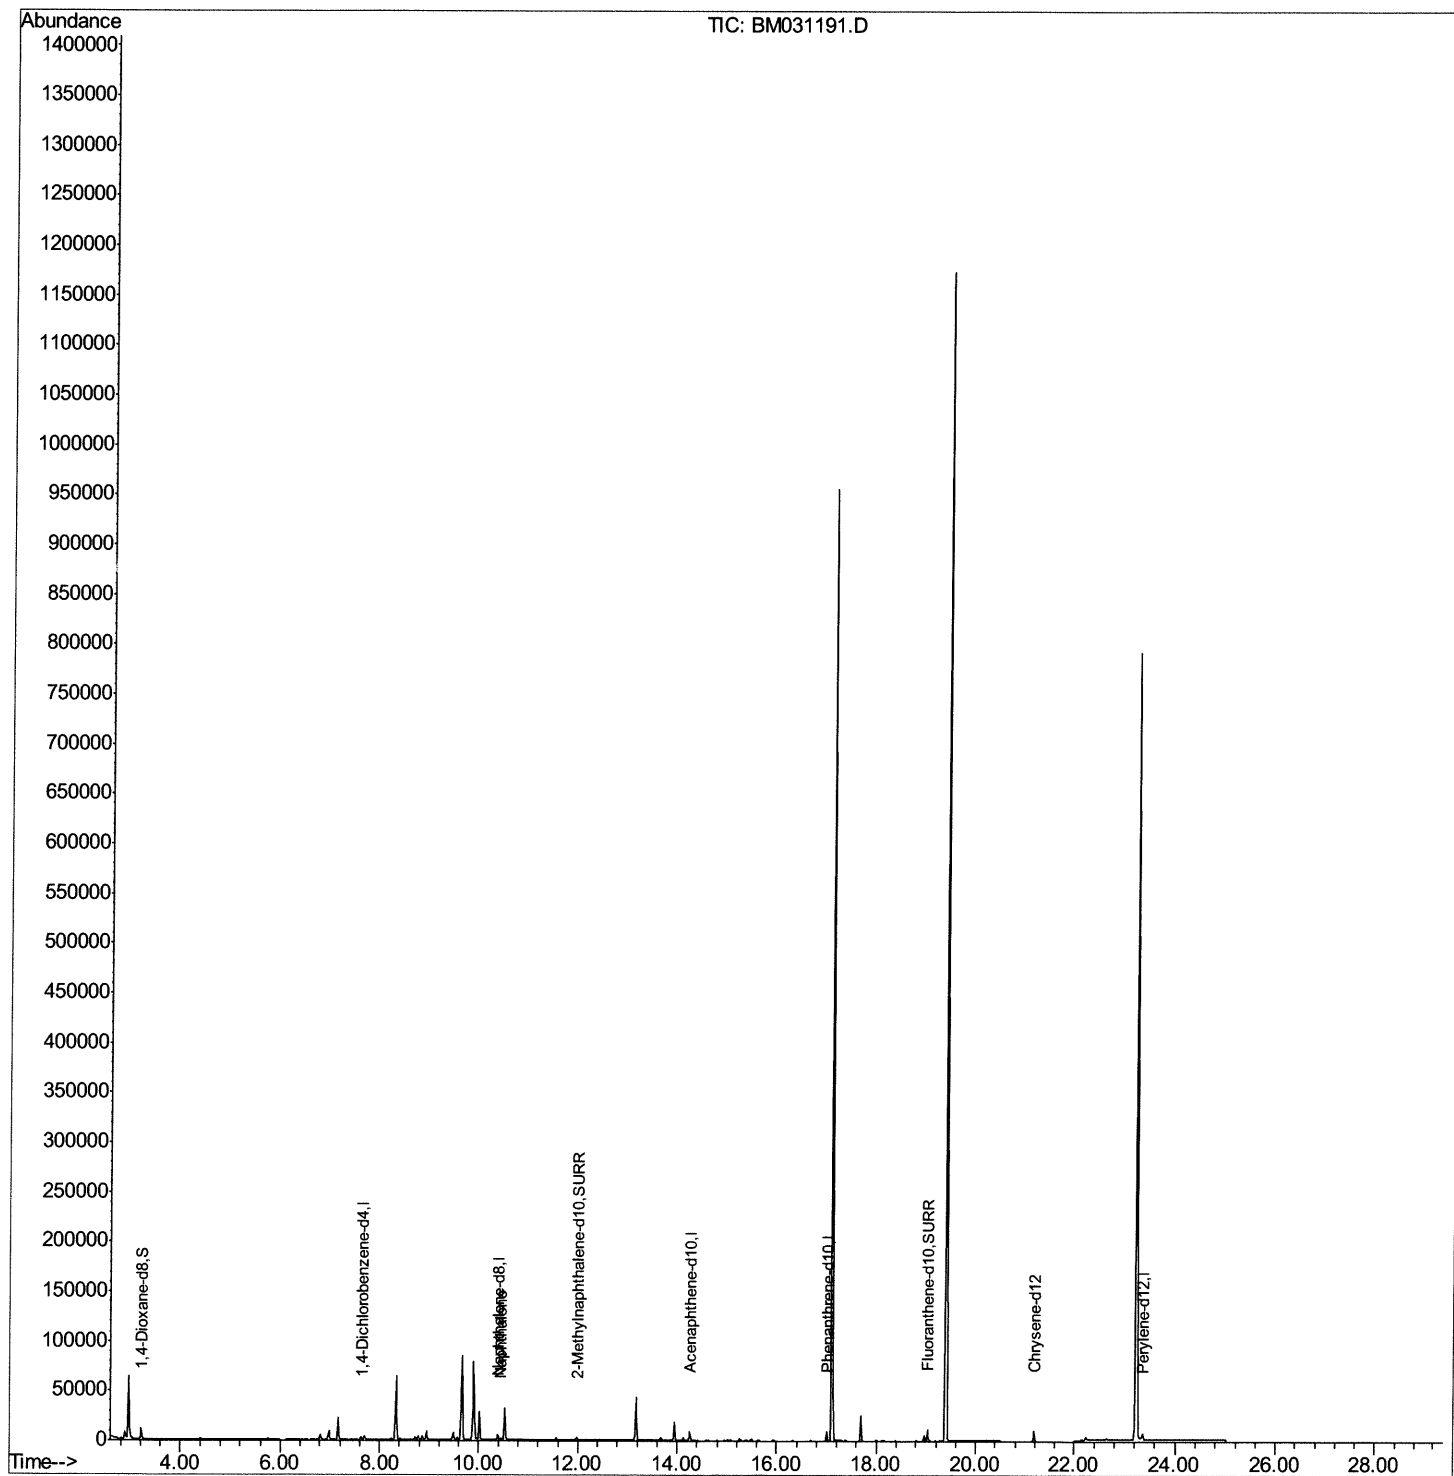




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM072621\
Data File : BM031191.D
Acq On : 27 Jul 2021 09:10
Operator : CG/JU
Sample : M3123-01
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0060

Manual Integrations
APPROVED

mohammad
7/27/2021 12:10:17 PM

Quant Time: Jul 27 10:12:43 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 22 01:52:16 2021
Response via : Initial Calibration

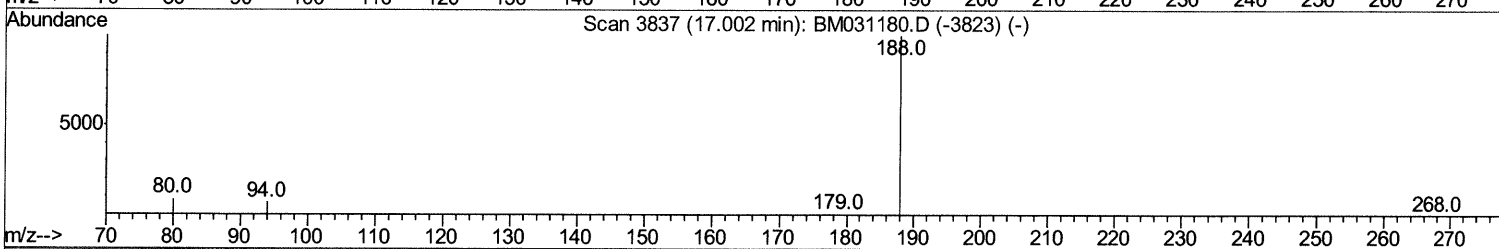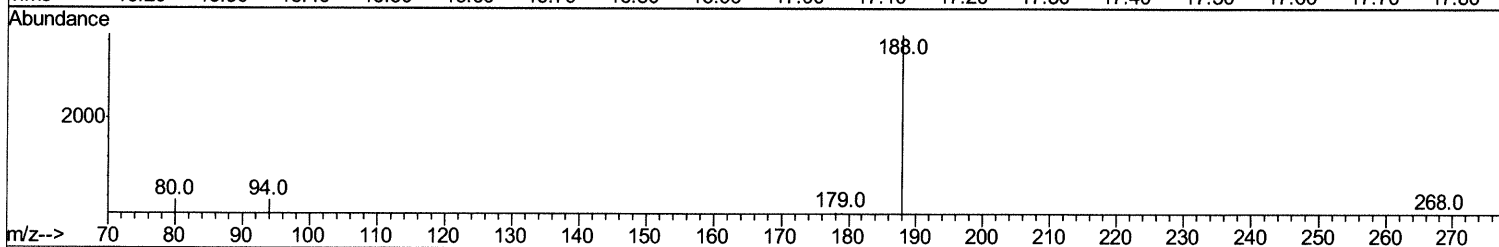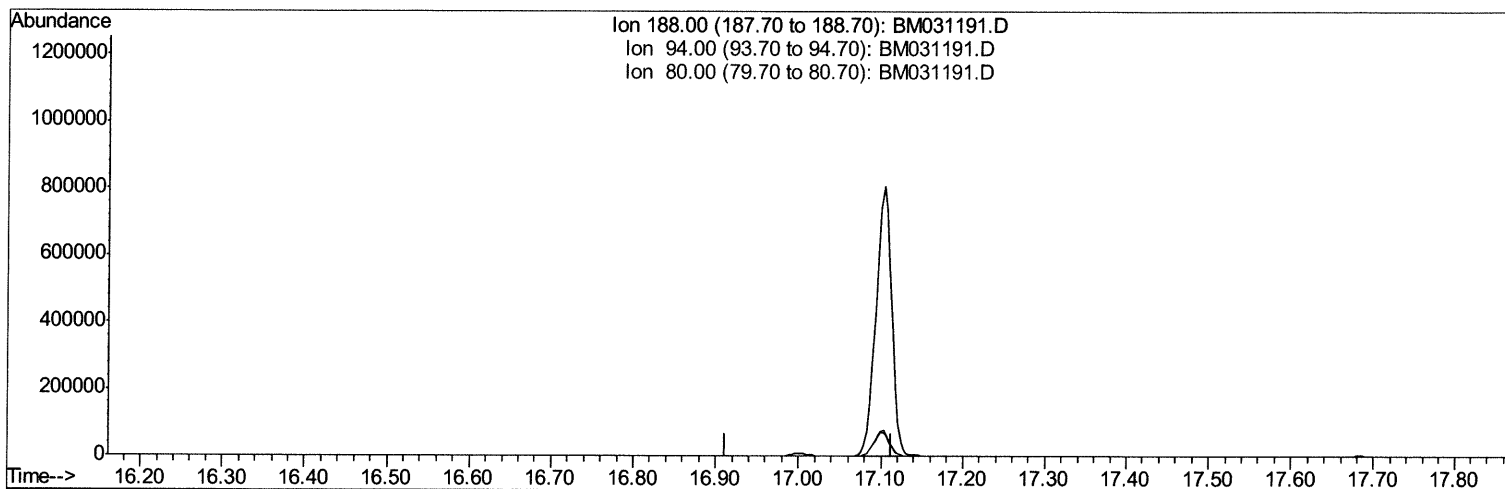

TIC: BM031191.D

(13) Phenanthrene-d10 (I)

17.013min (-17.013) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	7.90	0.00#
80.00	8.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM072621\
Data File : BM031191.D
Acq On : 27 Jul 2021 09:10
Operator : CG/JU
Sample : M3123-01
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0060

Manual Integrations
APPROVED

mohammad
7/27/2021 12:10:17 PM

Quant Time: Jul 27 10:12:43 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 22 01:52:16 2021
Response via : Initial Calibration

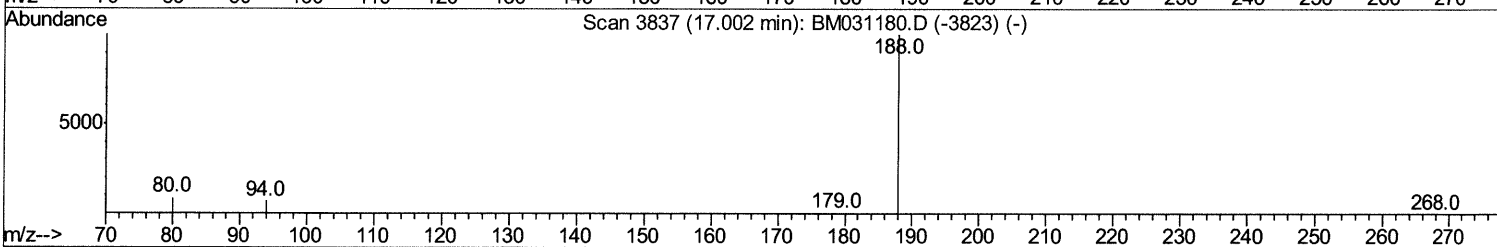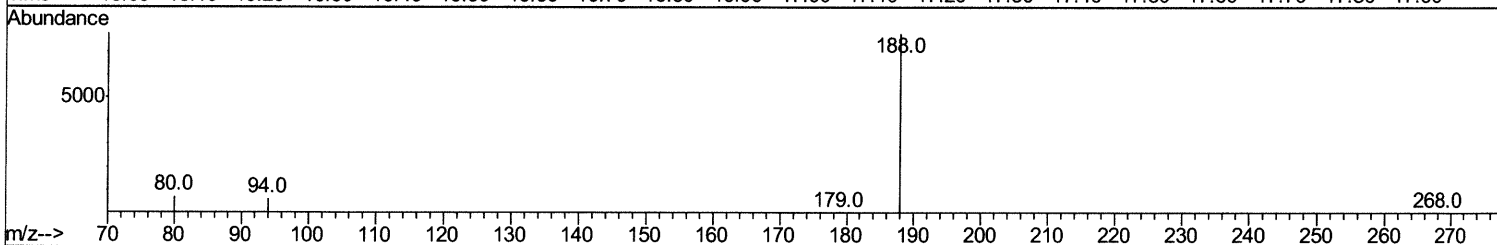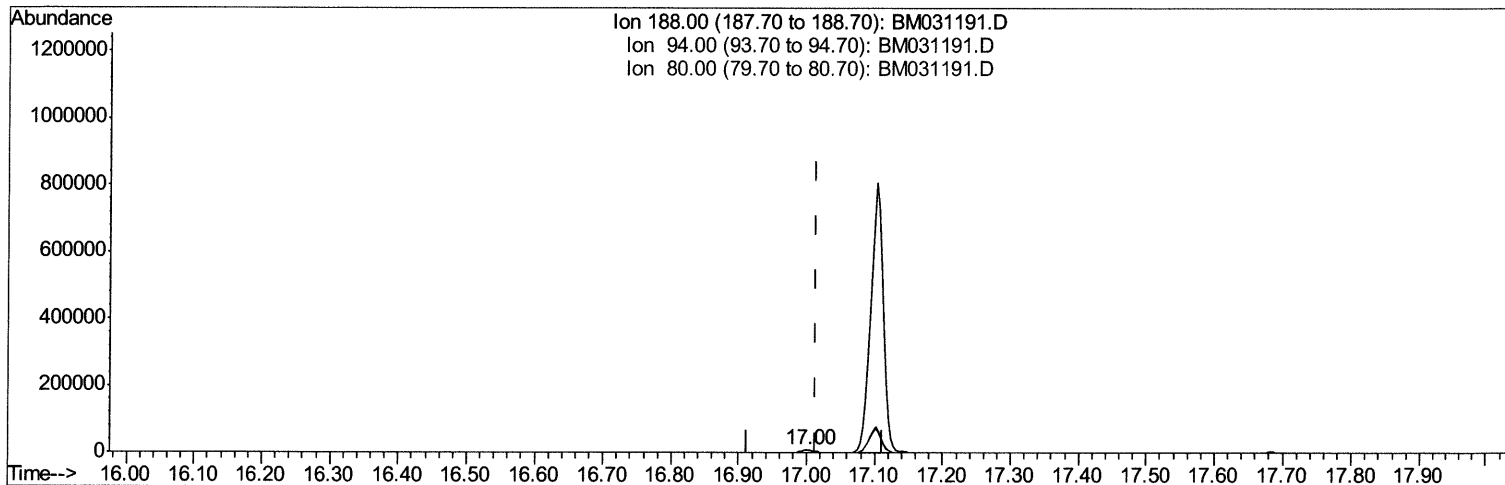

TIC: BM031191.D

(13) Phenanthrene-d10 (I)

17.003min (-0.010) 0.40ng/ul m

response 10751

Ion	Exp%	Act%
188.00	100	100
94.00	7.90	8.25
80.00	8.20	9.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM072621\
 Data File : BM031191.D
 Acq On : 27 Jul 2021 09:10
 Operator : CG/JU
 Sample : M3123-01
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0060

Manual Integrations
 APPROVED

mohammad
 7/27/2021 12:10:17 PM

Quant Time: Jul 27 10:20:51 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM072221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 22 01:52:16 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	1669	0.40	ng/ul	-0.01
4) Naphthalene-d8	10.39	136	6817	0.40	ng/ul	-0.01
9) Acenaphthene-d10	14.25	164	5086	0.40	ng/ul	-0.01
13) Phenanthrene-d10	17.00	188	10751m	0.40	ng/ul	-0.01
17) Chrysene-d12	21.19	240	9170	0.40	ng/ul	-0.01
23) Perylene-d12	23.36	264	8660	0.40	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.21	96	7651	4.36	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.98	152	4176	0.35	ng/ul	-0.01
18) Fluoranthene-d10	19.03	212	12658	0.45	ng/ul	-0.01
Target Compounds						
5) Naphthalene	10.44	128	641	0.031	ng/ul#	80

(#) = qualifier out of range (m) = manual integration (+) = signals summed