

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072621\
 Data File : BM031187.D
 Acq On : 27 Jul 2021 06:43
 Operator : CG/JU
 Sample : M3091-04
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0042

Manual Integrations
 APPROVED

mohammad
 7/27/2021 12:10:01 PM

Quant Time: Jul 27 07:21:53 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM072221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 27 07:10:34 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.632	152	1535	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.392	136	6364	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.258	164	4844	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.002	188	10703m	0.400	ng/ul	-0.01
17) Chrysene-d12	21.188	240	9435	0.400	ng/ul	-0.01
23) Perylene-d12	23.358	264	8657	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.210	96	6889	4.272	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.984	152	3900	0.349	ng/ul	-0.01
18) Fluoranthene-d10	19.031	212	12630	0.439	ng/ul	-0.01
Target Compounds						
					Qvalue	
5) Naphthalene	10.442	128	707	0.037	ng/ul#	79

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072621\
Data File : BM031187.D
Acq On : 27 Jul 2021 06:43
Operator : CG/JU
Sample : M3091-04
Misc :
ALS Vial : 33 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0042

Manual Integrations
APPROVED

mohammad
7/27/2021 12:10:01 PM




Quant Time: Jul 27 07:21:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 27 07:10:34 2021
Response via : Initial Calibration

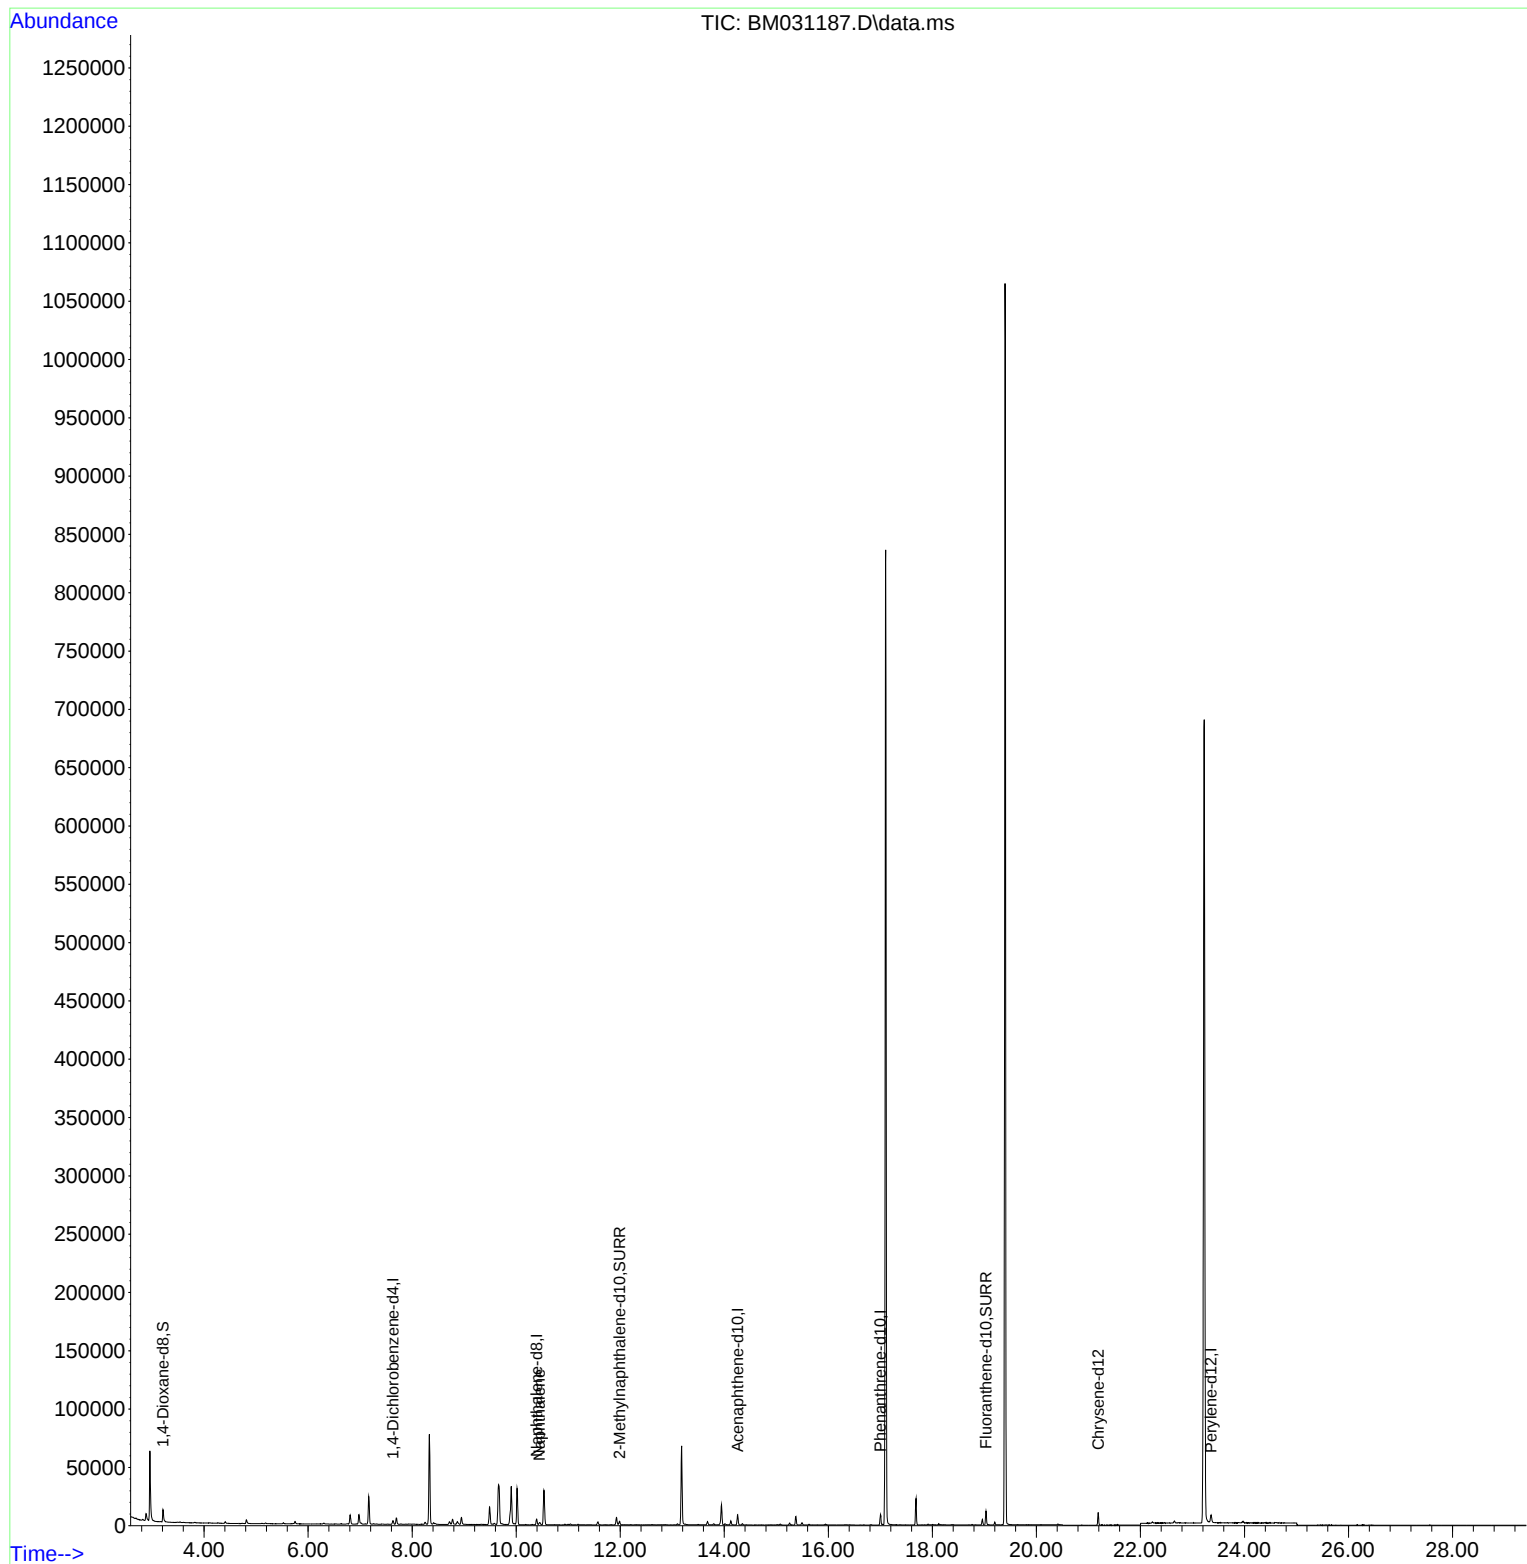

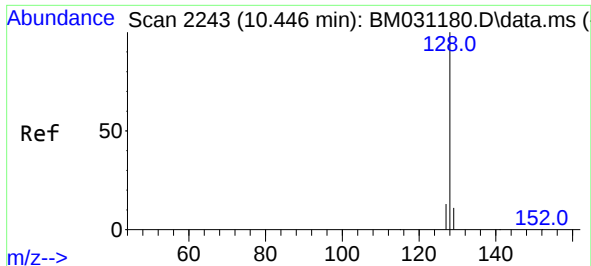

#5
Naphthalene
Concen: 0.037 ng/ul
RT: 10.442 min Scan# 2242
Delta R.T. -0.014 min
Lab File: BM031187.D
Acq: 27 Jul 2021 06:43

Tgt Ion:128 Resp: 707
Ion Ratio Lower Upper
128 100
129 23.1 10.2 15.4#
127 21.6 11.8 17.8#

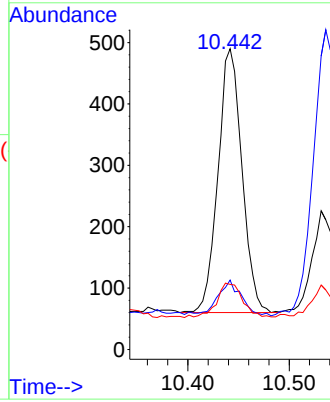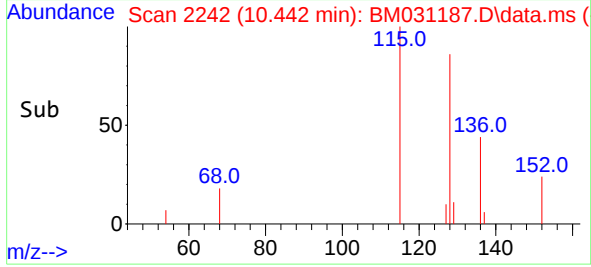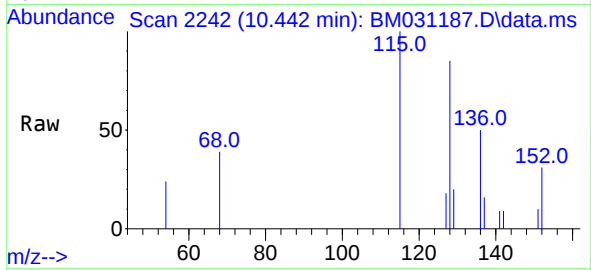

Instrument :
BNA_M
ClientSampleId :
C0042

Manual Integrations
APPROVED

mohammad
7/27/2021 12:10:01 PM