

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072621\
 Data File : BM031191.D
 Acq On : 27 Jul 2021 09:10
 Operator : CG/JU
 Sample : M2123-01
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0060

Manual Integrations
 APPROVED

mohammad
 7/27/2021 12:10:17 PM

Quant Time: Jul 27 10:13:05 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM072221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 22 01:52:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.632	152	1669	0.40	ng/ul	-0.01
4) Naphthalene-d8	10.392	136	6817	0.40	ng/ul	-0.01
9) Acenaphthene-d10	14.254	164	5086	0.40	ng/ul	-0.01
13) Phenanthrene-d10	17.003	188	10751m	0.40	ng/ul	-0.01
17) Chrysene-d12	21.188	240	9170	0.40	ng/ul	-0.01
23) Perylene-d12	23.360	264	8660	0.40	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.213	96	7651	4.36	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.984	152	4176	0.35	ng/ul	-0.01
18) Fluoranthene-d10	19.031	212	12658	0.45	ng/ul	-0.01
Target Compounds						
						Qvalue
5) Naphthalene	10.442	128	641	0.03	ng/ul#	80

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072621\
Data File : BM031191.D
Acq On : 27 Jul 2021 09:10
Operator : CG/JU
Sample : M2123-01
Misc :
ALS Vial : 37 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0060

Manual Integrations
APPROVED


mohammad
7/27/2021 12:10:17 PM

Quant Time: Jul 27 10:13:05 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 22 01:52:16 2021
Response via : Initial Calibration


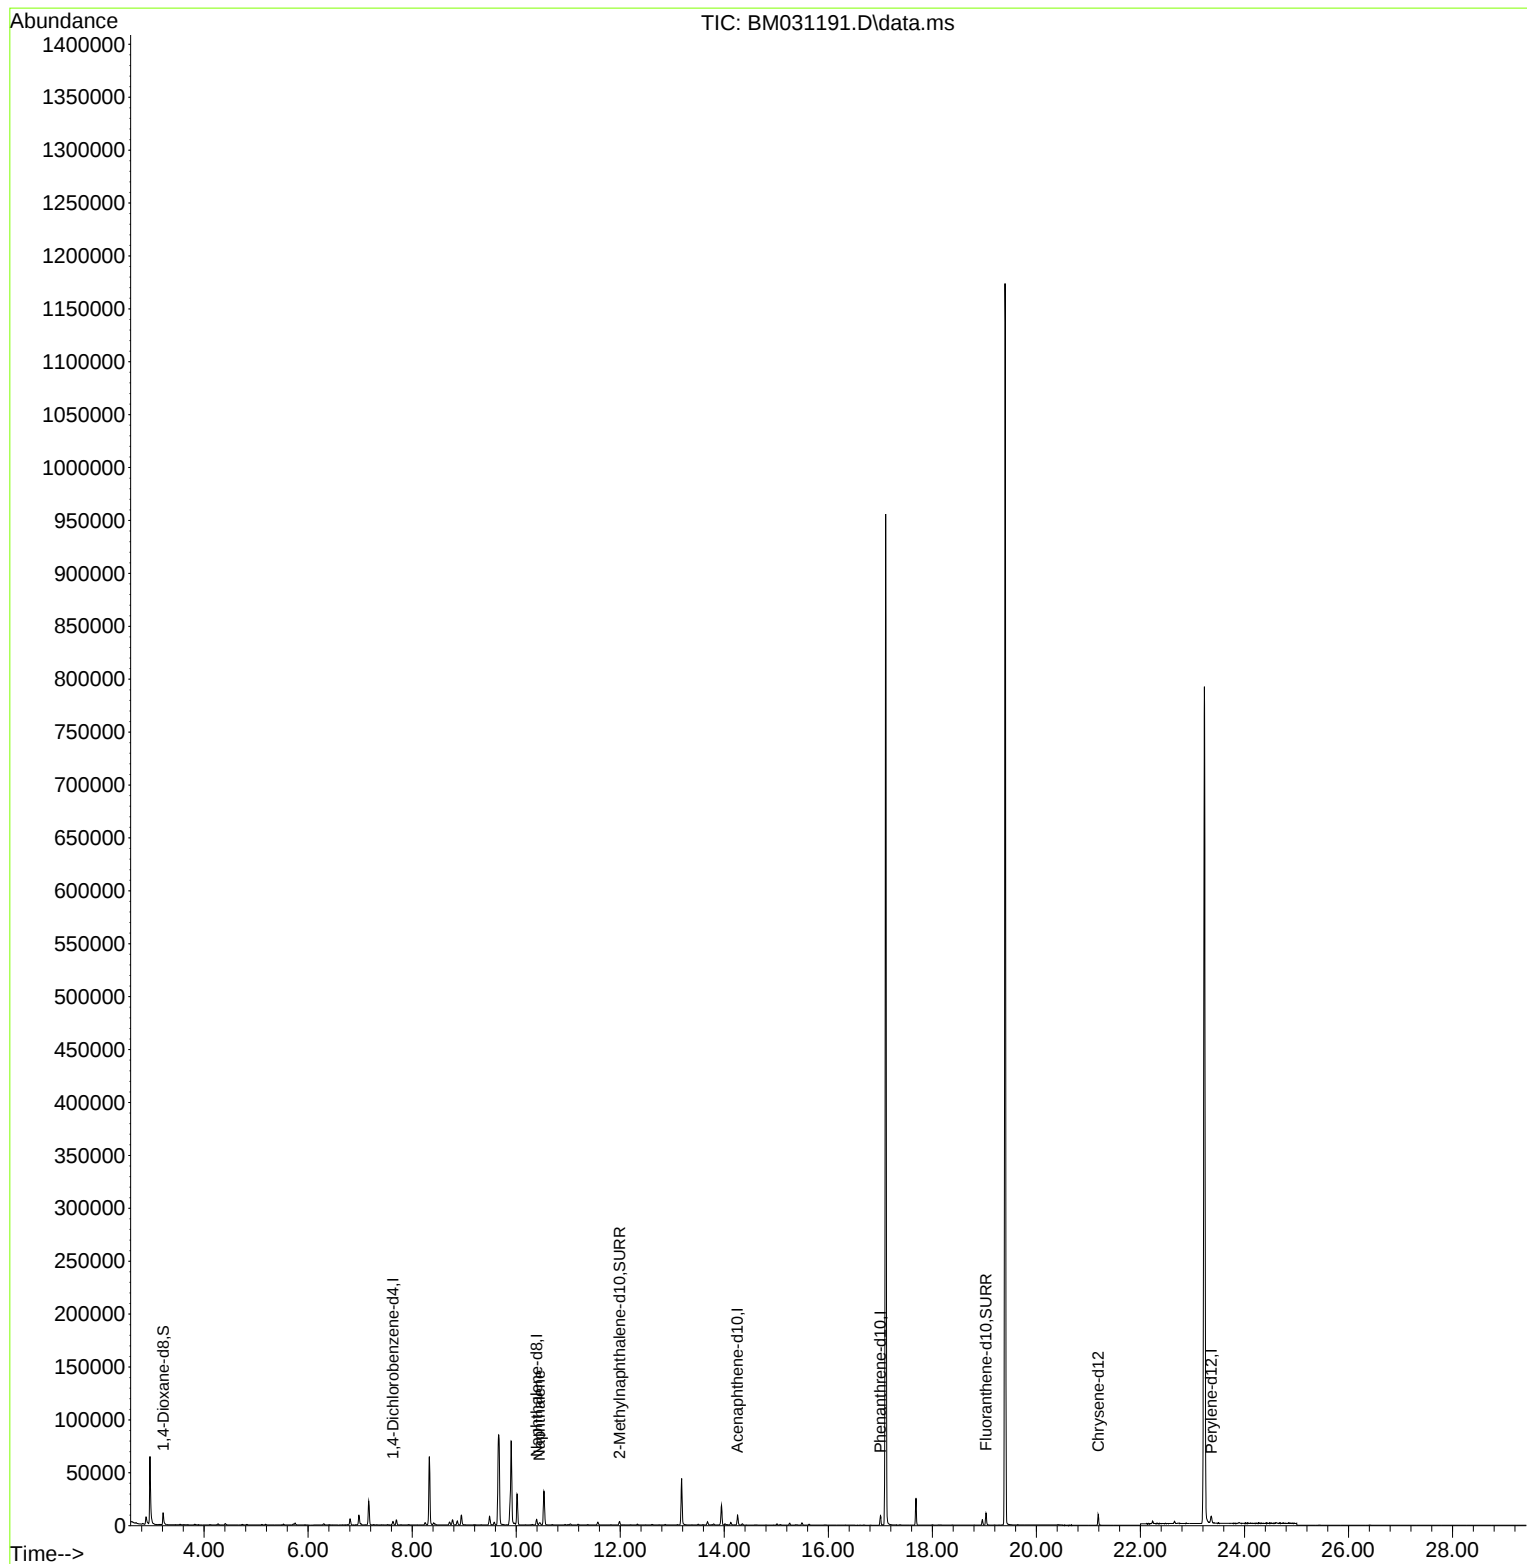


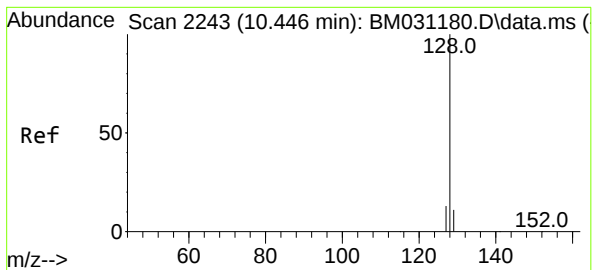

#5
Naphthalene
Concen: 0.03 ng/ul
RT: 10.442 min Scan# 2242
Delta R.T. -0.014 min
Lab File: BM031191.D
Acq: 27 Jul 2021 09:10

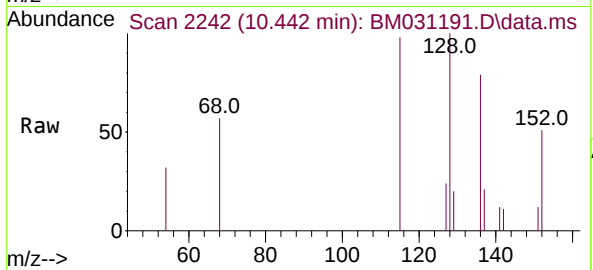

Tgt Ion	Ratio	Lower	Upper
128	100		
129	20.2	10.2	15.4#
127	23.8	11.8	17.8#

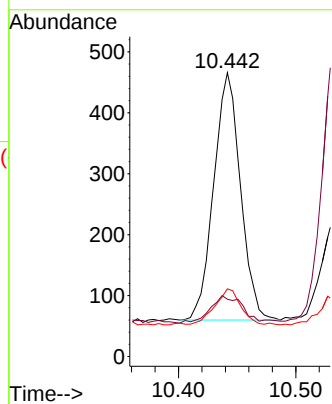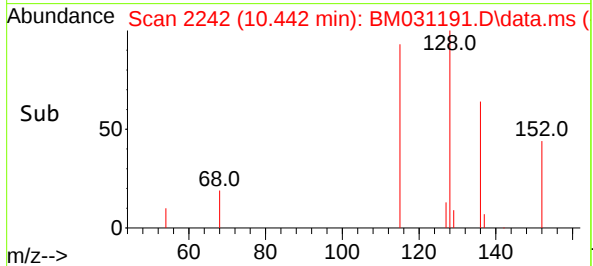

Instrument :
BNA_M
ClientSampleId :
C0060

Manual Integrations
APPROVED

mohammad
7/27/2021 12:10:17 PM