

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072623\
 Data File : BM041128.D
 Acq On : 26 Jul 2023 10:29
 Operator : MA/JU
 Sample : 03553-09
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jul 27 01:17:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 26 04:20:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.824	152	3057	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.625	136	10689	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.486	164	5724	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.244	188	11334	0.400	ng/ul	0.00
17) Chrysene-d12	21.454	240	9156	0.400	ng/ul	0.00
23) Perylene-d12	23.830	264	11593	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.246	96	9788	2.076	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.236	152	5412	0.355	ng/ul	0.00
18) Fluoranthene-d10	19.283	212	11504	0.462	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.645	202	1807	0.050	ng/ul#	1
26) Benzo(a)pyrene	23.670	252	3882	0.104	ng/ul#	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072623\
Data File : BM041128.D
Acq On : 26 Jul 2023 10:29
Operator : MA/JU
Sample : 03553-09
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jul 27 01:17:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 04:20:13 2023
Response via : Initial Calibration

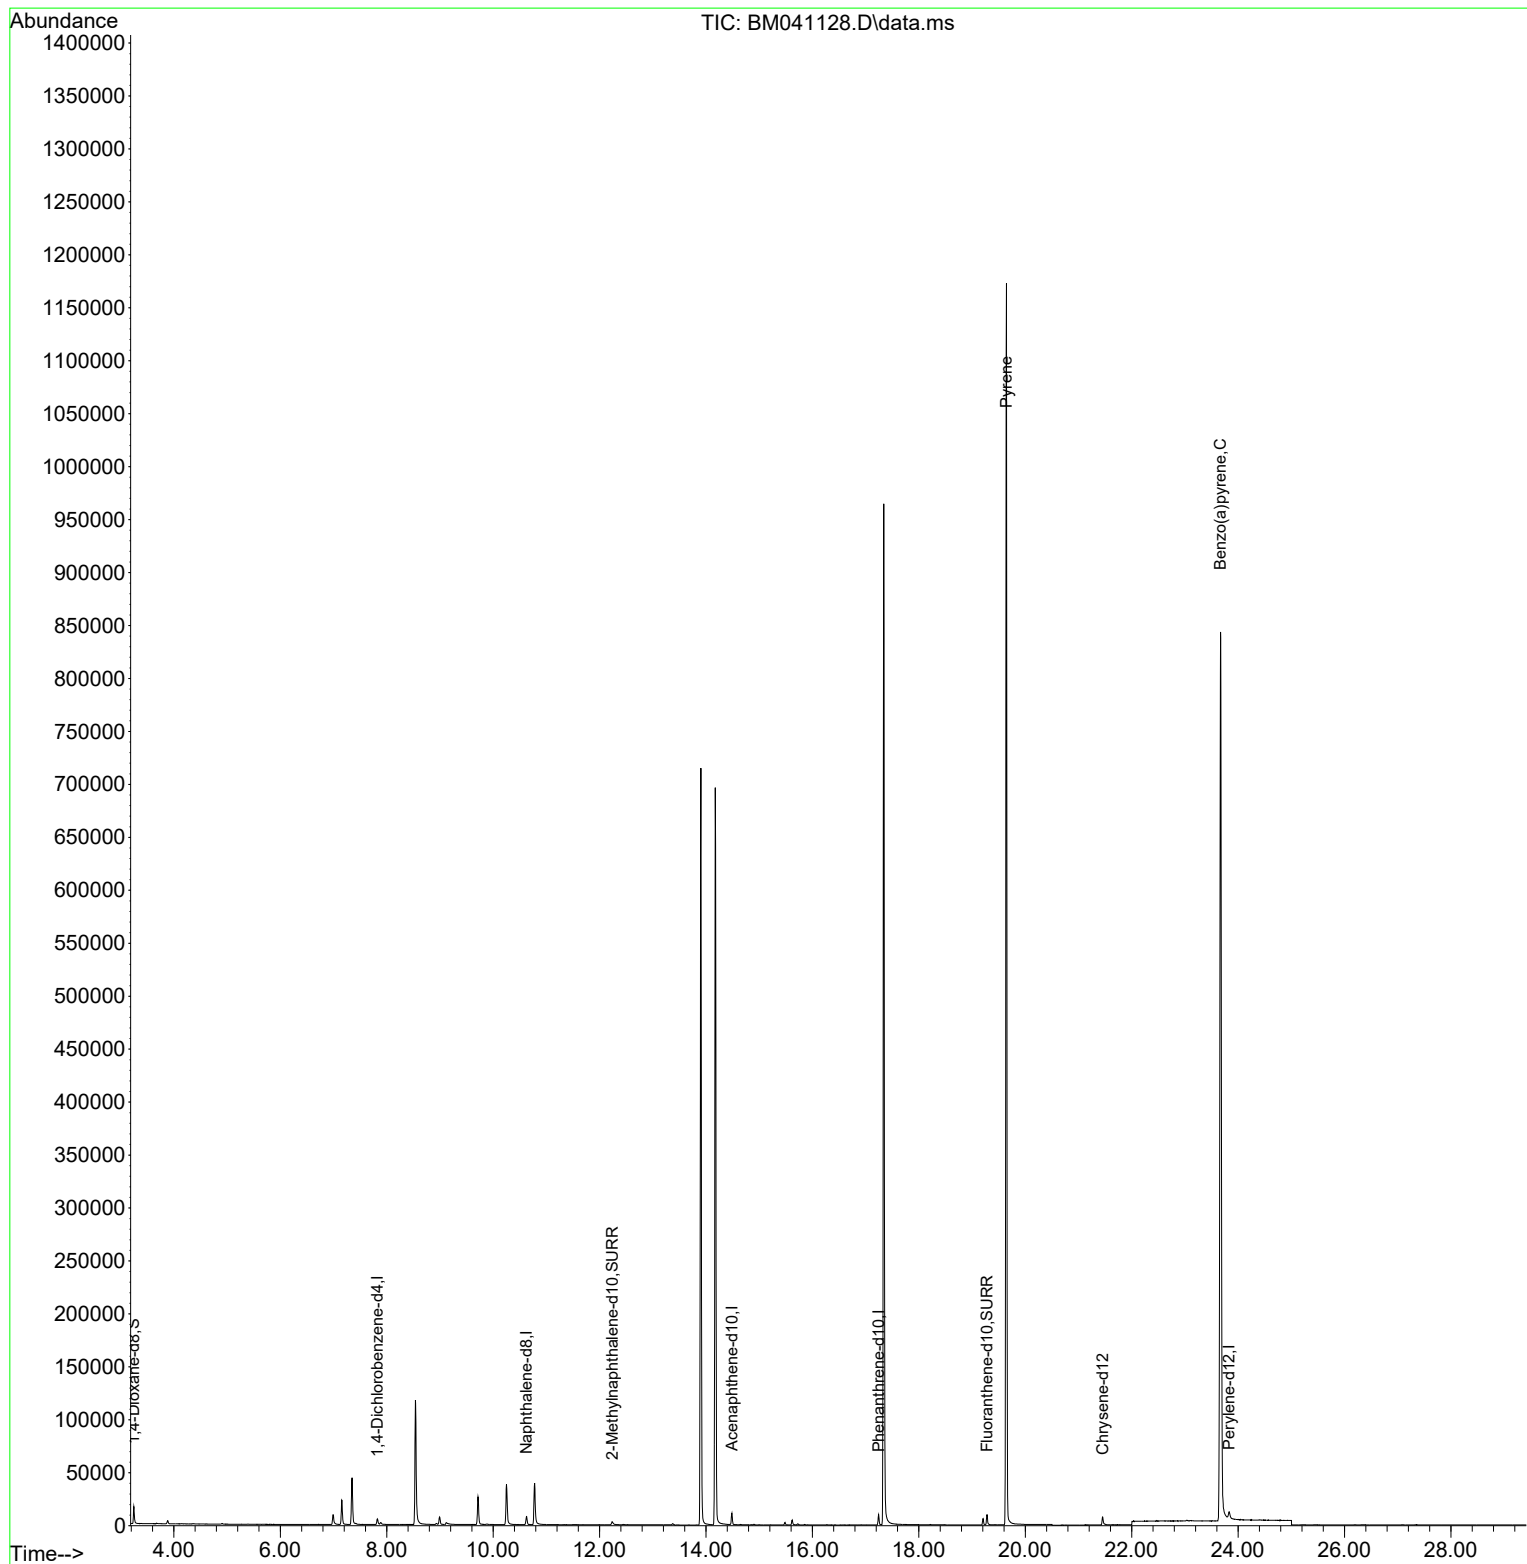

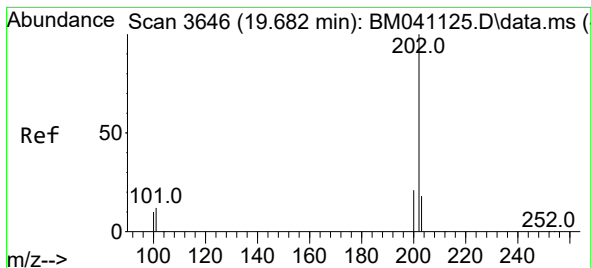

#20

Pyrene

Concen: 0.050 ng/ul

RT: 19.645 min Scan# 3

Delta R.T. -0.037 min


Lab File: BM041128.D

Acq: 26 Jul 2023 10:29

Instrument :

BNA_M

ClientSampleId :

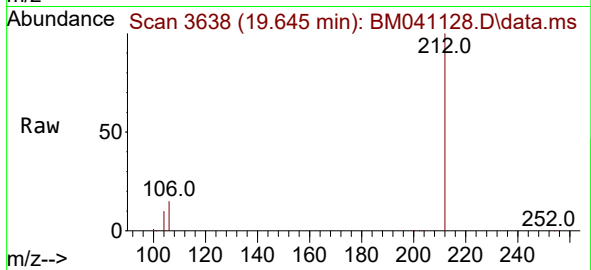




Tgt Ion:202 Resp: 1807

Ion Ratio Lower Upper

202 100

101 144.2 10.7 16.1#

100 1047.9 8.5 12.7#

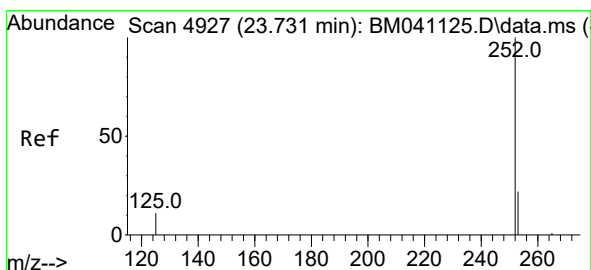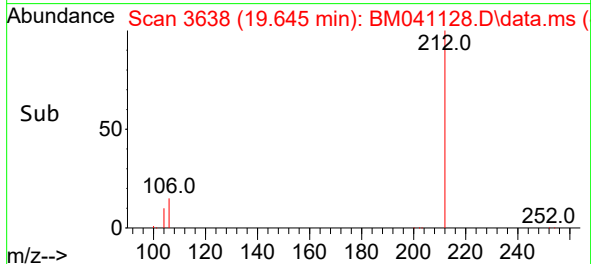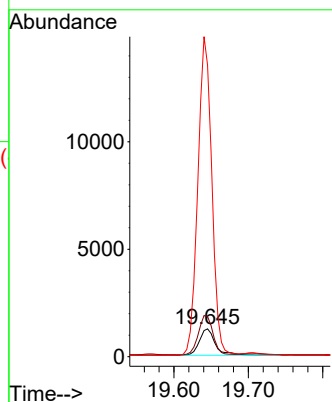

#26

Benzo(a)pyrene

Concen: 0.104 ng/ul

RT: 23.670 min Scan# 4906

Delta R.T. -0.059 min

Lab File: BM041128.D

Acq: 26 Jul 2023 10:29

Tgt Ion:252 Resp: 3882

Ion Ratio Lower Upper

252 100

253 49.5 26.7 40.1#

125 40.3 18.1 27.1#

