

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072623\
 Data File : BM041133.D
 Acq On : 26 Jul 2023 13:34
 Operator : MA/JU
 Sample : 03553-20
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jul 27 01:18:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 26 04:20:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.824	152	3311	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.631	136	11305	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.486	164	5871	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.244	188	11354	0.400	ng/ul	0.00
17) Chrysene-d12	21.463	240	9440	0.400	ng/ul	0.01
23) Perylene-d12	23.848	264	11351	0.400	ng/ul	# 0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.246	96	19915	3.899	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.231	152	5810	0.360	ng/ul	0.00
18) Fluoranthene-d10	19.283	212	11687	0.455	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.280	88	214	0.041	ng/ul#	1
26) Benzo(a)pyrene	23.687	252	3539	0.097	ng/ul#	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072623\
Data File : BM041133.D
Acq On : 26 Jul 2023 13:34
Operator : MA/JU
Sample : 03553-20
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Jul 27 01:18:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 04:20:13 2023
Response via : Initial Calibration

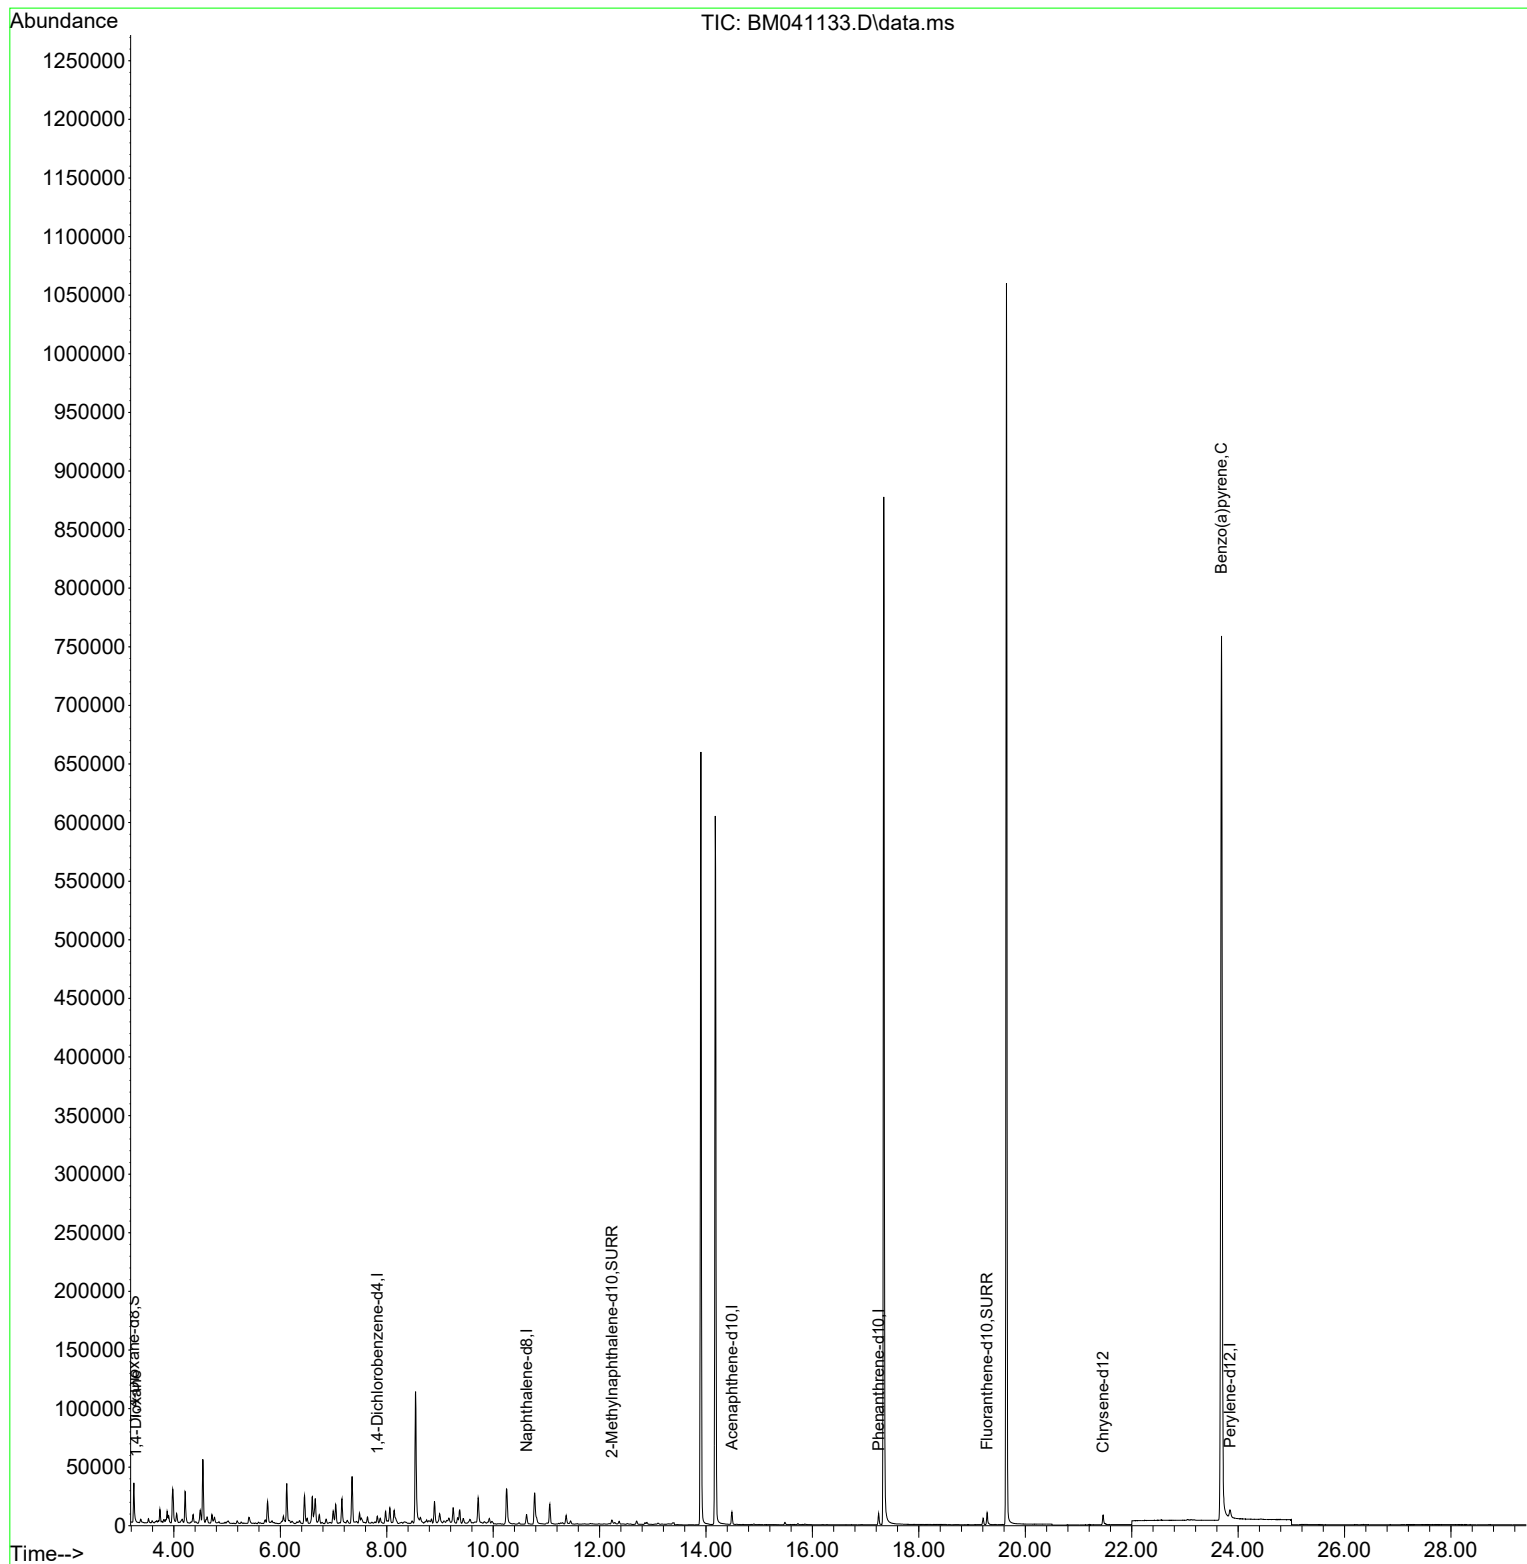



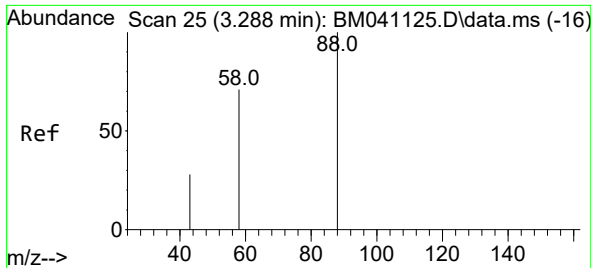


#2
1,4-Dioxane
Concen: 0.041 ng/ul
RT: 3.280 min Scan# 21
Delta R.T. -0.008 min
Lab File: BM041133.D
Acq: 26 Jul 2023 13:34

Instrument :
BNA_M
ClientSampleId :

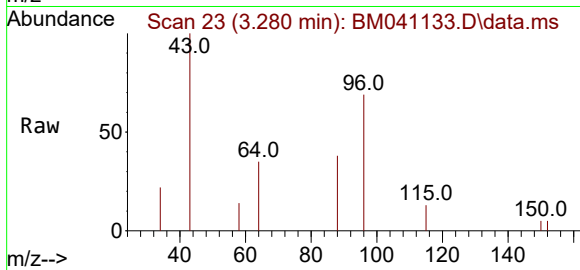

Tgt Ion: 88 Resp: 214
Ion Ratio Lower Upper
88 100
43 264.2 83.1 124.7#
58 36.8 38.8 58.2#

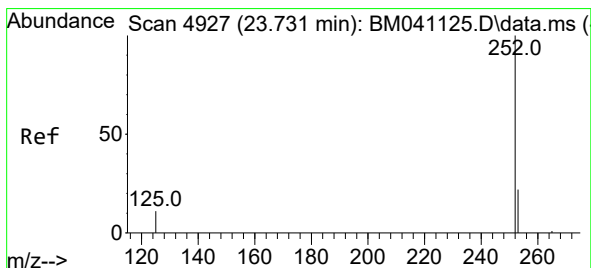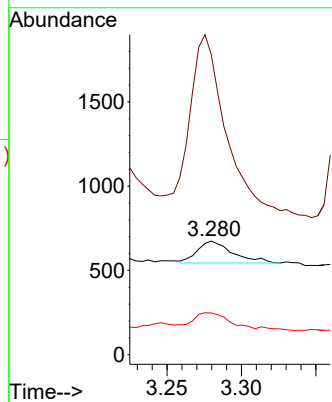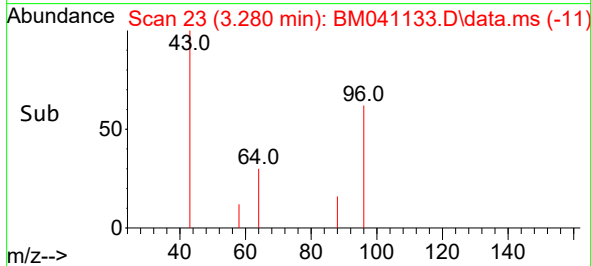

#26
Benzo(a)pyrene
Concen: 0.097 ng/ul
RT: 23.687 min Scan# 4912
Delta R.T. -0.041 min
Lab File: BM041133.D
Acq: 26 Jul 2023 13:34

Tgt Ion: 252 Resp: 3539
Ion Ratio Lower Upper
252 100
253 53.9 26.7 40.1#
125 43.2 18.1 27.1#

