

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072718\
 Data File : BM016118.D
 Acq On : 28 Jul 2018 03:11
 Operator : SJ/JU
 Sample : J4149-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JJ1G2

Manual Integrations
 APPROVED

Sohil
 7/30/2018 5:48:12 PM

Quant Time: Jul 28 04:35:46 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM071318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 27 23:04:38 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.20	152	57904	20.00	ng/ul	0.00
18) Naphthalene-d8	11.02	136	265225	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.83	164	155120	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.56	188	346614	20.00	ng/ul	0.00
77) Chrysene-d12	21.67	240	313982	20.00	ng/ul	0.00
85) Perylene-d12	24.03	264	257633	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.46	96	8752	6.65	ng/uL	0.00
5) Phenol-d5	7.36	99	27441	5.19	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.52	67	91648	27.53	ng/ul	0.00
9) 2-Chlorophenol-d4	7.73	132	96799	22.52	ng/ul	0.00
13) 4-Methylphenol-d8	8.92	113	57552	12.70	ng/ul	0.00
19) Nitrobenzene-d5	9.39	128	59520	31.25	ng/ul	0.00
22) 2-Nitrophenol-d4	10.11	143	69840	32.26	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.65	165	111130	26.50	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
43) Dimethylphthalate-d6	14.23	166	442528	31.30	ng/ul	0.00
46) Acenaphthylene-d8	14.52	160	486047	30.14	ng/ul	0.00
51) 4-Nitrophenol-d4	15.06	143	8799m	3.59	ng/ul	0.02
57) Fluorene-d10	15.82	176	375054	31.27	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.95	200	64441	27.86	ng/ul	0.00
70) Anthracene-d10	17.66	188	611128	34.44	ng/ul	0.00
78) Pyrene-d10	19.92	212	645988	44.39	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.89	264	507057	35.78	ng/ul	0.00

Target Compounds

				Ovalue	
44) Dimethylphthalate	14.28	163	22500	1.607	ng/ul# 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072718\
Data File : BM016118.D
Acq On : 28 Jul 2018 03:11
Operator : SJ/JU
Sample : J4149-02
Misc :
ALS Vial : 25 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
JJ1G2

Quant Time: Jul 28 04:35:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM071318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 27 23:04:38 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
7/30/2018 5:48:12 PM

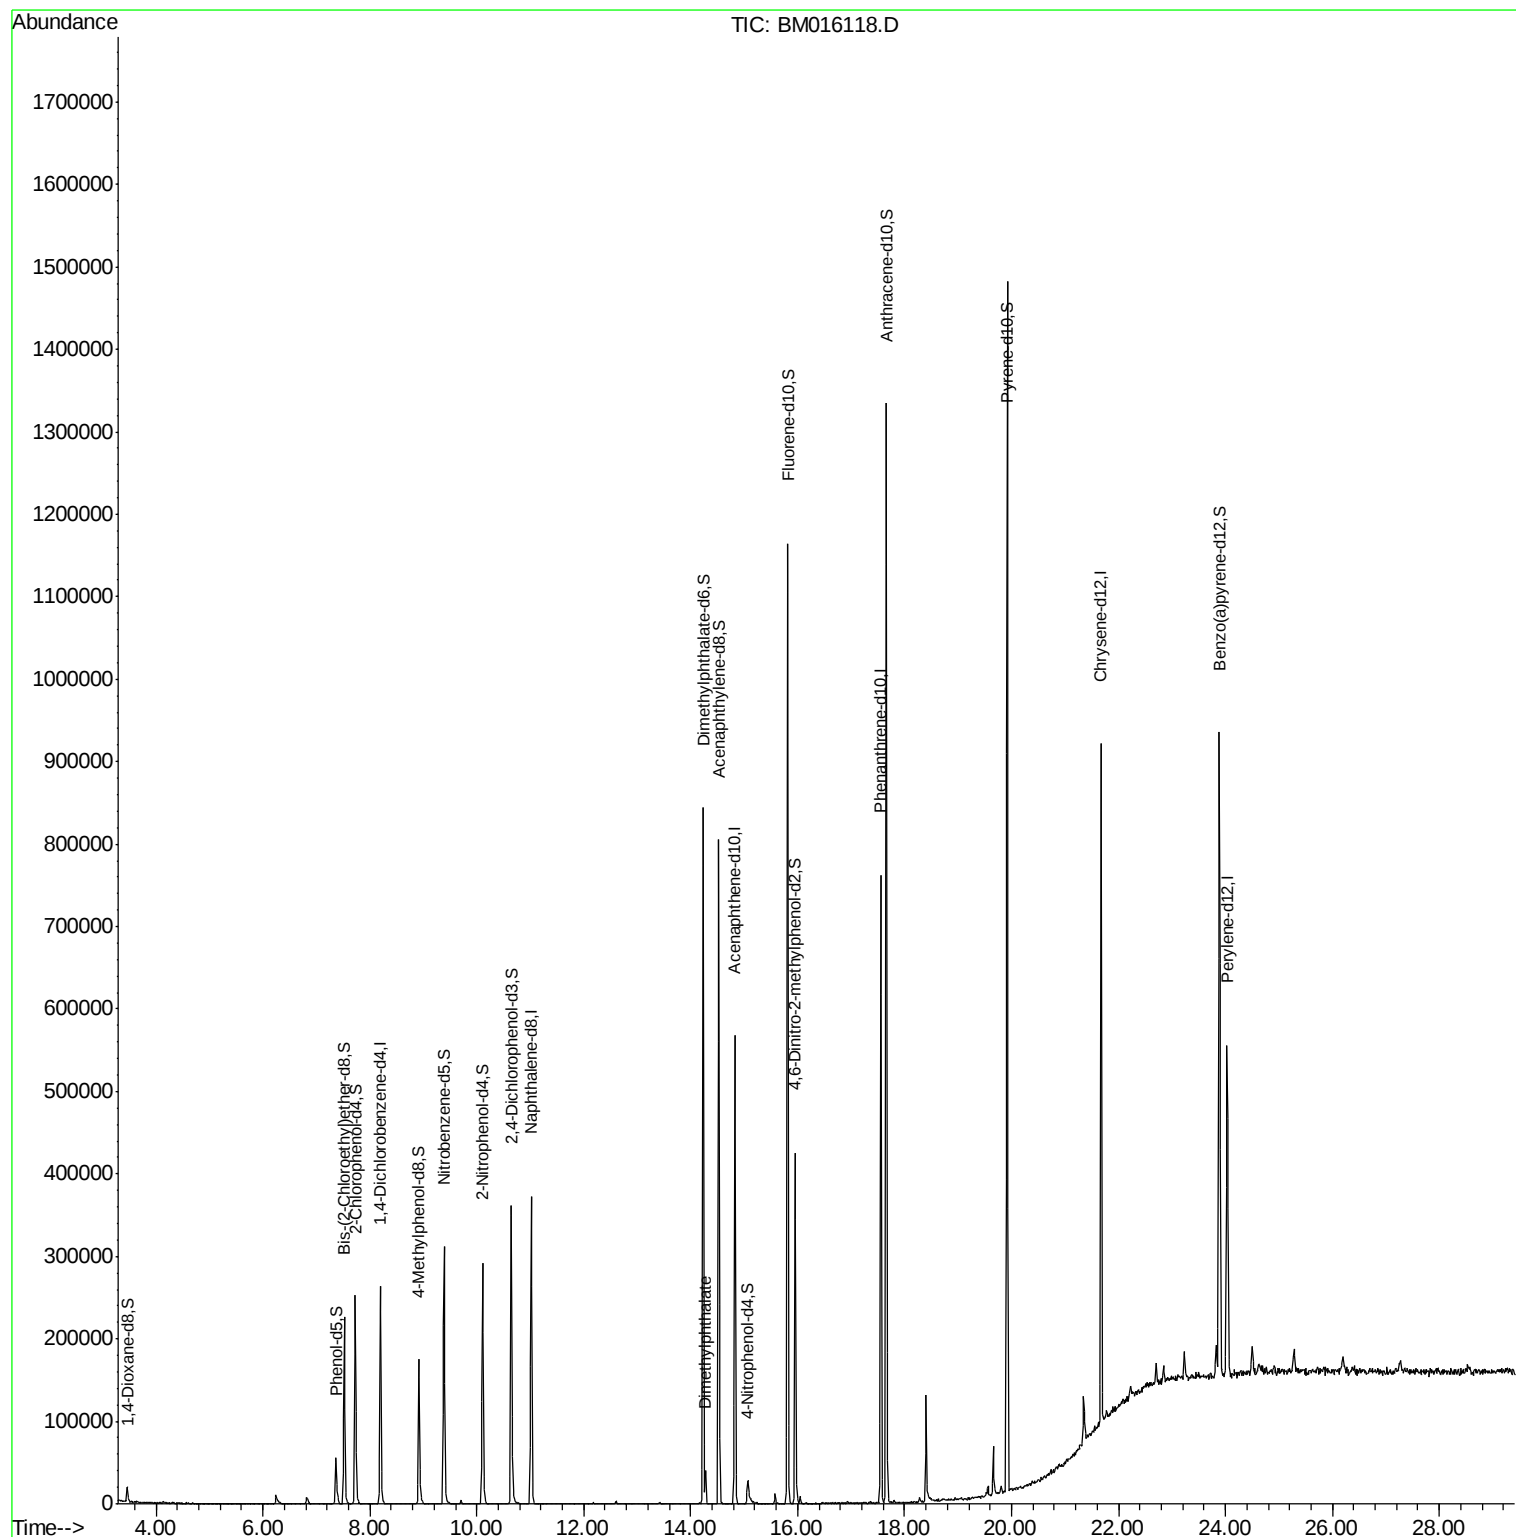

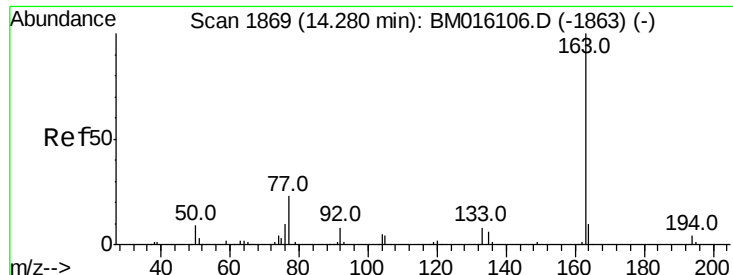

#44

Dimethylphthalate

Concen: 1.607 ng/ul

RT: 14.28 min Scan# 1869

Delta R.T. 0.00 min

Lab File: BM016118.D

Acq: 28 Jul 2018 03:11

Instrument :

BNA_M

ClientSampleId :

JJ1G2

Tot Ion:	163	Resp:	22500
Ion Ratio	Lower	Upper	
163	100		
194	2.2	3.2	4.8#
164	10.1	7.8	11.8

Manual Integrations
APPROVED

Sohil

7/30/2018 5:48:12 PM

