

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072723\
 Data File : BM041150.D
 Acq On : 27 Jul 2023 12:00
 Operator : MA/JU
 Sample : PB154091BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK091

Quant Time: Jul 28 03:29:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 26 04:20:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.828	152	2887	0.400	ng/ul	0.00
4) Naphthalene-d8	10.631	136	9203	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.486	164	4559	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.244	188	9655	0.400	ng/ul	0.00
17) Chrysene-d12	21.460	240	8195	0.400	ng/ul	0.01
23) Perylene-d12	23.827	264	11578	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.250	96	30781	6.911	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.247	152	4775	0.363	ng/ul	0.01
18) Fluoranthene-d10	19.283	212	9505	0.426	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.640	202	1535	0.047	ng/ul#	1
26) Benzo(a)pyrene	23.667	252	3526	0.094	ng/ul#	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072723\
Data File : BM041150.D
Acq On : 27 Jul 2023 12:00
Operator : MA/JU
Sample : PB154091BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK091

Quant Time: Jul 28 03:29:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 04:20:13 2023
Response via : Initial Calibration

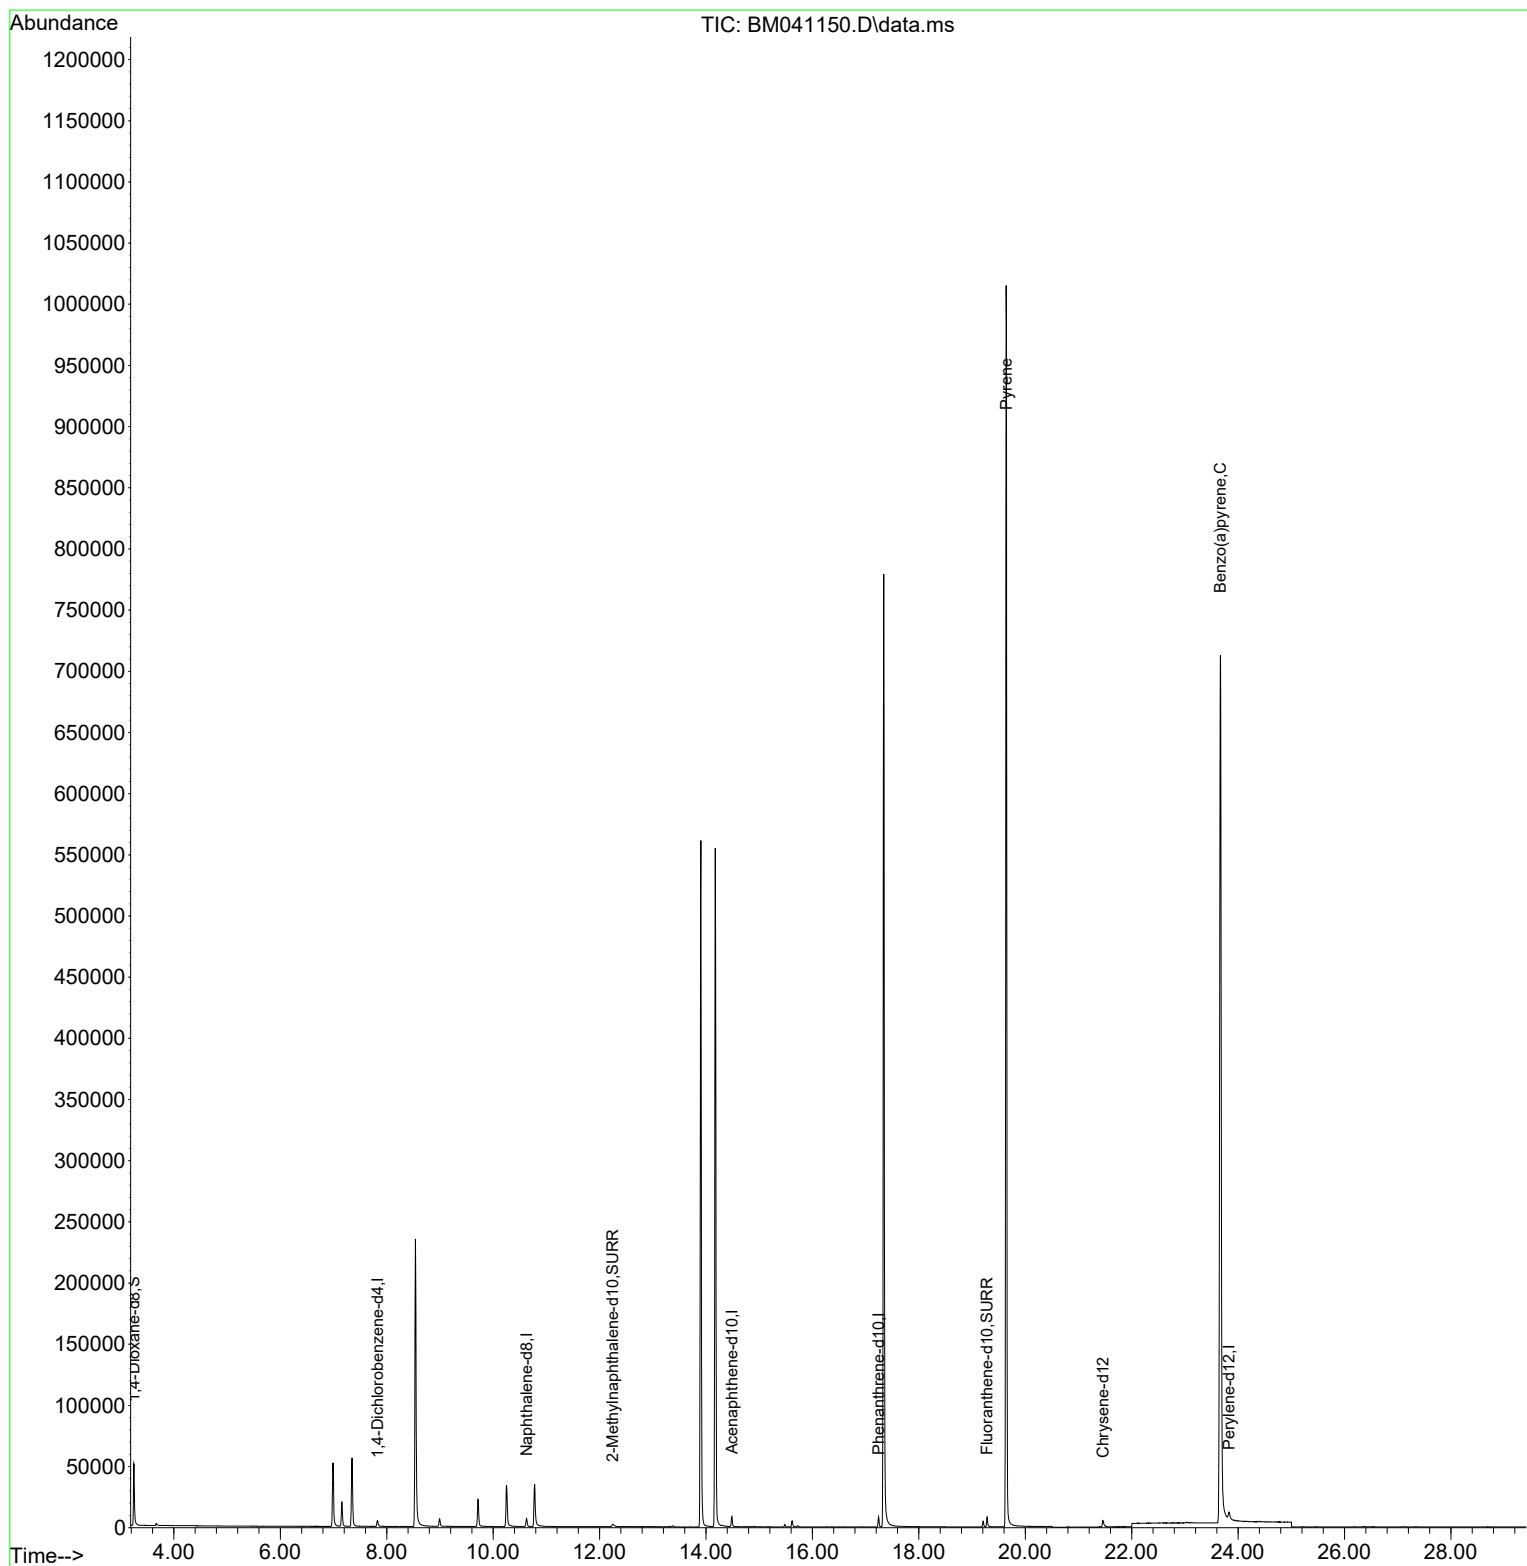

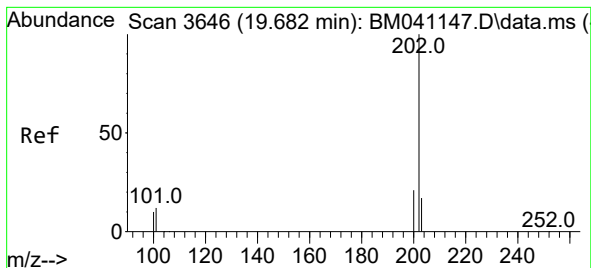

#20

Pyrene

Concen: 0.047 ng/ul

RT: 19.640 min Scan# 3

Delta R.T. -0.042 min

Lab File: BM041150.D

Acq: 27 Jul 2023 12:00

Instrument :

BNA_M

ClientSampleId :

SBLK091





Tgt Ion:202 Resp: 1535

Ion Ratio Lower Upper

202 100

101 154.1 10.7 16.1#

100 1158.1 8.5 12.7#

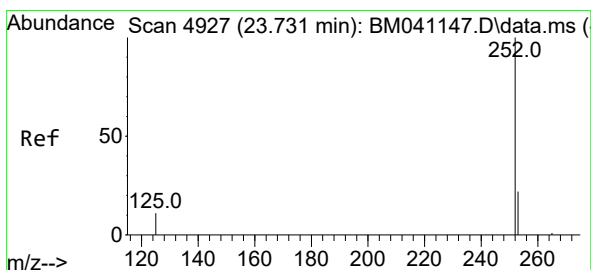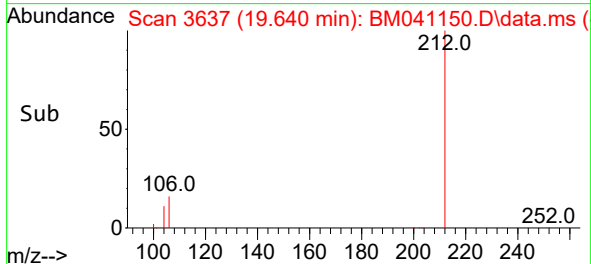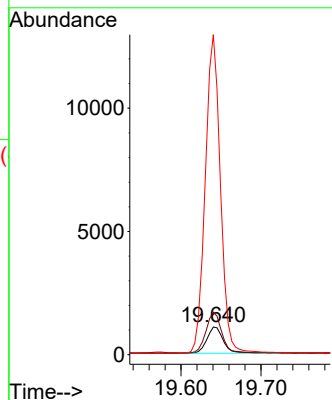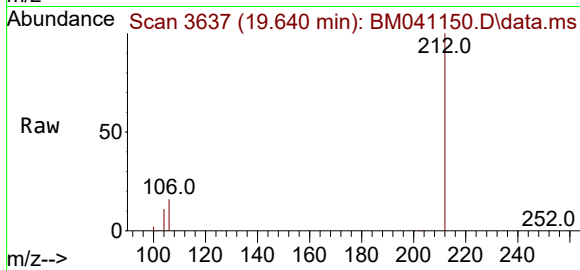

#26

Benzo(a)pyrene

Concen: 0.094 ng/ul

RT: 23.667 min Scan# 4905

Delta R.T. -0.062 min

Lab File: BM041150.D

Acq: 27 Jul 2023 12:00

Tgt Ion:252 Resp: 3526

Ion Ratio Lower Upper

252 100

253 50.7 26.7 40.1#

125 40.6 18.1 27.1#

