

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072723\
 Data File : BM041152.D
 Acq On : 27 Jul 2023 13:16
 Operator : MA/JU
 Sample : 03553-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A46Y5

Quant Time: Jul 28 03:29:38 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 26 04:20:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.828	152	3718	0.400	ng/ul	0.00
4) Naphthalene-d8	10.631	136	11876	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.486	164	5749	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.244	188	12531	0.400	ng/ul	0.00
17) Chrysene-d12	21.448	240	12454	0.400	ng/ul	0.00
23) Perylene-d12	23.825	264	15228	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.250	96	8447	1.473	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.242	152	4045	0.239	ng/ul	0.00
18) Fluoranthene-d10	19.278	212	11334	0.334	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.640	202	1944	0.039	ng/ul#	1
26) Benzo(a)pyrene	23.670	252	3952	0.080	ng/ul#	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072723\
Data File : BM041152.D
Acq On : 27 Jul 2023 13:16
Operator : MA/JU
Sample : 03553-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A46Y5

Quant Time: Jul 28 03:29:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 04:20:13 2023
Response via : Initial Calibration




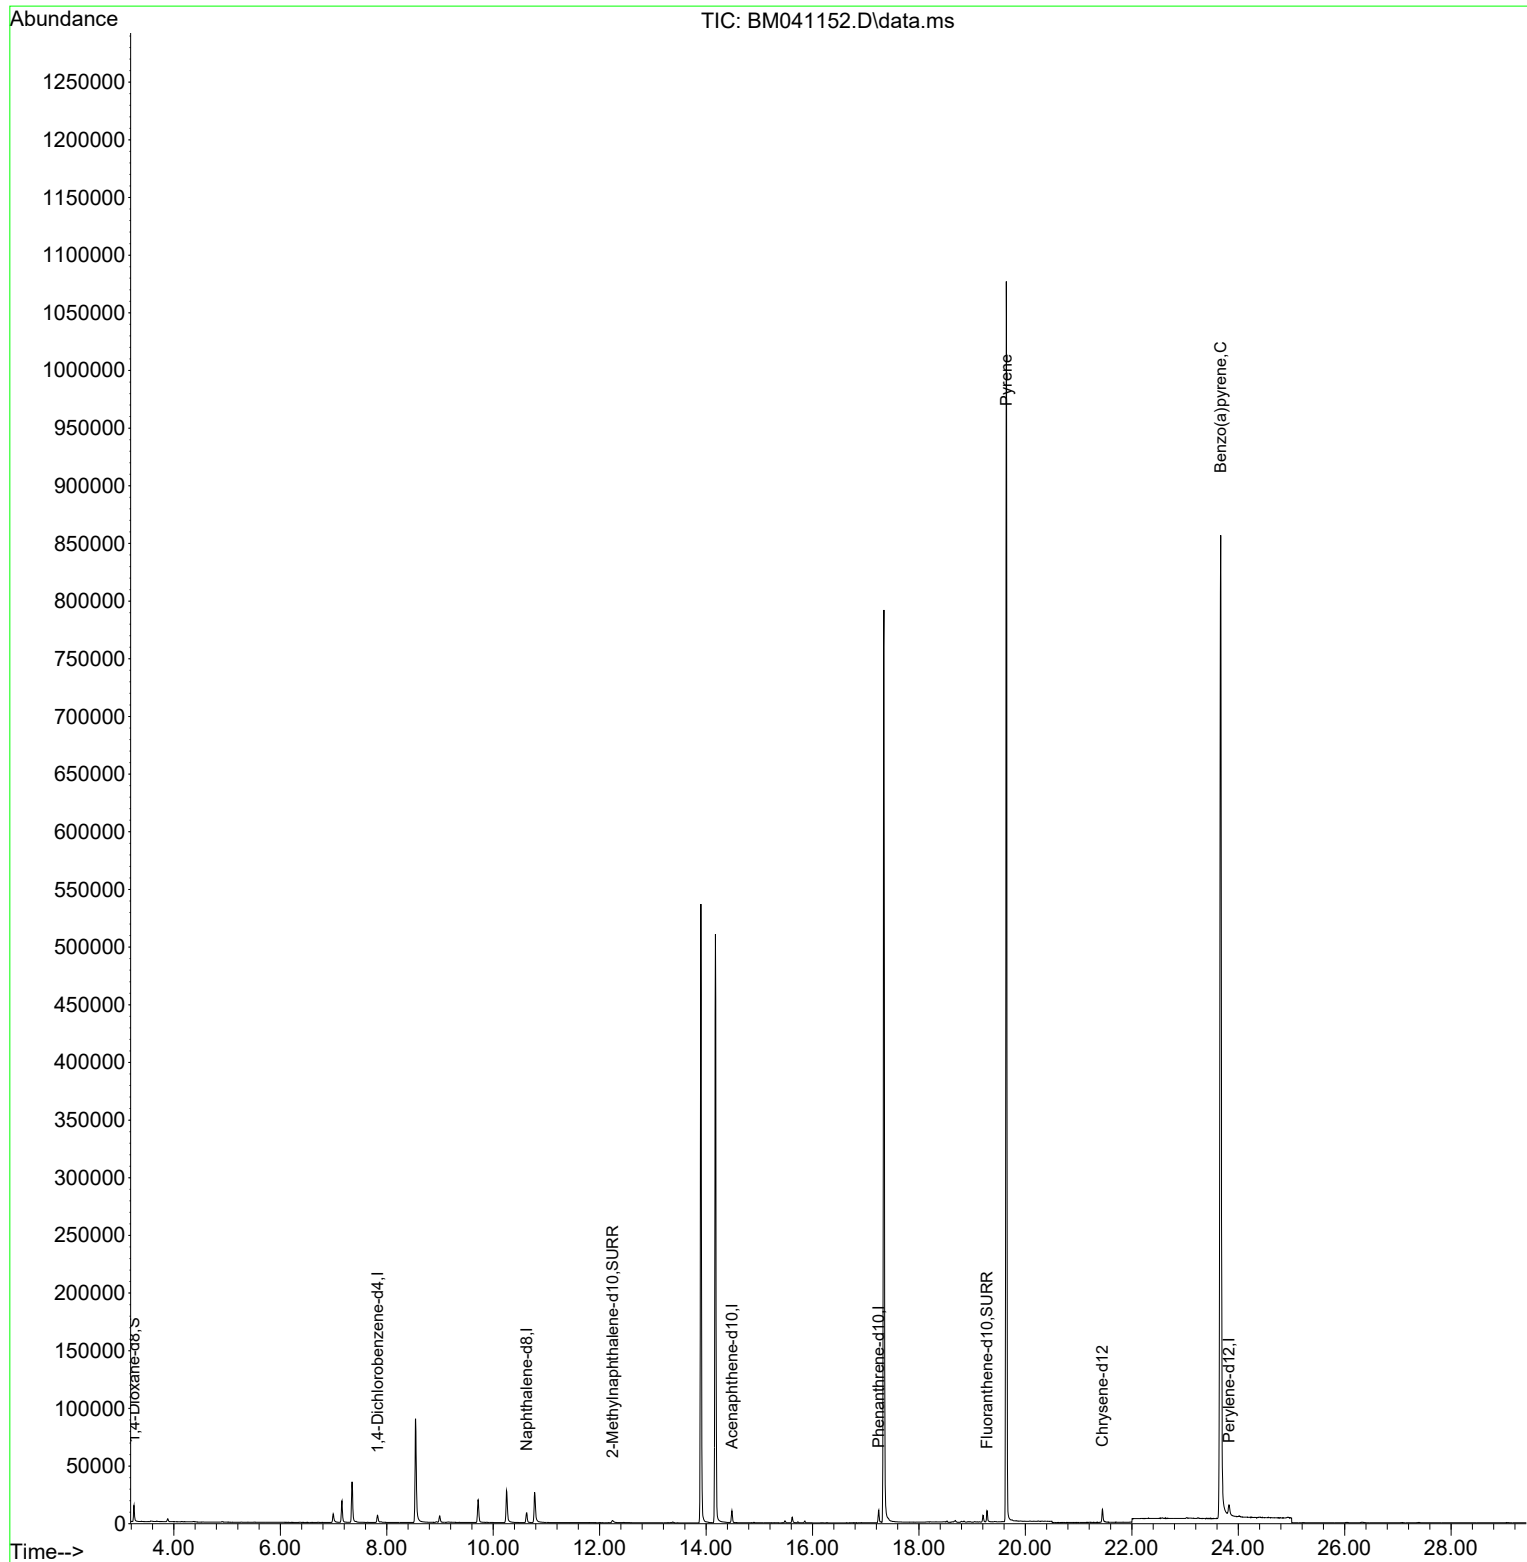


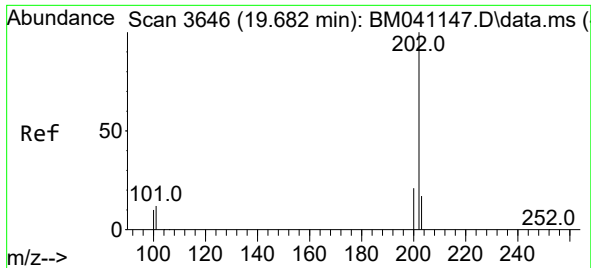

#20
Pyrene
Concen: 0.039 ng/ul
RT: 19.640 min Scan# 30
Delta R.T. -0.042 min
Lab File: BM041152.D
Acq: 27 Jul 2023 13:16

Instrument :
BNA_M
ClientSampleId :
A46Y5

Tgt Ion:202 Resp: 1944
Ion Ratio Lower Upper
202 100
101 142.8 10.7 16.1#
100 1065.9 8.5 12.7#

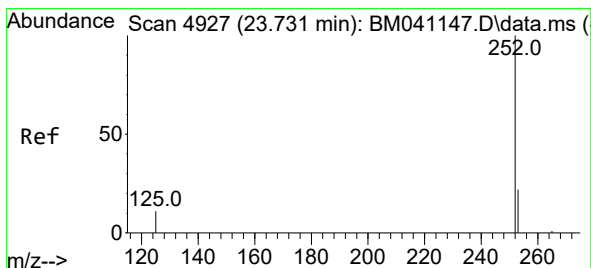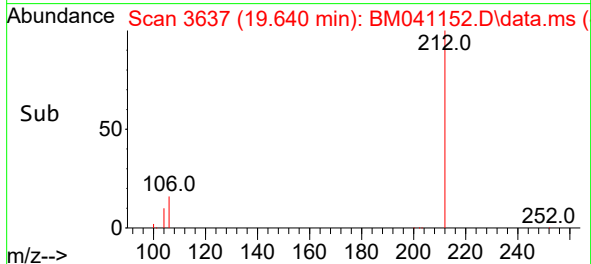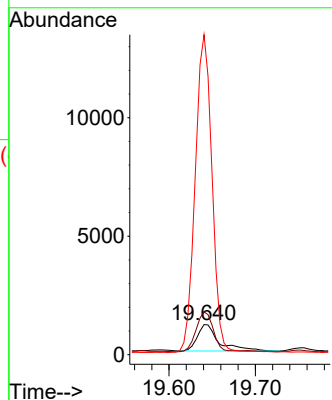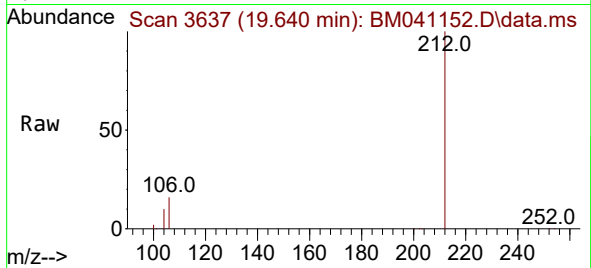

#26
Benzo(a)pyrene
Concen: 0.080 ng/ul
RT: 23.670 min Scan# 4906
Delta R.T. -0.059 min
Lab File: BM041152.D
Acq: 27 Jul 2023 13:16

Tgt Ion:252 Resp: 3952
Ion Ratio Lower Upper
252 100
253 50.9 26.7 40.1#
125 44.3 18.1 27.1#

