

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072723\
 Data File : BM041153.D
 Acq On : 27 Jul 2023 13:54
 Operator : MA/JU
 Sample : 03553-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A46Y8

Quant Time: Jul 28 03:29:44 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 26 04:20:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.828	152	3964	0.400	ng/ul	0.00
4) Naphthalene-d8	10.631	136	13002	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.486	164	6224	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.244	188	12287	0.400	ng/ul	0.00
17) Chrysene-d12	21.451	240	10403	0.400	ng/ul	0.00
23) Perylene-d12	23.830	264	12610	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.250	96	8959	1.465	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.236	152	4119	0.222	ng/ul	0.00
18) Fluoranthene-d10	19.282	212	8666	0.306	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.640	202	1343	0.033	ng/ul#	1
26) Benzo(a)pyrene	23.670	252	2940	0.072	ng/ul#	60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072723\
Data File : BM041153.D
Acq On : 27 Jul 2023 13:54
Operator : MA/JU
Sample : 03553-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A46Y8

Quant Time: Jul 28 03:29:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 04:20:13 2023
Response via : Initial Calibration




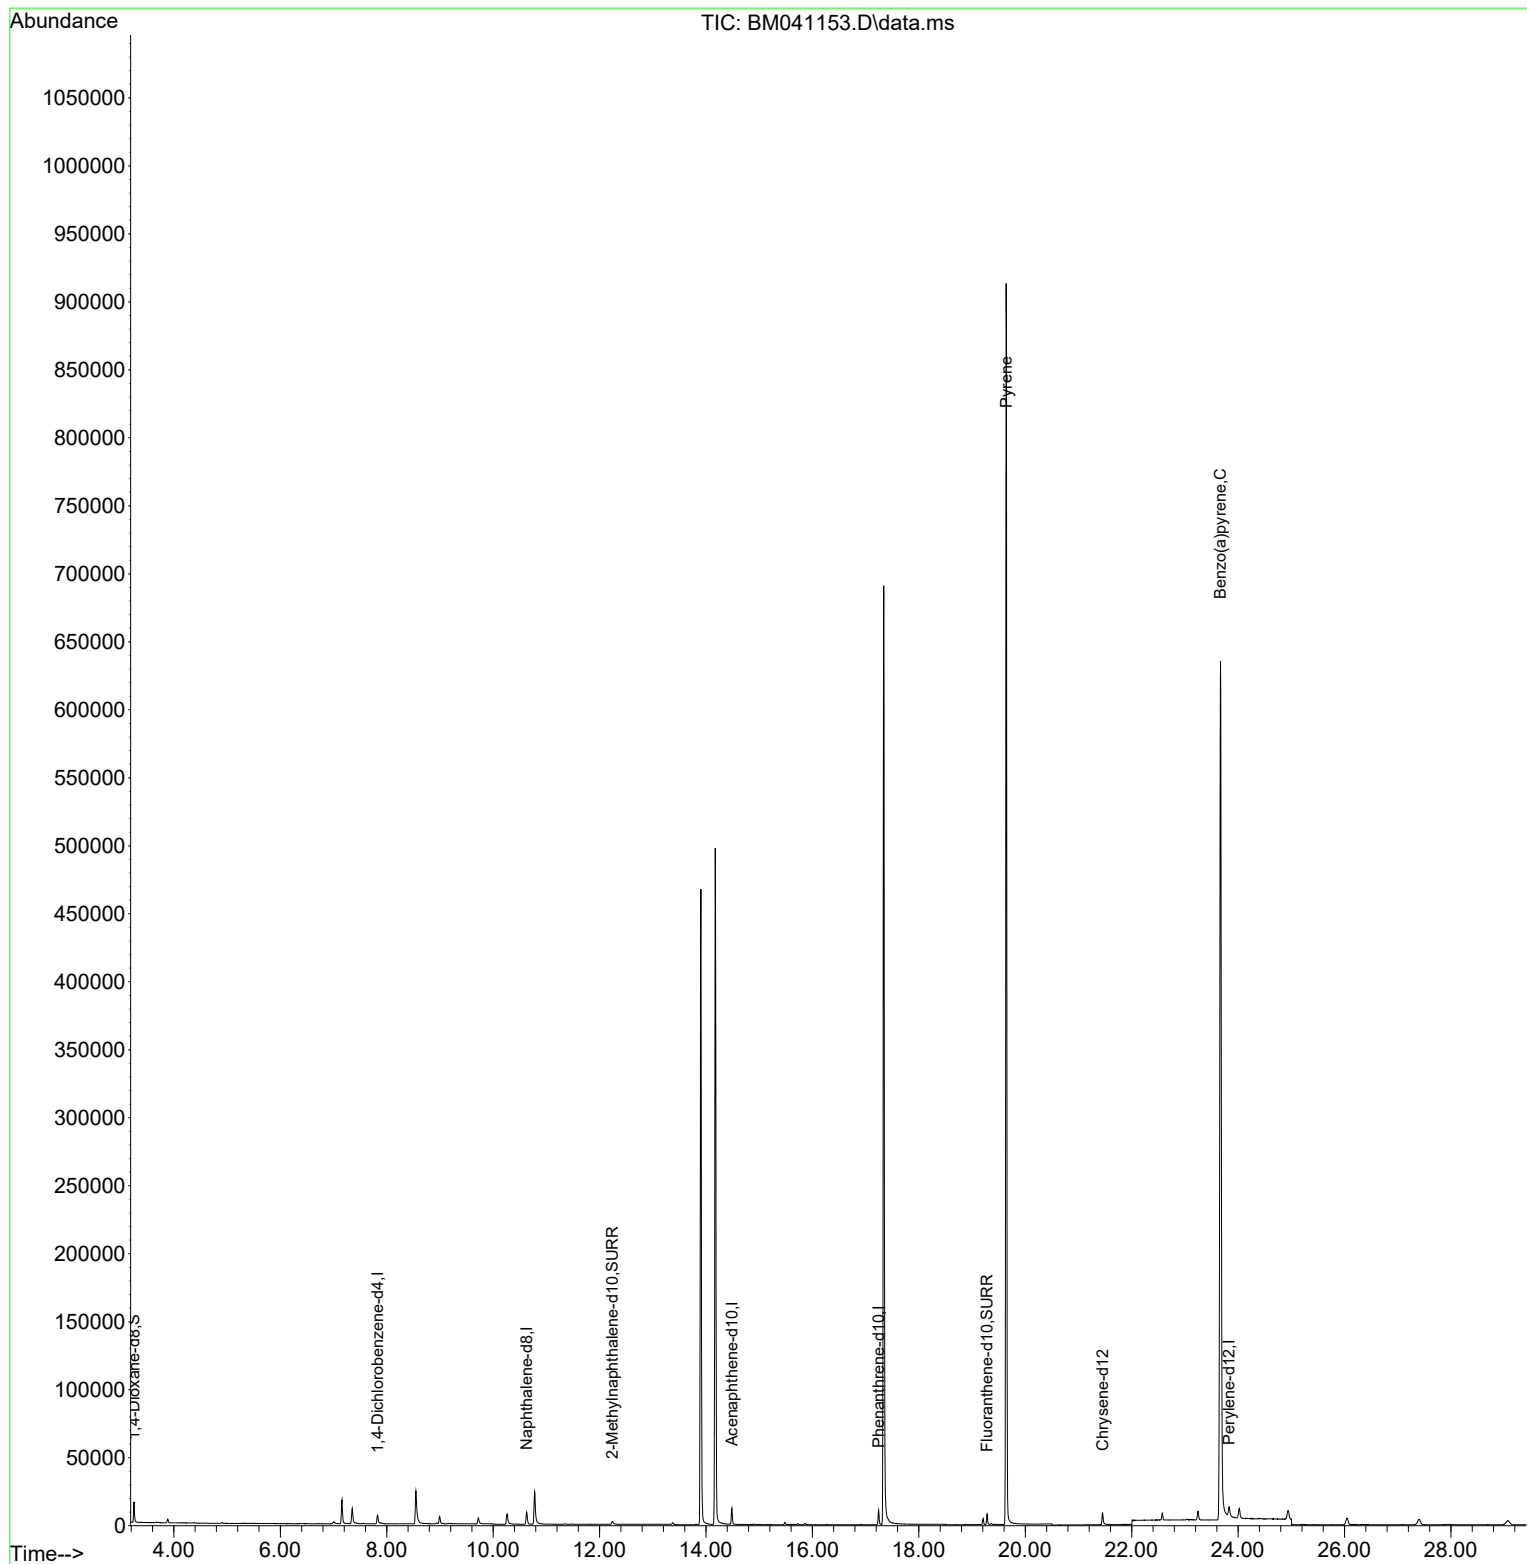


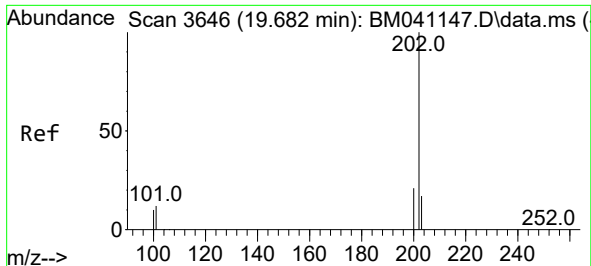

#20
Pyrene
Concen: 0.033 ng/ul
RT: 19.640 min Scan# 3
Delta R.T. -0.042 min
Lab File: BM041153.D
Acq: 27 Jul 2023 13:54

Instrument :
BNA_M
ClientSampleId :
A46Y8

Tgt Ion:202 Resp: 1343
Ion Ratio Lower Upper
202 100
101 153.2 10.7 16.1#
100 1146.5 8.5 12.7#

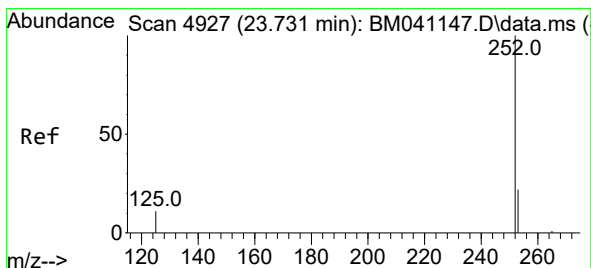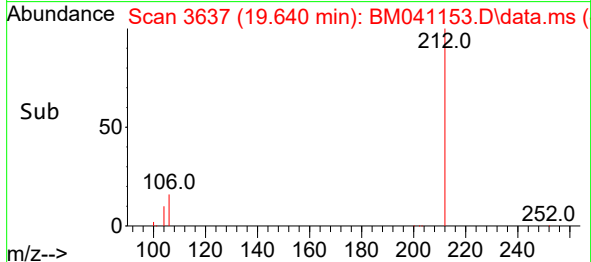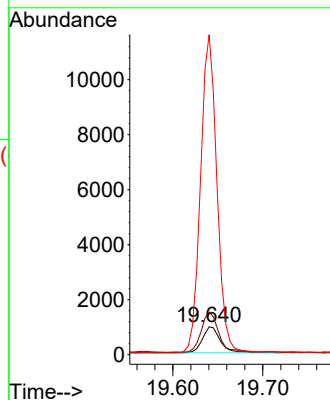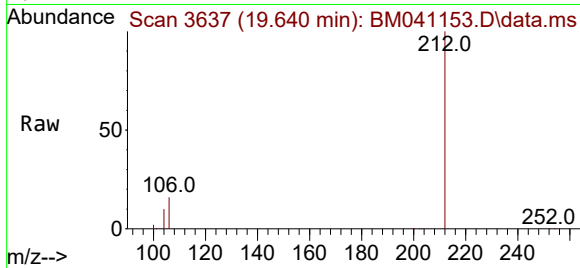

#26
Benzo(a)pyrene
Concen: 0.072 ng/ul
RT: 23.670 min Scan# 4906
Delta R.T. -0.059 min
Lab File: BM041153.D
Acq: 27 Jul 2023 13:54

Tgt Ion:252 Resp: 2940
Ion Ratio Lower Upper
252 100
253 54.2 26.7 40.1#
125 44.1 18.1 27.1#

