

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072723\
 Data File : BM041155.D
 Acq On : 27 Jul 2023 15:09
 Operator : MA/JU
 Sample : 03553-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A46Z6

Quant Time: Jul 28 03:29:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 26 04:20:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.828	152	3589	0.400	ng/ul	0.00
4) Naphthalene-d8	10.631	136	11639	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.486	164	5594	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.244	188	11687	0.400	ng/ul	0.00
17) Chrysene-d12	21.454	240	10030	0.400	ng/ul	0.00
23) Perylene-d12	23.828	264	12681	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.250	96	8548	1.544	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.242	152	3874	0.233	ng/ul	0.00
18) Fluoranthene-d10	19.283	212	9762	0.358	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.645	202	1616	0.041	ng/ul#	1
26) Benzo(a)pyrene	23.670	252	3461	0.085	ng/ul#	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072723\
Data File : BM041155.D
Acq On : 27 Jul 2023 15:09
Operator : MA/JU
Sample : 03553-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A46Z6

Quant Time: Jul 28 03:29:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 04:20:13 2023
Response via : Initial Calibration




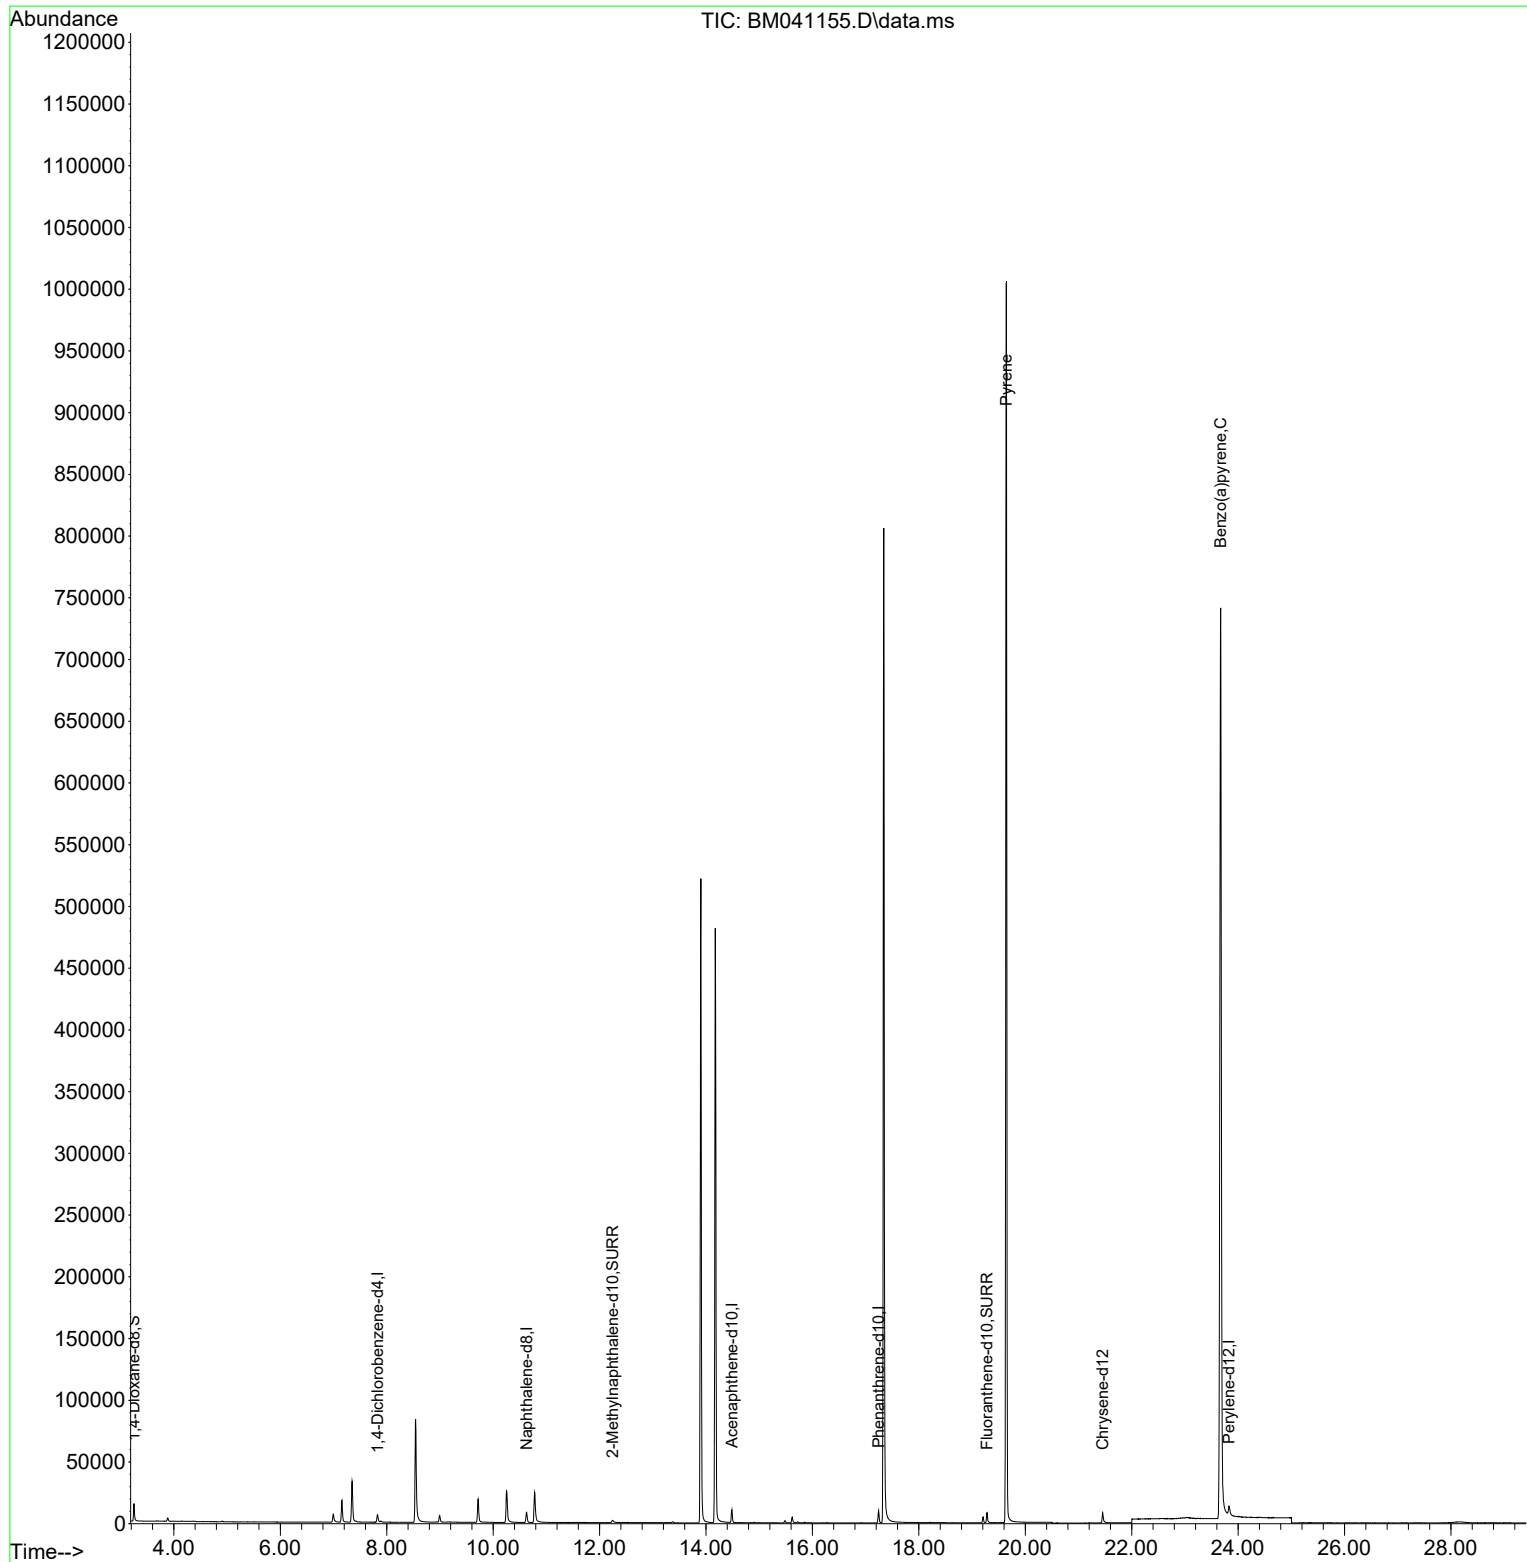


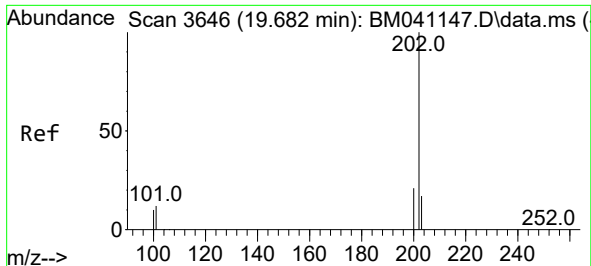

#20
Pyrene
Concen: 0.041 ng/ul
RT: 19.645 min Scan# 3646
Delta R.T. -0.037 min
Lab File: BM041155.D
Acq: 27 Jul 2023 15:09

Instrument :
BNA_M
ClientSampleId :
A46Z6

Tgt Ion:202 Resp: 1616
Ion Ratio Lower Upper
202 100
101 141.5 10.7 16.1#
100 1003.9 8.5 12.7#

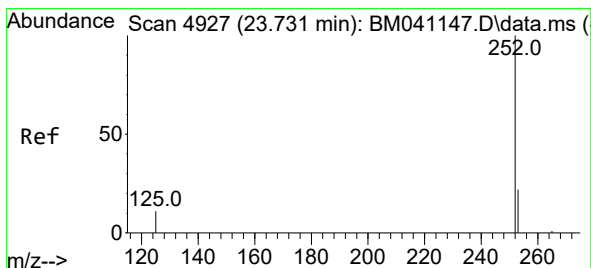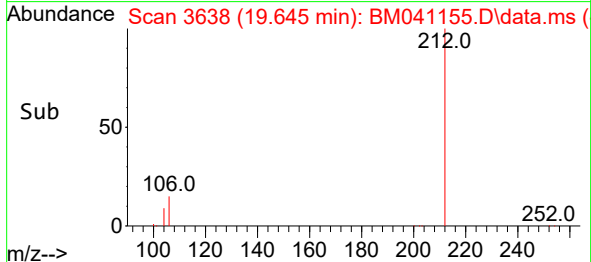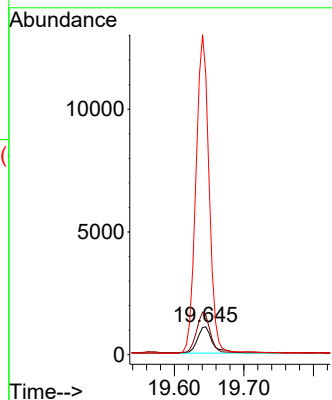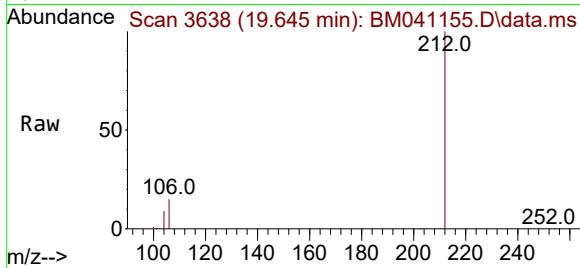

#26
Benzo(a)pyrene
Concen: 0.085 ng/ul
RT: 23.670 min Scan# 4906
Delta R.T. -0.059 min
Lab File: BM041155.D
Acq: 27 Jul 2023 15:09

Tgt Ion:252 Resp: 3461
Ion Ratio Lower Upper
252 100
253 50.2 26.7 40.1#
125 42.0 18.1 27.1#

