

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072820\
 Data File : BM026932.D
 Acq On : 29 Jul 2020 18:53
 Operator : JU/CG
 Sample : L1955-10
 Misc : MDL-WATER-03
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-03

Quant Time: Jul 30 01:22:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 30 01:20:34 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	53874	20.00	ng/ul	0.00
18) Naphthalene-d8	10.44	136	199215	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.30	164	124366	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	268159	20.00	ng/ul	0.00
78) Chrysene-d12	21.23	240	295390	20.00	ng/ul	-0.01
86) Perylene-d12	23.44	264	311633	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	8787	7.44	ng/uL	0.00
5) Phenol-d5	6.84	99	140669	29.81	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.01	67	102813	32.18	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	111622	31.60	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	109731	30.22	ng/ul	0.00
19) Nitrobenzene-d5	8.81	128	51058	32.95	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	47603	33.51	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	107501	31.70	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	128045	31.67	ng/ul	0.00
44) Dimethylphthalate-d6	13.71	166	319251	32.74	ng/ul	0.00
47) Acenaphthylene-d8	13.99	160	408093	32.89	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	50428	30.57	ng/ul	0.00
58) Fluorene-d10	15.29	176	283626	33.43	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.41	200	33862	28.33	ng/ul	0.00
71) Anthracene-d10	17.14	188	435428	32.49	ng/ul	0.00
79) Pyrene-d10	19.44	212	498536	31.64	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.31	264	547292	31.12	ng/ul	-0.01

Target Compounds

					Ovalue
2) 1,4-Dioxane	3.25	88	7400	5.042	ng/uL 95
4) Benzaldehyde	6.81	77	18890	4.913	ng/ul 94
6) Phenol	6.87	94	35758	7.080	ng/ul# 89
8) Bis(2-Chloroethyl)ether	7.10	93	29591	7.404	ng/ul 98
10) 2-Chlorophenol	7.24	128	28459	7.761	ng/ul 96
11) 2-Methylphenol	8.11	108	24344	6.737	ng/ul 93
12) 2,2'-oxybis(1-Chloropropan	8.20	45	23794	6.723	ng/ul# 93
14) Acetophenone	8.48	105	45870	7.613	ng/ul# 97
15) N-Nitroso-di-n-propylamine	8.47	70	25397	6.979	ng/ul 92
16) 4-Methylphenol	8.43	108	26487	6.879	ng/ul 88
17) Hexachloroethane	8.74	117	14204	8.127	ng/ul 93
20) Nitrobenzene	8.85	77	42137	8.394	ng/ul 99
21) Isophorone	9.38	82	60784	6.868	ng/ul 98
23) 2-Nitrophenol	9.56	139	12734	7.858	ng/ul 95
24) 2,4-Dimethylphenol	9.62	107	32666	7.717	ng/ul 96
25) Bis(2-Chloroethoxy)methane	9.86	93	36838	7.471	ng/ul 99
27) 2,4-Dichlorophenol	10.09	162	27528	8.333	ng/ul 94
28) Naphthalene	10.49	128	86759	7.795	ng/ul 98
30) 4-Chloroaniline	10.60	127	29708	7.285	ng/ul 91
31) Hexachlorobutadiene	10.80	225	20137	8.632	ng/ul 98
32) Caprolactam	11.36	113	6212	6.022	ng/ul 94
33) 4-Chloro-3-methylphenol	11.72	107	26236	7.123	ng/ul 97
34) 2-Methylnaphthalene	12.11	142	60761	7.722	ng/ul 99

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072820\
 Data File : BM026932.D
 Acq On : 29 Jul 2020 18:53
 Operator : JU/CG
 Sample : L1955-10
 Misc : MDL-WATER-03
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-03

Quant Time: Jul 30 01:22:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 30 01:20:34 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
35) 1-Methylnaphthalene	12.33	142	58502	7.609	ng/ul#	95
37) 1,2,4,5-Tetrachlorobenzene	12.48	216	35410	8.330	ng/ul	98
38) Hexachlorocyclopentadiene	12.48	237	17137	5.946	ng/ul	96
39) 2,4,6-Trichlorophenol	12.72	196	17267	7.089	ng/ul	94
40) 2,4,5-Trichlorophenol	12.79	196	19314	7.421	ng/ul	97
41) 1,1'-Biphenyl	13.13	154	80454	7.742	ng/ul	97
42) 2-Chloronaphthalene	13.17	162	65716	7.859	ng/ul	99
43) 2-Nitroaniline	13.37	65	17971	7.226	ng/ul	98
45) Dimethylphthalate	13.76	163	80323	7.848	ng/ul	100
46) 2,6-Dinitrotoluene	13.87	165	12608	6.987	ng/ul#	80
48) Acenaphthylene	14.02	152	97123	7.703	ng/ul	99
49) 3-Nitroaniline	14.19	138	11062	6.272	ng/ul	93
50) Acenaphthene	14.37	153	68303	7.863	ng/ul	99
51) 2,4-Dinitrophenol	14.40	184	3985	5.515	ng/ul#	84
53) 4-Nitrophenol	14.50	109	15903	9.624	ng/ul#	79
54) Dibenzofuran	14.70	168	97275	8.078	ng/ul	92
55) 2,4-Dinitrotoluene	14.65	165	19939	7.691	ng/ul	94
56) 2,3,4,6-Tetrachlorophenol	14.93	232	15343	7.514	ng/ul	95
57) Diethylphthalate	15.14	149	80061	7.801	ng/ul	97
59) Fluorene	15.35	166	79341	7.825	ng/ul	94
60) 4-Chlorophenyl-phenylether	15.35	204	40888	8.102	ng/ul	90
61) 4-Nitroaniline	15.35	138	14167	6.554	ng/ul#	87
64) 4,6-Dinitro-2-methylphenol	15.42	198	9660	7.112	ng/ul#	80
65) N-Nitrosodiphenylamine	15.56	169	65573	7.475	ng/ul	99
66) 4-Bromophenyl-phenylether	16.24	248	24554	7.805	ng/ul	95
67) Hexachlorobenzene	16.36	284	29766	8.344	ng/ul	94
68) Atrazine	16.51	200	22406	6.958	ng/ul	98
69) Pentachlorophenol	16.69	266	12038	6.781	ng/ul	92
70) Phenanthrene	17.08	178	128233	7.878	ng/ul	100
72) Anthracene	17.17	178	129955	7.767	ng/ul	98
73) 1,2,3,4-Tetrachlorobenzene	13.09	216	31866	7.564	ng/uL	96
74) Pentachlorobenzene	14.62	250	34020	8.329	ng/uL	98
75) Carbazole	17.44	167	109033	7.372	ng/ul	98
76) Di-n-butylphthalate	18.03	149	119227	6.853	ng/ul	98
77) Fluoranthene	19.10	202	149498	7.778	ng/ul	97
80) Pvrene	19.47	202	162324	7.553	ng/ul#	95
81) Butylbenzylphthalate	20.38	149	48378	6.054	ng/ul	97
82) 3,3'-Dichlorobenzidine	21.15	252	34076	4.879	ng/ul	91
83) Benzo(a)anthracene	21.22	228	156331	7.678	ng/ul	100
84) Bis(2-ethylhexyl)phthalate	21.18	149	73624	6.145	ng/ul	97
85) Chrysene	21.27	228	154769	7.795	ng/ul	99
87) Di-n-octyl phthalate	22.05	149	121639	5.312	ng/ul	100
88) Benzo(b)fluoranthene	22.78	252	157478	7.064	ng/ul	99
89) Benzo(k)fluoranthene	22.82	252	164217	7.677	ng/ul	99
91) Benzo(a)pyrene	23.35	252	155966	7.753	ng/ul	97
92) Indeno(1,2,3-cd)pyrene	25.65	276	195908	7.850	ng/ul	97
93) Dibenzo(a,h)anthracene	25.66	278	167444	7.933	ng/ul	98
94) Benzo(a,h,i)perylene	26.32	276	163911	7.943	ng/ul	99


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072820\
Data File : BM026932.D
Acq On : 29 Jul 2020 18:53
Operator : JU/CG
Sample : L1955-10
Misc : MDL-WATER-03
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-03

Quant Time: Jul 30 01:22:04 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 30 01:20:34 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)

(#) = qualifier out of range (m) = manual integration (+) = signals summed						



#2

1,4-Dioxane

Concen: 5.042 ng/uL

RT: 3.25 min Scan# 88

Delta R.T. -0.00 min

Lab File: BM026932.D

Acq: 29 Jul 2020 18:53

Instrument :

BNA_M

ClientSampleId :

MDL-WATER-03


Tot Ion: 88 Resp: 7400

Ion Ratio Lower Upper

88 100

43 26.0 24.7 37.1




58 60.9 50.8 76.2



Abundance Ion 88.00 (87.70 to 88.70): BM026932.D (-54) (-)

Ion 43.00 (42.70 to 43.70): BM026932.D (-54) (-)

Ion 58.00 (57.70 to 58.70): BM026932.D (-54) (-)

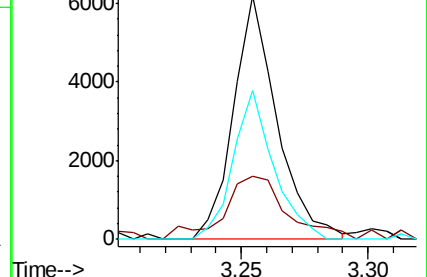

#4

Benzaldehyde

Concen: 4.913 ng/uL

RT: 6.81 min Scan# 693

Delta R.T. -0.00 min

Lab File: BM026932.D

Acq: 29 Jul 2020 18:53


Tgt Ion: 77 Resp: 18890

Ion Ratio Lower Upper

77 100

105 85.8 64.9 97.3



106 84.0 62.5 93.7




Abundance Ion 77.00 (76.70 to 77.70): BM026932.D (-659) (-)

Ion 105.00 (104.70 to 105.70): BM026932.D (-659) (-)

Ion 106.00 (105.70 to 106.70): BM026932.D (-659) (-)

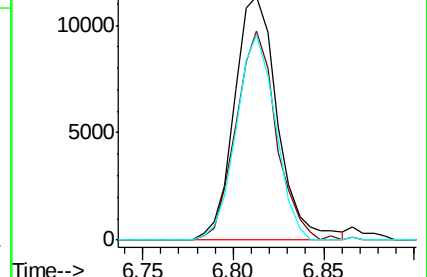



#6

Phenol

Concen: 7.080 ng/ul

RT: 6.87 min Scan# 702

Delta R.T. -0.01 min

Lab File: BM026932.D

Acq: 29 Jul 2020 18:53

Instrument :





BNA_M

ClientSampleId :

MDL-WATER-03

Tot Ion: 94 Resp: 35758

Ion	Ratio	Lower	Upper
94	100		
65	40.4	26.2	39.4#
66	54.0	38.2	57.2

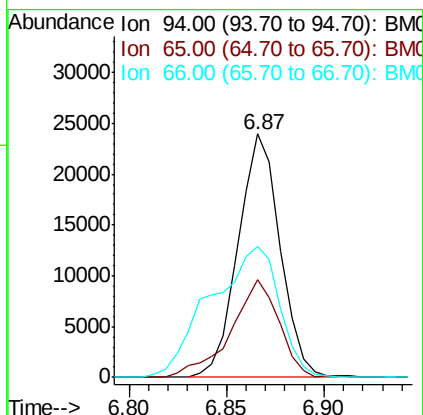

#8

Bis(2-Chloroethyl)ether

Concen: 7.404 ng/ul

RT: 7.10 min Scan# 741




Delta R.T. -0.01 min


Lab File: BM026932.D

Acq: 29 Jul 2020 18:53

Tgt Ion: 93 Resp: 29591

Ion	Ratio	Lower	Upper
93	100		
63	79.2	62.9	94.3
95	33.1	24.6	37.0

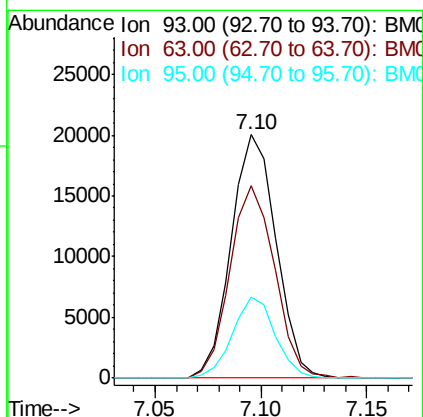

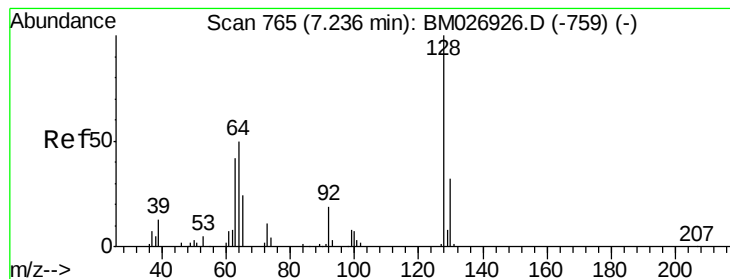

#10

2-Chlorophenol

Concen: 7.761 ng/ul

RT: 7.24 min Scan# 765

Delta R.T. -0.01 min

Lab File: BM026932.D

Acq: 29 Jul 2020 18:53

Instrument :

BNA_M

ClientSampleId :

MDL-WATER-03


Tot Ion:128 Resp: 28459

Ion Ratio Lower Upper




128 100

64 51.4 43.4 65.2

130 30.7 26.3 39.5



Abundance Ion 128.00 (127.70 to 128.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 130.00 (129.70 to 130.70): E

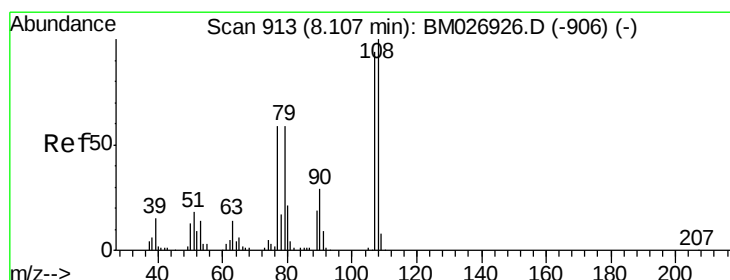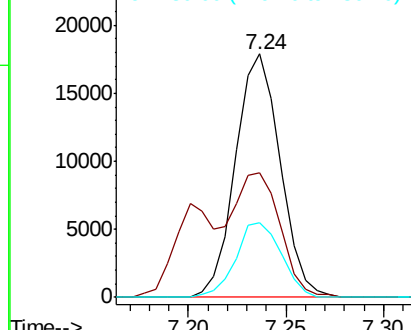

#11

2-Methylphenol

Concen: 6.737 ng/ul

RT: 8.11 min Scan# 913

Delta R.T. -0.00 min

Lab File: BM026932.D


Acq: 29 Jul 2020 18:53

Tgt Ion:108 Resp: 24344



Ion Ratio Lower Upper


108 100

107 97.6 72.5 108.7



Abundance Ion 108.00 (107.70 to 108.70): E
Ion 107.00 (106.70 to 107.70): E

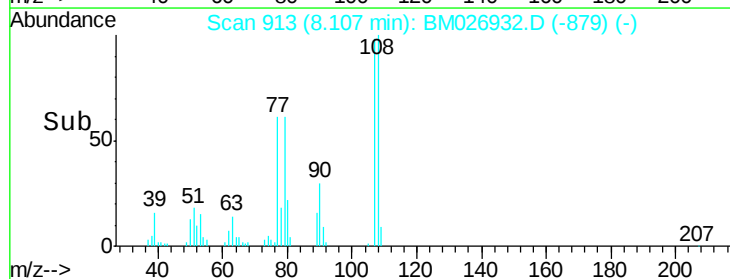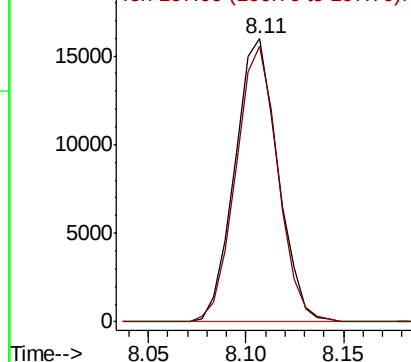







#12
2,2'-oxvbis(1-Chloropropane)
Concen: 6.723 ng/ul
RT: 8.20 min Scan# 929
Delta R.T. -0.01 min
Lab File: BM026932.D
Acq: 29 Jul 2020 18:53

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-03

Tot Ion: 45 Resp: 23794
Ion Ratio Lower Upper
45 100
77 30.7 19.7 29.5#
79 18.7 14.9 22.3




Abundance Ion 45.00 (44.70 to 45.70): BM0
Ion 77.00 (76.70 to 77.70): BM0
Ion 79.00 (78.70 to 79.70): BM0


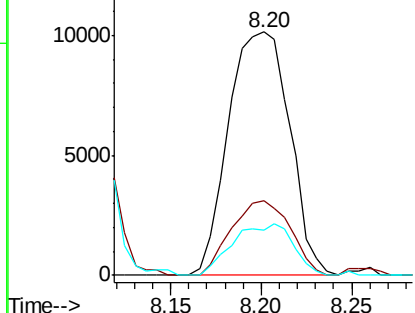



#14
Acetophenone
Concen: 7.613 ng/ul
RT: 8.48 min Scan# 976
Delta R.T. -0.01 min
Lab File: BM026932.D
Acq: 29 Jul 2020 18:53

Tgt Ion: 105 Resp: 45870
Ion Ratio Lower Upper
105 100
77 92.3 74.0 111.0
51 27.8 17.3 25.9#



Abundance Ion 105.00 (104.70 to 105.70): E
Ion 77.00 (76.70 to 77.70): BM0
Ion 51.00 (50.70 to 51.70): BM0

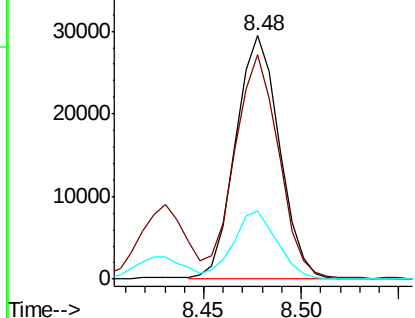



#15

N-Nitroso-di-n-propylamine

Concen: 6.979 ng/ul

RT: 8.47 min Scan# 975

Delta R.T. -0.00 min

Lab File: BM026932.D

Acq: 29 Jul 2020 18:53

Instrument :

BNA_M

ClientSampleId :

MDL-WATER-03

Tot Ion: 70 Resp: 25397


Ion Ratio Lower Upper

70 100

42 50.5 34.2 51.4

101 8.1 6.4 9.6

130 15.6 13.2 19.8






Abundance Ion 70.00 (69.70 to 70.70): BM0

Ion 42.00 (41.70 to 42.70): BM0

Ion 101.00 (100.70 to 101.70): E

Ion 130.00 (129.70 to 130.70): E

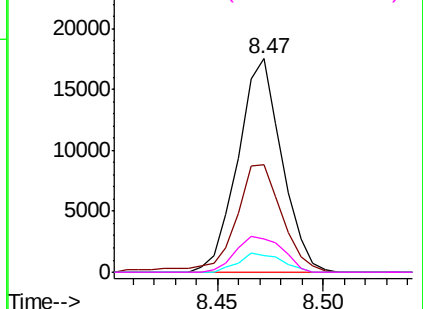

#16

4-Methylphenol

Concen: 6.879 ng/ul

RT: 8.43 min Scan# 968

Delta R.T. -0.01 min

Lab File: BM026932.D


Acq: 29 Jul 2020 18:53

Tgt Ion: 108 Resp: 26487

Ion Ratio Lower Upper



108 100


107 124.2 88.8 133.2



Abundance Ion 108.00 (107.70 to 108.70): E

Ion 107.00 (106.70 to 107.70): E

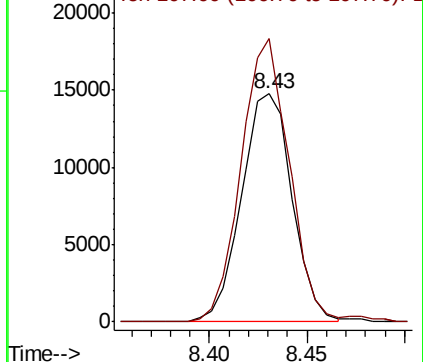







#17
Hexachloroethane
Concen: 8.127 ng/ul
RT: 8.74 min Scan# 1021
Delta R.T. -0.01 min
Lab File: BM026932.D
Acq: 29 Jul 2020 18:53

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-03

Tot Ion:117 Resp: 14204
Ion Ratio Lower Upper
117 100
201 108.9 80.8 121.2
199 66.3 50.3 75.5




Abundance Ion 117.00 (116.70 to 117.70): E
Ion 201.00 (200.70 to 201.70): E
Ion 199.00 (198.70 to 199.70): E


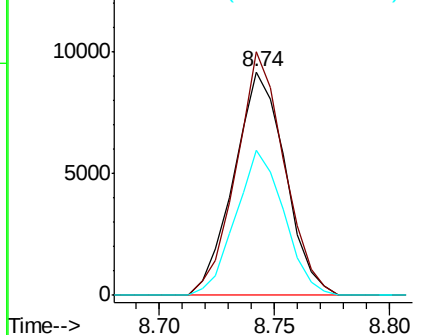



#20
Nitrobenzene
Concen: 8.394 ng/ul
RT: 8.85 min Scan# 1039
Delta R.T. -0.01 min
Lab File: BM026932.D
Acq: 29 Jul 2020 18:53

Tgt Ion: 77 Resp: 42137
Ion Ratio Lower Upper
77 100
123 35.3 28.3 42.5
65 15.3 11.0 16.6



Abundance Ion 77.00 (76.70 to 77.70): BM0
Ion 123.00 (122.70 to 123.70): E
Ion 65.00 (64.70 to 65.70): BM0

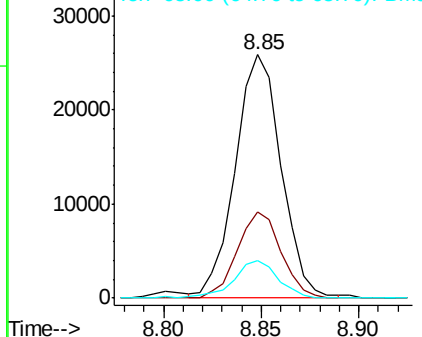

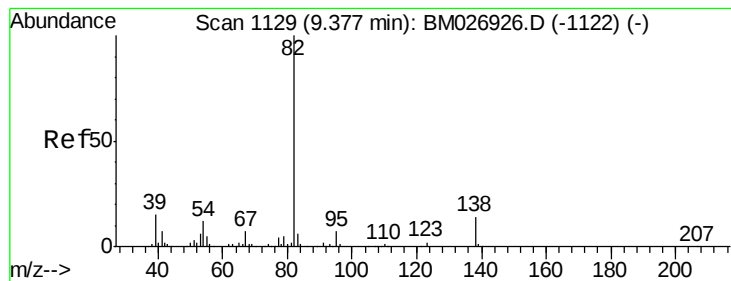

#21

Isophorone

Concen: 6.868 ng/ul

RT: 9.38 min Scan# 1129

Delta R.T. -0.01 min

Lab File: BM026932.D

Acq: 29 Jul 2020 18:53

Instrument :

BNA_M

ClientSampleId :

MDL-WATER-03





Tot Ion: 82 Resp: 60784

Ion Ratio Lower Upper

82 100

95 8.4 6.0 9.0

138 15.4 11.5 17.3

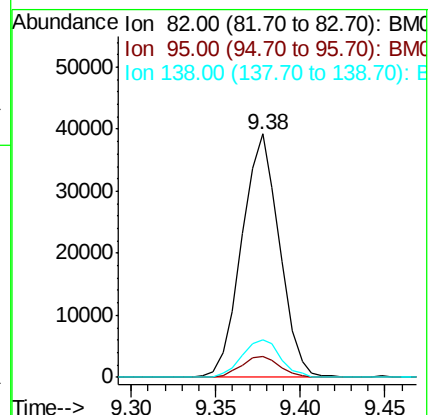

#23

2-Nitrophenol

Concen: 7.858 ng/ul

RT: 9.56 min Scan# 1160

Delta R.T. -0.00 min

Lab File: BM026932.D

Acq: 29 Jul 2020 18:53




Tgt Ion: 139 Resp: 12734


Ion Ratio Lower Upper

139 100

65 70.8 53.3 79.9

109 43.2 32.6 49.0



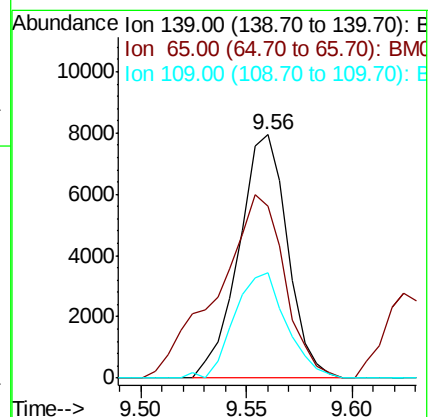





#24
 2,4-Dimethylphenol
 Concen: 7.717 ng/ul
 RT: 9.62 min Scan# 1171
 Delta R.T. -0.01 min
 Lab File: BM026932.D
 Acq: 29 Jul 2020 18:53




Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-03


Tot Ion:107 Resp: 32666
 Ion Ratio Lower Upper
 107 100
 121 47.6 35.5 53.3
 122 78.9 61.0 91.4

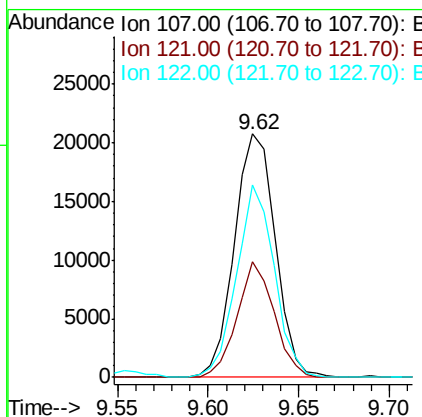

#25
 Bis(2-Chloroethoxy)methane
 Concen: 7.471 ng/ul
 RT: 9.86 min Scan# 1211
 Delta R.T. -0.01 min
 Lab File: BM026932.D
 Acq: 29 Jul 2020 18:53

Tgt Ion: 93 Resp: 36838
 Ion Ratio Lower Upper
 93 100
 95 32.7 25.7 38.5
 123 9.6 7.8 11.8

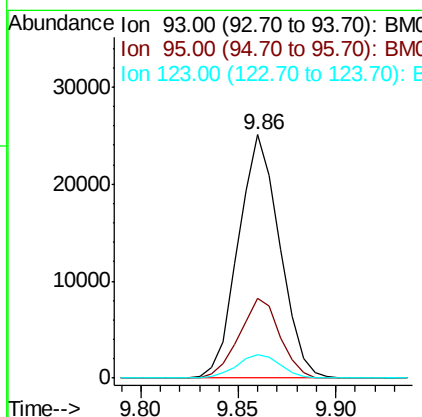

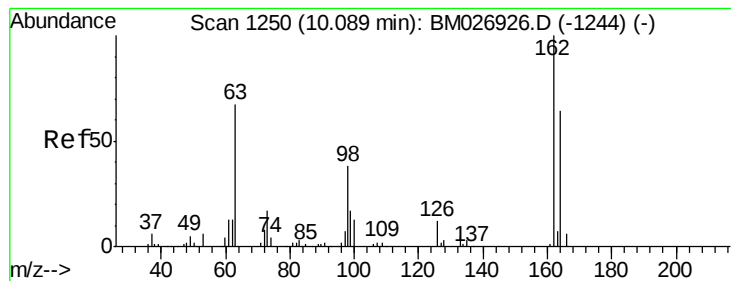

#27

2,4-Dichlorophenol

Concen: 8.333 ng/ul

RT: 10.09 min Scan# 1250

Delta R.T. -0.01 min

Lab File: BM026932.D

Acq: 29 Jul 2020 18:53

Instrument :

BNA_M

ClientSampleId :

MDL-WATER-03


Tot Ion:162 Resp: 27528

Ion Ratio Lower Upper

162 100

164 72.8 52.4 78.6




98 40.6 32.2 48.2



Abundance Ion 162.00 (161.70 to 162.70): E

Ion 164.00 (163.70 to 164.70): E

Ion 98.00 (97.70 to 98.70): BM

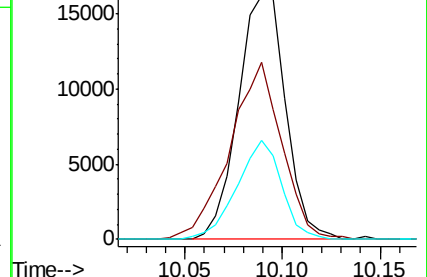

#28

Naphthalene

Concen: 7.795 ng/ul

RT: 10.49 min Scan# 1318

Delta R.T. -0.01 min

Lab File: BM026932.D

Acq: 29 Jul 2020 18:53


Tgt Ion:128 Resp: 86759

Ion Ratio Lower Upper

128 100

129 11.3 8.3 12.5



127 14.6 11.0 16.6




Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

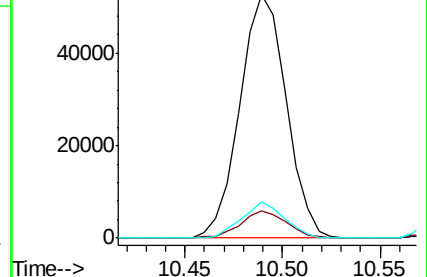

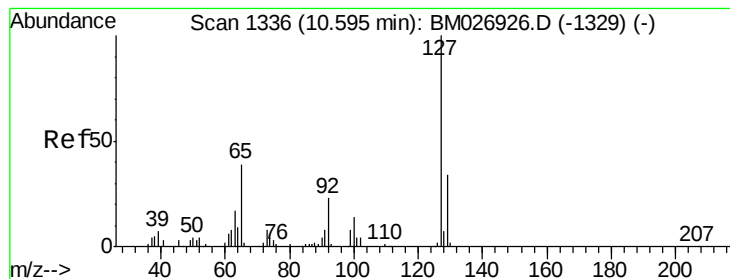

#30

4-Chloroaniline

Concen: 7.285 ng/ul

RT: 10.60 min Scan# 1336

Delta R.T. -0.01 min

Lab File: BM026932.D

Acq: 29 Jul 2020 18:53

Instrument :

BNA_M

ClientSampleId :


MDL-WATER-03

Tot Ion:127 Resp: 29708

Ion Ratio Lower Upper




127 100

129 35.4 24.3 36.5



Abundance Ion 127.00 (126.70 to 127.70): E

Ion 129.00 (128.70 to 129.70): E

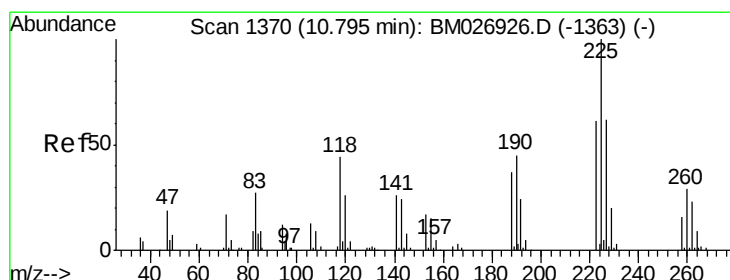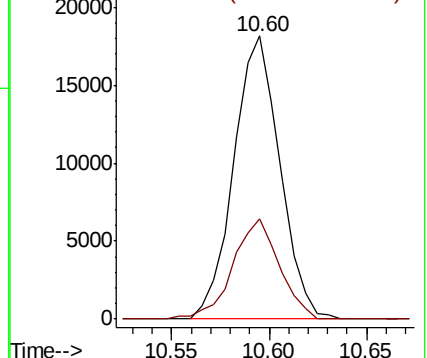

#31

Hexachlorobutadiene

Concen: 8.632 ng/ul

RT: 10.80 min Scan# 1370

Delta R.T. -0.01 min

Lab File: BM026932.D

Acq: 29 Jul 2020 18:53


Tgt Ion:225 Resp: 20137

Ion Ratio Lower Upper

225 100

223 60.5 51.4 77.0



227 66.7 53.1 79.7




Abundance Ion 225.00 (224.70 to 225.70): E

Ion 223.00 (222.70 to 223.70): E

Ion 227.00 (226.70 to 227.70): E

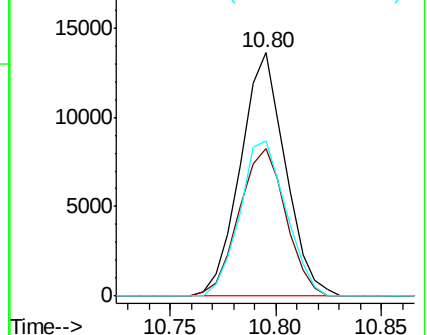

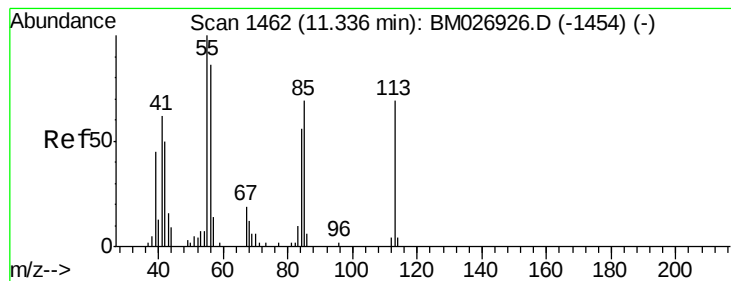

#32

Caprolactam

Concen: 6.022 ng/ul

RT: 11.36 min Scan# 1466

Delta R.T. 0.02 min

Lab File: BM026932.D

Acq: 29 Jul 2020 18:53

Instrument :

BNA_M

ClientSampleId :

MDL-WATER-03


Tot Ion:113 Resp: 6212

Ion Ratio Lower Upper

113 100

55 137.9 119.7 179.5




56 111.0 90.2 135.2



Abundance Ion 113.00 (112.70 to 113.70): E

Ion 55.00 (54.70 to 55.70): BM0

Ion 56.00 (55.70 to 56.70): BM0

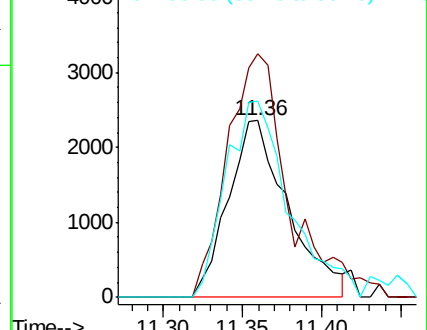

#33

4-Chloro-3-methylphenol

Concen: 7.123 ng/ul

RT: 11.72 min Scan# 1528

Delta R.T. -0.01 min

Lab File: BM026932.D

Acq: 29 Jul 2020 18:53


Tgt Ion:107 Resp: 26236

Ion Ratio Lower Upper

107 100

144 23.3 20.6 30.8



142 76.8 59.9 89.9




Abundance Ion 107.00 (106.70 to 107.70): E

Ion 144.00 (143.70 to 144.70): E

Ion 142.00 (141.70 to 142.70): E

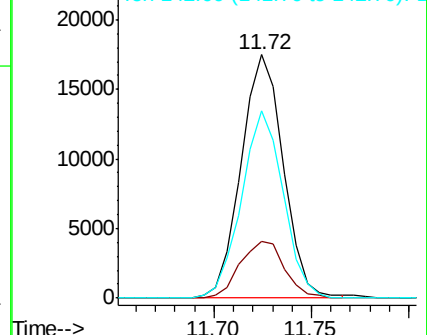



#34

2-Methylnaphthalene

Concen: 7.722 ng/ul

RT: 12.11 min Scan# 1593

Delta R.T. -0.01 min

Lab File: BM026932.D

Acq: 29 Jul 2020 18:53

Instrument :

BNA_M

ClientSampleId :


MDL-WATER-03

Tot Ion:142 Resp: 60761

Ion Ratio Lower Upper




142 100

141 88.1 71.1 106.7



Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

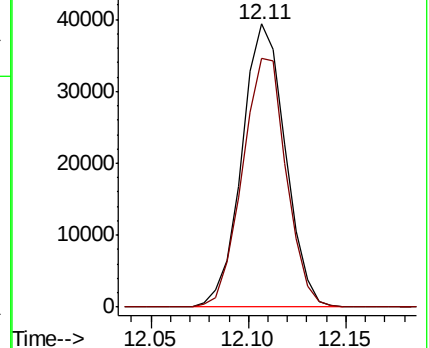

#35

1-Methylnaphthalene

Concen: 7.609 ng/ul

RT: 12.33 min Scan# 1631

Delta R.T. -0.01 min

Lab File: BM026932.D

Acq: 29 Jul 2020 18:53


Tgt Ion:142 Resp: 58502

Ion Ratio Lower Upper

142 100

141 96.6 73.3 109.9



116 5.6 3.4 5.0#




Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 116.00 (115.70 to 116.70): E

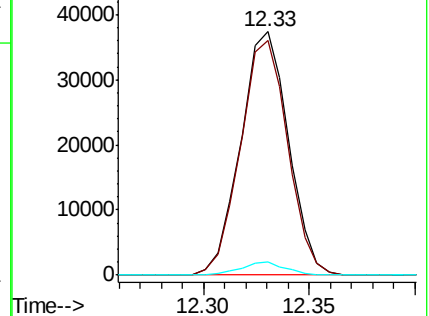







#37
 1,2,4,5-Tetrachlorobenzene
 Concen: 8.330 ng/ul
 RT: 12.48 min Scan# 1657
 Delta R.T. -0.01 min
 Lab File: BM026932.D
 Acq: 29 Jul 2020 18:53

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-03

Tot Ion:216 Resp: 35410
 Ion Ratio Lower Upper
 216 100
 214 78.9 64.2 96.4
 179 21.1 16.2 24.4
 108 23.2 16.7 25.1




Abundance Ion 216.00 (215.70 to 216.70): E
 Ion 214.00 (213.70 to 214.70): E
 Ion 179.00 (178.70 to 179.70): E
 Ion 108.00 (107.70 to 108.70): E


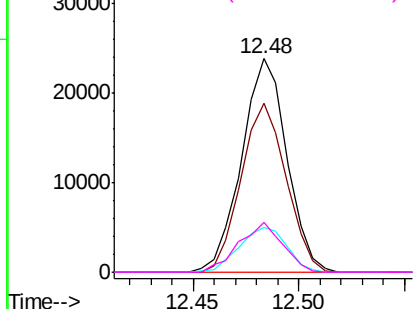



#38
 Hexachlorocyclopentadiene
 Concen: 5.946 ng/ul
 RT: 12.48 min Scan# 1656
 Delta R.T. -0.00 min
 Lab File: BM026932.D
 Acq: 29 Jul 2020 18:53

Tgt Ion:237 Resp: 17137
 Ion Ratio Lower Upper
 237 100
 235 65.7 49.8 74.8
 272 12.2 10.1 15.1



Abundance Ion 237.00 (236.70 to 237.70): E
 Ion 235.00 (234.70 to 235.70): E
 Ion 272.00 (271.70 to 272.70): E




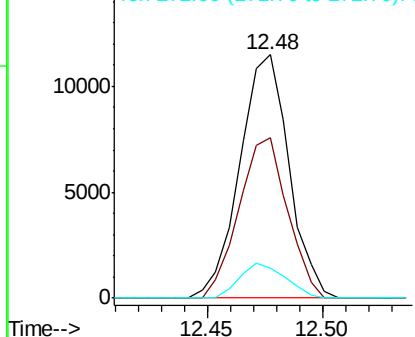




#39
 2,4,6-Trichlorophenol
 Concen: 7.089 ng/ul
 RT: 12.72 min Scan# 1698
 Delta R.T. -0.01 min
 Lab File: BM026932.D
 Acq: 29 Jul 2020 18:53




Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-03


Tot Ion:196 Resp: 17267
 Ion Ratio Lower Upper
 196 100
 198 92.3 79.0 118.6
 200 31.5 23.3 34.9

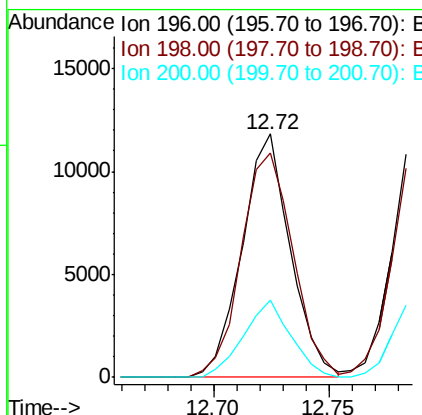

#40
 2,4,5-Trichlorophenol
 Concen: 7.421 ng/ul
 RT: 12.79 min Scan# 1709
 Delta R.T. -0.01 min
 Lab File: BM026932.D
 Acq: 29 Jul 2020 18:53

Tgt Ion:196 Resp: 19314
 Ion Ratio Lower Upper
 196 100
 198 96.7 79.0 118.6
 200 34.8 25.4 38.2

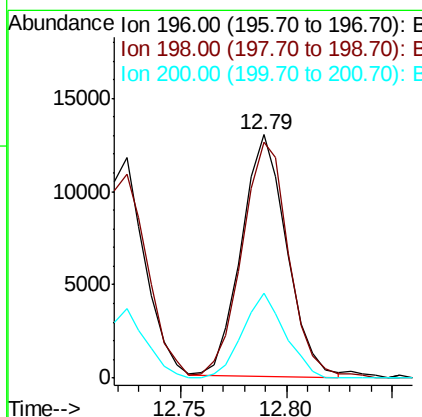







#41
 1,1'-Biphenyl
 Concen: 7.742 ng/ul
 RT: 13.13 min Scan# 1767
 Delta R.T. -0.01 min
 Lab File: BM026932.D
 Acq: 29 Jul 2020 18:53

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-03

Tot Ion	Ratio	Lower	Upper
154	100		
153	41.1	31.4	47.2
76	12.4	10.8	16.2




Abundance Ion 154.00 (153.70 to 154.70): E
 Ion 153.00 (152.70 to 153.70): E
 Ion 76.00 (75.70 to 76.70): BM


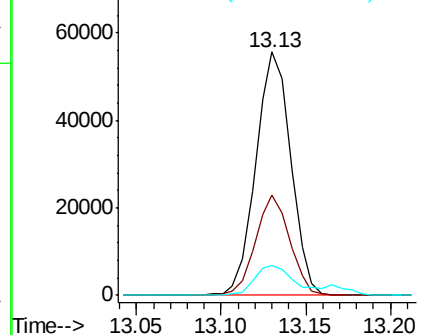



#42
 2-Chloronaphthalene
 Concen: 7.859 ng/ul
 RT: 13.17 min Scan# 1773
 Delta R.T. -0.01 min
 Lab File: BM026932.D
 Acq: 29 Jul 2020 18:53

Tgt Ion	Ratio	Lower	Upper
162	100		
164	32.2	26.4	39.6
127	38.3	30.6	45.8



Abundance Ion 162.00 (161.70 to 162.70): E
 Ion 164.00 (163.70 to 164.70): E
 Ion 127.00 (126.70 to 127.70): E




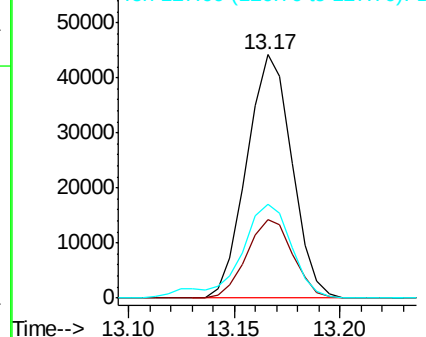




#43
2-Nitroaniline
Concen: 7.226 ng/ul
RT: 13.37 min Scan# 1807
Delta R.T. -0.00 min
Lab File: BM026932.D
Acq: 29 Jul 2020 18:53




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-03


Tot Ion: 65 Resp: 17971
Ion Ratio Lower Upper
65 100
92 61.6 51.0 76.6
138 84.6 67.3 100.9

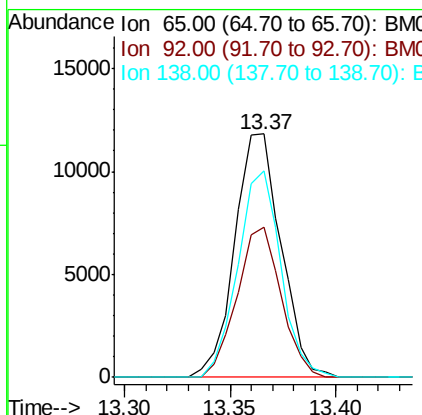

#45
Dimethylphthalate
Concen: 7.848 ng/ul
RT: 13.76 min Scan# 1874
Delta R.T. -0.01 min
Lab File: BM026932.D
Acq: 29 Jul 2020 18:53

Tgt Ion:163 Resp: 80323
Ion Ratio Lower Upper
163 100
194 4.1 3.0 4.6
164 10.6 8.6 12.8



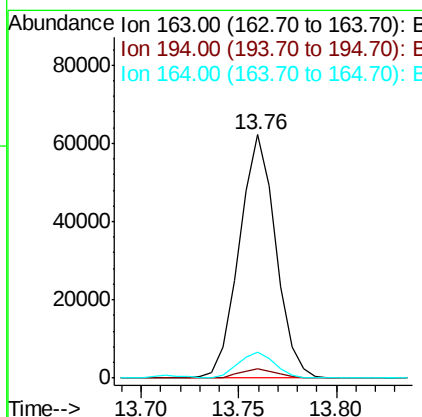





#46
2,6-Dinitrotoluene
Concen: 6.987 ng/ul
RT: 13.87 min Scan# 1892
Delta R.T. -0.01 min
Lab File: BM026932.D
Acq: 29 Jul 2020 18:53




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-03


Tot Ion:165 Resp: 12608
Ion Ratio Lower Upper
165 100
89 88.7 55.0 82.4#
121 27.2 19.0 28.6

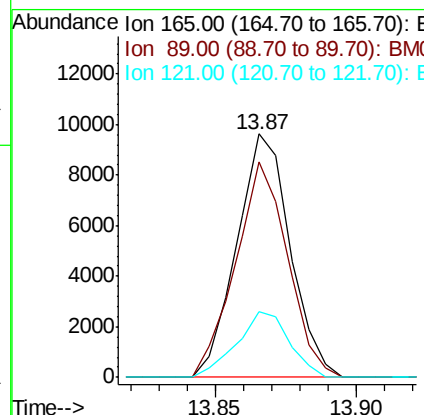

#48
Acenaphthylene
Concen: 7.703 ng/ul
RT: 14.02 min Scan# 1918
Delta R.T. -0.01 min
Lab File: BM026932.D
Acq: 29 Jul 2020 18:53

Tgt Ion:152 Resp: 97123
Ion Ratio Lower Upper
152 100
151 19.2 15.8 23.6
153 13.0 10.7 16.1

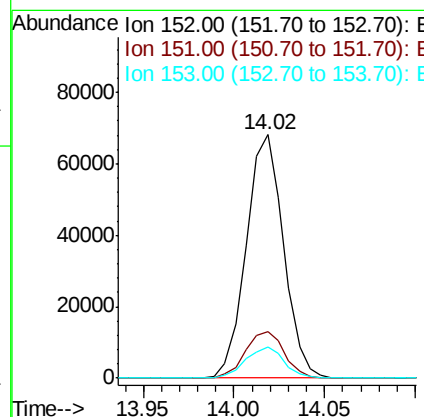







#49
3-Nitroaniline
Concen: 6.272 ng/ul
RT: 14.19 min Scan# 1948
Delta R.T. -0.00 min
Lab File: BM026932.D
Acq: 29 Jul 2020 18:53

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-03

Tot Ion:138 Resp: 11062
Ion Ratio Lower Upper
138 100
108 16.0 11.4 17.2
92 127.5 108.7 163.1




Abundance Ion 138.00 (137.70 to 138.70): E
Ion 108.00 (107.70 to 108.70): E
Ion 92.00 (91.70 to 92.70): B


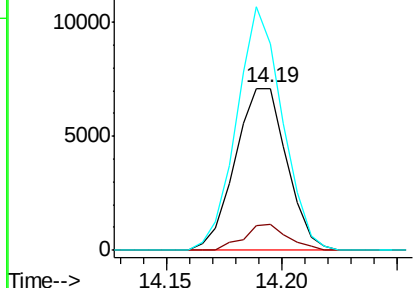



#50
Acenaphthene
Concen: 7.863 ng/ul
RT: 14.37 min Scan# 1977
Delta R.T. -0.00 min
Lab File: BM026932.D
Acq: 29 Jul 2020 18:53

Tgt Ion:153 Resp: 68303
Ion Ratio Lower Upper
153 100
152 46.0 37.8 56.6
154 88.4 70.5 105.7



Abundance Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E
Ion 154.00 (153.70 to 154.70): E




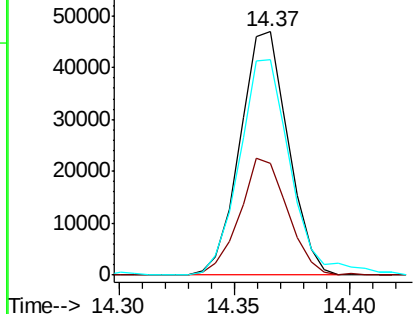




#51
 2,4-Dinitrophenol
 Concen: 5.515 ng/ul
 RT: 14.40 min Scan# 1983
 Delta R.T. -0.00 min
 Lab File: BM026932.D
 Acq: 29 Jul 2020 18:53




Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-03


Tot Ion:184 Resp: 3985
 Ion Ratio Lower Upper
 184 100
 63 97.8 57.8 86.8#
 154 68.0 55.0 82.4

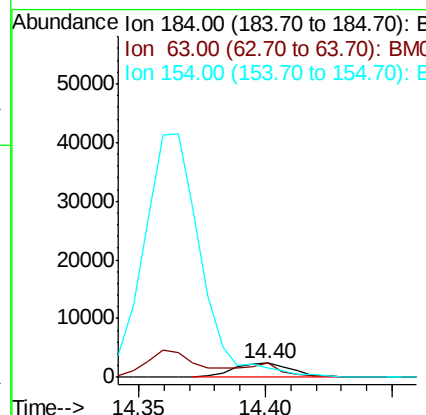

#53
 4-Nitrophenol
 Concen: 9.624 ng/ul
 RT: 14.50 min Scan# 2000
 Delta R.T. -0.01 min
 Lab File: BM026932.D
 Acq: 29 Jul 2020 18:53

Tgt Ion:109 Resp: 15903
 Ion Ratio Lower Upper
 109 100
 139 83.8 92.3 138.5#
 65 128.6 116.6 174.8

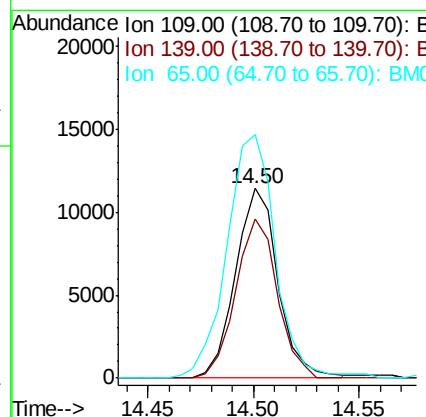



#54

Dibenzofuran

Concen: 8.078 ng/ul

RT: 14.70 min Scan# 2034

Delta R.T. -0.01 min

Lab File: BM026932.D

Acq: 29 Jul 2020 18:53

Instrument :

BNA_M

ClientSampleId :


MDL-WATER-03

Tot Ion:168 Resp: 97275

Ion Ratio Lower Upper

168 100

139 43.5 30.8 46.2



Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

14.70



60000

40000

20000

0

Time-->



#55

2,4-Dinitrotoluene

Concen: 7.691 ng/ul

RT: 14.65 min Scan# 2026

Delta R.T. -0.01 min

Lab File: BM026932.D

Acq: 29 Jul 2020 18:53


Tgt Ion:165 Resp: 19939

Ion Ratio Lower Upper

165 100

63 62.4 46.2 69.4

182 2.7 2.4 3.6



Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BM

Ion 182.00 (181.70 to 182.70): E

20000


15000


10000

5000

0

Time-->









#56
 2,3,4,6-Tetrachlorophenol
 Concen: 7.514 ng/ul
 RT: 14.93 min Scan# 2073
 Delta R.T. -0.00 min
 Lab File: BM026932.D
 Acq: 29 Jul 2020 18:53




Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-03


Tot Ion	Ratio	Lower	Upper
232	100		
131	44.9	39.4	59.2
130	2.9	2.6	4.0
166	31.0	26.7	40.1

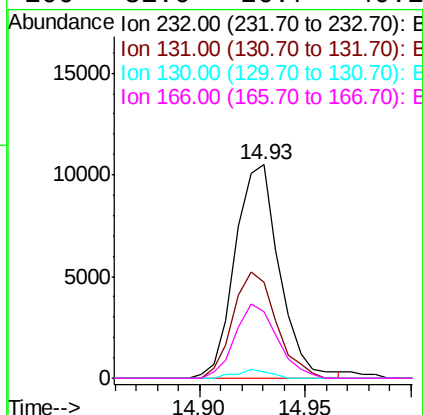

#57
 Diethylphthalate
 Concen: 7.801 ng/ul
 RT: 15.14 min Scan# 2108
 Delta R.T. -0.01 min
 Lab File: BM026932.D
 Acq: 29 Jul 2020 18:53

Tgt Ion	Ratio	Lower	Upper
149	100		
177	19.4	17.0	25.4
150	11.3	9.2	13.8

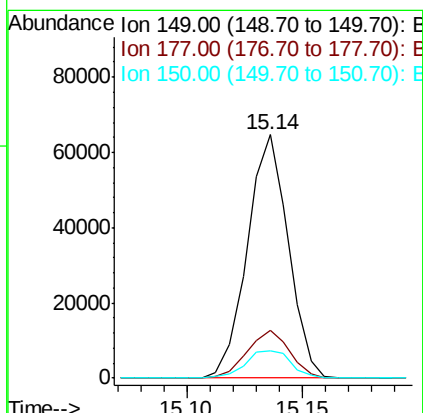



#59

Fluorene

Concen: 7.825 ng/ul

RT: 15.35 min Scan# 2144

Delta R.T. -0.01 min

Lab File: BM026932.D

Acq: 29 Jul 2020 18:53

Instrument :

BNA_M

ClientSampleId :

MDL-WATER-03


Tot Ion:166 Resp: 79341

Ion Ratio Lower Upper

166 100

165 104.4 78.2 117.2




167 14.5 10.3 15.5

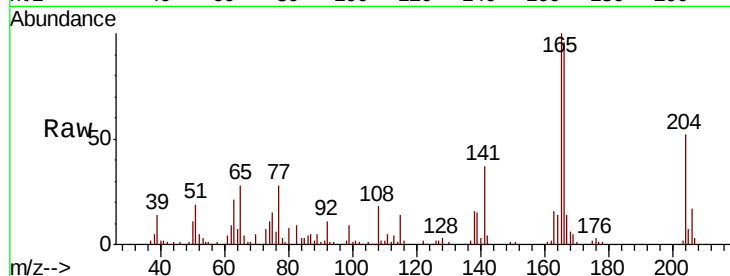

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

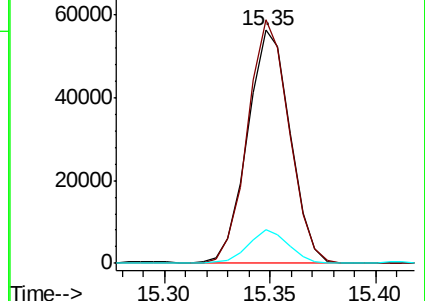

#60

4-Chlorophenyl-phenylether

Concen: 8.102 ng/ul

RT: 15.35 min Scan# 2144

Delta R.T. -0.01 min

Lab File: BM026932.D

Acq: 29 Jul 2020 18:53


Tgt Ion:204 Resp: 40888

Ion Ratio Lower Upper

204 100

206 33.1 26.0 39.0



141 71.1 48.3 72.5




Abundance Ion 204.00 (203.70 to 204.70): E

Ion 206.00 (205.70 to 206.70): E

Ion 141.00 (140.70 to 141.70): E



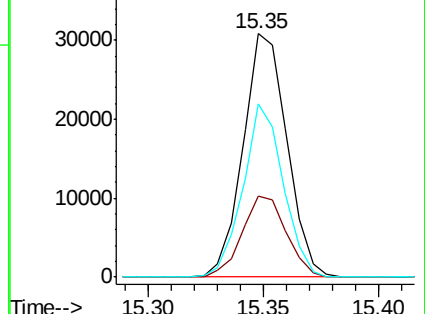





#61
4-Nitroaniline
Concen: 6.554 ng/ul
RT: 15.35 min Scan# 2145
Delta R.T. -0.01 min
Lab File: BM026932.D
Acq: 29 Jul 2020 18:53




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-03


Tot Ion:138 Resp: 14167
Ion Ratio Lower Upper
138 100
92 63.0 49.9 74.9
108 119.4 78.9 118.3#

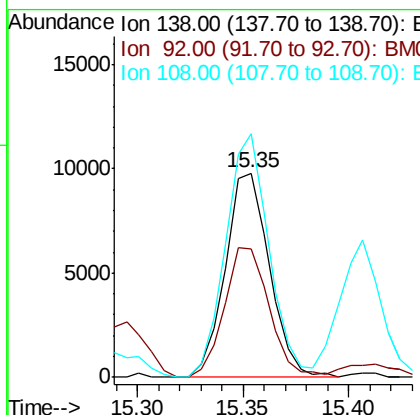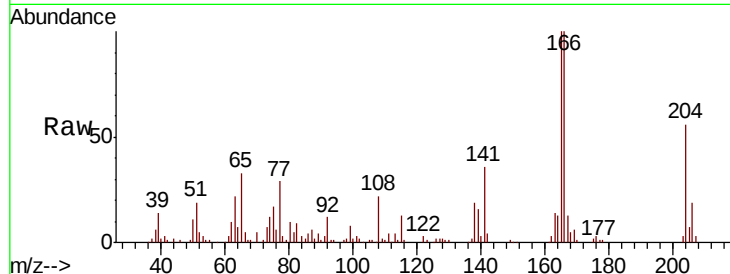

#64
4,6-Dinitro-2-methylphenol
Concen: 7.112 ng/ul
RT: 15.42 min Scan# 2156
Delta R.T. -0.01 min
Lab File: BM026932.D
Acq: 29 Jul 2020 18:53

Tgt Ion:198 Resp: 9660
Ion Ratio Lower Upper
198 100
182 7.9 4.2 6.4#
77 49.6 29.3 43.9#



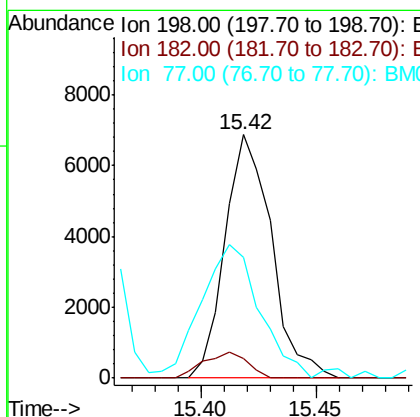
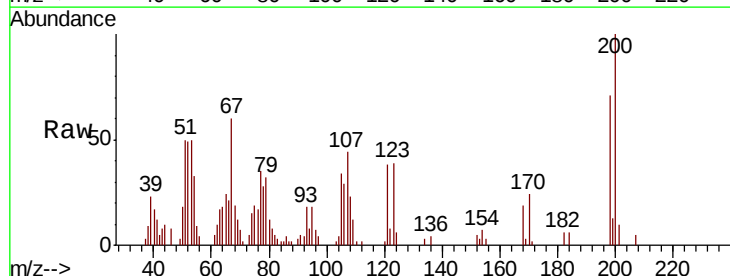




#65
N-Nitrosodiphenylamine
Concen: 7.475 ng/ul
RT: 15.56 min Scan# 2180
Delta R.T. -0.01 min
Lab File: BM026932.D
Acq: 29 Jul 2020 18:53




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-03


Tot Ion:169 Resp: 65573
Ion Ratio Lower Upper
169 100
168 70.0 54.6 82.0
167 36.3 29.1 43.7

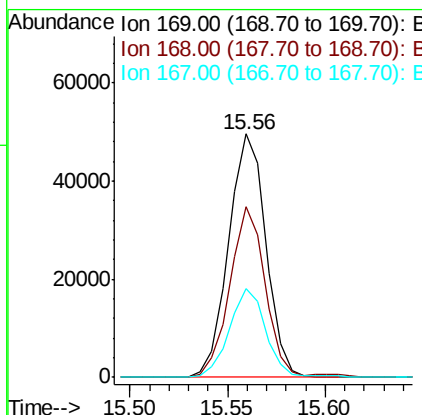

#66
4-Bromophenyl-phenylether
Concen: 7.805 ng/ul
RT: 16.24 min Scan# 2296
Delta R.T. -0.01 min
Lab File: BM026932.D
Acq: 29 Jul 2020 18:53

Tgt Ion:248 Resp: 24554
Ion Ratio Lower Upper
248 100
250 99.1 78.2 117.4
141 81.0 57.5 86.3

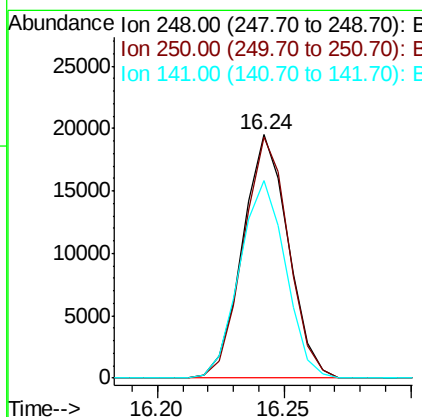



#67

Hexachlorobenzene

Concen: 8.344 ng/ul

RT: 16.36 min Scan# 2316

Delta R.T. -0.00 min

Lab File: BM026932.D

Acq: 29 Jul 2020 18:53

Instrument :

BNA_M

ClientSampleId :

MDL-WATER-03


Tot Ion:284 Resp: 29766

Ion Ratio Lower Upper

284 100

142 42.6 31.7 47.5




249 28.3 25.7 38.5

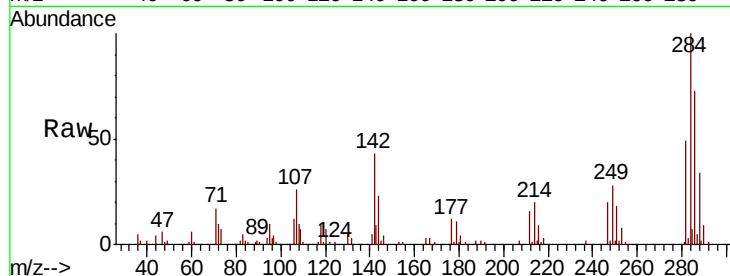

Abundance Ion 284.00 (283.70 to 284.70): E

Ion 142.00 (141.70 to 142.70): E

Ion 249.00 (248.70 to 249.70): E

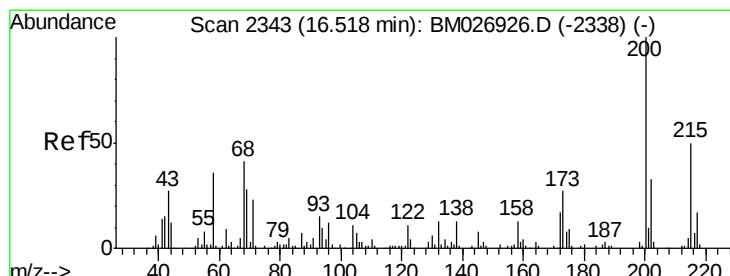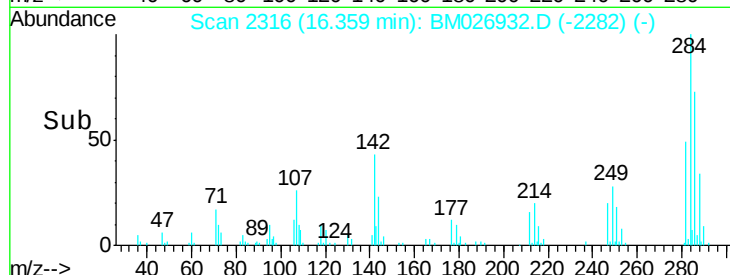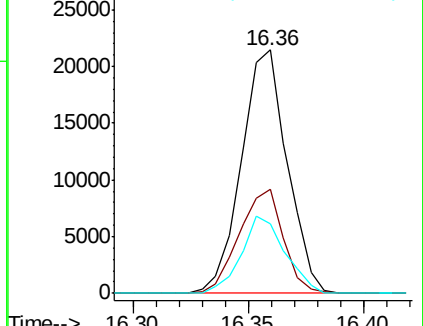

#68

Atrazine

Concen: 6.958 ng/ul

RT: 16.51 min Scan# 2342

Delta R.T. -0.01 min

Lab File: BM026932.D

Acq: 29 Jul 2020 18:53


Tgt Ion:200 Resp: 22406

Ion Ratio Lower Upper

200 100

173 25.8 22.4 33.6



215 47.4 38.6 58.0




Abundance Ion 200.00 (199.70 to 200.70): E

Ion 173.00 (172.70 to 173.70): E

Ion 215.00 (214.70 to 215.70): E

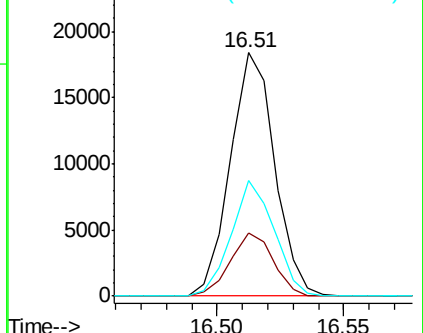







#69
 Pentachlorophenol
 Concen: 6.781 ng/ul
 RT: 16.69 min Scan# 2373
 Delta R.T. -0.01 min
 Lab File: BM026932.D
 Acq: 29 Jul 2020 18:53

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-03

Tot Ion:266 Resp: 12038
 Ion Ratio Lower Upper
 266 100
 264 53.8 49.3 73.9
 268 58.5 50.5 75.7




Abundance Ion 265.70 (265.40 to 266.40): E
 Ion 264.00 (263.70 to 264.70): E
 Ion 268.00 (267.70 to 268.70): E


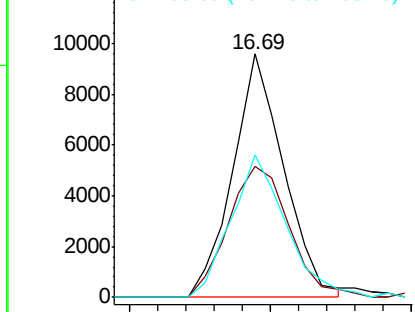



#70
 Phenanthrene
 Concen: 7.878 ng/ul
 RT: 17.08 min Scan# 2439
 Delta R.T. -0.01 min
 Lab File: BM026932.D
 Acq: 29 Jul 2020 18:53

Tgt Ion:178 Resp: 128233
 Ion Ratio Lower Upper
 178 100
 179 15.2 12.0 18.0
 176 18.4 14.7 22.1



Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 179.00 (178.70 to 179.70): E
 Ion 176.00 (175.70 to 176.70): E

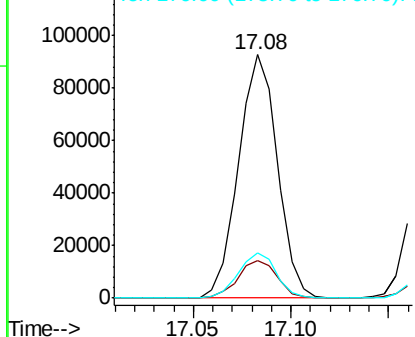



#72

Anthracene

Concen: 7.767 ng/uL

RT: 17.17 min Scan# 2454

Delta R.T. -0.01 min

Lab File: BM026932.D

Acq: 29 Jul 2020 18:53

Instrument :

BNA_M

ClientSampleId :

MDL-WATER-03


Tot Ion:178 Resp: 129955

Ion Ratio Lower Upper

178 100

179 14.3 11.8 17.6




176 17.6 15.0 22.6



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

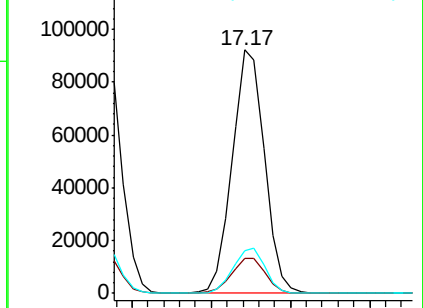

#73

1,2,3,4-Tetrachlorobenzene

Concen: 7.564 ng/uL

RT: 13.09 min Scan# 1761

Delta R.T. -0.01 min

Lab File: BM026932.D

Acq: 29 Jul 2020 18:53


Tgt Ion:216 Resp: 31866

Ion Ratio Lower Upper

216 100

214 81.0 62.6 94.0



218 51.9 38.1 57.1




Abundance Ion 216.00 (215.70 to 216.70): E

Ion 214.00 (213.70 to 214.70): E

Ion 218.00 (217.70 to 218.70): E

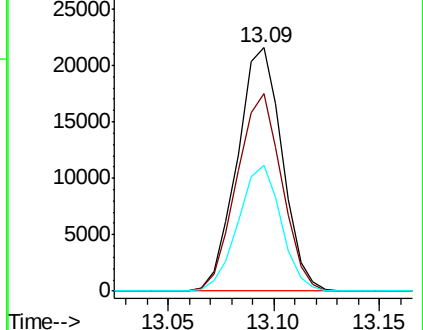



#74

Pentachlorobenzene

Concen: 8.329 ng/uL

RT: 14.62 min Scan# 2021

Delta R.T. -0.01 min

Lab File: BM026932.D

Acq: 29 Jul 2020 18:53

Instrument :

BNA_M

ClientSampleId :

MDL-WATER-03


Tot Ion:250 Resp: 34020

Ion Ratio Lower Upper

250 100

248 64.1 49.6 74.4




252 63.1 51.7 77.5



Abundance Ion 250.00 (249.70 to 250.70): E

Ion 248.00 (247.70 to 248.70): E

Ion 252.00 (251.70 to 252.70): E

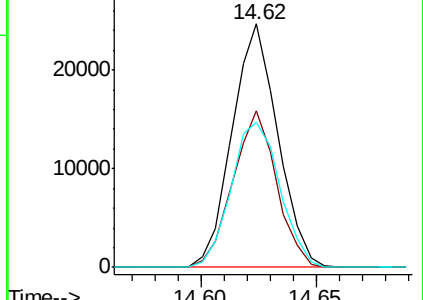

#75

Carbazole

Concen: 7.372 ng/uL

RT: 17.44 min Scan# 2499

Delta R.T. -0.01 min

Lab File: BM026932.D

Acq: 29 Jul 2020 18:53


Tgt Ion:167 Resp: 109033

Ion Ratio Lower Upper

167 100

166 21.0 17.1 25.7



139 14.3 10.1 15.1




Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E




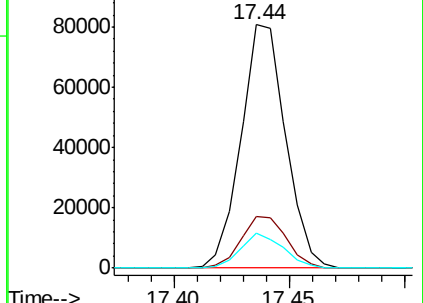


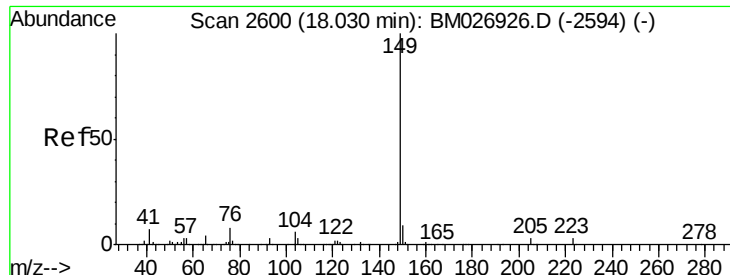

#76
Di-n-butylphthalate
Concen: 6.853 ng/ul
RT: 18.03 min Scan# 2600
Delta R.T. -0.01 min
Lab File: BM026932.D
Acq: 29 Jul 2020 18:53




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-03


Tot Ion:149 Resp: 119227
Ion Ratio Lower Upper
149 100
150 9.3 7.6 11.4
104 7.1 4.7 7.1

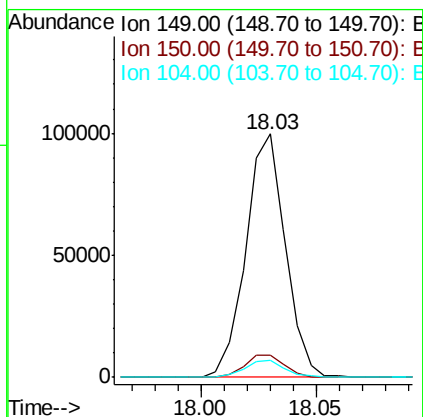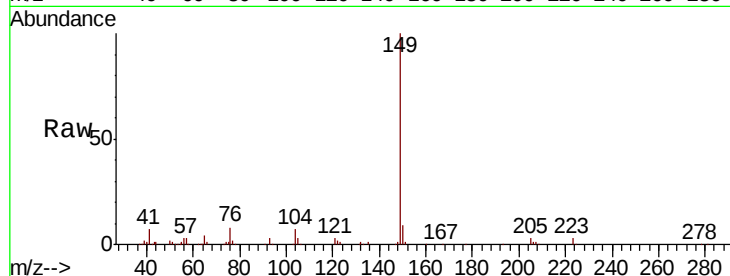

#77
Fluoranthene
Concen: 7.778 ng/ul
RT: 19.10 min Scan# 2782
Delta R.T. -0.01 min
Lab File: BM026932.D
Acq: 29 Jul 2020 18:53

Tgt Ion:202 Resp: 149498
Ion Ratio Lower Upper
202 100
101 8.2 7.7 11.5
100 7.2 6.2 9.4



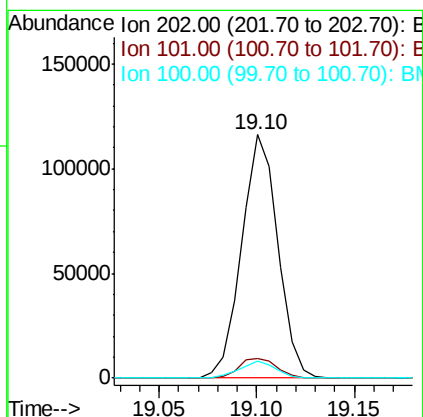





#80
Pvrene
Concen: 7.553 ng/ul
RT: 19.47 min Scan# 2844
Delta R.T. -0.01 min
Lab File: BM026932.D
Acq: 29 Jul 2020 18:53




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-03


Tot Ion	Ratio	Lower	Upper
202	100		
101	8.8	9.4	14.2#
100	9.3	8.2	12.4

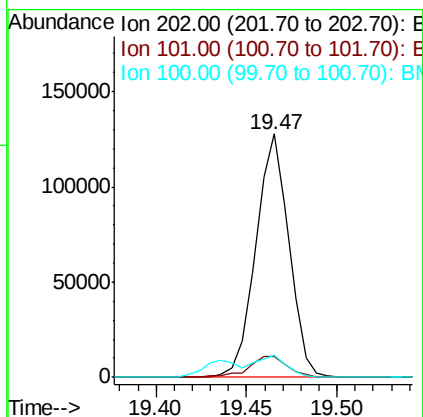

#81
Butylbenzylphthalate
Concen: 6.054 ng/ul
RT: 20.38 min Scan# 3000
Delta R.T. -0.01 min
Lab File: BM026932.D
Acq: 29 Jul 2020 18:53

Tgt Ion	Ratio	Lower	Upper
149	100		
91	83.3	64.2	96.2
206	19.8	15.8	23.6

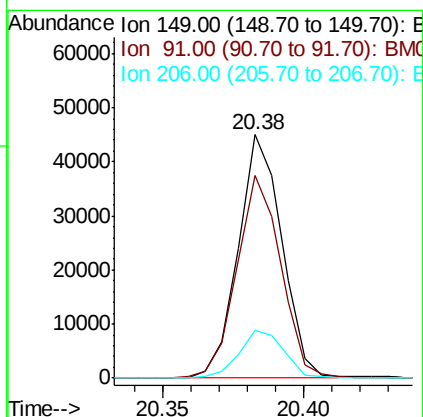







#82
 3,3'-Dichlorobenzidine
 Concen: 4.879 ng/ul
 RT: 21.15 min Scan# 3131
 Delta R.T. -0.01 min
 Lab File: BM026932.D
 Acq: 29 Jul 2020 18:53

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-03

Tot Ion:252 Resp: 34076
 Ion Ratio Lower Upper
 252 100
 254 71.6 51.4 77.2
 126 9.4 8.7 13.1




Abundance Ion 252.00 (251.70 to 252.70): E
 Ion 254.00 (253.70 to 254.70): E
 Ion 126.00 (125.70 to 126.70): E


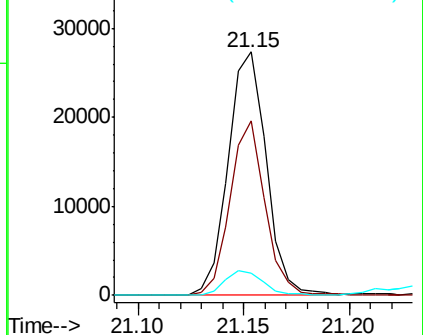



#83
 Benzo(a)anthracene
 Concen: 7.678 ng/ul
 RT: 21.22 min Scan# 3142
 Delta R.T. -0.01 min
 Lab File: BM026932.D
 Acq: 29 Jul 2020 18:53

Tgt Ion:228 Resp: 156331
 Ion Ratio Lower Upper
 228 100
 229 18.9 15.4 23.2
 226 26.1 20.9 31.3



Abundance Ion 228.00 (227.70 to 228.70): E
 Ion 229.00 (228.70 to 229.70): E
 Ion 226.00 (225.70 to 226.70): E

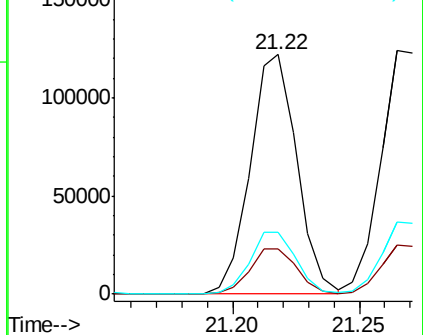



#84

Bis(2-ethylhexyl)phthalate

Concen: 6.145 ng/ul

RT: 21.18 min Scan# 3135

Delta R.T. -0.01 min

Lab File: BM026932.D

Acq: 29 Jul 2020 18:53

Instrument :

BNA_M

ClientSampleId :

MDL-WATER-03


Tot Ion:149 Resp: 73624

Ion Ratio Lower Upper

149 100

167 27.5 20.6 31.0




279 4.5 3.0 4.6



Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

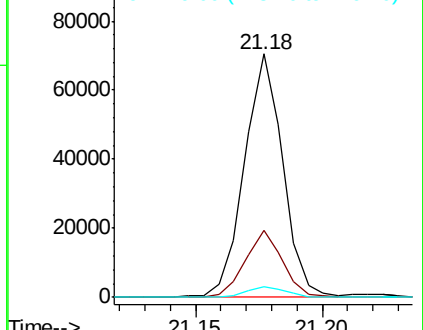

#85

Chrysene

Concen: 7.795 ng/ul

RT: 21.27 min Scan# 3150

Delta R.T. -0.01 min

Lab File: BM026932.D

Acq: 29 Jul 2020 18:53


Tgt Ion:228 Resp: 154769

Ion Ratio Lower Upper

228 100

226 29.5 23.2 34.8



229 20.0 15.5 23.3




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E




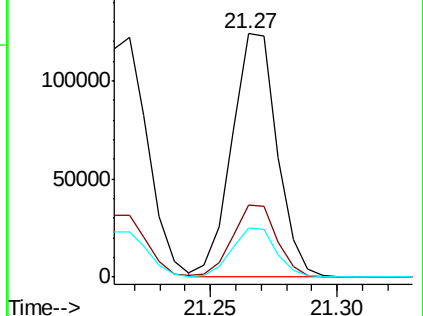




#87
 Di-n-octyl phthalate
 Concen: 5.312 ng/ul
 RT: 22.05 min Scan# 3283
 Delta R.T. -0.02 min
 Lab File: BM026932.D
 Acq: 29 Jul 2020 18:53

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-03




Tgt Ion:149 Resp: 121639

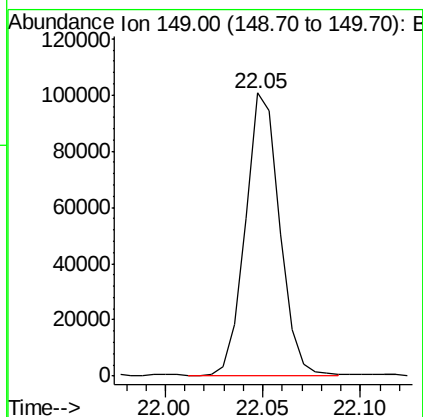


#88
 Benzo(b)fluoranthene
 Concen: 7.064 ng/ul
 RT: 22.78 min Scan# 3408
 Delta R.T. -0.01 min
 Lab File: BM026932.D
 Acq: 29 Jul 2020 18:53

Tgt Ion:252 Resp: 157478

Ion	Ratio	Lower	Upper
252	100		
253	21.4	17.6	26.4
125	8.2	6.6	10.0

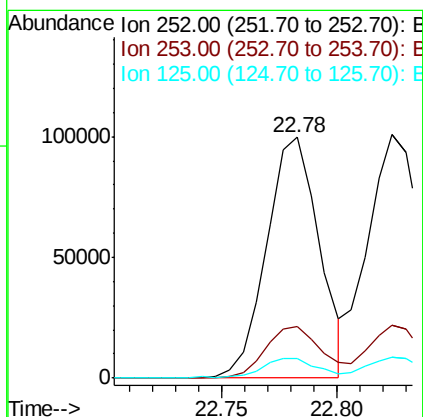



#89

Benzo(k)fluoranthene

Concen: 7.677 ng/ul

RT: 22.82 min Scan# 3415

Delta R.T. -0.02 min

Lab File: BM026932.D

Acq: 29 Jul 2020 18:53

Instrument :

BNA_M

ClientSampleId :

MDL-WATER-03


Tot Ion:252 Resp: 164217

Ion Ratio Lower Upper

252 100

253 21.9 17.4 26.2

125 8.5 7.3 10.9






Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

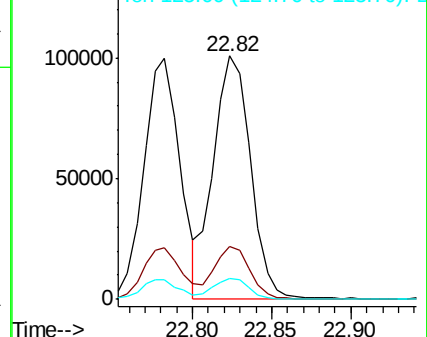

#91

Benzo(a)pyrene

Concen: 7.753 ng/ul

RT: 23.35 min Scan# 3504

Delta R.T. -0.01 min

Lab File: BM026932.D

Acq: 29 Jul 2020 18:53


Tgt Ion:252 Resp: 155966

Ion Ratio Lower Upper

252 100

253 21.1 17.7 26.5

125 8.6 8.2 12.2






Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E




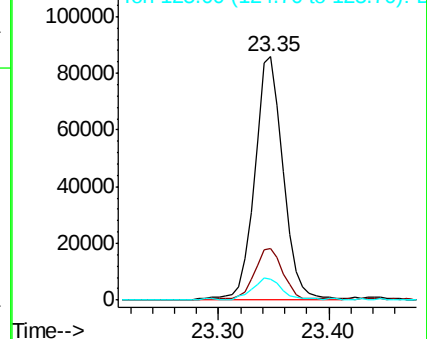




#92
 Indeno(1,2,3-cd)pyrene
 Concen: 7.850 ng/ul
 RT: 25.65 min Scan# 3895
 Delta R.T. -0.03 min
 Lab File: BM026932.D
 Acq: 29 Jul 2020 18:53




Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-03


Tot Ion:276 Resp: 195908
 Ion Ratio Lower Upper
 276 100
 138 18.7 17.0 25.4
 277 24.7 20.6 30.8

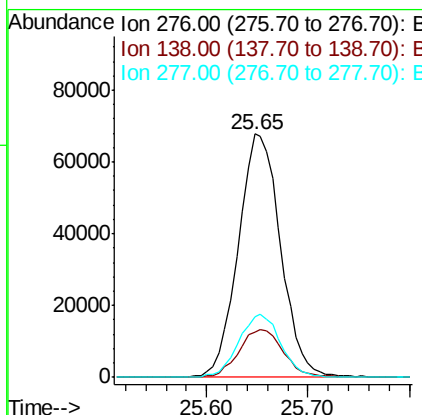

#93
 Dibenzo(a,h)anthracene
 Concen: 7.933 ng/ul
 RT: 25.66 min Scan# 3898
 Delta R.T. -0.02 min
 Lab File: BM026932.D
 Acq: 29 Jul 2020 18:53

Tgt Ion:278 Resp: 167444
 Ion Ratio Lower Upper
 278 100
 139 12.8 10.9 16.3
 279 23.6 19.4 29.2

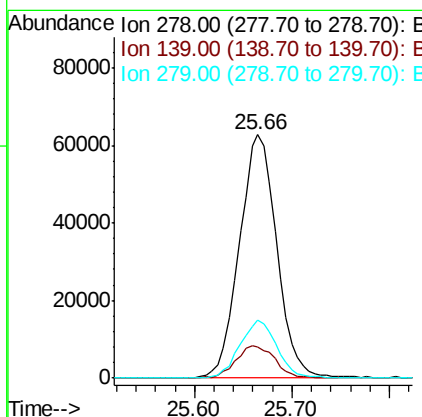



#94

Benzo(a,h,i)perylene

Concen: 7.943 ng/ul

RT: 26.32 min Scan# 4009

Delta R.T. -0.03 min

Lab File: BM026932.D

Acq: 29 Jul 2020 18:53

Instrument :

BNA_M

ClientSampleId :

MDL-WATER-03


Tot Ion:276 Resp: 163911

Ion Ratio Lower Upper

276 100

138 18.1 14.9 22.3

277 23.8 19.1 28.7



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

