

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072820\
 Data File : BM026891.D
 Acq On : 28 Jul 2020 15:16
 Operator : JU/CG
 Sample : L3388-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AD6

Quant Time: Jul 28 16:04:16 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 28 10:40:31 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	67198	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	248432	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.31	164	152729	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.05	188	312851	20.00	ng/ul	0.00
78) Chrysene-d12	21.24	240	319240	20.00	ng/ul	0.00
86) Perylene-d12	23.46	264	325450	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	10753	7.30	ng/uL	0.00
5) Phenol-d5	6.84	99	80012	13.59	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.01	67	60317	15.14	ng/ul	0.00
9) 2-Chlorophenol-d4	7.21	132	57955	13.15	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	63636	14.05	ng/ul	0.00
19) Nitrobenzene-d5	8.81	128	29402	15.22	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	24812	14.01	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	57307	13.55	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	82863	16.43	ng/ul	0.00
44) Dimethylphthalate-d6	13.72	166	205404	17.15	ng/ul	0.00
47) Acenaphthylene-d8	14.00	160	231304	15.18	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	22363	11.04	ng/ul	0.00
58) Fluorene-d10	15.30	176	162776	15.62	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.41	200	14180	10.17	ng/ul	0.00
71) Anthracene-d10	17.15	188	236014	15.09	ng/ul	0.00
79) Pyrene-d10	19.44	212	247916	14.56	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.32	264	239703	13.05	ng/ul	0.00


Target Compounds				Ovalue
45) Dimethylphthalate	13.77	163	25219	2.006 ng/ul#


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072820\
Data File : BM026891.D
Acq On : 28 Jul 2020 15:16
Operator : JU/CG
Sample : L3388-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD6

Quant Time: Jul 28 16:04:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 28 10:40:31 2020
Response via : Initial Calibration

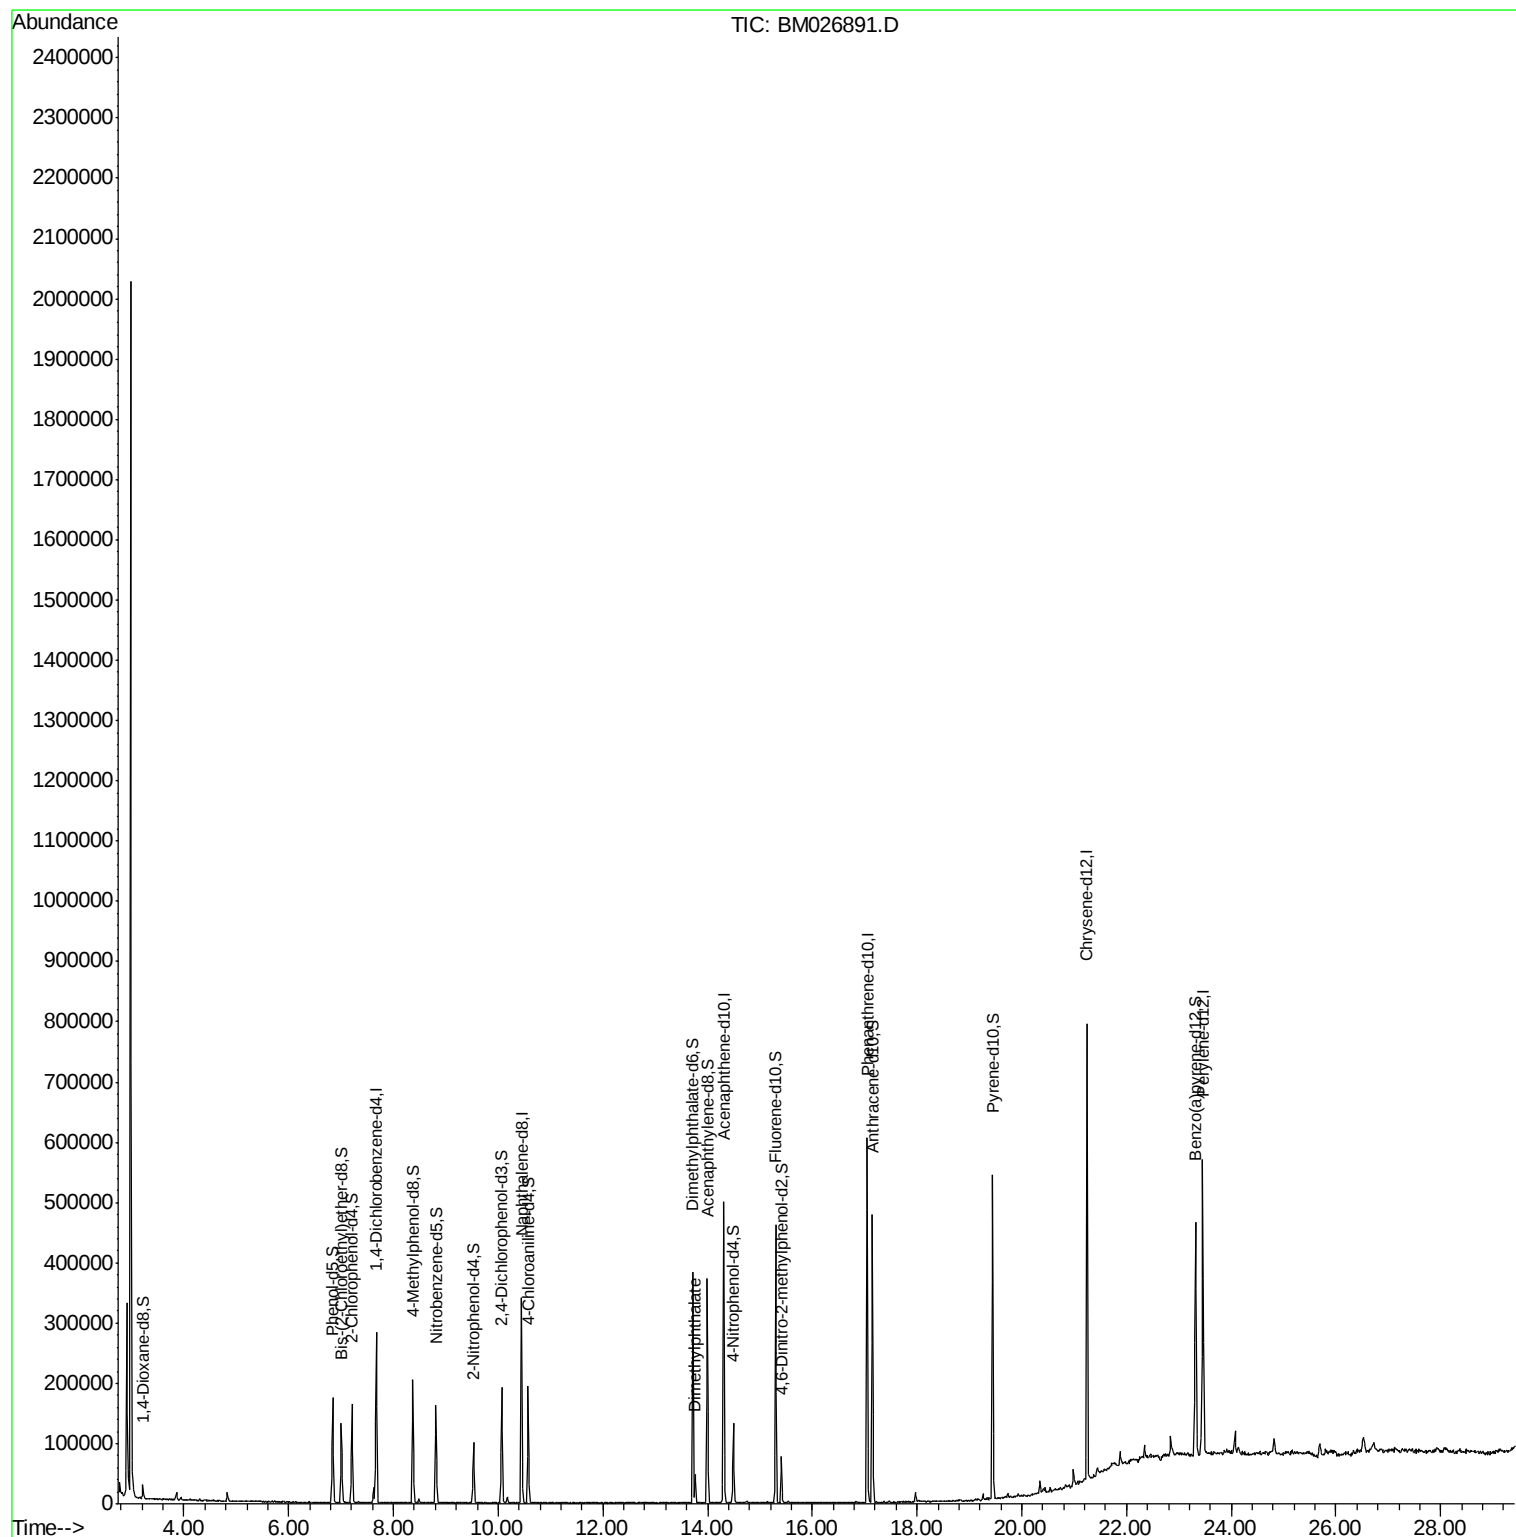

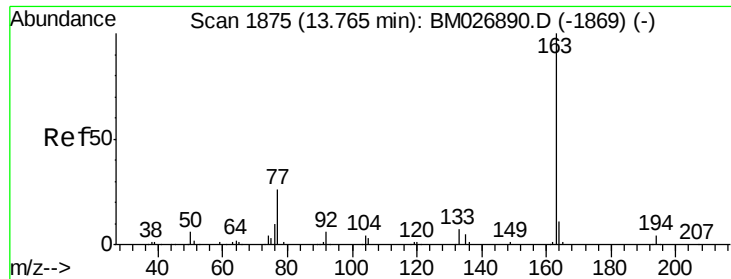

#45

Dimethylphthalate

Concen: 2.006 ng/ul

RT: 13.77 min Scan# 1875

Delta R.T. -0.01 min

Lab File: BM026891.D

Acq: 28 Jul 2020 15:16

Instrument :

BNA_M

ClientSampleId :

C0AD6


Tot Ion:163 Resp: 25219

Ion Ratio Lower Upper

163 100

194 2.9 3.0 4.6#

164 11.9 8.6 12.8

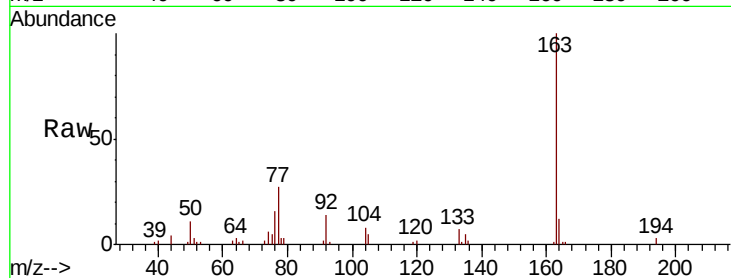

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

