

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072820\
 Data File : BM026893.D
 Acq On : 28 Jul 2020 16:30
 Operator : JU/CG
 Sample : L3388-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AD9

Quant Time: Jul 28 17:01:26 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 28 10:40:31 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	81204	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	306296	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.31	164	185502	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.05	188	387969	20.00	ng/ul	0.00
78) Chrysene-d12	21.25	240	392807	20.00	ng/ul	0.00
86) Perylene-d12	23.46	264	408708	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.23	96	8718	4.90	ng/uL	0.00
5) Phenol-d5	6.84	99	94369	13.27	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.01	67	68539	14.23	ng/ul	0.00
9) 2-Chlorophenol-d4	7.21	132	68202	12.81	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	78156	14.28	ng/ul	0.00
19) Nitrobenzene-d5	8.81	128	34860	14.63	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	31056	14.22	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	71053	13.63	ng/ul	0.00
29) 4-Chloroaniline-d4	10.58	131	94733	15.24	ng/ul	0.00
44) Dimethylphthalate-d6	13.72	166	240294	16.52	ng/ul	0.00
47) Acenaphthylene-d8	13.99	160	289531	15.64	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	30200	12.28	ng/ul	0.00
58) Fluorene-d10	15.30	176	201406	15.92	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.41	200	19933	11.53	ng/ul	0.00
71) Anthracene-d10	17.15	188	296301	15.28	ng/ul	0.00
79) Pyrene-d10	19.44	212	316553	15.11	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.32	264	313311	13.58	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.77	163	26403	1.730	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072820\
Data File : BM026893.D
Acq On : 28 Jul 2020 16:30
Operator : JU/CG
Sample : L3388-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD9

Quant Time: Jul 28 17:01:26 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 28 10:40:31 2020
Response via : Initial Calibration

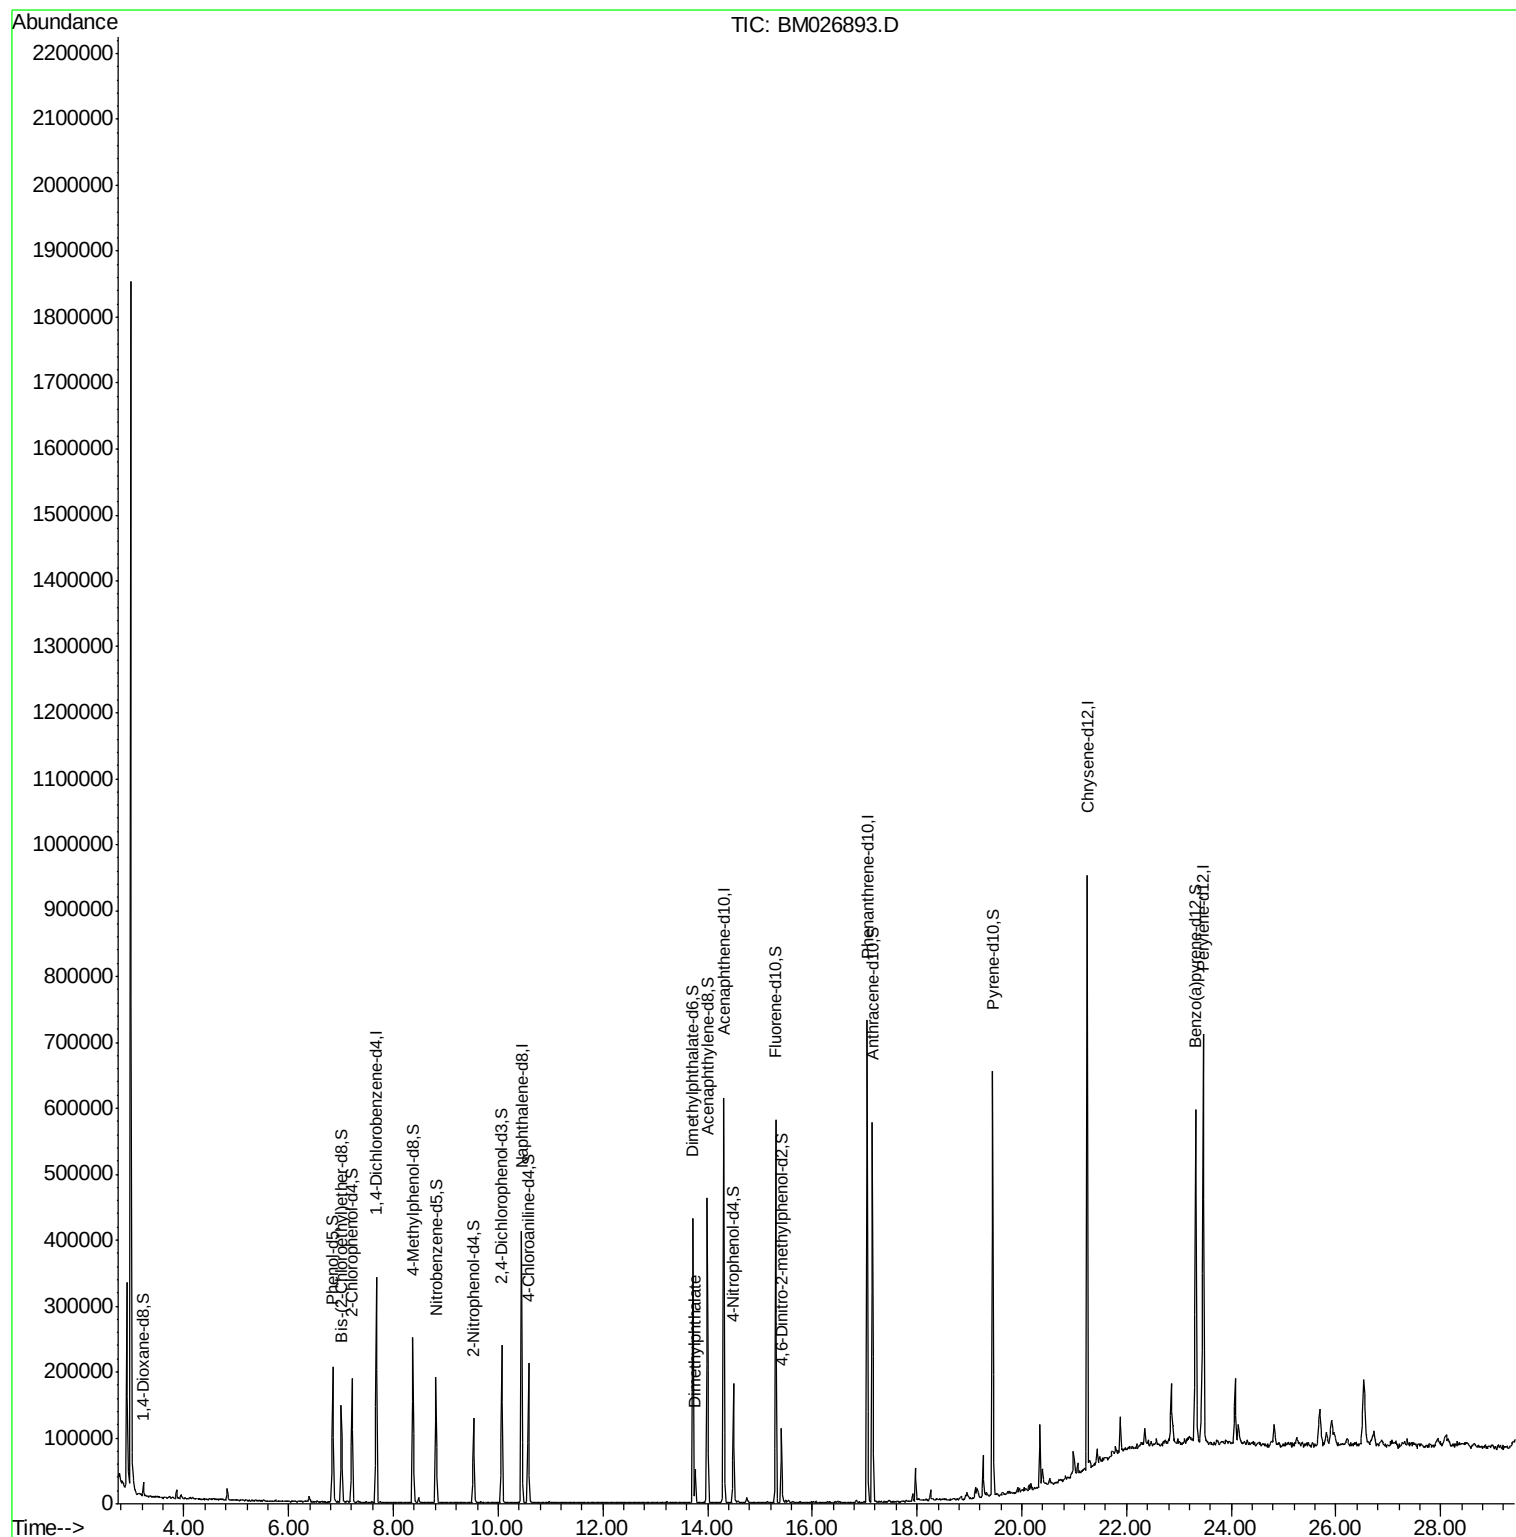

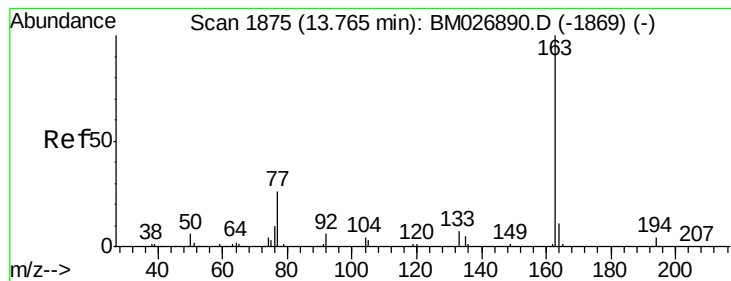

#45

Dimethylphthalate

Concen: 1.730 ng/ul

RT: 13.77 min Scan# 1875

Delta R.T. -0.01 min

Lab File: BM026893.D

Acq: 28 Jul 2020 16:30

Instrument :

BNA_M

ClientSampleId :

C0AD9


Tot Ion:163 Resp: 26403

Ion Ratio Lower Upper

163 100

194 4.4 3.0 4.6

164 10.5 8.6 12.8

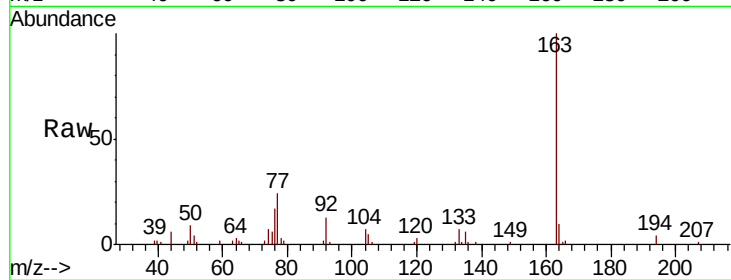

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

