

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072820\
 Data File : BM026913.D
 Acq On : 29 Jul 2020 05:22
 Operator : JU/CG
 Sample : L3443-02
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AA7

Quant Time: Jul 29 06:34:32 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 29 02:24:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	68028	20.00	ng/ul	0.00
18) Naphthalene-d8	10.44	136	247684	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.30	164	153383	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	316619	20.00	ng/ul	0.00
78) Chrysene-d12	21.23	240	343274	20.00	ng/ul	-0.01
86) Perylene-d12	23.44	264	361456	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	10207	6.85	ng/uL	0.00
5) Phenol-d5	6.84	99	44641	7.49	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.01	67	115511	28.63	ng/ul	0.00
9) 2-Chlorophenol-d4	7.21	132	105642	23.68	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	66630	14.53	ng/ul	0.00
19) Nitrobenzene-d5	8.81	128	59739	31.01	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	58323	33.02	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	122981	29.17	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	13410	2.67	ng/ul	0.00
44) Dimethylphthalate-d6	13.72	166	421436	35.04	ng/ul	0.00
47) Acenaphthylene-d8	13.99	160	481509	31.46	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	14661	7.21	ng/ul	-0.01
58) Fluorene-d10	15.29	176	360255	34.43	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.41	200	48774	34.56	ng/ul	0.00
71) Anthracene-d10	17.14	188	486269	30.73	ng/ul	0.00
79) Pyrene-d10	19.44	212	626768	34.23	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.30	264	583368	28.60	ng/ul	-0.02


Target Compounds					Ovalue	
45) Dimethylphthalate	13.76	163	48038	3.806	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072820\
Data File : BM026913.D
Acq On : 29 Jul 2020 05:22
Operator : JU/CG
Sample : L3443-02
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA7

Quant Time: Jul 29 06:34:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 29 02:24:07 2020
Response via : Initial Calibration

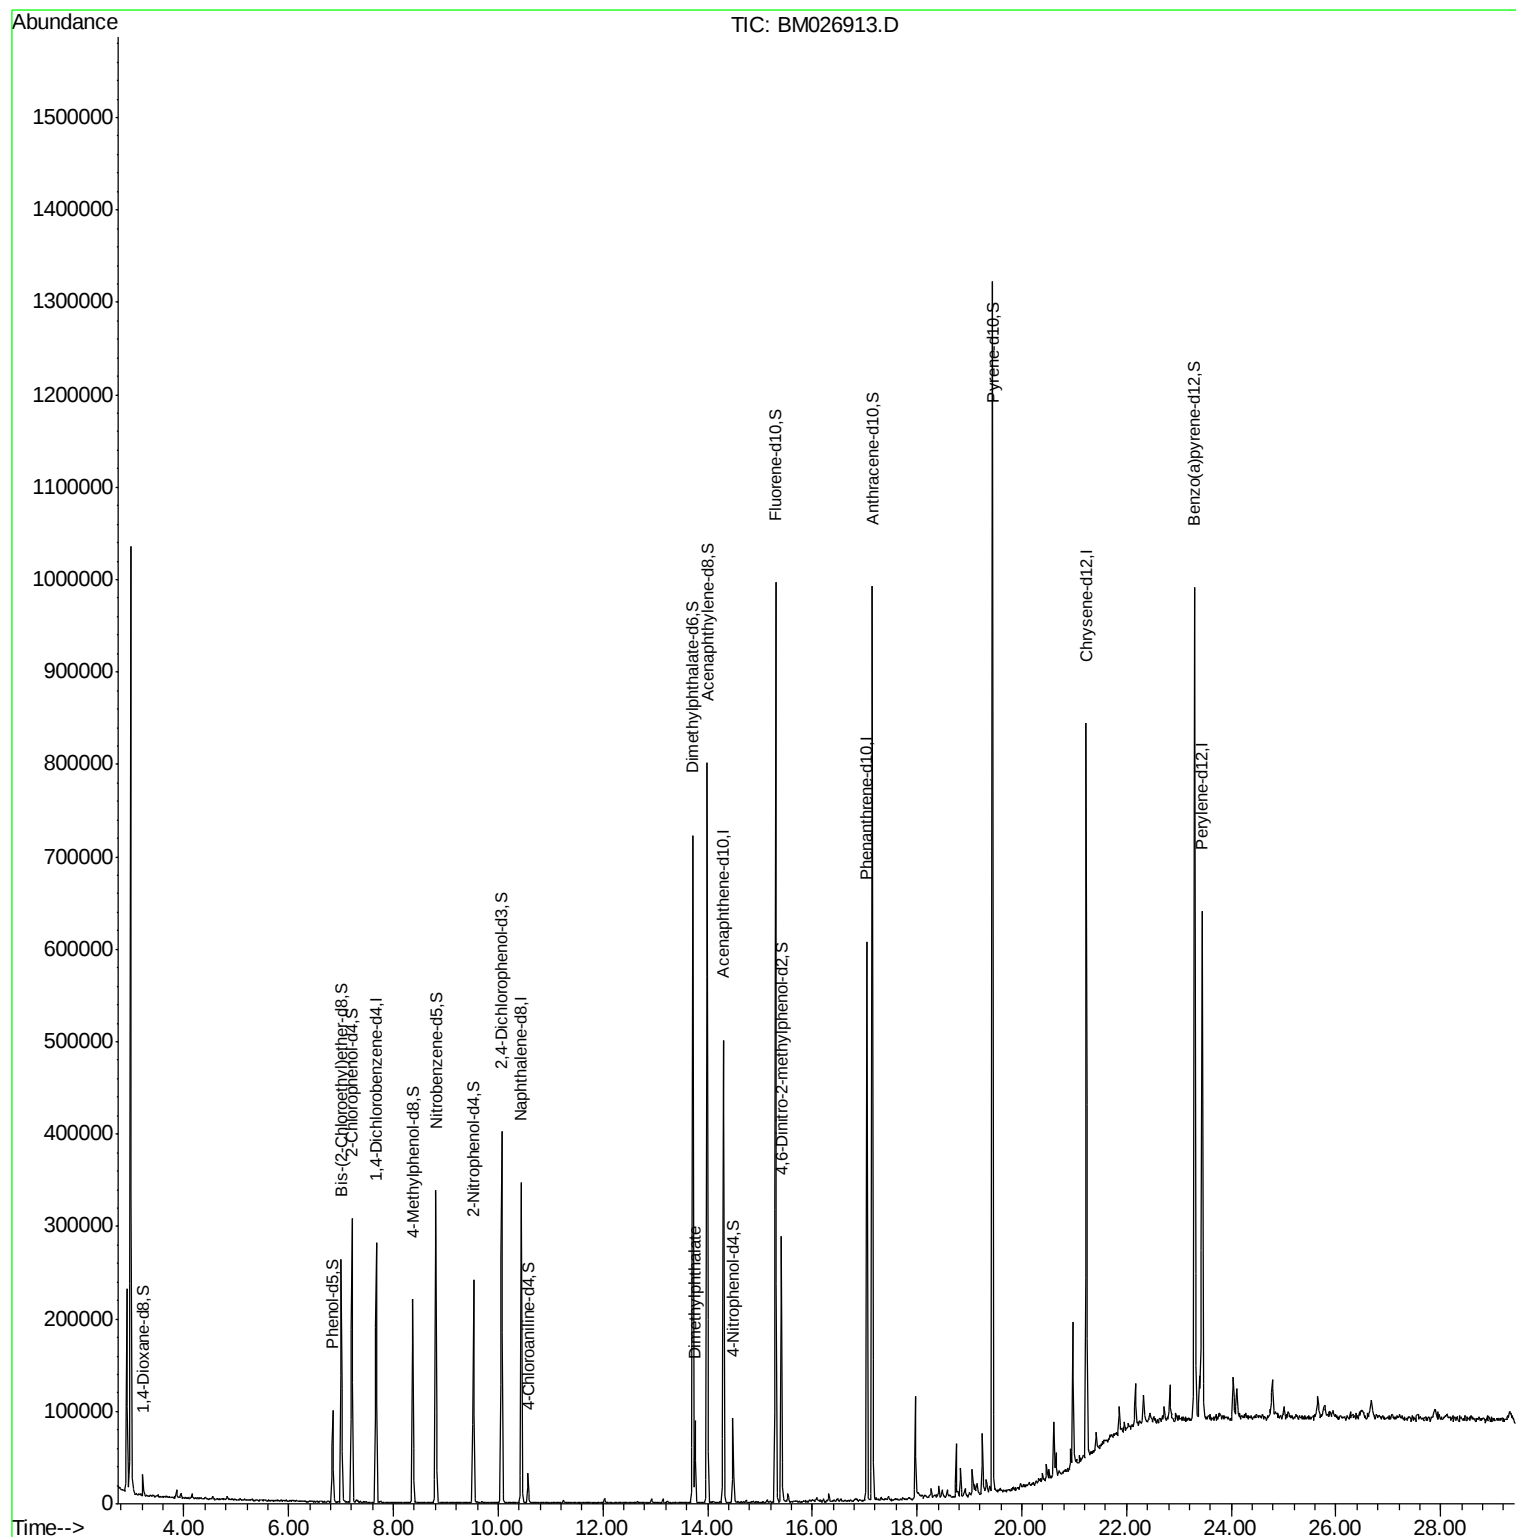


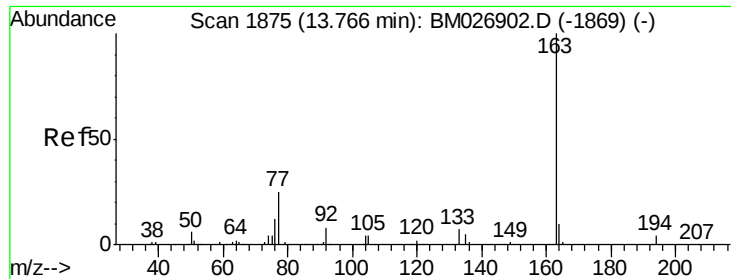

#45
 Dimethylphthalate
 Concen: 3.806 ng/ul
 RT: 13.76 min Scan# 1874
 Delta R.T. -0.01 min
 Lab File: BM026913.D
 Acq: 29 Jul 2020 05:22

Instrument :
 BNA_M
 ClientSampleId :
 C0AA7

Tot Ion	Ratio	Lower	Upper
163	100		
194	3.5	3.0	4.6
164	10.1	8.6	12.8

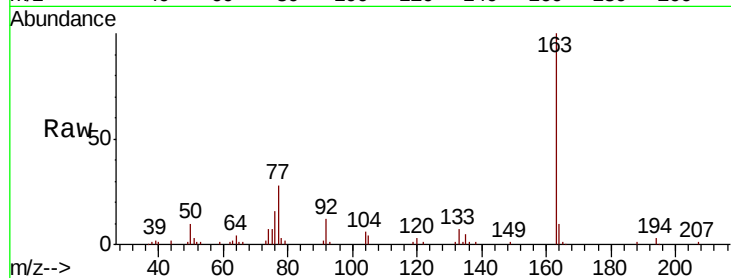

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

