

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072820\
 Data File : BM026930.D
 Acq On : 29 Jul 2020 17:39
 Operator : JU/CG
 Sample : L1955-09
 Misc : PBBL-WATER-02
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleID :
 MDL-WATER-02

Manual Integrations
 APPROVED

mohammad
 7/30/2020 3:32:41 PM

Quant Time: Jul 29 18:18:07 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 29 02:24:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	61314	20.00	ng/ul	0.00
18) Naphthalene-d8	10.44	136	229514	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.30	164	145640	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	311740	20.00	ng/ul	0.00
78) Chrysene-d12	21.24	240	341845	20.00	ng/ul	0.00
86) Perylene-d12	23.45	264	358195	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	9452	7.03	ng/uL	0.00
5) Phenol-d5	6.84	99	148944	27.73	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.01	67	104751	28.81	ng/ul	0.00
9) 2-Chlorophenol-d4	7.21	132	116682	29.02	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	114435	27.69	ng/ul	0.00
19) Nitrobenzene-d5	8.81	128	52967	29.67	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	50893	31.10	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	113664	29.09	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	136535	29.31	ng/ul	0.00
44) Dimethylphthalate-d6	13.71	166	334598	29.30	ng/ul	0.00
47) Acenaphthylene-d8	13.99	160	428260	29.47	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	54753	28.35	ng/ul	0.00
58) Fluorene-d10	15.29	176	294653	29.66	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.41	200	35348	25.44	ng/ul	0.00
71) Anthracene-d10	17.14	188	462238	29.67	ng/ul	0.00
79) Pyrene-d10	19.44	212	518172	28.42	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.31	264	564996	27.95	ng/ul	0.00

Target Compounds

				Ovalue	
2) 1,4-Dioxane	3.25	88	7265	4.349	ng/uL 96
4) Benzaldehyde	6.81	77	20641m	4.717	ng/ul
6) Phenol	6.87	94	37442	6.514	ng/ul# 90
8) Bis(2-Chloroethyl)ether	7.10	93	30335	6.669	ng/ul 93
10) 2-Chlorophenol	7.24	128	27732	6.645	ng/ul 96
11) 2-Methylphenol	8.11	108	24268	5.901	ng/ul 91
12) 2,2'-oxybis(1-Chloropropan	8.20	45	24648	6.119	ng/ul# 92
14) Acetophenone	8.48	105	45241	6.597	ng/ul# 93
15) N-Nitroso-di-n-propylamine	8.47	70	25104	6.061	ng/ul# 90
16) 4-Methylphenol	8.43	108	27771	6.337	ng/ul 99
17) Hexachloroethane	8.74	117	14202	7.140	ng/ul 97
20) Nitrobenzene	8.85	77	42062	7.273	ng/ul 96
21) Isophorone	9.38	82	62930	6.172	ng/ul# 97
23) 2-Nitrophenol	9.56	139	13912	7.452	ng/ul 95
24) 2,4-Dimethylphenol	9.62	107	32043	6.571	ng/ul 95
25) Bis(2-Chloroethoxy)methane	9.86	93	36714	6.463	ng/ul 100
27) 2,4-Dichlorophenol	10.09	162	27764	7.295	ng/ul 92
28) Naphthalene	10.49	128	88315	6.887	ng/ul 98
30) 4-Chloroaniline	10.60	127	28987	6.170	ng/ul 92
31) Hexachlorobutadiene	10.80	225	20446	7.608	ng/ul 97
32) Caprolactam	11.36	113	6662	5.605	ng/ul 84
33) 4-Chloro-3-methylphenol	11.72	107	27118	6.391	ng/ul 96
34) 2-Methylnaphthalene	12.11	142	61628	6.798	ng/ul 99

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072820\
 Data File : BM026930.D
 Acq On : 29 Jul 2020 17:39
 Operator : JU/CG
 Sample : L1955-09
 Misc : PBBL-WATER-02
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-02

Manual Integrations
 APPROVED

mohammad
 7/30/2020 3:32:41 PM

Quant Time: Jul 29 18:18:07 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 29 02:24:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
35) 1-Methylnaphthalene	12.33	142	60287	6.806	ng/ul	97
37) 1,2,4,5-Tetrachlorobenzene	12.48	216	33639	6.758	ng/ul	98
38) Hexachlorocyclopentadiene	12.48	237	17286	5.121	ng/ul#	95
39) 2,4,6-Trichlorophenol	12.72	196	17658	6.190	ng/ul	97
40) 2,4,5-Trichlorophenol	12.80	196	20149	6.611	ng/ul	92
41) 1,1'-Biphenyl	13.13	154	81154	6.668	ng/ul	95
42) 2-Chloronaphthalene	13.17	162	66567	6.797	ng/ul	97
43) 2-Nitroaniline	13.37	65	18488	6.348	ng/ul	95
45) Dimethylphthalate	13.76	163	80897	6.750	ng/ul	98
46) 2,6-Dinitrotoluene	13.87	165	13371	6.328	ng/ul#	85
48) Acenaphthylene	14.02	152	97443	6.599	ng/ul	99
49) 3-Nitroaniline	14.19	138	11533	5.584	ng/ul	97
50) Acenaphthene	14.37	153	69776	6.859	ng/ul	95
51) 2,4-Dinitrophenol	14.39	184	4474	5.288	ng/ul#	80
53) 4-Nitrophenol	14.50	109	15878	8.205	ng/ul#	82
54) Dibenzofuran	14.70	168	98144	6.960	ng/ul	99
55) 2,4-Dinitrotoluene	14.65	165	20533	6.763	ng/ul	100
56) 2,3,4,6-Tetrachlorophenol	14.93	232	16068	6.720	ng/ul	98
57) Diethylphthalate	15.14	149	81009	6.741	ng/ul	98
59) Fluorene	15.35	166	82416	6.941	ng/ul	99
60) 4-Chlorophenyl-phenylether	15.35	204	41643	7.046	ng/ul	99
61) 4-Nitroaniline	15.35	138	14341	5.665	ng/ul	90
64) 4,6-Dinitro-2-methylphenol	15.42	198	9870	6.250	ng/ul#	86
65) N-Nitrosodiphenylamine	15.56	169	68212	6.689	ng/ul	97
66) 4-Bromophenyl-phenylether	16.24	248	24820	6.787	ng/ul#	89
67) Hexachlorobenzene	16.36	284	29678	7.156	ng/ul	92
68) Atrazine	16.51	200	21929	5.858	ng/ul	100
69) Pentachlorophenol	16.69	266	12999	6.299	ng/ul	97
70) Phenanthrene	17.08	178	129962	6.868	ng/ul	99
72) Anthracene	17.17	178	132139	6.794	ng/ul	98
73) 1,2,3,4-Tetrachlorobenzene	13.09	216	33910	6.924	ng/uL	99
74) Pentachlorobenzene	14.62	250	33705	7.098	ng/uL	97
75) Carbazole	17.44	167	112682	6.554	ng/ul	99
76) Di-n-butylphthalate	18.03	149	123187	6.091	ng/ul	99
77) Fluoranthene	19.10	202	148244	6.635	ng/ul	96
80) Pvrene	19.47	202	163425	6.571	ng/ul#	95
81) Butylbenzylphthalate	20.39	149	48800	5.277	ng/ul	100
82) 3,3'-Dichlorobenzidine	21.15	252	35037	4.335	ng/ul	98
83) Benzo(a)anthracene	21.22	228	158534	6.728	ng/ul	99
84) Bis(2-ethylhexyl)phthalate	21.18	149	76953	5.550	ng/ul	99
85) Chrysene	21.27	228	155776	6.780	ng/ul	99
87) Di-n-octyl phthalate	22.05	149	125203	4.757	ng/ul	100
88) Benzo(b)fluoranthene	22.79	252	161258	6.293	ng/ul	99
89) Benzo(k)fluoranthene	22.83	252	166055	6.753	ng/ul	99
91) Benzo(a)pyrene	23.35	252	156736	6.779	ng/ul	99
92) Indeno(1,2,3-cd)pyrene	25.66	276	195961	6.832	ng/ul	98
93) Dibenzo(a,h)anthracene	25.67	278	167405	6.900	ng/ul	97
94) Benzo(a,h,i)perylene	26.33	276	164967	6.955	ng/ul	98

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072820\
Data File : BM026930.D
Acq On : 29 Jul 2020 17:39
Operator : JU/CG
Sample : L1955-09
Misc : PBBL-WATER-02
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-02

Manual Integrations
APPROVED

mohammad
7/30/2020 3:32:41 PM

Quant Time: Jul 29 18:18:07 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 29 02:24:07 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072820\
Data File : BM026930.D
Acq On : 29 Jul 2020 17:39
Operator : JU/CG
Sample : L1955-09
Misc : PBBL-WATER-02
ALS Vial : 47 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
MDL-WATER-02

Manual Integrations
APPROVED

mohammad
7/30/2020 3:32:41 PM

Quant Time: Jul 29 18:18:07 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 29 02:24:07 2020
Response via : Initial Calibration

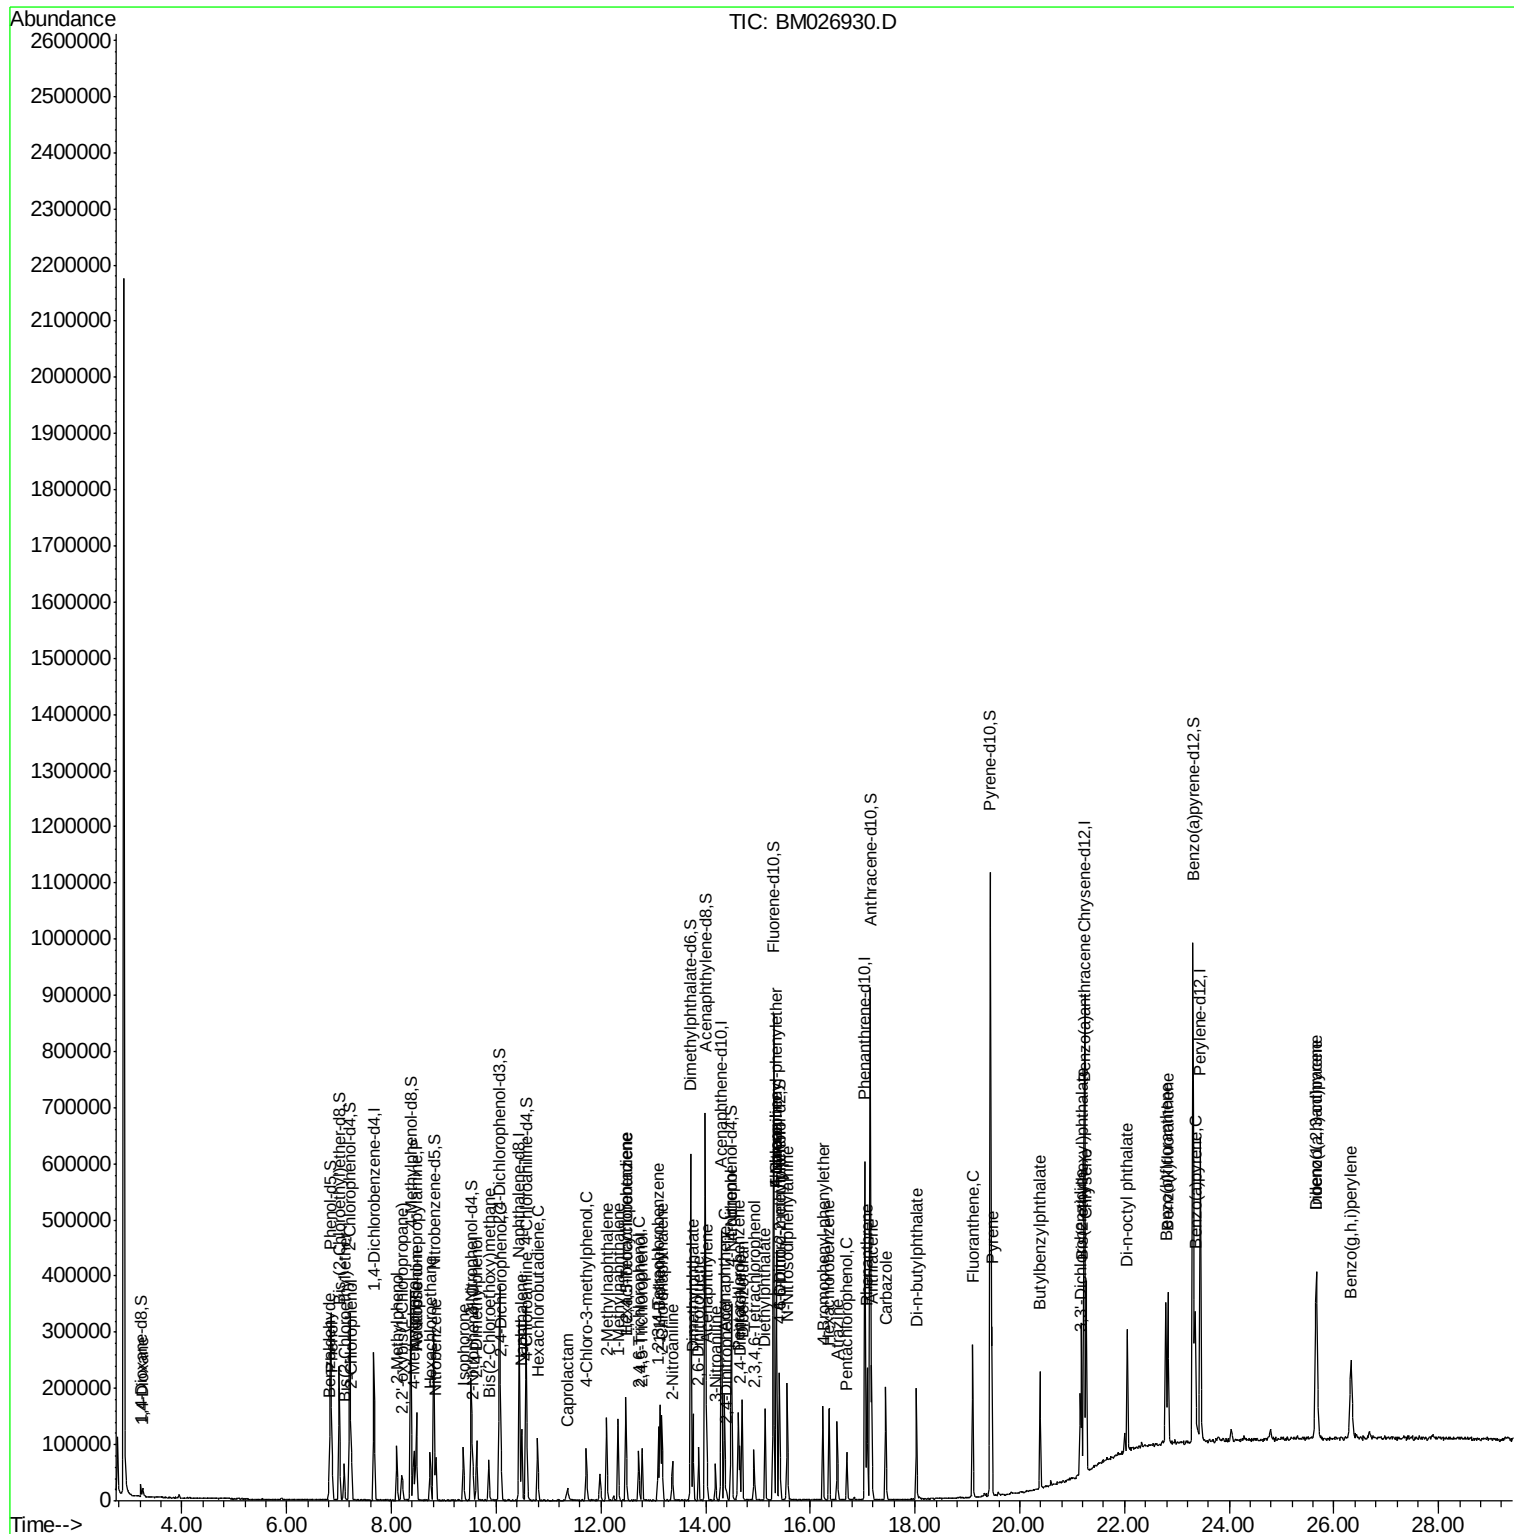



#2

1,4-Dioxane

Concen: 4.349 ng/uL

RT: 3.25 min Scan# 88

Delta R.T. -0.00 min

Lab File: BM026930.D

Acq: 29 Jul 2020 17:39

Instrument :

BNA_M


ClientSampleId :

MDL-WATER-02

Tot Ion:	88	Resp:	7265
Ion	Ratio	Lower	Upper
88	100		
43	34.0	24.7	37.1
58	65.6	50.8	76.2

Manual Integrations
APPROVED

mohammad
7/30/2020 3:32:41 PM





Abundance Ion 88.00 (87.70 to 88.70): BM026926.D (-83) (-)

Ion 43.00 (42.70 to 43.70): BM026926.D (-83) (-)

Ion 58.00 (57.70 to 58.70): BM026926.D (-83) (-)

Time-->



#4

Benzaldehyde

Concen: 4.717 ng/uL m


RT: 6.81 min Scan# 693

Delta R.T. -0.00 min

Lab File: BM026930.D

Acq: 29 Jul 2020 17:39

Tgt Ion:	77	Resp:	20641
Ion	Ratio	Lower	Upper
77	100		
105	81.8	64.9	97.3
106	78.3	62.5	93.7





Abundance Ion 77.00 (76.70 to 77.70): BM026926.D (-687) (-)

Ion 105.00 (104.70 to 105.70): BM026926.D (-687) (-)

Ion 106.00 (105.70 to 106.70): BM026926.D (-687) (-)

Time-->





#6

Phenol

Concen: 6.514 ng/ul

RT: 6.87 min Scan# 702

Delta R.T. -0.01 min

Lab File: BM026930.D

Acq: 29 Jul 2020 17:39

Instrument :

BNA_M





ClientSampleId :

MDL-WATER-02

Tot Ion:	94	Resp:	37442
Ion	Ratio	Lower	Upper
94	100		
65	41.3	26.2	39.4#
66	52.7	38.2	57.2

Manual Integrations
APPROVED

mohammad
7/30/2020 3:32:41 PM

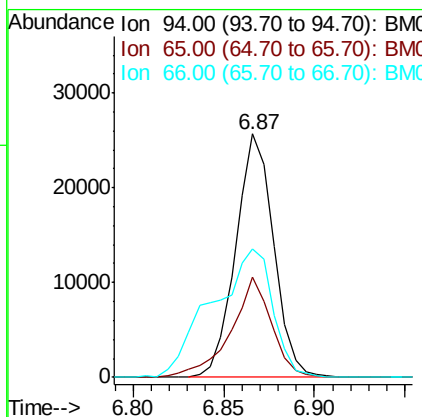

#8

Bis(2-Chloroethyl)ether

Concen: 6.669 ng/ul




RT: 7.10 min Scan# 741


Delta R.T. -0.01 min

Lab File: BM026930.D

Acq: 29 Jul 2020 17:39

Tgt Ion:	93	Resp:	30335
Ion	Ratio	Lower	Upper
93	100		
63	70.2	62.9	94.3
95	29.8	24.6	37.0

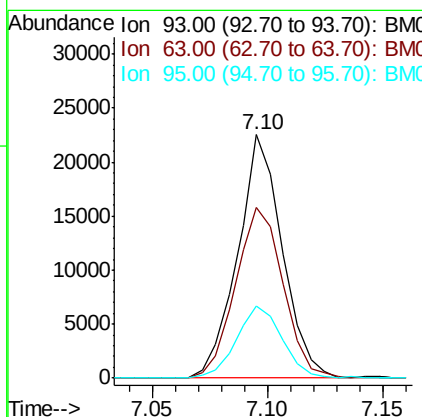



#10

2-Chlorophenol

Concen: 6.645 ng/ul

RT: 7.24 min Scan# 765

Delta R.T. -0.01 min

Lab File: BM026930.D

Acq: 29 Jul 2020 17:39

Instrument :

BNA_M





ClientSampleId :

MDL-WATER-02

Tot Ion:	128	Resp:	27732
Ion Ratio	Lower	Upper	
128	100		
64	57.6	43.4	65.2
130	31.9	26.3	39.5

Manual Integrations
APPROVED

mohammad
7/30/2020 3:32:41 PM

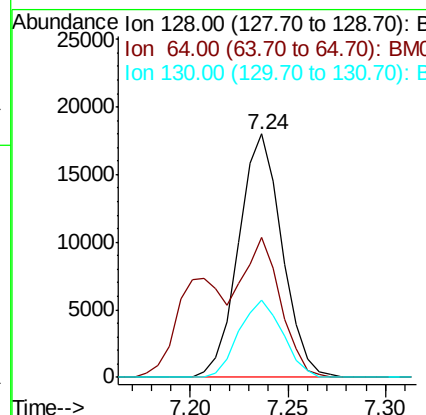

#11

2-Methylphenol

Concen: 5.901 ng/ul




RT: 8.11 min Scan# 913


Delta R.T. -0.00 min

Lab File: BM026930.D

Acq: 29 Jul 2020 17:39

Tgt Ion:	108	Resp:	24268
Ion Ratio	Lower	Upper	
108	100		
107	82.1	72.5	108.7

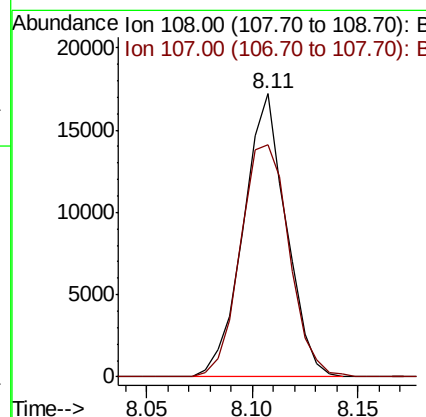




#12
2,2'-oxvbis(1-Chloropropane)
Concen: 6.119 ng/ul
RT: 8.20 min Scan# 929
Delta R.T. -0.01 min
Lab File: BM026930.D
Acq: 29 Jul 2020 17:39

Instrument :
BNA_M
ClientSampled :
MDL-WATER-02




Tot Ion	Ratio	Lower	Upper
45	100		
77	31.3	19.7	29.5#
79	18.2	14.9	22.3

Manual Integrations
APPROVED

mohammad
7/30/2020 3:32:41 PM




Abundance Ion 45.00 (44.70 to 45.70): BM0
Ion 77.00 (76.70 to 77.70): BM0
Ion 79.00 (78.70 to 79.70): BM0


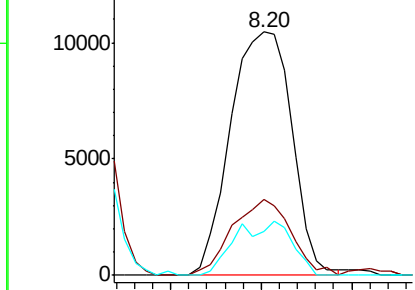



#14
Acetophenone
Concen: 6.597 ng/ul
RT: 8.48 min Scan# 976
Delta R.T. -0.01 min
Lab File: BM026930.D
Acq: 29 Jul 2020 17:39

Tgt Ion	Ratio	Lower	Upper
105	100		
77	97.2	74.0	111.0
51	28.2	17.3	25.9#



Abundance Ion 105.00 (104.70 to 105.70): E
Ion 77.00 (76.70 to 77.70): BM0
Ion 51.00 (50.70 to 51.70): BM0

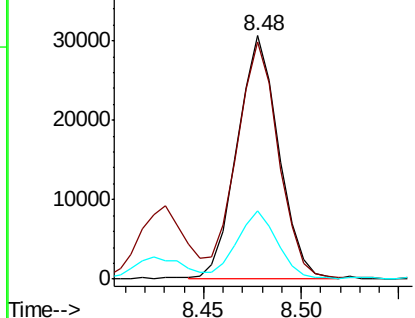







#15
N-Nitroso-di-n-propylamine
Concen: 6.061 ng/ul
RT: 8.47 min Scan# 975
Delta R.T. -0.00 min
Lab File: BM026930.D
Acq: 29 Jul 2020 17:39

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-02

Tot Ion	Ion	Ratio	Lower	Upper
70	100			
42	51.9	34.2	51.4#	
101	8.3	6.4	9.6	
130	18.2	13.2	19.8	




Manual Integrations
APPROVED


mohammad
7/30/2020 3:32:41 PM

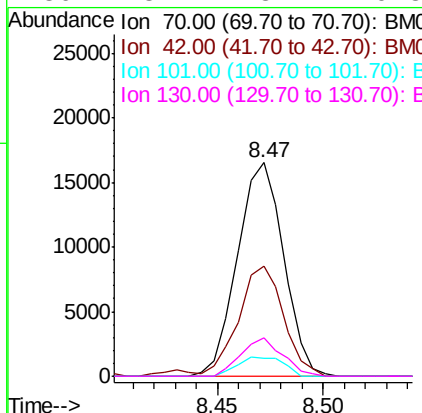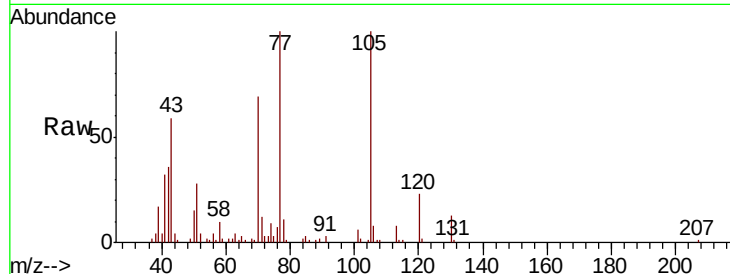

#16
4-Methylphenol
Concen: 6.337 ng/ul
RT: 8.43 min Scan# 968
Delta R.T. -0.01 min
Lab File: BM026930.D
Acq: 29 Jul 2020 17:39

Tgt Ion	Ion	Ratio	Lower	Upper
108	100			
107	112.3	88.8	133.2	

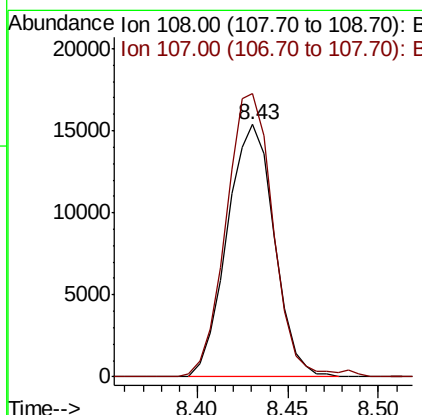



#17

Hexachloroethane

Concen: 7.140 ng/ul

RT: 8.74 min Scan# 1021

Delta R.T. -0.01 min

Lab File: BM026930.D

Acq: 29 Jul 2020 17:39

Instrument :

BNA_M





ClientSampleId :

MDL-WATER-02

Tot Ion	Ratio	Lower	Upper
117	100		
201	97.2	80.8	121.2
199	65.1	50.3	75.5

Manual Integrations
APPROVED

mohammad
7/30/2020 3:32:41 PM

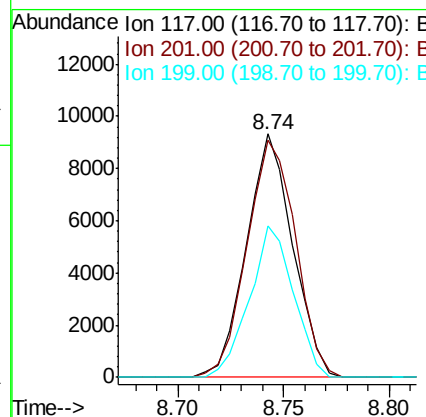

#20

Nitrobenzene

Concen: 7.273 ng/ul




RT: 8.85 min Scan# 1039


Delta R.T. -0.01 min

Lab File: BM026930.D

Acq: 29 Jul 2020 17:39

Tgt Ion	Ratio	Lower	Upper
77	100		
123	32.1	28.3	42.5
65	13.5	11.0	16.6

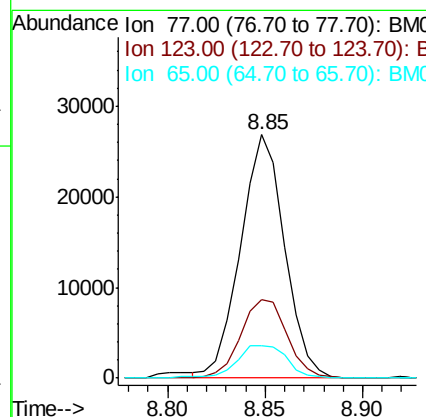

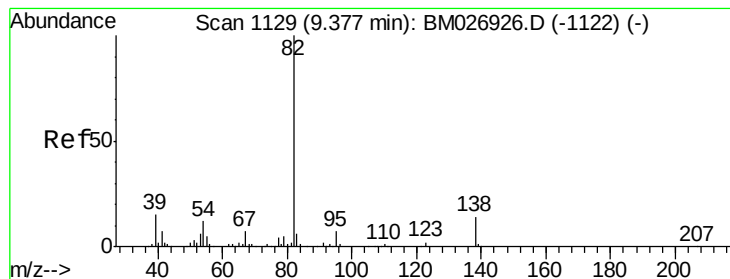

#21

Isophorone

Concen: 6.172 ng/ul

RT: 9.38 min Scan# 1129

Delta R.T. -0.01 min

Lab File: BM026930.D

Acq: 29 Jul 2020 17:39

Instrument :

BNA_M





ClientSampleId :

MDL-WATER-02

Tot Ion:	82	Resp:	62930
Ion	Ratio	Lower	Upper
82	100		
95	9.1	6.0	9.0#
138	15.3	11.5	17.3

Manual Integrations
APPROVED

mohammad
7/30/2020 3:32:41 PM

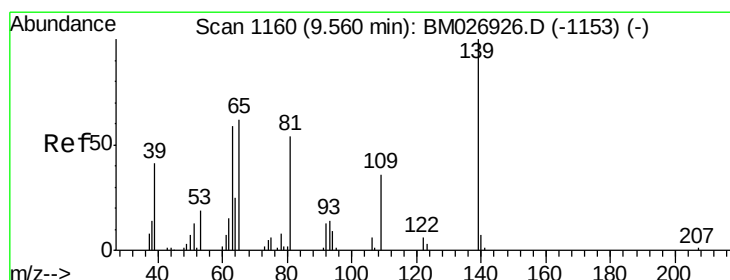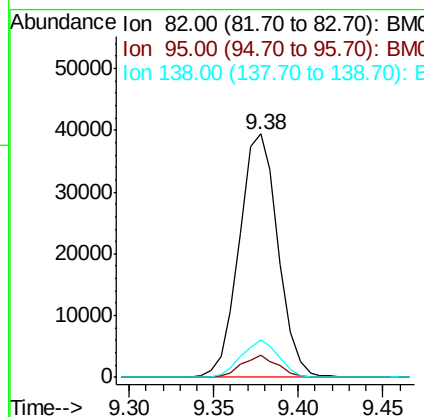

#23

2-Nitrophenol

Concen: 7.452 ng/ul




RT: 9.56 min Scan# 1160


Delta R.T. -0.00 min

Lab File: BM026930.D

Acq: 29 Jul 2020 17:39

Tgt Ion:	139	Resp:	13912
Ion	Ratio	Lower	Upper
139	100		
65	70.9	53.3	79.9
109	44.3	32.6	49.0

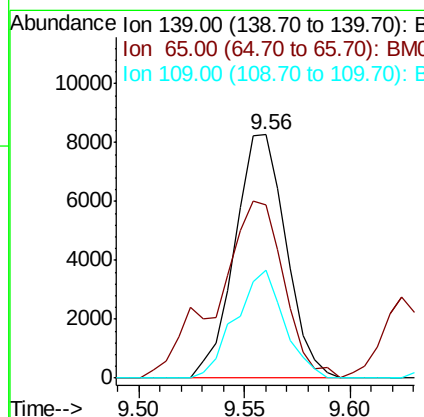

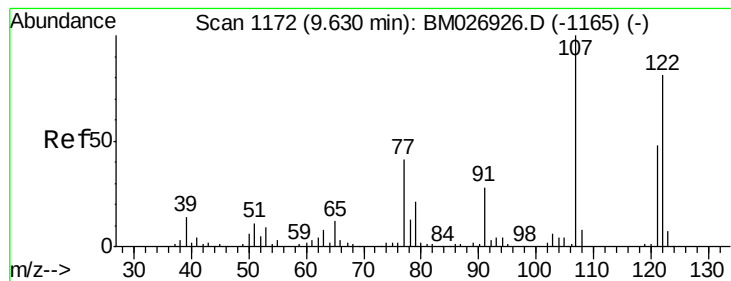





#24
 2,4-Dimethylphenol
 Concen: 6.571 ng/ul
 RT: 9.62 min Scan# 1171
 Delta R.T. -0.01 min
 Lab File: BM026930.D
 Acq: 29 Jul 2020 17:39

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-02

Tot Ion:	107	Resp:	32043
Ion Ratio	Lower	Upper	
107	100		
121	41.0	35.5	53.3
122	72.5	61.0	91.4




Manual Integrations
 APPROVED


mohammad
 7/30/2020 3:32:41 PM

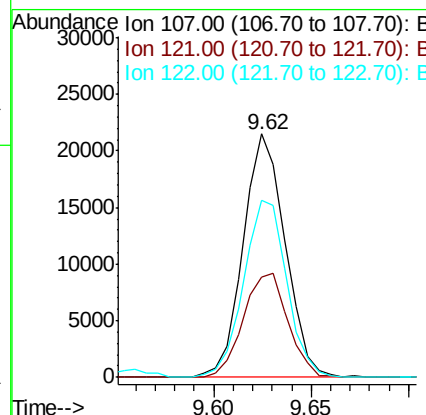

#25
 Bis(2-Chloroethoxy)methane
 Concen: 6.463 ng/ul
 RT: 9.86 min Scan# 1211
 Delta R.T. -0.01 min
 Lab File: BM026930.D
 Acq: 29 Jul 2020 17:39

Tgt Ion:	93	Resp:	36714
Ion Ratio	Lower	Upper	
93	100		
95	31.9	25.7	38.5
123	9.6	7.8	11.8

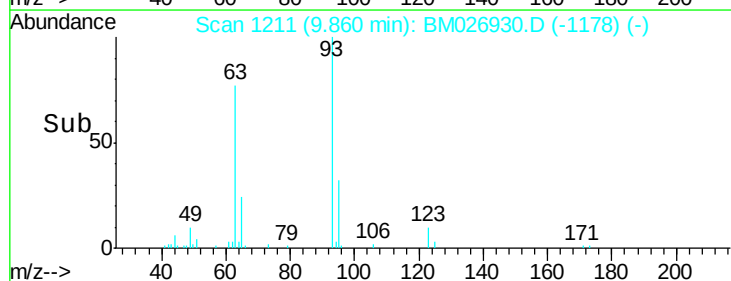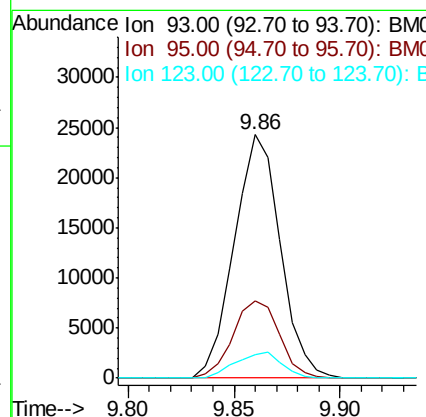







#27
 2,4-Dichlorophenol
 Concen: 7.295 ng/ul
 RT: 10.09 min Scan# 1250
 Delta R.T. -0.01 min
 Lab File: BM026930.D
 Acq: 29 Jul 2020 17:39

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-02

Tot Ion	Ratio	Lower	Upper
162	100		
164	75.5	52.4	78.6
98	40.0	32.2	48.2




Manual Integrations
 APPROVED


mohammad
 7/30/2020 3:32:41 PM

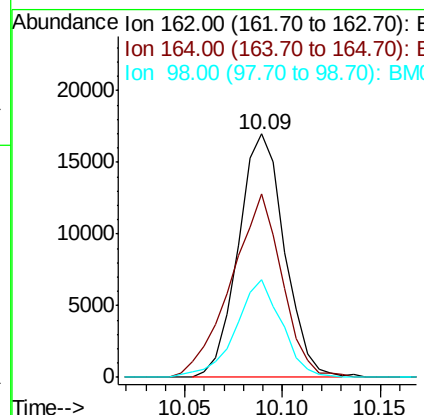

#28
 Naphthalene
 Concen: 6.887 ng/ul
 RT: 10.49 min Scan# 1318
 Delta R.T. -0.01 min
 Lab File: BM026930.D
 Acq: 29 Jul 2020 17:39

Tgt Ion	Ratio	Lower	Upper
128	100		
129	10.5	8.3	12.5
127	12.4	11.0	16.6

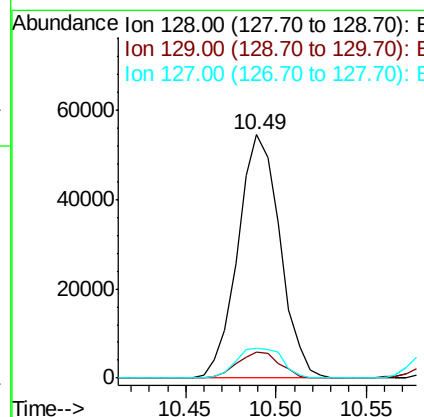







#30
4-Chloroaniline
Concen: 6.170 ng/ul
RT: 10.60 min Scan# 1336
Delta R.T. -0.01 min
Lab File: BM026930.D
Acq: 29 Jul 2020 17:39

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-02

Tot Ion	Ratio	Lower	Upper
127	100		
129	34.9	24.3	36.5




Manual Integrations
APPROVED


mohammad
7/30/2020 3:32:41 PM

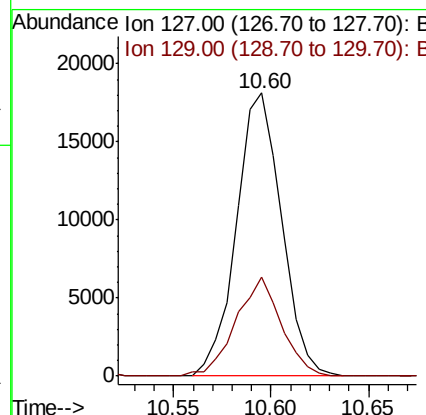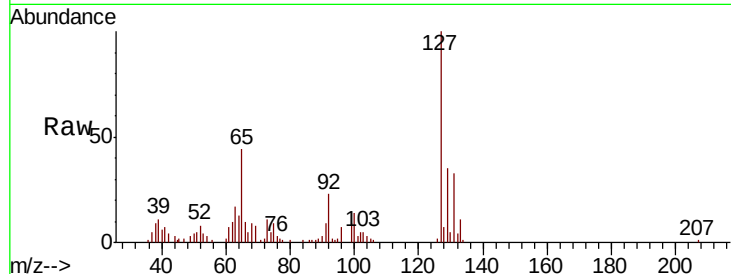

#31
Hexachlorobutadiene
Concen: 7.608 ng/ul
RT: 10.80 min Scan# 1370
Delta R.T. -0.01 min
Lab File: BM026930.D
Acq: 29 Jul 2020 17:39

Tgt Ion	Ratio	Lower	Upper
225	100		
223	63.0	51.4	77.0
227	63.0	53.1	79.7

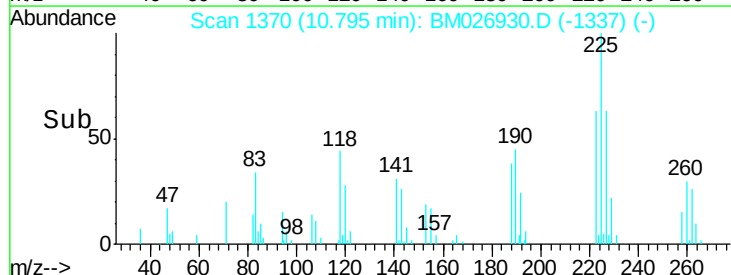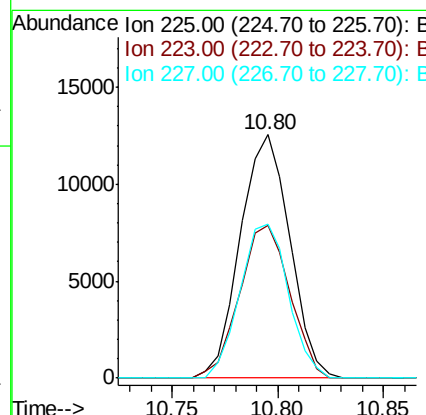







#32
 Caprolactam
 Concen: 5.605 ng/ul
 RT: 11.36 min Scan# 1466
 Delta R.T. 0.02 min
 Lab File: BM026930.D
 Acq: 29 Jul 2020 17:39

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-02

Tot Ion	Ratio	Lower	Upper
113	100		
55	125.0	119.7	179.5
56	99.9	90.2	135.2




Manual Integrations
 APPROVED


mohammad
 7/30/2020 3:32:41 PM

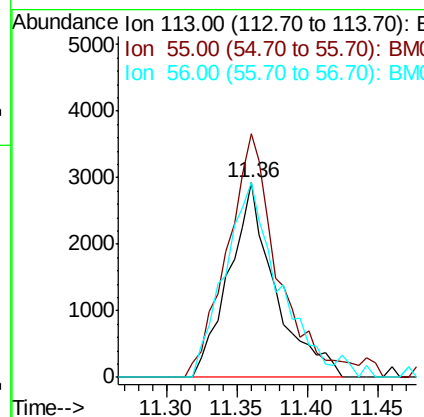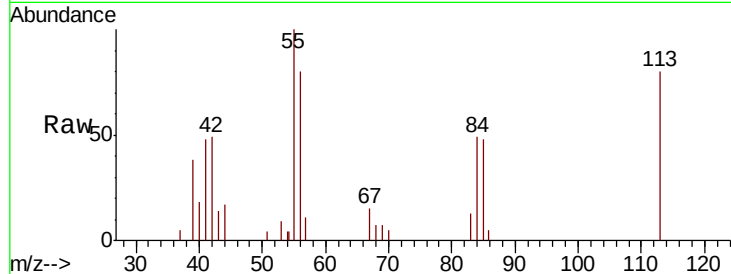

#33
 4-Chloro-3-methylphenol
 Concen: 6.391 ng/ul
 RT: 11.72 min Scan# 1528
 Delta R.T. -0.01 min
 Lab File: BM026930.D
 Acq: 29 Jul 2020 17:39

Tgt Ion	Ratio	Lower	Upper
107	100		
144	24.1	20.6	30.8
142	78.5	59.9	89.9

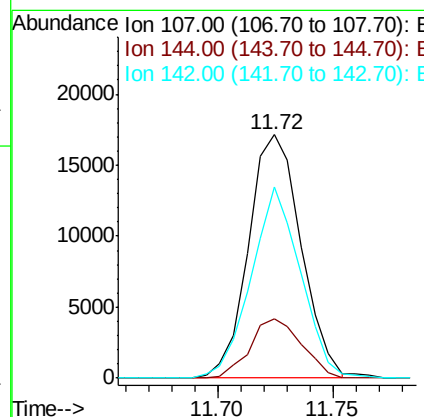







#34
2-Methylnaphthalene
Concen: 6.798 ng/ul
RT: 12.11 min Scan# 1593
Delta R.T. -0.01 min
Lab File: BM026930.D
Acq: 29 Jul 2020 17:39

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-02

Tot Ion:142 Resp: 61628
Ion Ratio Lower Upper
142 100
141 88.3 71.1 106.7




Manual Integrations
APPROVED


mohammad
7/30/2020 3:32:41 PM

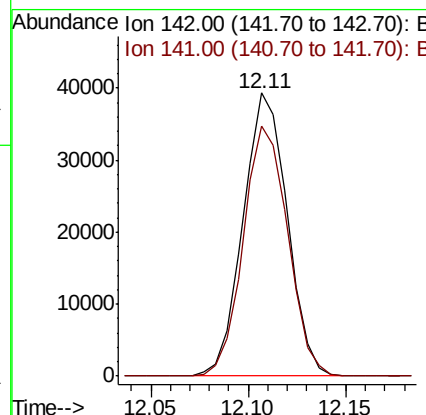

#35
1-Methylnaphthalene
Concen: 6.806 ng/ul
RT: 12.33 min Scan# 1631
Delta R.T. -0.01 min
Lab File: BM026930.D
Acq: 29 Jul 2020 17:39

Tgt Ion:142 Resp: 60287
Ion Ratio Lower Upper
142 100
141 88.2 73.3 109.9
116 4.5 3.4 5.0

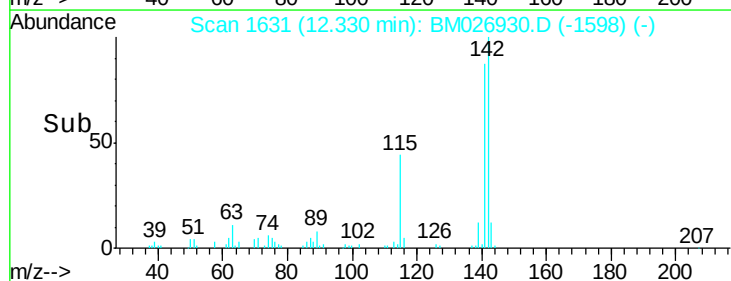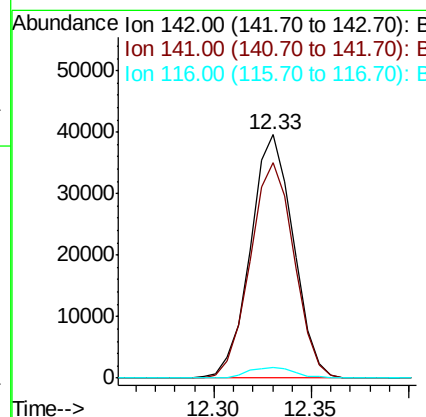

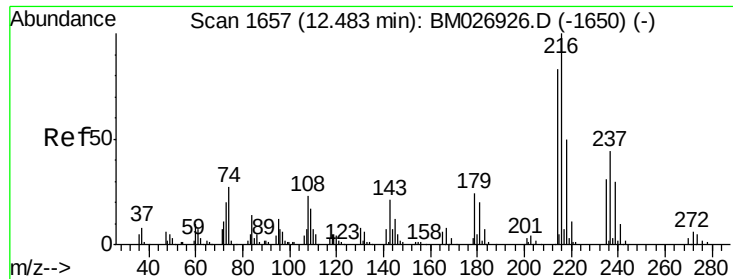





#37
 1,2,4,5-Tetrachlorobenzene
 Concen: 6.758 ng/ul
 RT: 12.48 min Scan# 1657
 Delta R.T. -0.01 min
 Lab File: BM026930.D
 Acq: 29 Jul 2020 17:39

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-02

Tot Ion:	216	Resp:	33639
Ion Ratio	Lower	Upper	
216	100		
214	79.3	64.2	96.4
179	22.3	16.2	24.4
108	21.1	16.7	25.1




Manual Integrations
 APPROVED


mohammad
 7/30/2020 3:32:41 PM

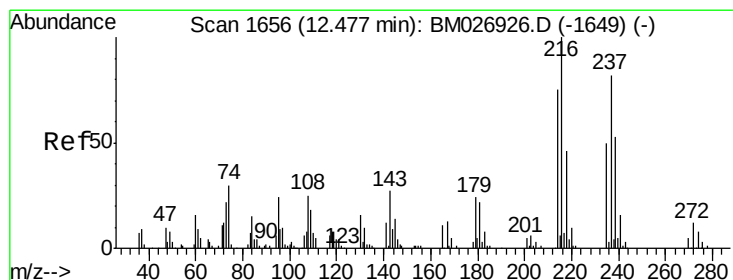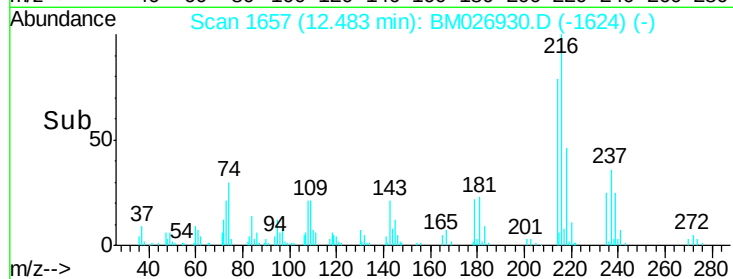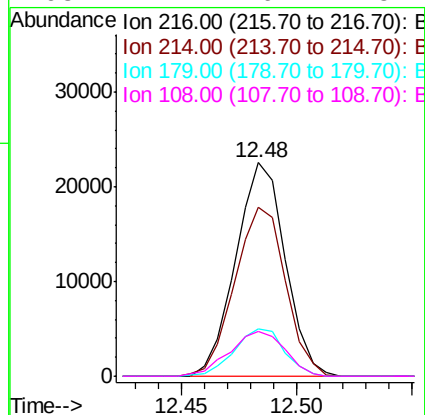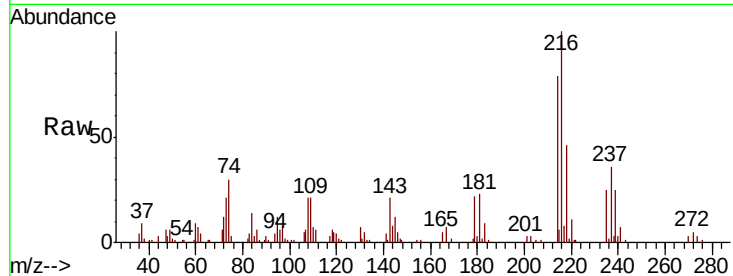

#38
 Hexachlorocyclopentadiene
 Concen: 5.121 ng/ul
 RT: 12.48 min Scan# 1656
 Delta R.T. -0.00 min
 Lab File: BM026930.D
 Acq: 29 Jul 2020 17:39

Tgt Ion:	237	Resp:	17286
Ion Ratio	Lower	Upper	
237	100		
235	65.5	49.8	74.8
272	9.3	10.1	15.1#

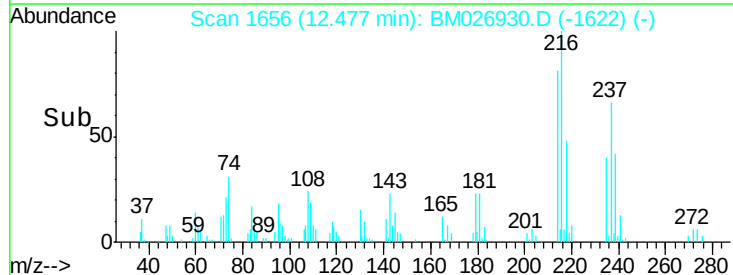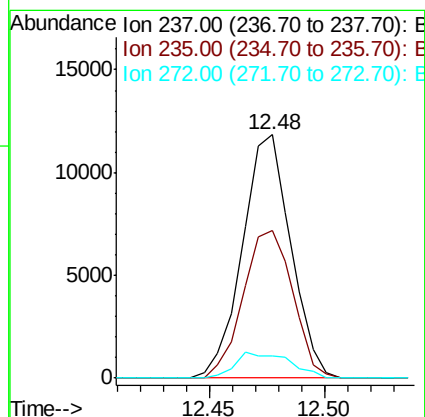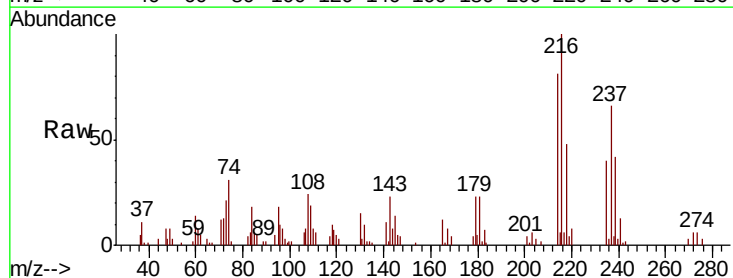







#39
 2,4,6-Trichlorophenol
 Concen: 6.190 ng/ul
 RT: 12.72 min Scan# 1698
 Delta R.T. -0.01 min
 Lab File: BM026930.D
 Acq: 29 Jul 2020 17:39

Instrument :
 BNA_M
 ClientSampled :
 MDL-WATER-02

Tot Ion	Ratio	Lower	Upper
196	100		
198	95.6	79.0	118.6
200	31.1	23.3	34.9




Manual Integrations
 APPROVED


mohammad
 7/30/2020 3:32:41 PM

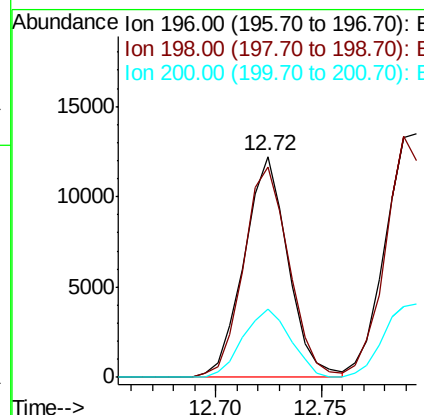

#40
 2,4,5-Trichlorophenol
 Concen: 6.611 ng/ul
 RT: 12.80 min Scan# 1710
 Delta R.T. -0.00 min
 Lab File: BM026930.D
 Acq: 29 Jul 2020 17:39

Tgt Ion	Ratio	Lower	Upper
196	100		
198	89.0	79.0	118.6
200	30.3	25.4	38.2

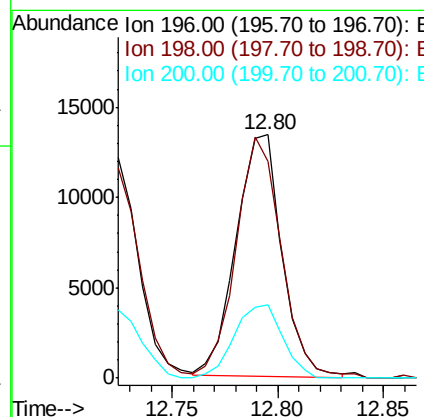

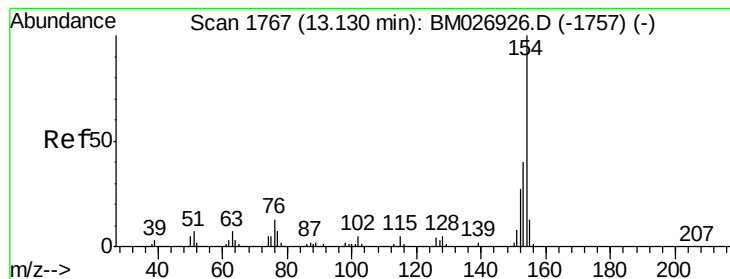


#41
 1,1'-Biphenyl
 Concen: 6.668 ng/ul
 RT: 13.13 min Scan# 1767
 Delta R.T. -0.01 min
 Lab File: BM026930.D
 Acq: 29 Jul 2020 17:39

Instrument :
 BNA_M
 ClientSampled :
 MDL-WATER-02




Tot Ion	Ratio	Lower	Upper
154	100		
153	43.5	31.4	47.2
76	13.1	10.8	16.2

Manual Integrations
 APPROVED

mohammad
 7/30/2020 3:32:41 PM




Abundance Ion 154.00 (153.70 to 154.70): E
 Ion 153.00 (152.70 to 153.70): E
 Ion 76.00 (75.70 to 76.70): BM

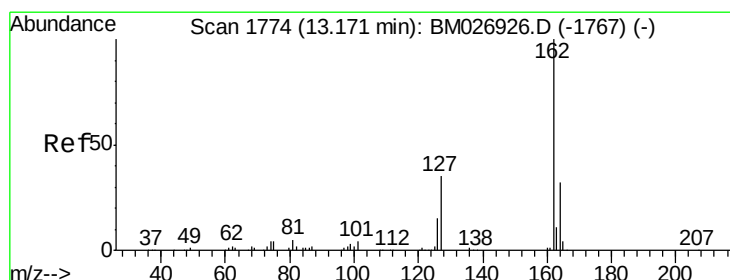
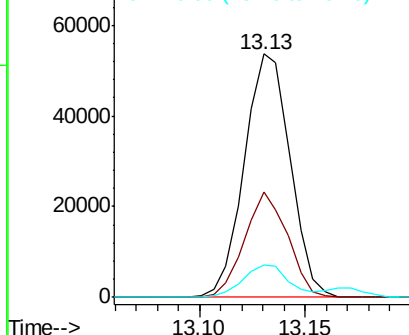



#42
 2-Chloronaphthalene
 Concen: 6.797 ng/ul
 RT: 13.17 min Scan# 1773
 Delta R.T. -0.01 min
 Lab File: BM026930.D
 Acq: 29 Jul 2020 17:39

Tgt Ion	Ratio	Lower	Upper
162	100		
164	33.7	26.4	39.6
127	40.8	30.6	45.8



Abundance Ion 162.00 (161.70 to 162.70): E
 Ion 164.00 (163.70 to 164.70): E
 Ion 127.00 (126.70 to 127.70): E

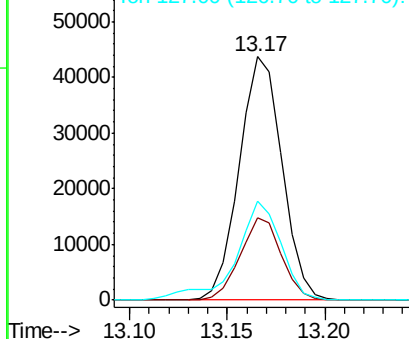







#43
2-Nitroaniline
Concen: 6.348 ng/ul
RT: 13.37 min Scan# 1807
Delta R.T. -0.00 min
Lab File: BM026930.D
Acq: 29 Jul 2020 17:39

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-02

Tot Ion	Ratio	Lower	Upper
65	100		
92	60.0	51.0	76.6
138	78.7	67.3	100.9




Manual Integrations
APPROVED


mohammad
7/30/2020 3:32:41 PM

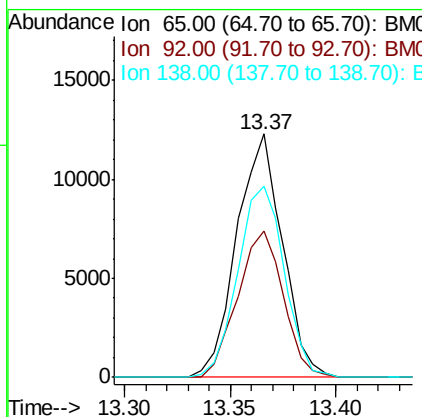

#45
Dimethylphthalate
Concen: 6.750 ng/ul
RT: 13.76 min Scan# 1874
Delta R.T. -0.01 min
Lab File: BM026930.D
Acq: 29 Jul 2020 17:39

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.2	3.0	4.6
164	10.0	8.6	12.8

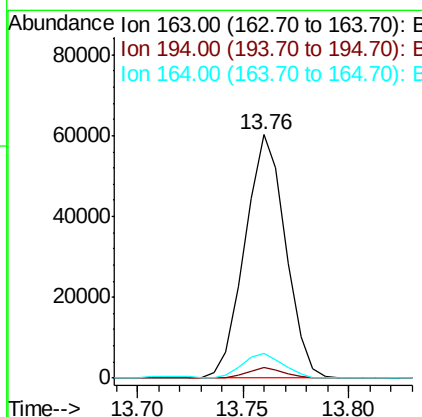







#46
 2,6-Dinitrotoluene
 Concen: 6.328 ng/ul
 RT: 13.87 min Scan# 1892
 Delta R.T. -0.01 min
 Lab File: BM026930.D
 Acq: 29 Jul 2020 17:39

Instrument :
 BNA_M
 ClientSampleID :
 MDL-WATER-02

Tot Ion	Ratio	Lower	Upper
165	100		
89	84.0	55.0	82.4#
121	21.1	19.0	28.6




Manual Integrations
 APPROVED


mohammad
 7/30/2020 3:32:41 PM

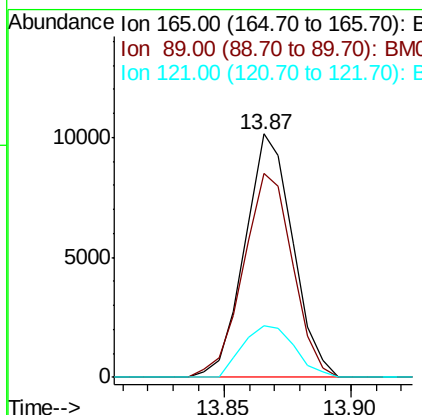

#48
 Acenaphthylene
 Concen: 6.599 ng/ul
 RT: 14.02 min Scan# 1918
 Delta R.T. -0.01 min
 Lab File: BM026930.D
 Acq: 29 Jul 2020 17:39

Tgt Ion	Ratio	Lower	Upper
152	100		
151	20.2	15.8	23.6
153	14.1	10.7	16.1

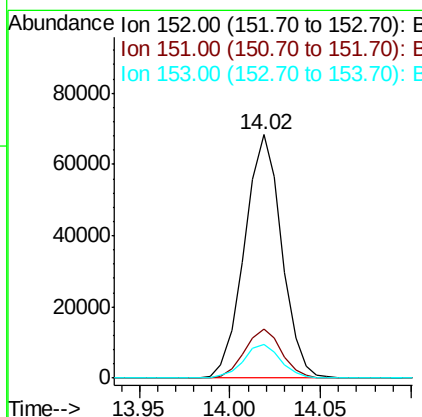







#49
3-Nitroaniline
Concen: 5.584 ng/ul
RT: 14.19 min Scan# 1948
Delta R.T. -0.00 min
Lab File: BM026930.D
Acq: 29 Jul 2020 17:39

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-02

Tot Ion	Ratio	Lower	Upper
138	100		
108	13.6	11.4	17.2
92	132.2	108.7	163.1




Manual Integrations
APPROVED


mohammad
7/30/2020 3:32:41 PM

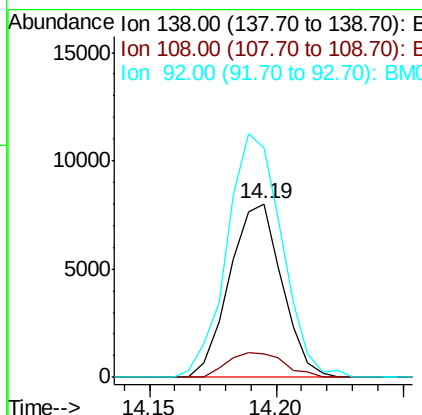

#50
Acenaphthene
Concen: 6.859 ng/ul
RT: 14.37 min Scan# 1977
Delta R.T. -0.00 min
Lab File: BM026930.D
Acq: 29 Jul 2020 17:39

Tgt Ion	Ratio	Lower	Upper
153	100		
152	44.4	37.8	56.6
154	83.5	70.5	105.7

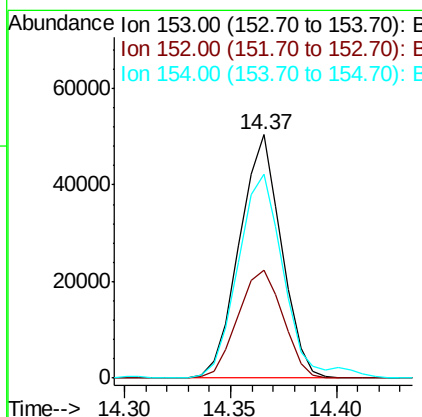







#51
 2,4-Dinitrophenol
 Concen: 5.288 ng/ul
 RT: 14.39 min Scan# 1982
 Delta R.T. -0.01 min
 Lab File: BM026930.D
 Acq: 29 Jul 2020 17:39

Instrument :
 BNA_M
 ClientSampled :
 MDL-WATER-02

Tot Ion	Ratio	Lower	Upper
184	100		
63	89.3	57.8	86.8#
154	52.4	55.0	82.4#




Manual Integrations
 APPROVED


mohammad
 7/30/2020 3:32:41 PM

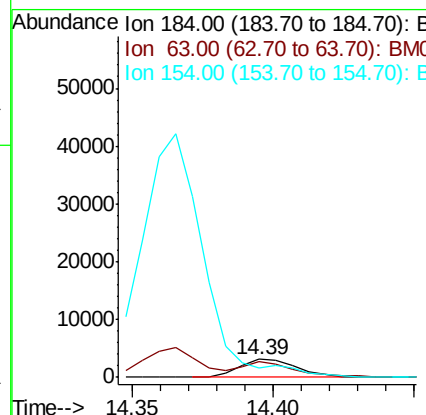

#53
 4-Nitrophenol
 Concen: 8.205 ng/ul
 RT: 14.50 min Scan# 2000
 Delta R.T. -0.01 min
 Lab File: BM026930.D
 Acq: 29 Jul 2020 17:39

Tgt Ion	Ratio	Lower	Upper
109	100		
139	88.6	92.3	138.5#
65	129.5	116.6	174.8

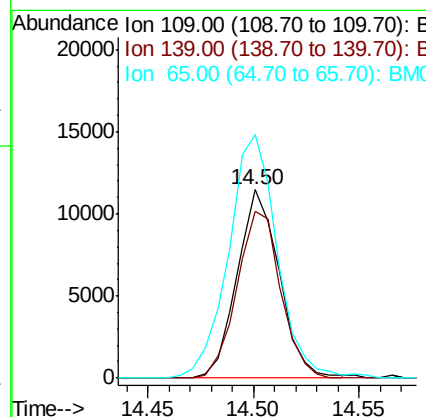



#54

Dibenzofuran

Concen: 6.960 ng/ul

RT: 14.70 min Scan# 2034

Delta R.T. -0.01 min

Lab File: BM026930.D

Acq: 29 Jul 2020 17:39

Instrument :

BNA_M

ClientSampleId :

MDL-WATER-02

Tot Ion:168 Resp: 98144

Ion Ratio Lower Upper





168 100

139 39.1 30.8 46.2

Manual Integrations
APPROVED

mohammad

7/30/2020 3:32:41 PM

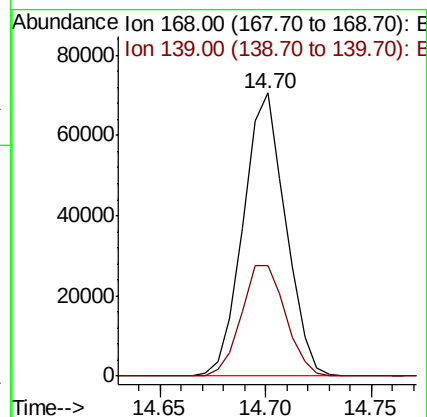

#55

2,4-Dinitrotoluene

Concen: 6.763 ng/ul

RT: 14.65 min Scan# 2026

Delta R.T. -0.01 min

Lab File: BM026930.D

Acq: 29 Jul 2020 17:39




Tgt Ion:165 Resp: 20533


Ion Ratio Lower Upper

165 100

63 58.1 46.2 69.4

182 2.8 2.4 3.6

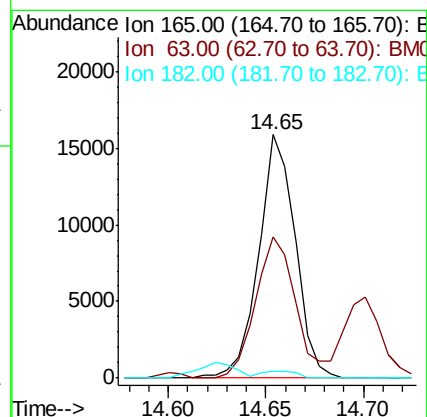

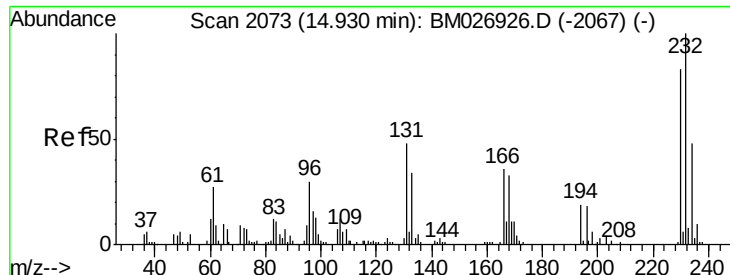





#56
 2,3,4,6-Tetrachlorophenol
 Concen: 6.720 ng/ul
 RT: 14.93 min Scan# 2073
 Delta R.T. -0.00 min
 Lab File: BM026930.D
 Acq: 29 Jul 2020 17:39

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-02

Tot Ion	Ratio	Lower	Upper
232	100		
131	50.2	39.4	59.2
130	2.9	2.6	4.0
166	31.9	26.7	40.1




Manual Integrations
 APPROVED


mohammad
 7/30/2020 3:32:41 PM

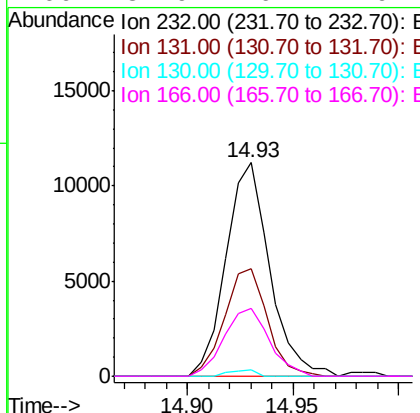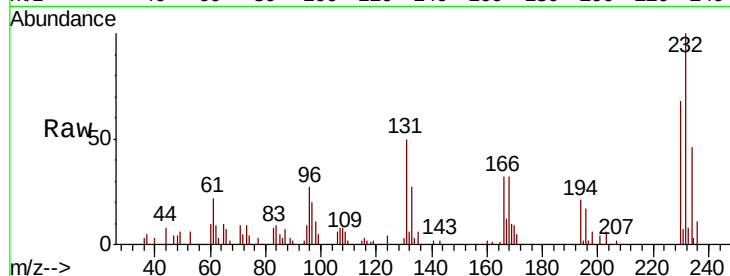

#57
 Diethylphthalate
 Concen: 6.741 ng/ul
 RT: 15.14 min Scan# 2108
 Delta R.T. -0.01 min
 Lab File: BM026930.D
 Acq: 29 Jul 2020 17:39

Tgt Ion	Ratio	Lower	Upper
149	100		
177	20.4	17.0	25.4
150	12.9	9.2	13.8

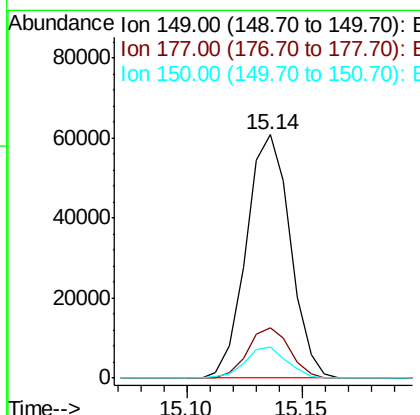

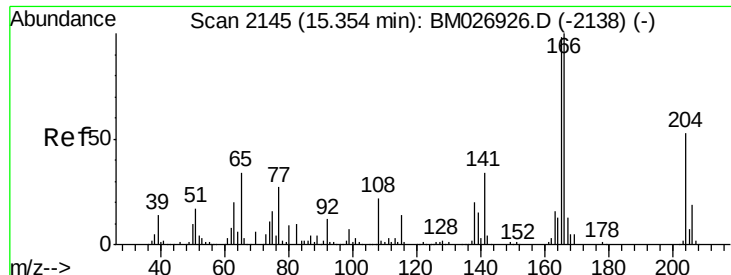

#59

Fluorene

Concen: 6.941 ng/ul

RT: 15.35 min Scan# 2144

Delta R.T. -0.01 min

Lab File: BM026930.D

Acq: 29 Jul 2020 17:39

Instrument :

BNA_M

ClientSampleId :

MDL-WATER-02

Tot Ion:166 Resp: 82416

Ion Ratio Lower Upper

166 100

165 96.9 78.2 117.2


167 12.8 10.3 15.5

Manual Integrations

APPROVED

mohammad




7/30/2020 3:32:41 PM



Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

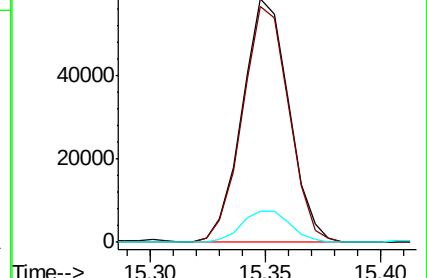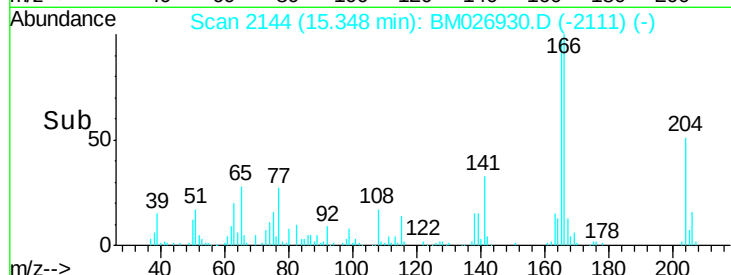

#60

4-Chlorophenyl-phenylether

Concen: 7.046 ng/ul

RT: 15.35 min Scan# 2145

Delta R.T. -0.01 min

Lab File: BM026930.D

Acq: 29 Jul 2020 17:39


Tgt Ion:204 Resp: 41643

Ion Ratio Lower Upper

204 100

206 31.7 26.0 39.0



141 60.4 48.3 72.5




Abundance Ion 204.00 (203.70 to 204.70): E

Ion 206.00 (205.70 to 206.70): E

Ion 141.00 (140.70 to 141.70): E

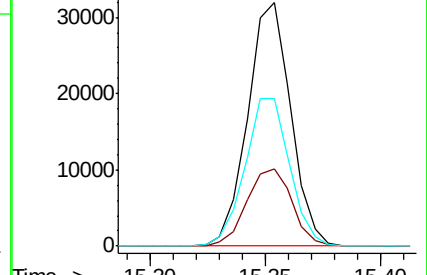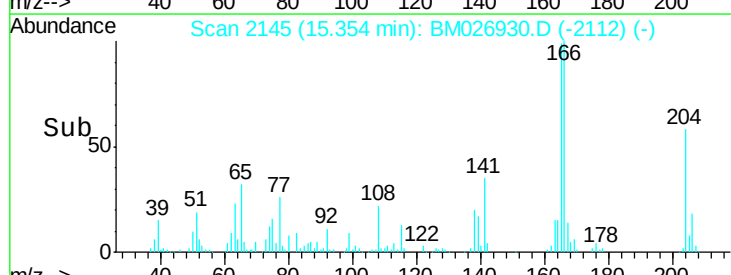







#61
 4-Nitroaniline
 Concen: 5.665 ng/ul
 RT: 15.35 min Scan# 2145
 Delta R.T. -0.01 min
 Lab File: BM026930.D
 Acq: 29 Jul 2020 17:39

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-02

Tot Ion	Ratio	Lower	Upper
138	100		
92	55.2	49.9	74.9
108	108.9	78.9	118.3




Manual Integrations
 APPROVED


mohammad
 7/30/2020 3:32:41 PM

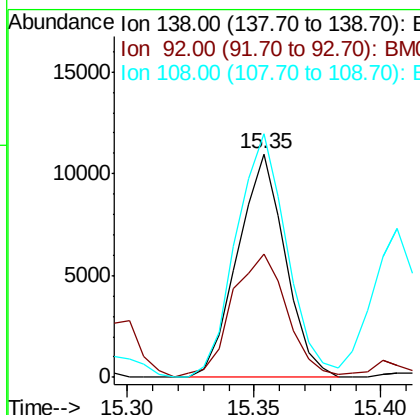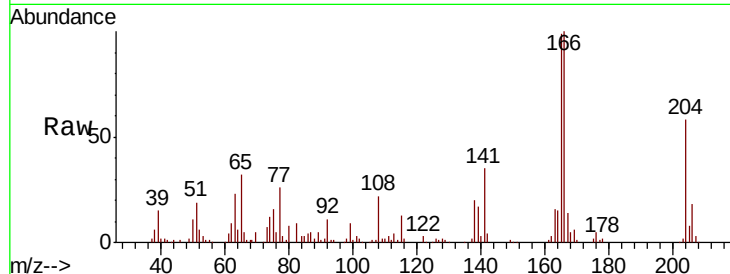

#64
 4,6-Dinitro-2-methylphenol
 Concen: 6.250 ng/ul
 RT: 15.42 min Scan# 2156
 Delta R.T. -0.01 min
 Lab File: BM026930.D
 Acq: 29 Jul 2020 17:39

Tgt Ion	Ratio	Lower	Upper
198	100		
182	6.4	4.2	6.4
77	45.9	29.3	43.9#

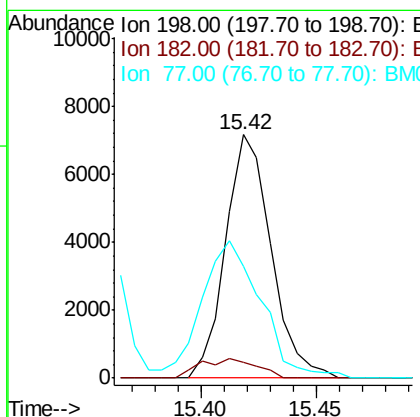







#65
N-Nitrosodiphenylamine
Concen: 6.689 ng/ul
RT: 15.56 min Scan# 2180
Delta R.T. -0.01 min
Lab File: BM026930.D
Acq: 29 Jul 2020 17:39

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-02

Tot Ion	Ratio	Lower	Upper
169	100		
168	66.2	54.6	82.0
167	34.7	29.1	43.7




Manual Integrations
APPROVED


mohammad
7/30/2020 3:32:41 PM

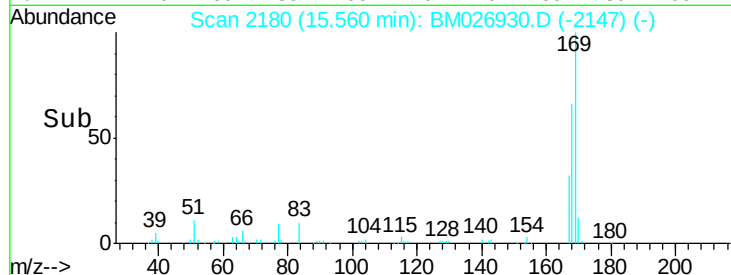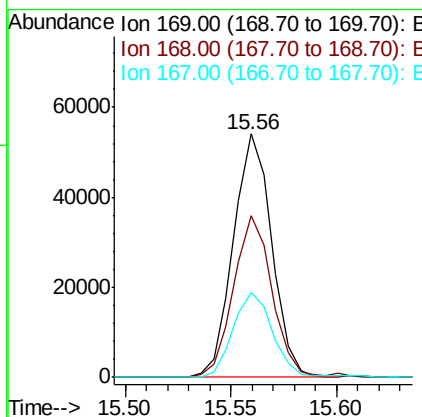

#66
4-Bromophenyl-phenylether
Concen: 6.787 ng/ul
RT: 16.24 min Scan# 2296
Delta R.T. -0.01 min
Lab File: BM026930.D
Acq: 29 Jul 2020 17:39

Tgt Ion	Ratio	Lower	Upper
248	100		
250	100.6	78.2	117.4
141	89.7	57.5	86.3

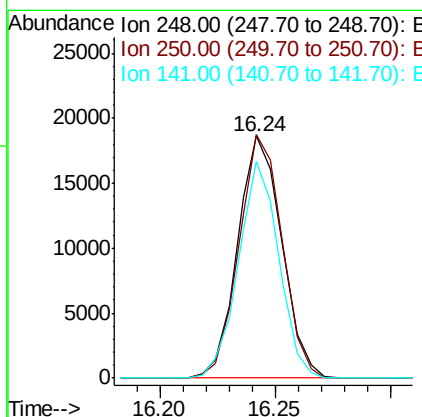

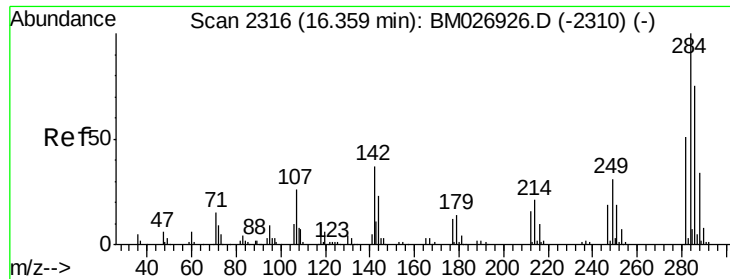





#67
Hexachlorobenzene
Concen: 7.156 ng/ul
RT: 16.36 min Scan# 2316
Delta R.T. -0.00 min
Lab File: BM026930.D
Acq: 29 Jul 2020 17:39

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-02

Tot Ion	Ratio	Lower	Upper
284	100		
142	33.7	31.7	47.5
249	28.7	25.7	38.5




Manual Integrations
APPROVED


mohammad
7/30/2020 3:32:41 PM

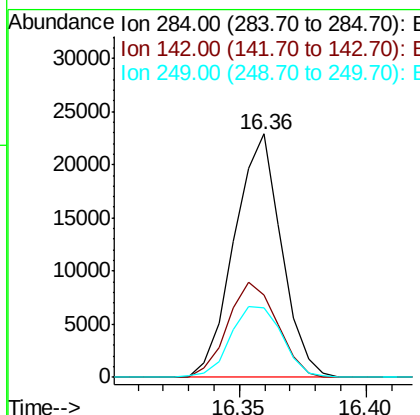

#68
Atrazine
Concen: 5.858 ng/ul
RT: 16.51 min Scan# 2342
Delta R.T. -0.01 min
Lab File: BM026930.D
Acq: 29 Jul 2020 17:39

Tgt Ion	Ratio	Lower	Upper
200	100		
173	27.9	22.4	33.6
215	48.6	38.6	58.0

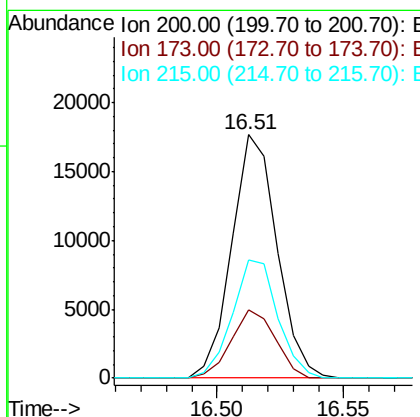




#69
 Pentachlorophenol
 Concen: 6.299 ng/ul
 RT: 16.69 min Scan# 2373
 Delta R.T. -0.01 min
 Lab File: BM026930.D
 Acq: 29 Jul 2020 17:39

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-02

Tot Ion	Ratio	Lower	Upper
266	100		
264	64.4	49.3	73.9
268	61.8	50.5	75.7

Manual Integrations
 APPROVED

mohammad
 7/30/2020 3:32:41 PM






Abundance

Ion 265.70 (265.40 to 266.40): E


Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

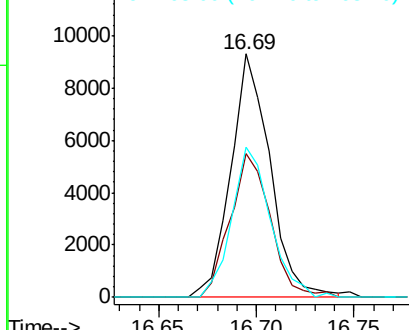

#70
 Phenanthrene
 Concen: 6.868 ng/ul
 RT: 17.08 min Scan# 2439
 Delta R.T. -0.01 min
 Lab File: BM026930.D
 Acq: 29 Jul 2020 17:39

Tgt Ion	Ratio	Lower	Upper
178	100		
179	14.9	12.0	18.0
176	18.7	14.7	22.1






Abundance

Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

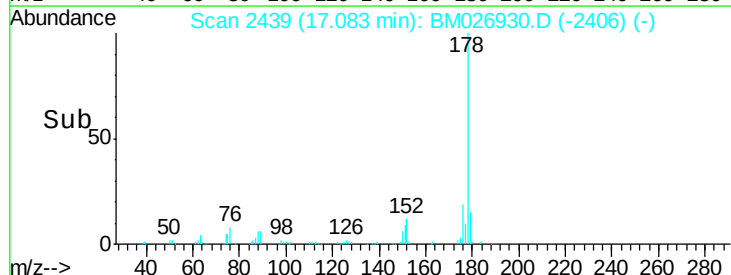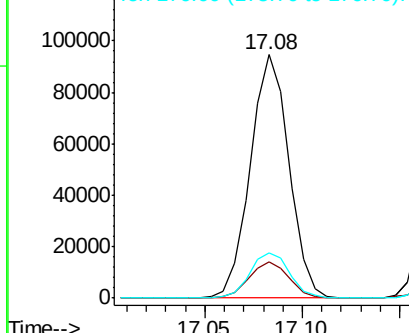

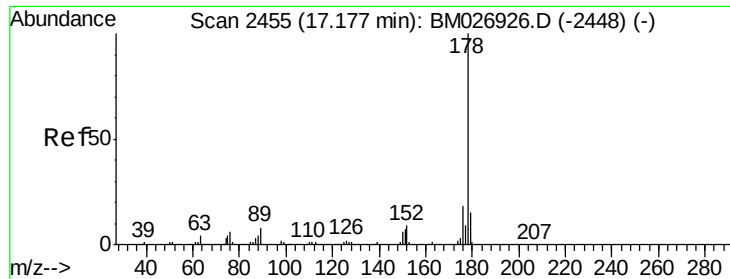

#72

Anthracene

Concen: 6.794 ng/ul

RT: 17.17 min Scan# 2454

Delta R.T. -0.01 min

Lab File: BM026930.D

Acq: 29 Jul 2020 17:39

Instrument :

BNA_M


ClientSampleId :

MDL-WATER-02




Tot Ion:	178	Resp:	132139
Ion Ratio	Lower	Upper	
178	100		
179	15.7	11.8	17.6
176	18.3	15.0	22.6

Manual Integrations
APPROVED

mohammad
7/30/2020 3:32:41 PM

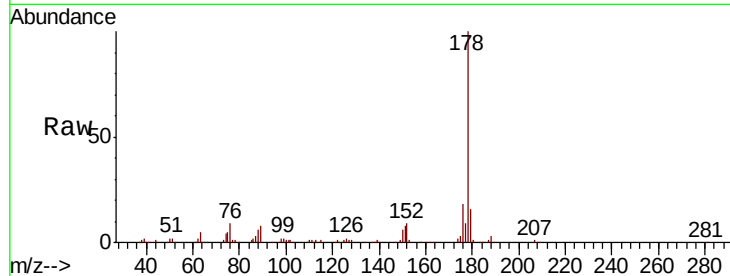

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

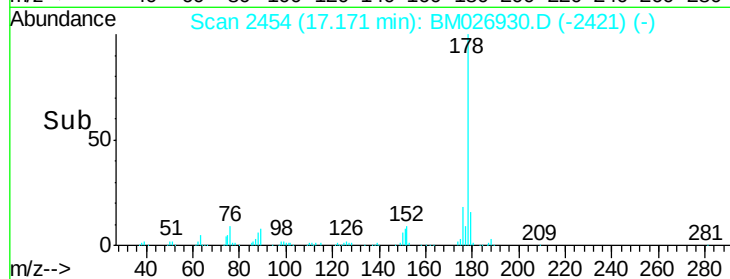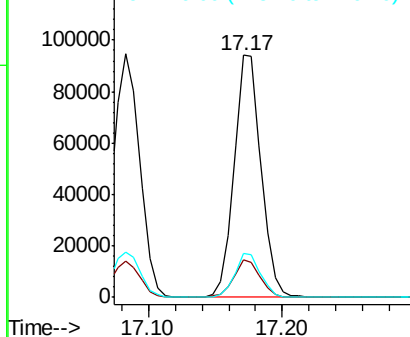

#73

1,2,3,4-Tetrachlorobenzene

Concen: 6.924 ng/uL


RT: 13.09 min Scan# 1761

Delta R.T. -0.01 min



Lab File: BM026930.D


Acq: 29 Jul 2020 17:39

Tgt Ion:	216	Resp:	33910
Ion Ratio	Lower	Upper	
216	100		
214	76.9	62.6	94.0
218	46.7	38.1	57.1



Abundance Ion 216.00 (215.70 to 216.70): E
Ion 214.00 (213.70 to 214.70): E
Ion 218.00 (217.70 to 218.70): E

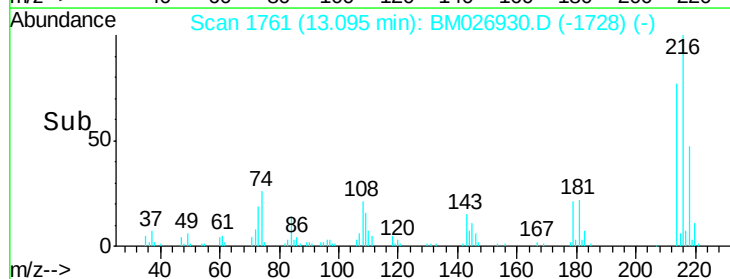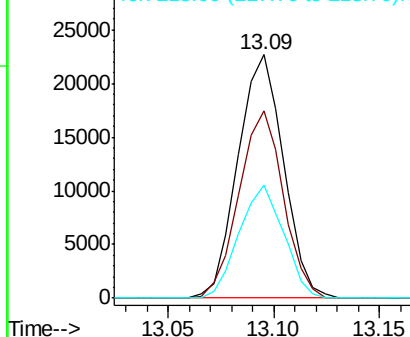







#74
 Pentachlorobenzene
 Concen: 7.098 ng/uL
 RT: 14.62 min Scan# 2021
 Delta R.T. -0.01 min
 Lab File: BM026930.D
 Acq: 29 Jul 2020 17:39

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-02

Tot Ion	Ratio	Lower	Upper
250	100		
248	64.0	49.6	74.4
252	61.6	51.7	77.5




Manual Integrations
 APPROVED


mohammad
 7/30/2020 3:32:41 PM

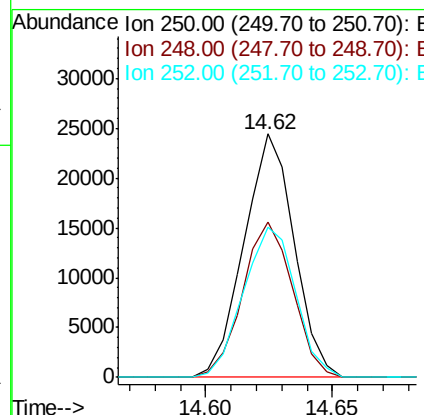

#75
 Carbazole
 Concen: 6.554 ng/uL
 RT: 17.44 min Scan# 2500
 Delta R.T. -0.01 min
 Lab File: BM026930.D
 Acq: 29 Jul 2020 17:39

Tgt Ion	Ratio	Lower	Upper
167	100		
166	21.4	17.1	25.7
139	13.4	10.1	15.1

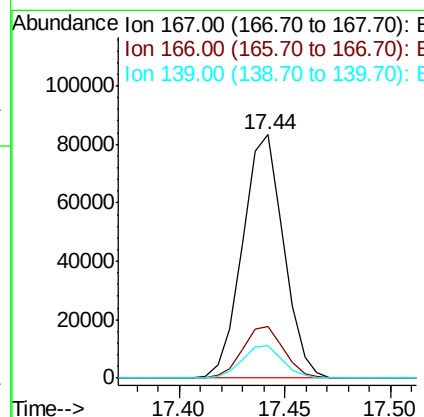

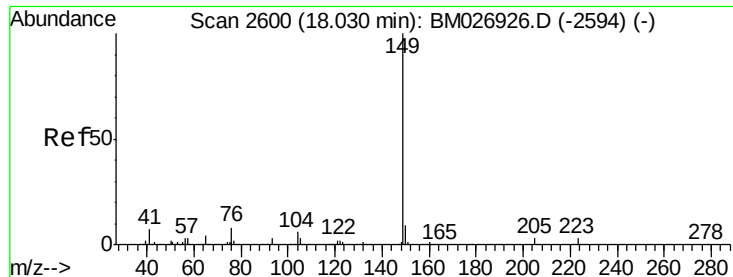





#76
Di-n-butylphthalate
Concen: 6.091 ng/ul
RT: 18.03 min Scan# 2600
Delta R.T. -0.01 min
Lab File: BM026930.D
Acq: 29 Jul 2020 17:39

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-02

Tot Ion:	149	Resp:	123187
Ion Ratio	Lower	Upper	
149	100		
150	9.2	7.6	11.4
104	6.7	4.7	7.1




Manual Integrations
APPROVED


mohammad
7/30/2020 3:32:41 PM

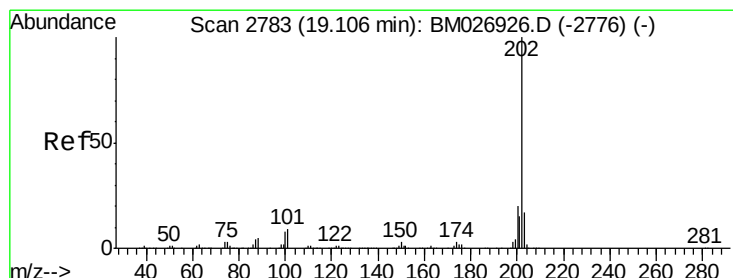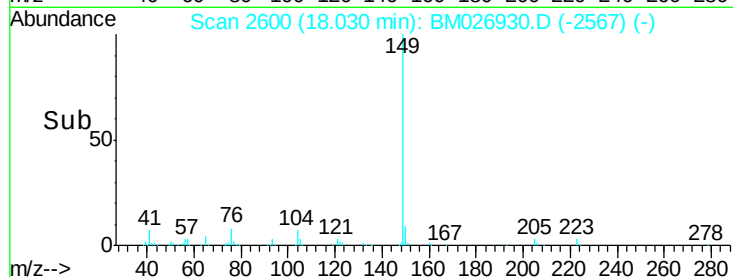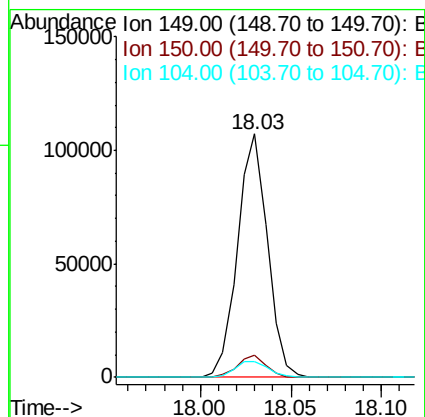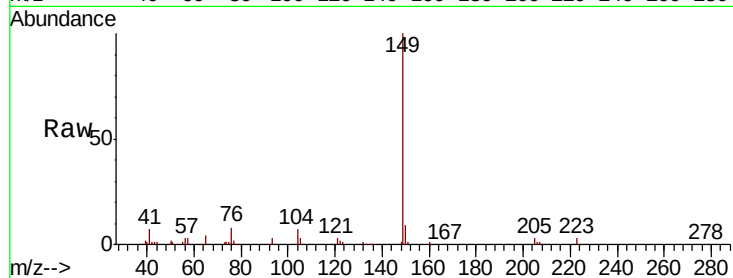

#77
Fluoranthene
Concen: 6.635 ng/ul
RT: 19.10 min Scan# 2782
Delta R.T. -0.01 min
Lab File: BM026930.D
Acq: 29 Jul 2020 17:39

Tgt Ion:	202	Resp:	148244
Ion Ratio	Lower	Upper	
202	100		
101	8.3	7.7	11.5
100	6.5	6.2	9.4

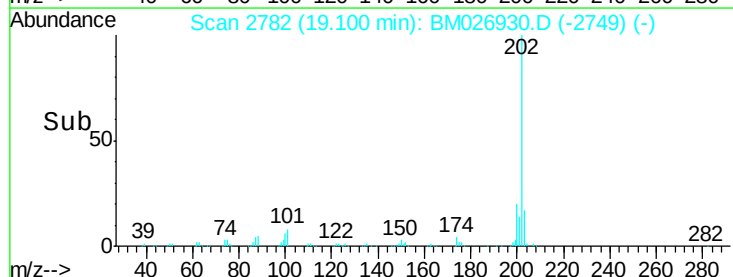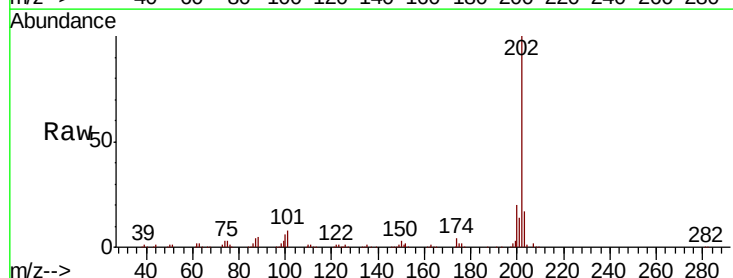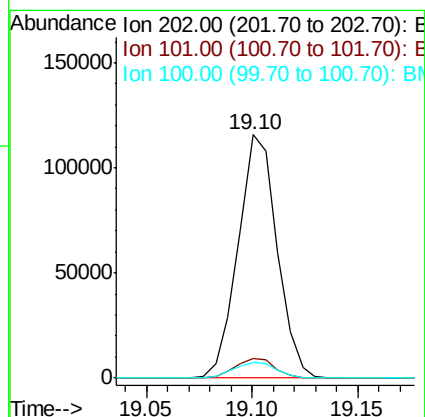







#80
Pvrene
Concen: 6.571 ng/ul
RT: 19.47 min Scan# 2844
Delta R.T. -0.01 min
Lab File: BM026930.D
Acq: 29 Jul 2020 17:39

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-02

Tot Ion	Ratio	Resp Lower	Upper
202	100		
101	9.4	9.4	14.2#
100	8.8	8.2	12.4




Manual Integrations
APPROVED


mohammad
7/30/2020 3:32:41 PM

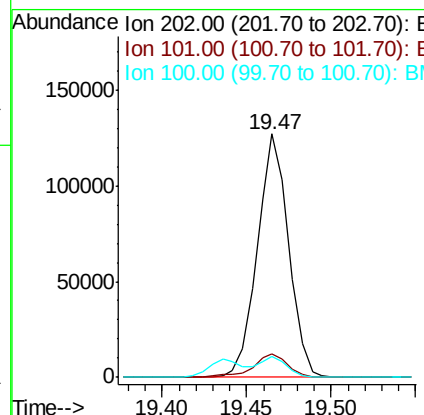

#81
Butylbenzylphthalate
Concen: 5.277 ng/ul
RT: 20.39 min Scan# 3001
Delta R.T. -0.01 min
Lab File: BM026930.D
Acq: 29 Jul 2020 17:39

Tgt Ion	Ratio	Resp Lower	Upper
149	100		
91	80.5	64.2	96.2
206	19.7	15.8	23.6

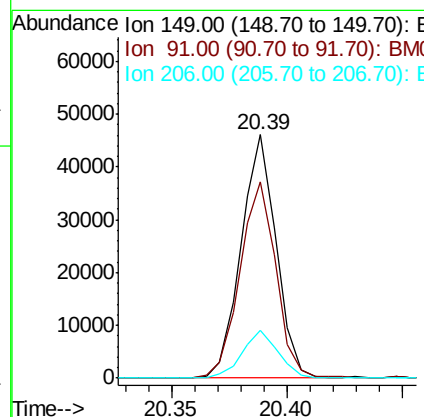



#82

3,3'-Dichlorobenzidine

Concen: 4.335 ng/ul

RT: 21.15 min Scan# 3131

Delta R.T. -0.01 min

Lab File: BM026930.D

Acq: 29 Jul 2020 17:39

Instrument :

BNA_M


ClientSampleId :

MDL-WATER-02




Tot Ion:	252	Resp:	35037
Ion Ratio	Lower	Upper	
252	100		
254	62.9	51.4	77.2
126	10.3	8.7	13.1

Manual Integrations
APPROVED

mohammad
7/30/2020 3:32:41 PM



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 254.00 (253.70 to 254.70): E
Ion 126.00 (125.70 to 126.70): E

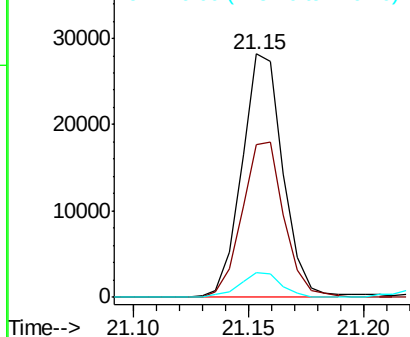

#83

Benzo(a)anthracene

Concen: 6.728 ng/ul


RT: 21.22 min Scan# 3142

Delta R.T. -0.01 min



Lab File: BM026930.D


Acq: 29 Jul 2020 17:39

Tgt Ion:	228	Resp:	158534
Ion Ratio	Lower	Upper	
228	100		
229	19.2	15.4	23.2
226	26.5	20.9	31.3



Abundance Ion 228.00 (227.70 to 228.70): E
Ion 229.00 (228.70 to 229.70): E
Ion 226.00 (225.70 to 226.70): E

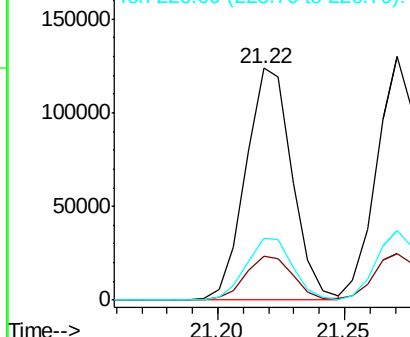







#84
 Bis(2-ethylhexyl)phthalate
 Concen: 5.550 ng/ul
 RT: 21.18 min Scan# 3136
 Delta R.T. -0.01 min
 Lab File: BM026930.D
 Acq: 29 Jul 2020 17:39

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-02

Tot Ion	Ratio	Lower	Upper
149	100		
167	26.5	20.6	31.0
279	4.3	3.0	4.6




Manual Integrations
 APPROVED


mohammad
 7/30/2020 3:32:41 PM

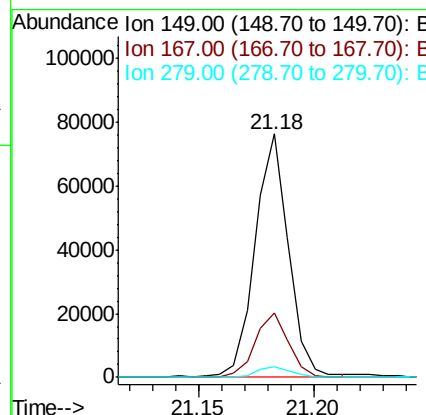

#85
 Chrysene
 Concen: 6.780 ng/ul
 RT: 21.27 min Scan# 3151
 Delta R.T. -0.01 min
 Lab File: BM026930.D
 Acq: 29 Jul 2020 17:39

Tgt Ion	Ratio	Lower	Upper
228	100		
226	28.5	23.2	34.8
229	19.1	15.5	23.3

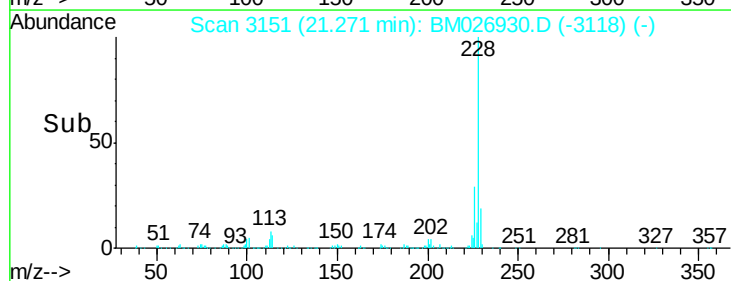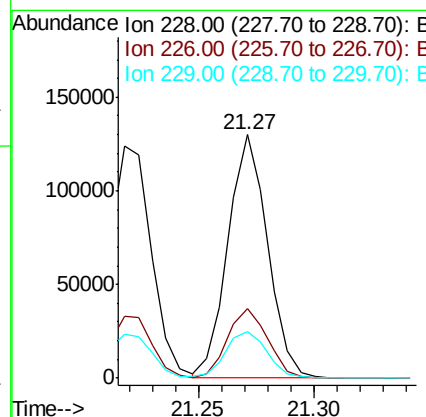

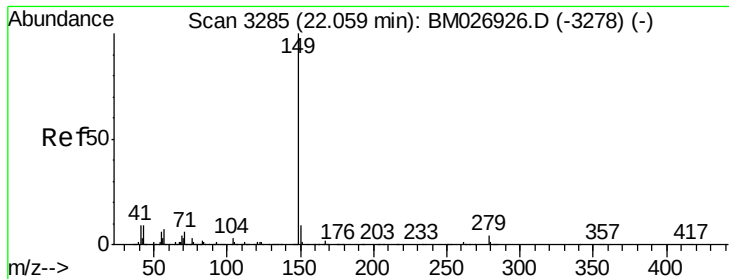





#87
Di-n-octyl phthalate
Concen: 4.757 ng/ul
RT: 22.05 min Scan# 3284
Delta R.T. -0.01 min
Lab File: BM026930.D
Acq: 29 Jul 2020 17:39

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-02

Tgt Ion:149 Resp: 125203




Manual Integrations
APPROVED


mohammad
7/30/2020 3:32:41 PM

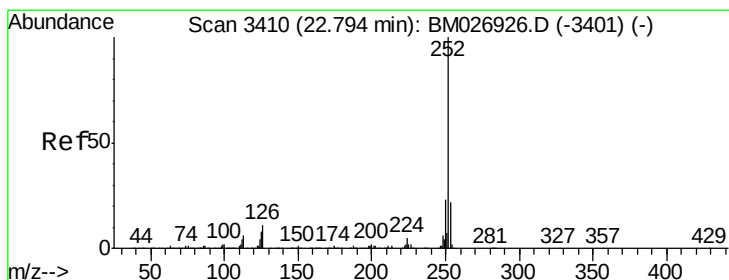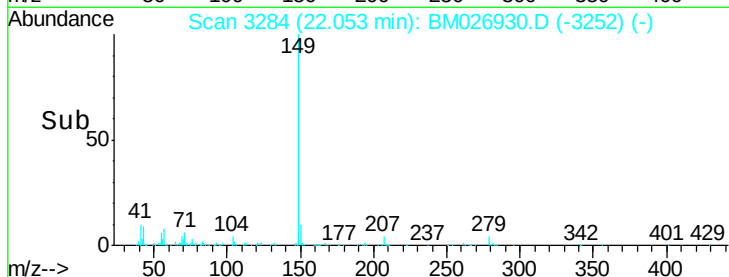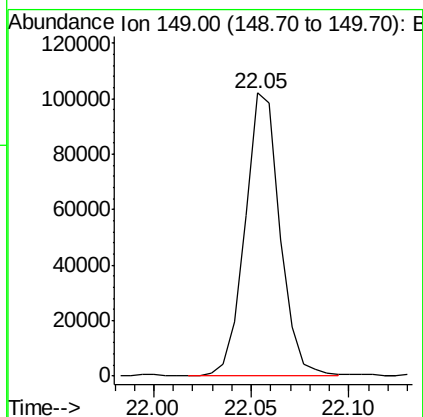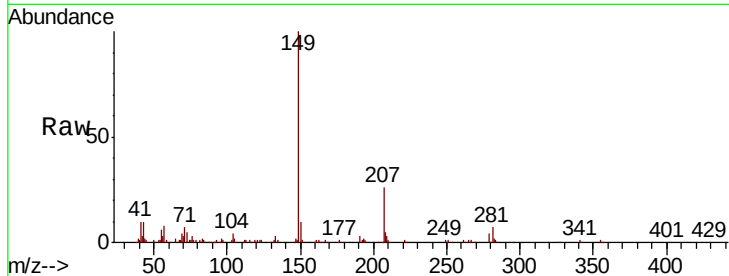

#88
Benzo(b)fluoranthene
Concen: 6.293 ng/ul
RT: 22.79 min Scan# 3409
Delta R.T. -0.01 min
Lab File: BM026930.D
Acq: 29 Jul 2020 17:39

Tgt Ion:252 Resp: 161258
Ion Ratio Lower Upper
252 100
253 22.4 17.6 26.4
125 7.2 6.6 10.0

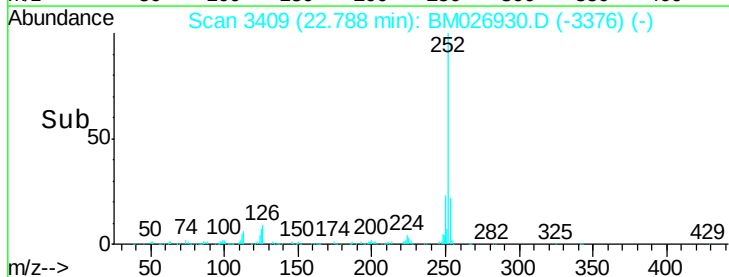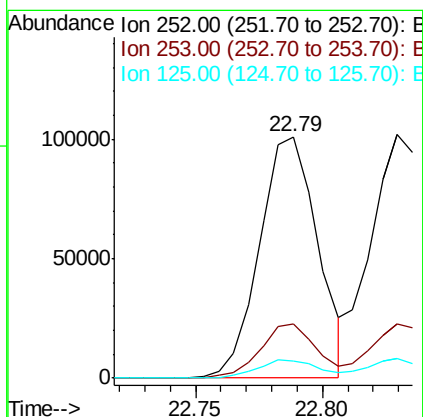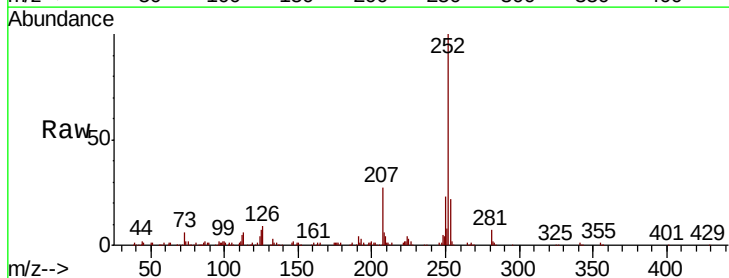




#89
Benzo(k)fluoranthene
Concen: 6.753 ng/ul
RT: 22.83 min Scan# 3416
Delta R.T. -0.01 min
Lab File: BM026930.D
Acq: 29 Jul 2020 17:39

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-02

Tot Ion	Ratio	Lower	Upper
252	100		
253	22.1	17.4	26.2
125	8.2	7.3	10.9

Manual Integrations
APPROVED

mohammad
7/30/2020 3:32:41 PM






Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

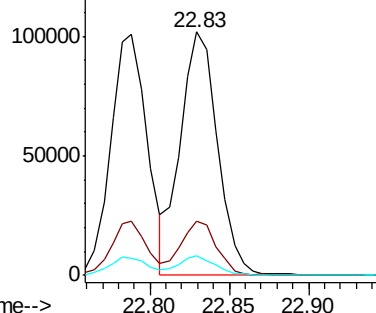

#91
Benzo(a)pyrene
Concen: 6.779 ng/ul
RT: 23.35 min Scan# 3505
Delta R.T. -0.01 min
Lab File: BM026930.D
Acq: 29 Jul 2020 17:39




Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.1	17.7	26.5
125	8.6	8.2	12.2


Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

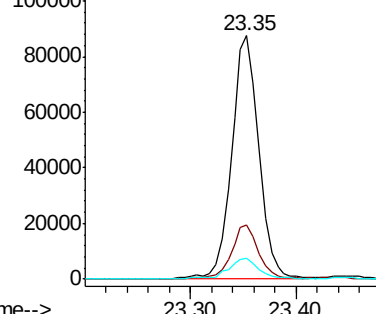

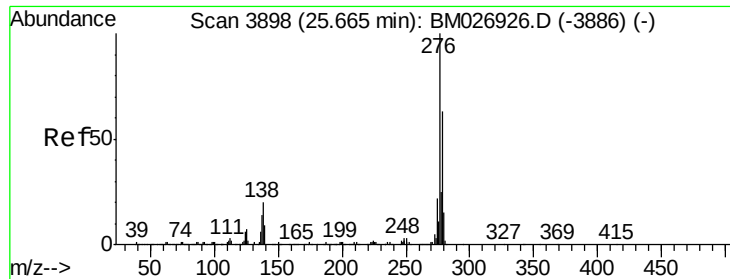





#92
Indeno(1,2,3-cd)pyrene
Concen: 6.832 ng/ul
RT: 25.66 min Scan# 3898
Delta R.T. -0.01 min
Lab File: BM026930.D
Acq: 29 Jul 2020 17:39

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-02

Tot Ion	Ratio	Lower	Upper
276	100		
138	19.8	17.0	25.4
277	24.8	20.6	30.8




Manual Integrations
APPROVED


mohammad
7/30/2020 3:32:41 PM

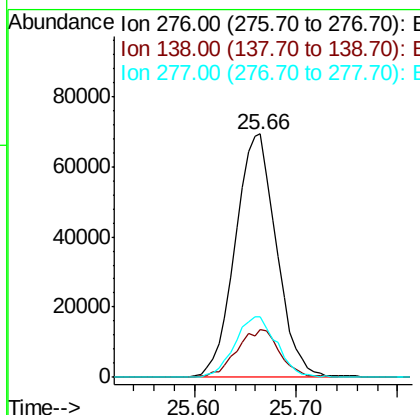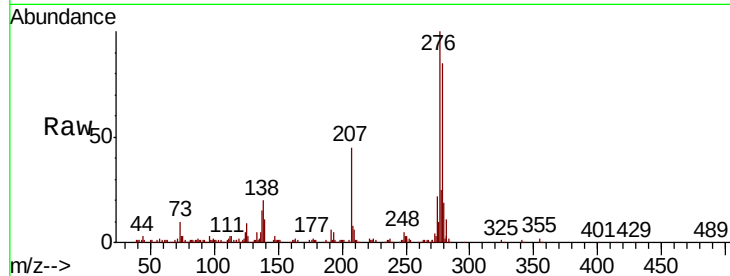

#93
Dibenzo(a,h)anthracene
Concen: 6.900 ng/ul
RT: 25.67 min Scan# 3899
Delta R.T. -0.01 min
Lab File: BM026930.D
Acq: 29 Jul 2020 17:39

Tgt Ion	Ratio	Lower	Upper
278	100		
139	11.6	10.9	16.3
279	23.1	19.4	29.2

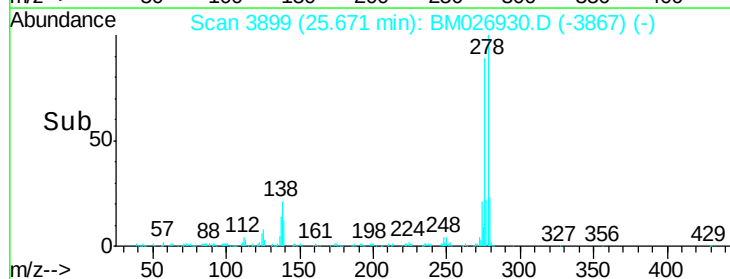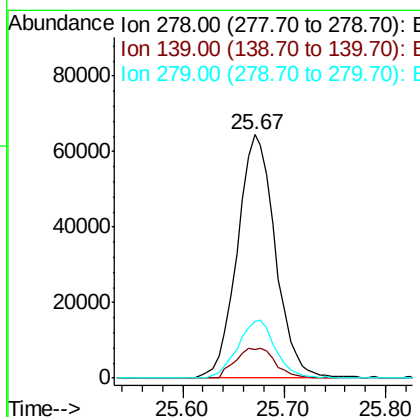



#94
 Benzo(a,h,i)perylene
 Concen: 6.955 ng/ul
 RT: 26.33 min Scan# 4011
 Delta R.T. -0.02 min
 Lab File: BM026930.D
 Acq: 29 Jul 2020 17:39

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-02

Tot Ion:	276	Resp:	164967
Ion Ratio	Lower	Upper	
276	100		
138	17.6	14.9	22.3
277	22.7	19.1	28.7

Manual Integrations
 APPROVED

mohammad
 7/30/2020 3:32:41 PM

