
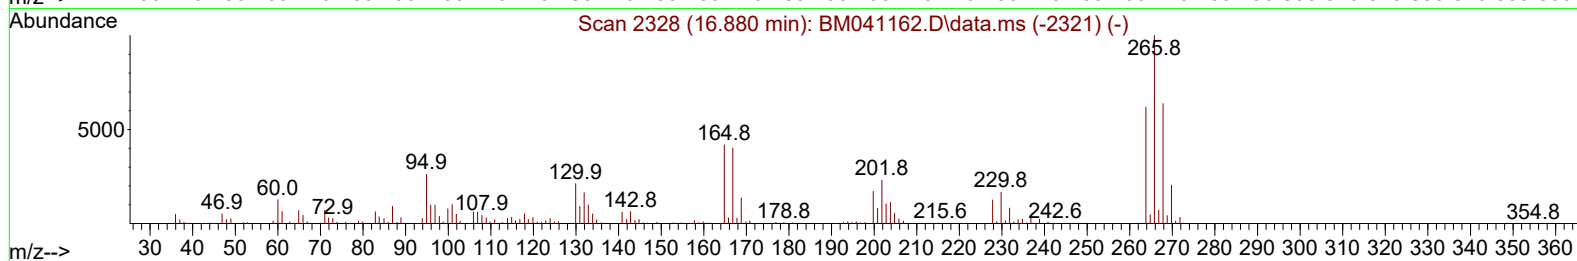
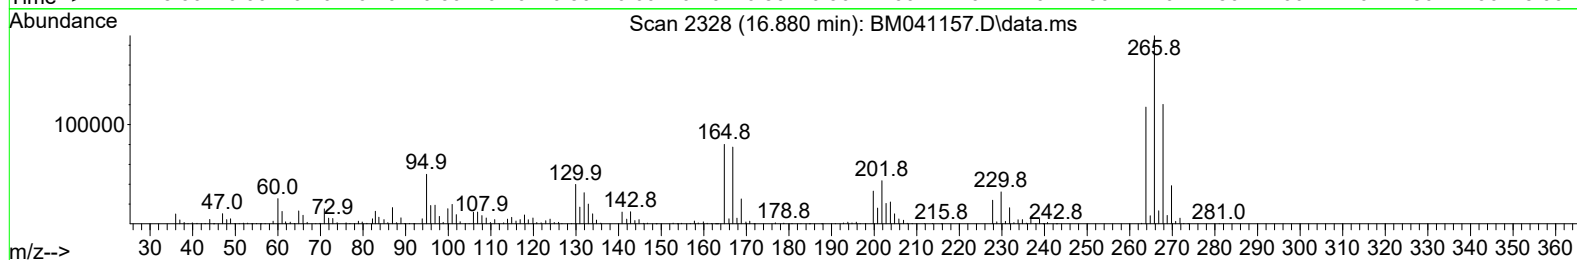


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072823\
Data File : BM041157.D
Acq On : 28 Jul 2023 09:37
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 04:31:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 29 00:19:24 2023
Response via : Initial Calibration

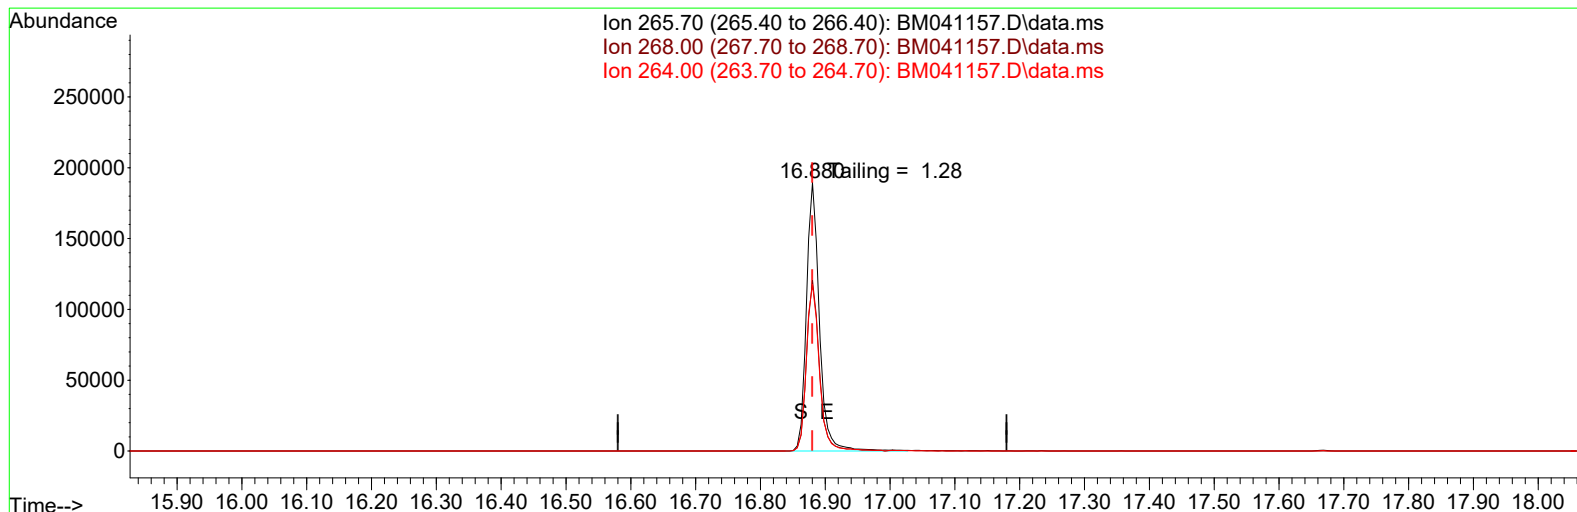

TIC: BM041157.D\data.ms

(70) Pentachlorophenol (C)




16.880min (+ 0.000) 0.00 ng

response 264374

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.49
264.00	61.80	62.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072823\
 Data File : BM041157.D
 Acq On : 28 Jul 2023 09:37
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 04:31:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 29 00:19:24 2023
 Response via : Initial Calibration

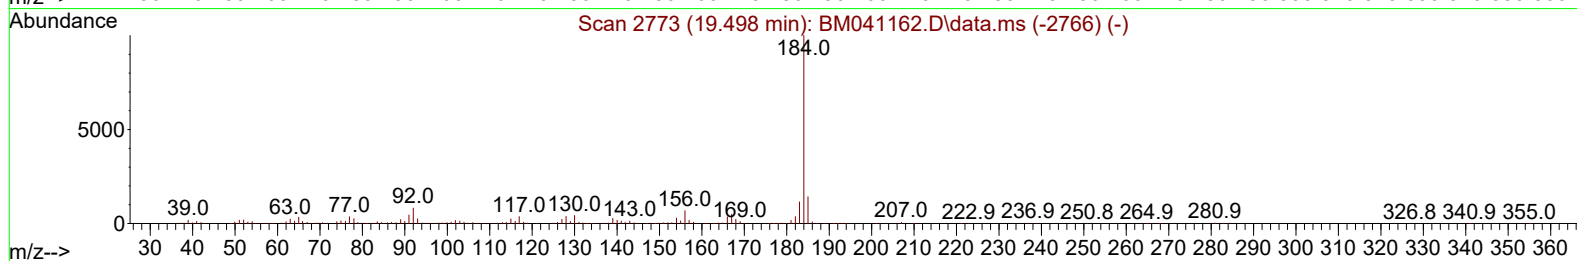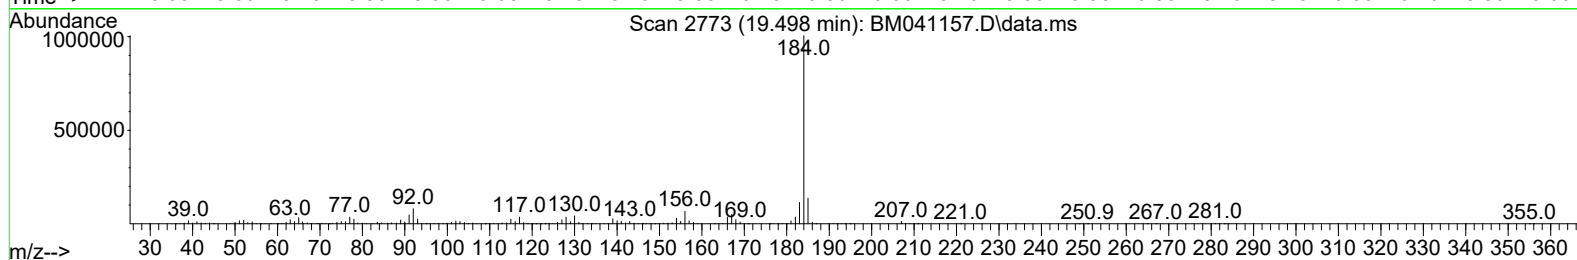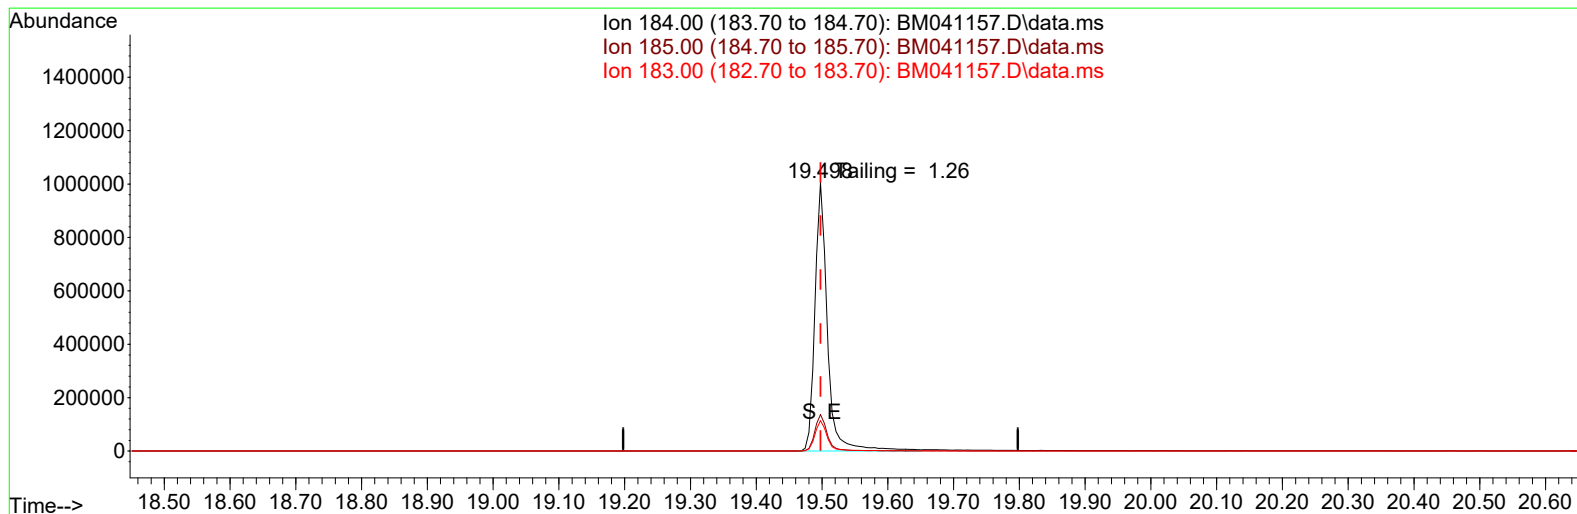

TIC: BM041157.D\data.ms

(77) Benzidine

19.498min (-0.000) 0.00 ng

response 1327248

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.60
183.00	11.50	11.35
0.00	0.00	0.00