
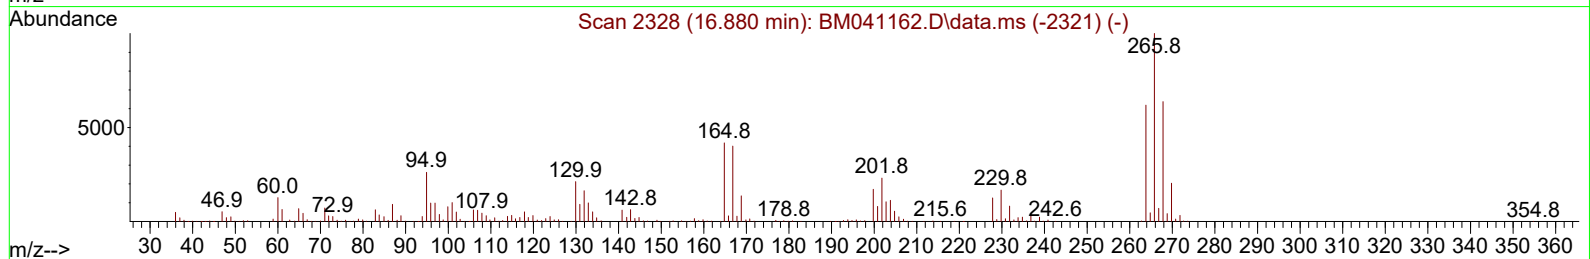
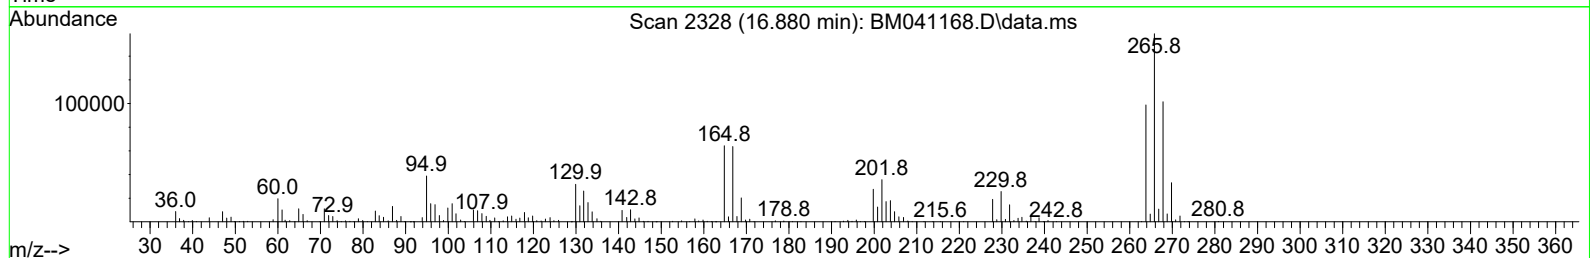


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072823\
Data File : BM041168.D
Acq On : 28 Jul 2023 16:33
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 04:32:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 29 00:19:24 2023
Response via : Initial Calibration

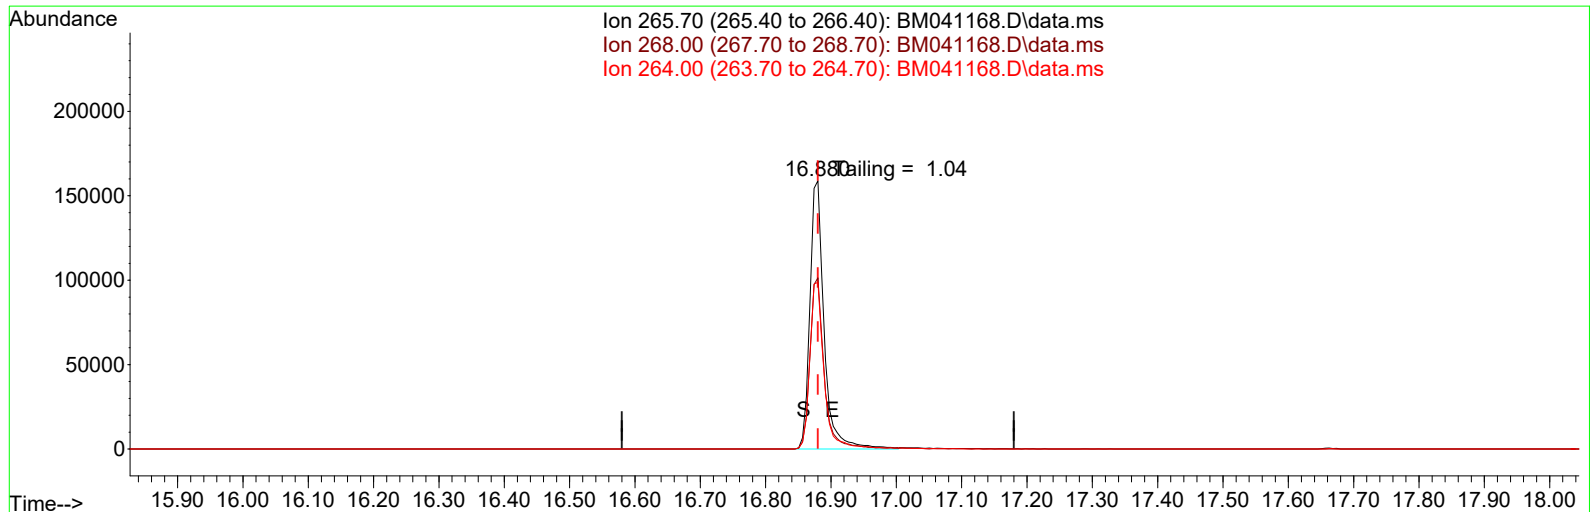

TIC: BM041168.D\data.ms

(70) Pentachlorophenol (C)




16.880min (-0.000) 0.00 ng

response 242566

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.83
264.00	61.80	62.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072823\
Data File : BM041168.D
Acq On : 28 Jul 2023 16:33
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 04:32:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 29 00:19:24 2023
Response via : Initial Calibration

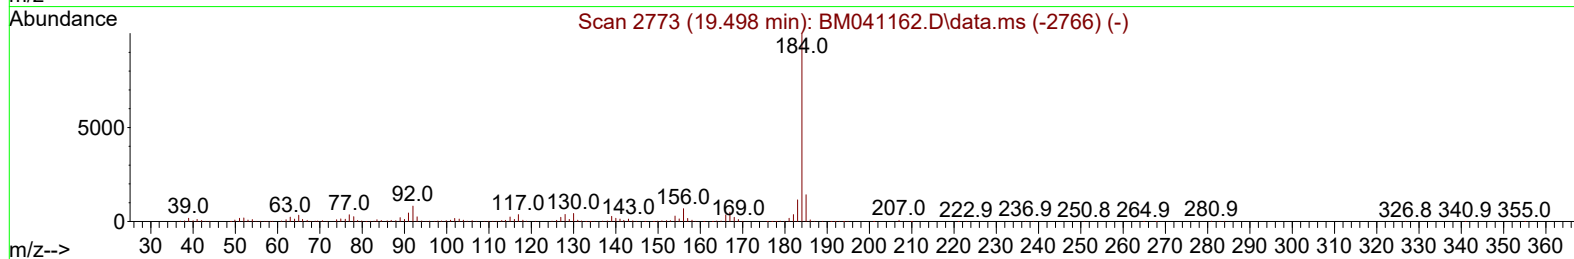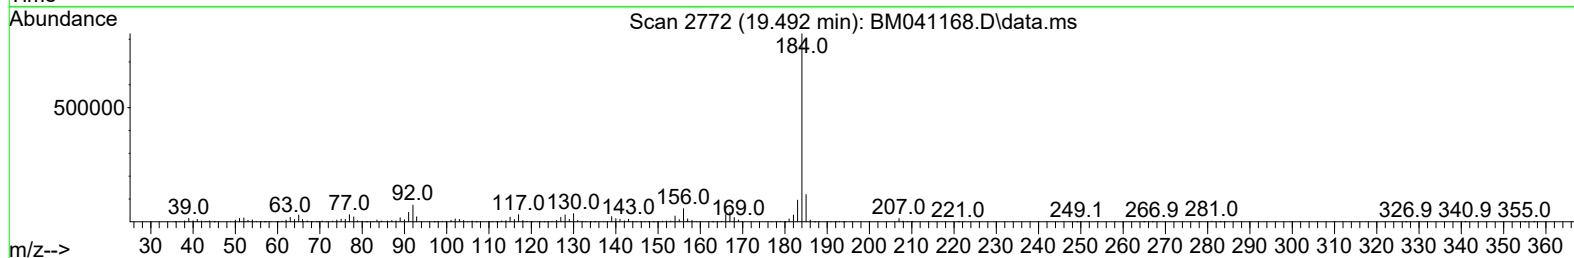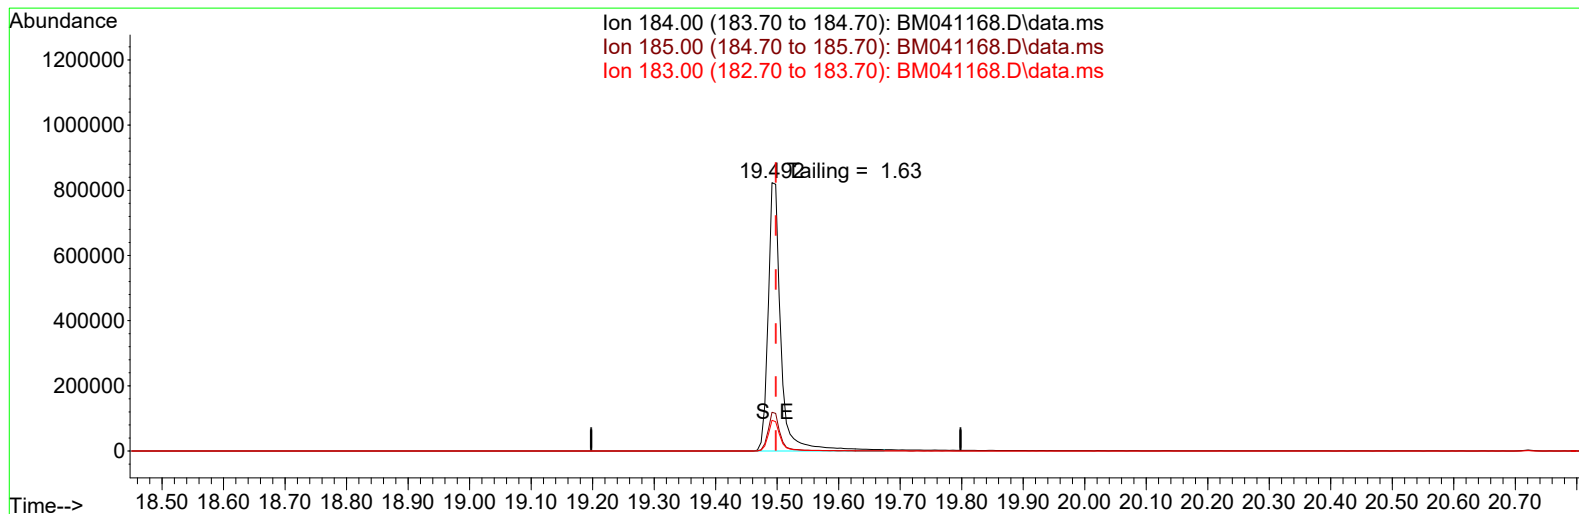

TIC: BM041168.D\data.ms

(77) Benzidine**19.492min (-0.006) 1371060.88 ng****response 1214682**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.46
183.00	11.50	11.47
0.00	0.00	0.00