

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072823\
 Data File : BM041170.D
 Acq On : 28 Jul 2023 17:49
 Operator : MA/JU
 Sample : PB154028BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB154028BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM041170.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.916	290	294	302	rBV	97426	138649	1.51%	0.291%
2	5.375	365	372	396	rBV	4542328	6296231	68.53%	13.224%
3	6.981	638	645	666	rBV	3960036	6283057	68.39%	13.197%
4	7.804	778	785	798	rBV	650253	1021594	11.12%	2.146%
5	8.981	977	985	1002	rBV	2280736	3806978	41.44%	7.996%
6	10.616	1255	1263	1283	rBV	739802	1302519	14.18%	2.736%
7	13.092	1676	1684	1699	rBV	5489561	7951232	86.54%	16.701%
8	14.469	1909	1918	1936	rBV	1011291	1515149	16.49%	3.182%
9	15.968	2166	2173	2186	rBV	3940775	5461642	59.45%	11.472%
10	17.227	2381	2387	2405	rBV	1110977	1599426	17.41%	3.359%
11	17.515	2430	2436	2448	rBV2	78368	123827	1.35%	0.260%
12	19.868	2830	2836	2849	rBV	7892181	9187635	100.00%	19.298%
13	21.433	3097	3102	3109	rBV	1059152	1453513	15.82%	3.053%
14	23.803	3499	3505	3518	rVB	753603	1469016	15.99%	3.085%




Sum of corrected areas: 47610468

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072823\
Data File : BM041170.D
Acq On : 28 Jul 2023 17:49
Operator : MA/JU
Sample : PB154028BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB154028BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

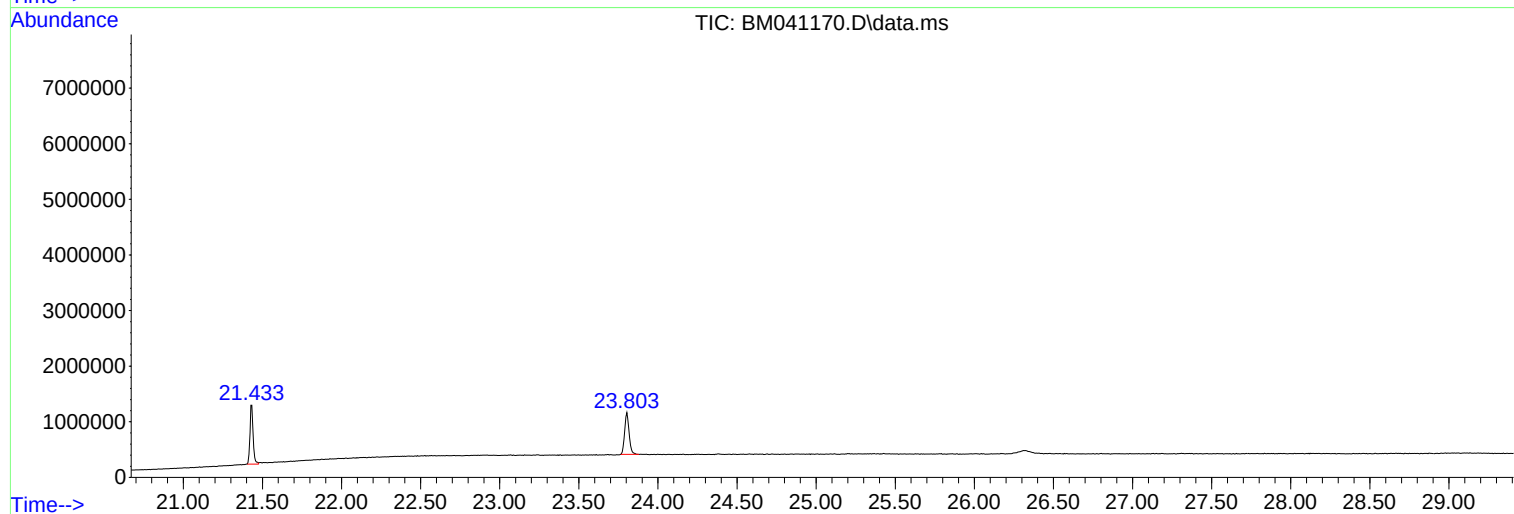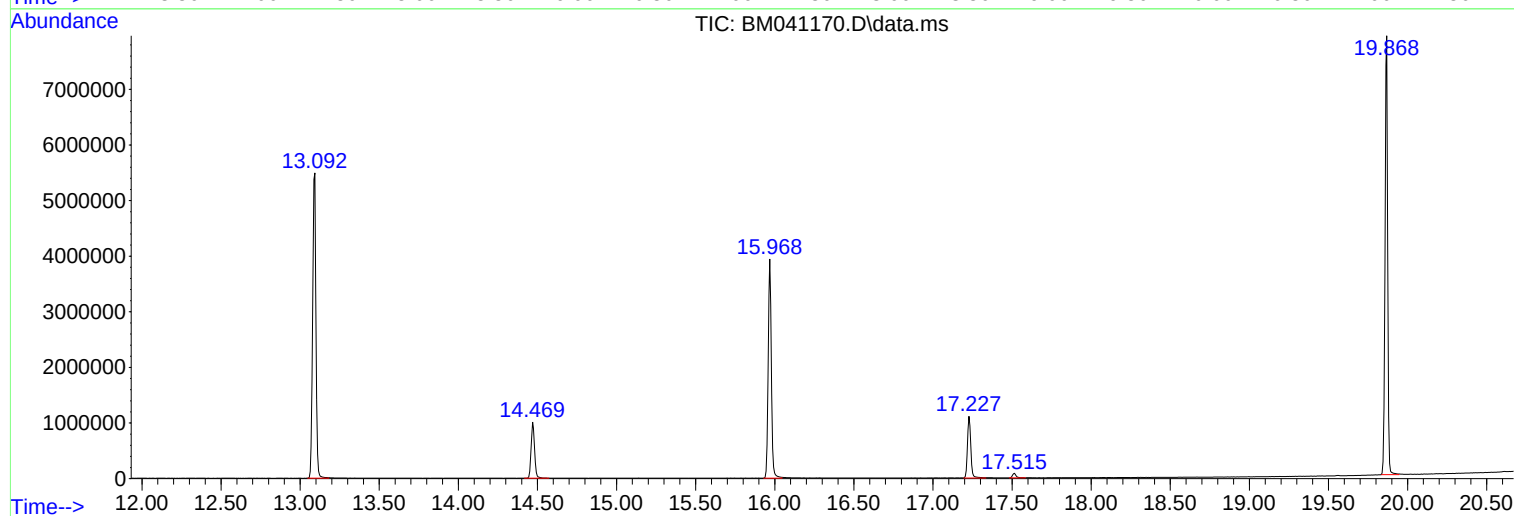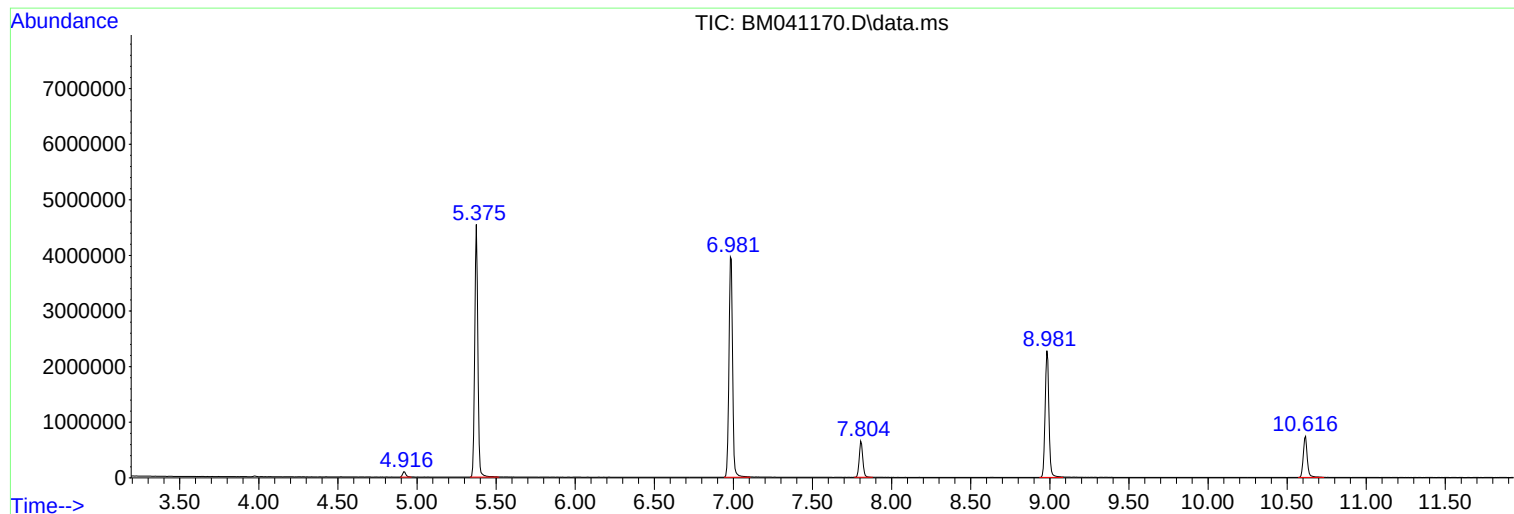

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072823\
Data File : BM041170.D
Acq On : 28 Jul 2023 17:49
Operator : MA/JU
Sample : PB154028BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB154028BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.916	2.71 ng	138649	1,4-Dichlorobenzene-d4	7.804

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23		
3	Propane, 2-ethoxy-2-methyl-	102	C6H14O	000637-92-3	17		
4	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
5	4-Penten-2-one, 4-methyl-	98	C6H10O	003744-02-3	9		

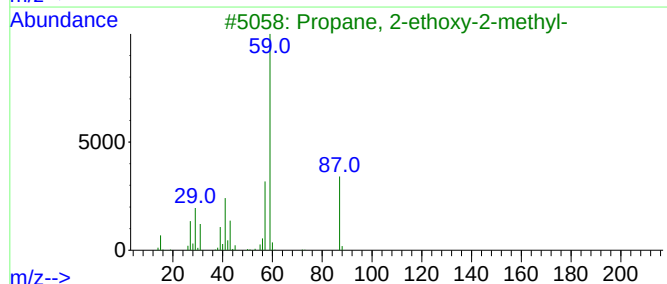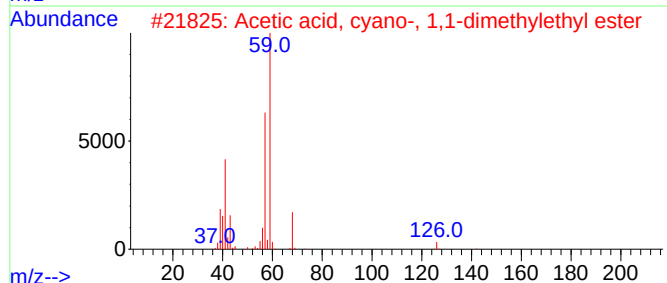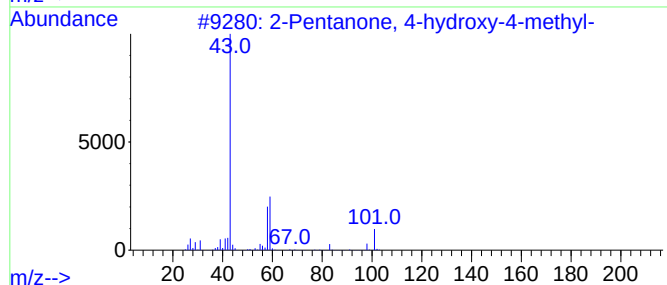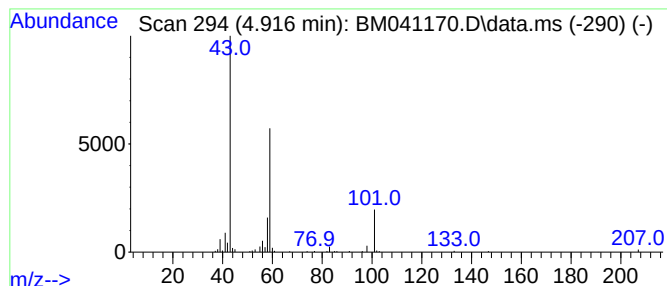

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072823\
Data File : BM041170.D
Acq On : 28 Jul 2023 17:49
Operator : MA/JU
Sample : PB154028BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB154028BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.916	2.7	ng	138649	1	7.804	1021590	20.0