

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
 Data File : BM046926.D
 Acq On : 30 Jul 2024 19:24
 Operator : MA/JU
 Sample : P3336-17
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F7E45

Quant Time: Jul 31 00:00:56 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 04:18:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.447	152	2201	0.400	ng/ul	0.00
4) Naphthalene-d8	10.205	136	6153	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.095	164	4059	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.854	188	8720	0.400	ng/ul	0.00
17) Chrysene-d12	21.067	240	5776	0.400	ng/ul	0.00
23) Perylene-d12	23.188	264	6832	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.084	96	6092	3.953	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.800	152	2495	0.255	ng/ul	-0.01
18) Fluoranthene-d10	18.895	212	5078	0.270	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.262	202	912	0.035	ng/ul#	1
26) Benzo(a)pyrene	23.054	252	1466	0.068	ng/ul#	28


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
Data File : BM046926.D
Acq On : 30 Jul 2024 19:24
Operator : MA/JU
Sample : P3336-17
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7E45

Quant Time: Jul 31 00:00:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 04:18:24 2024
Response via : Initial Calibration

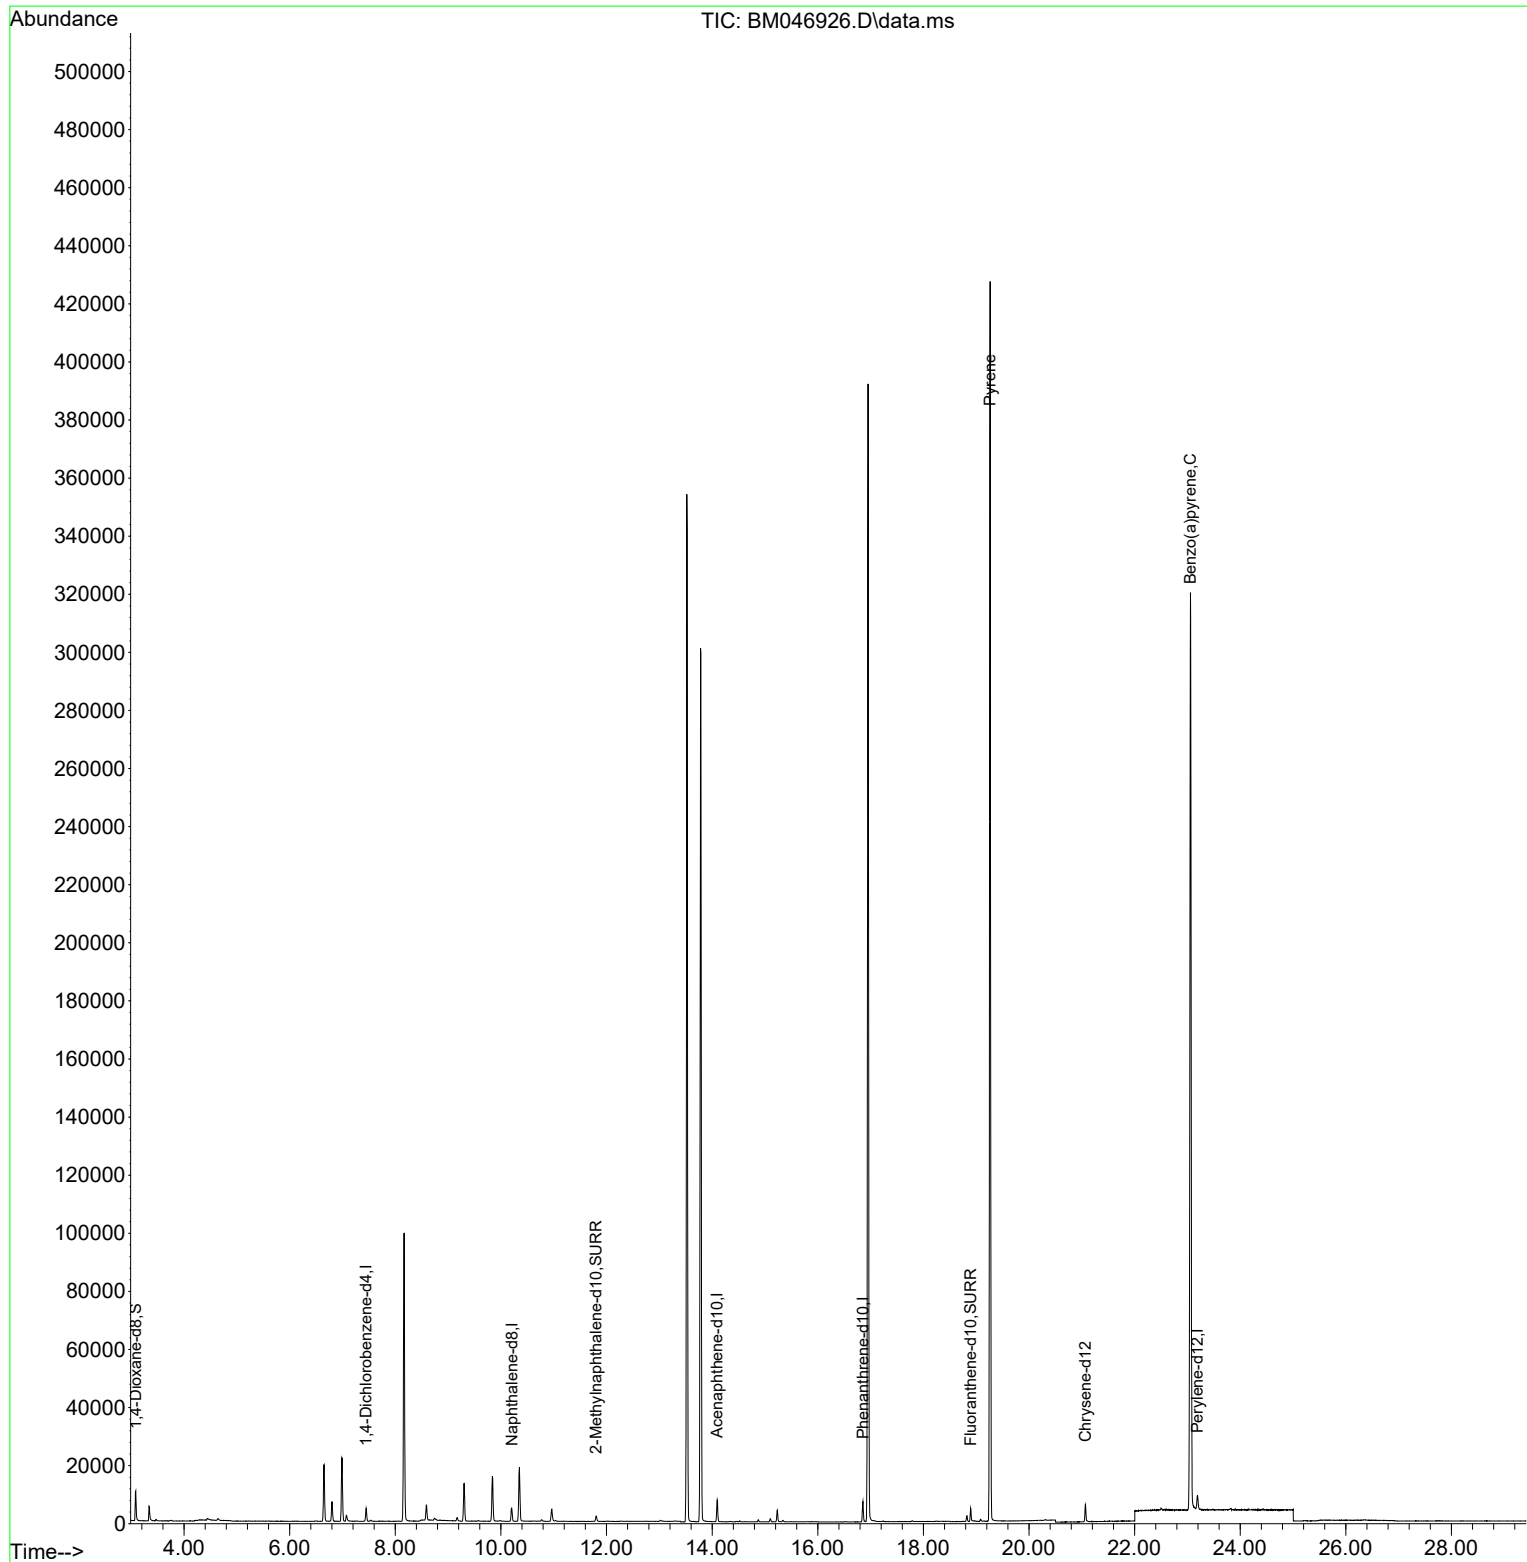

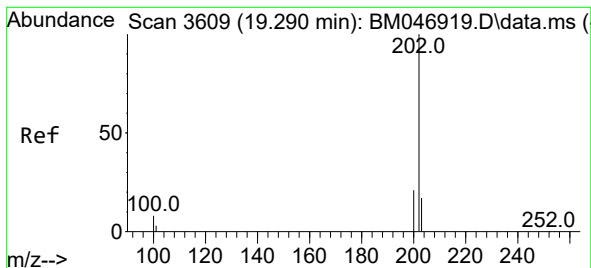

#20

Pyrene

Concen: 0.035 ng/ul

RT: 19.262 min Scan# 3

Delta R.T. -0.033 min

Lab File: BM046926.D

Acq: 30 Jul 2024 19:24

Instrument :

BNA_M

ClientSampleId :

F7E45





Tgt Ion:202 Resp: 912

Ion Ratio Lower Upper

202 100

101 157.5 5.2 7.8#

100 1204.9 4.3 6.5#

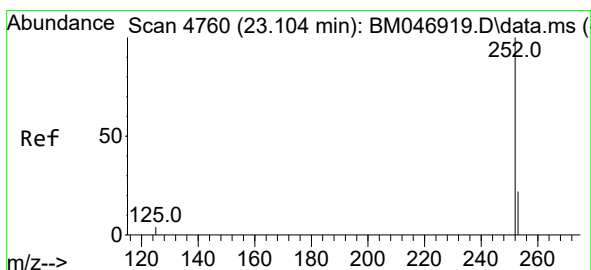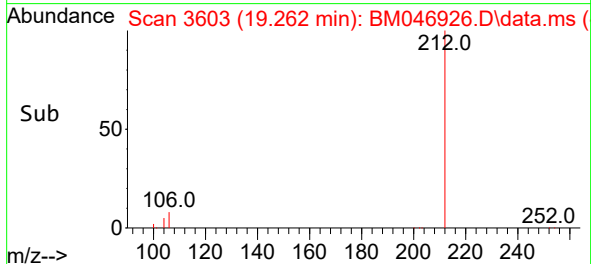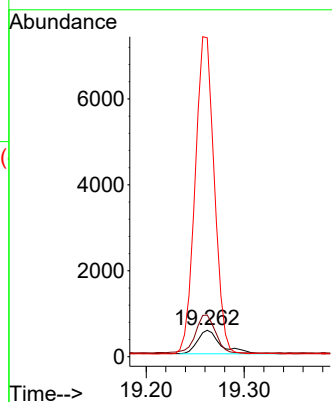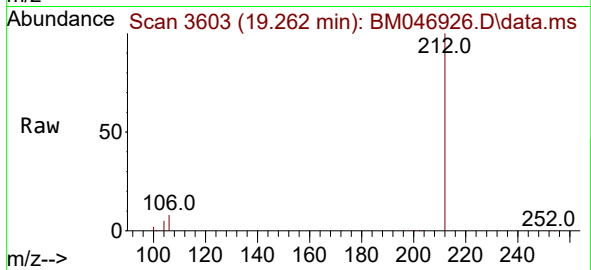

#26

Benzo(a)pyrene

Concen: 0.068 ng/ul

RT: 23.054 min Scan# 4743

Delta R.T. -0.050 min

Lab File: BM046926.D

Acq: 30 Jul 2024 19:24

Tgt Ion:252 Resp: 1466

Ion Ratio Lower Upper

252 100

253 70.9 26.0 39.0#

125 41.3 7.8 11.8#

