

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
 Data File : BM046931.D
 Acq On : 30 Jul 2024 22:28
 Operator : MA/JU
 Sample : P3336-13
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F7E41

Quant Time: Jul 31 00:01:45 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 04:18:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.447	152	3529	0.400	ng/ul	0.00
4) Naphthalene-d8	10.200	136	6002	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.095	164	4267	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-16.86
17) Chrysene-d12	21.067	240	6112	0.400	ng/ul	0.00
23) Perylene-d12	23.189	264	7152	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.084	96	10369	4.196	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.800	152	4222	0.443	ng/ul	-0.01
18) Fluoranthene-d10	18.895	212	9303	0.467	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.262	202	1634	0.059	ng/ul#	1
26) Benzo(a)pyrene	23.054	252	2545	0.113	ng/ul#	53


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
Data File : BM046931.D
Acq On : 30 Jul 2024 22:28
Operator : MA/JU
Sample : P3336-13
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7E41

Quant Time: Jul 31 00:01:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 04:18:24 2024
Response via : Initial Calibration

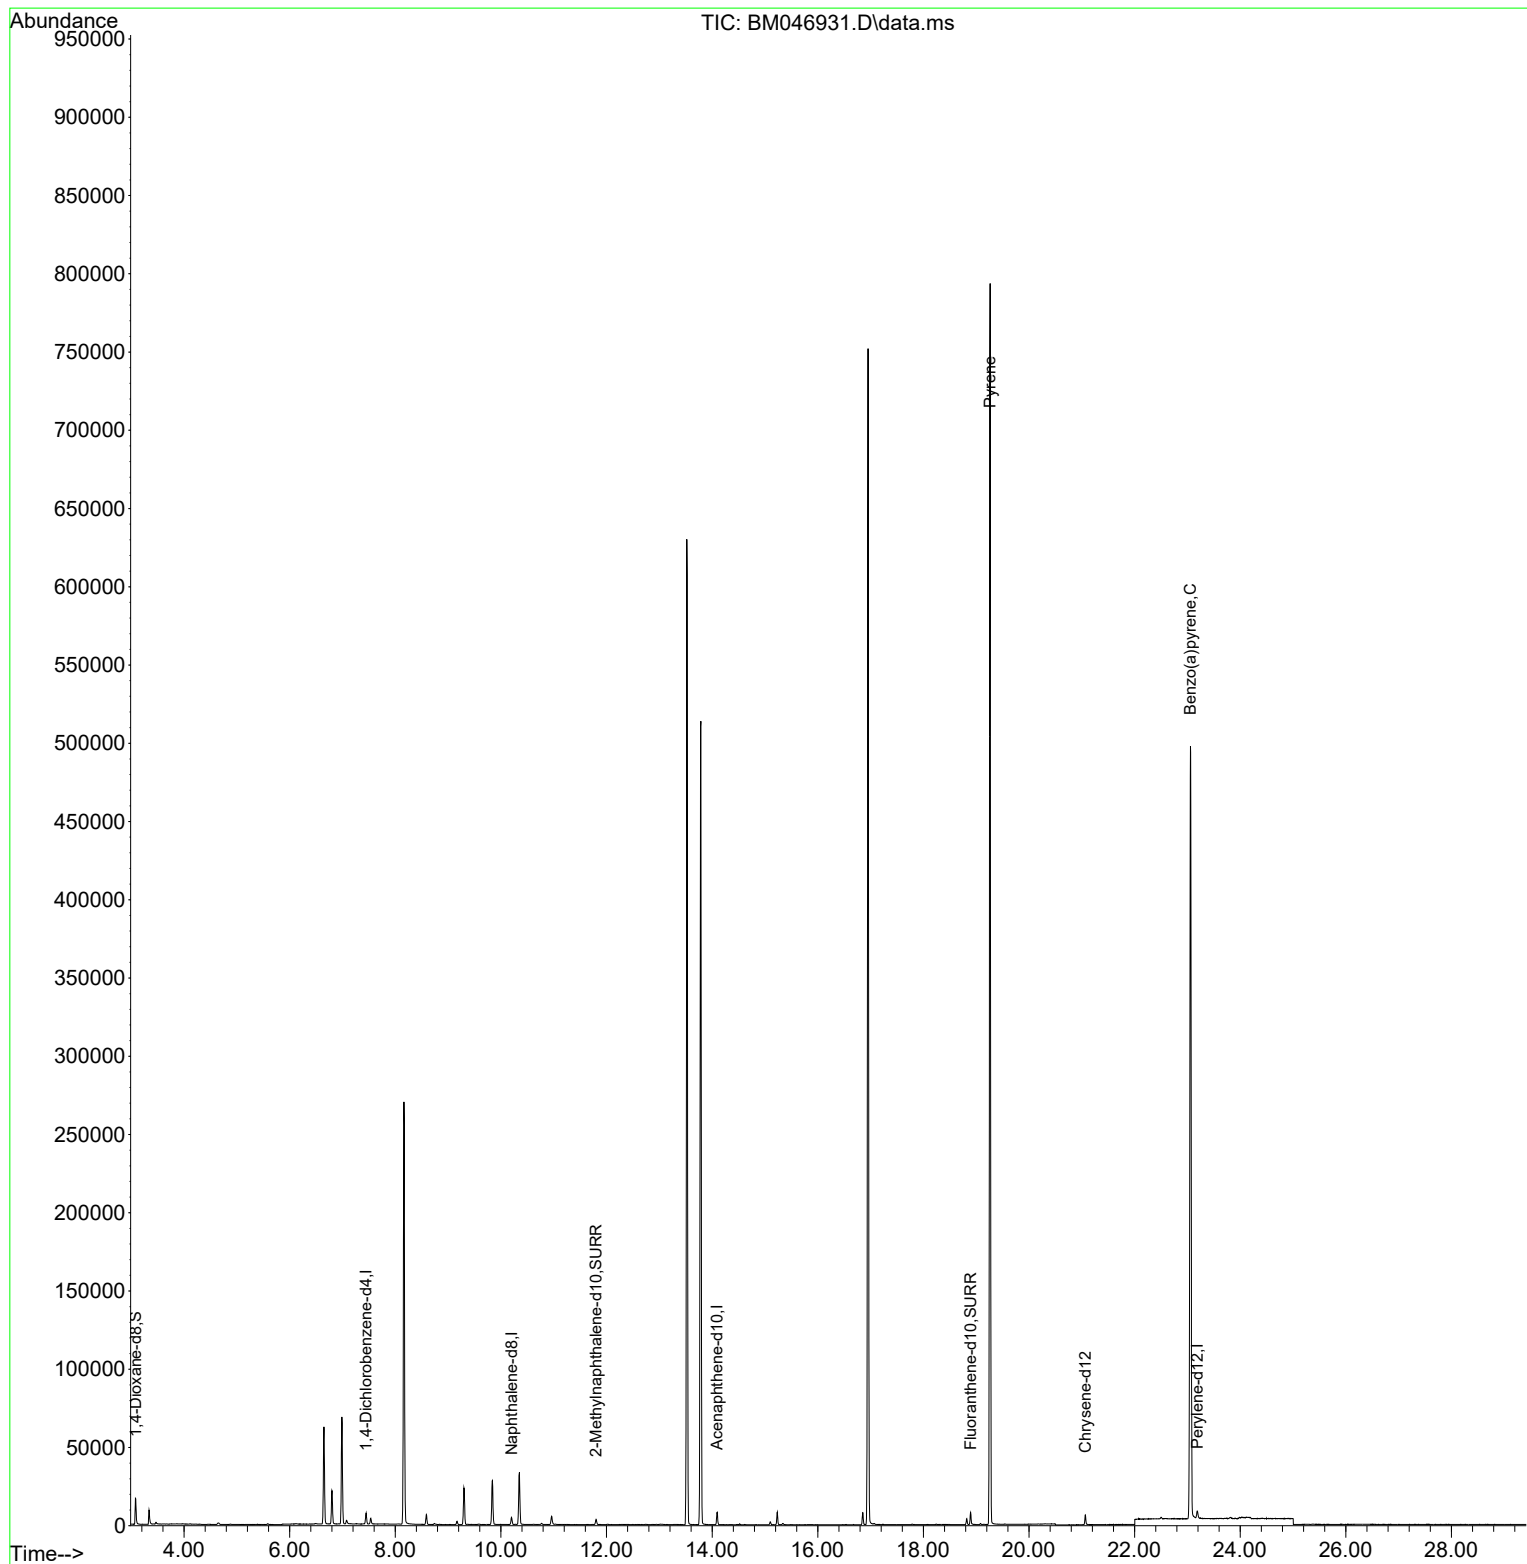

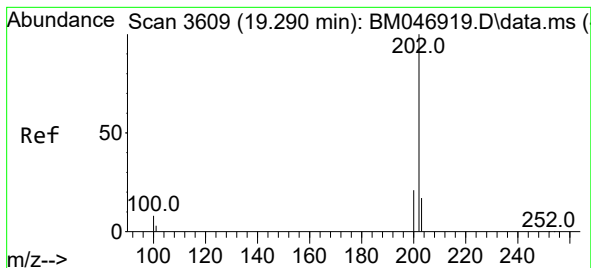

#20

Pyrene

Concen: 0.059 ng/ul

RT: 19.262 min Scan# 3

Delta R.T. -0.033 min

Lab File: BM046931.D

Acq: 30 Jul 2024 22:28

Instrument :

BNA_M

ClientSampleId :

F7E41





Tgt Ion:202 Resp: 1634

Ion Ratio Lower Upper

202 100

101 153.8 5.2 7.8#

100 1250.0 4.3 6.5#

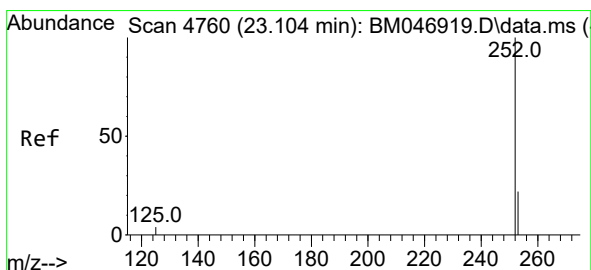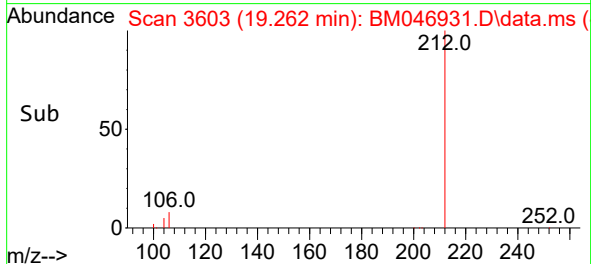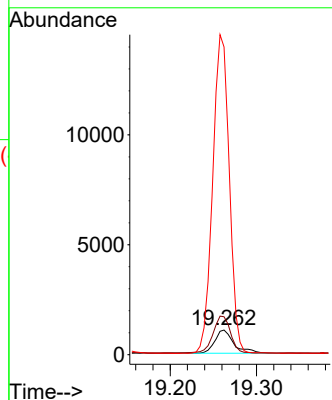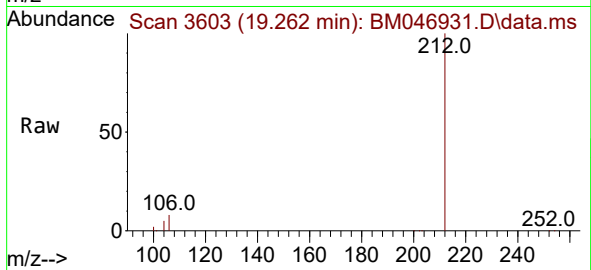

#26

Benzo(a)pyrene

Concen: 0.113 ng/ul

RT: 23.054 min Scan# 4743

Delta R.T. -0.050 min

Lab File: BM046931.D

Acq: 30 Jul 2024 22:28

Tgt Ion:252 Resp: 2545

Ion Ratio Lower Upper

252 100

253 55.1 26.0 39.0#

125 34.7 7.8 11.8#

