




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
Data File : BM046892.D
Acq On : 29 Jul 2024 20:23
Operator : MA/JU
Sample : P3336-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7E87

Manual IntegrationsAPPROVED

Quant Time: Jul 30 00:02:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 24 15:10:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/30/2024
Supervised By :mohammad ahmed 08/03/2024

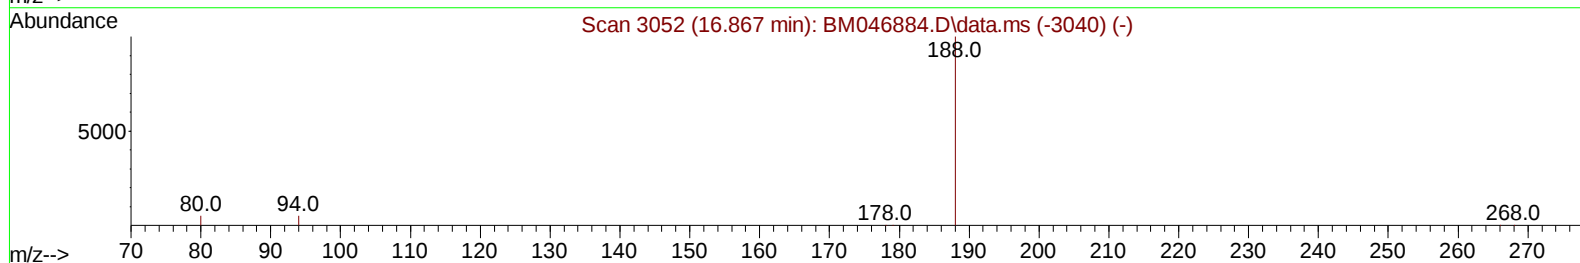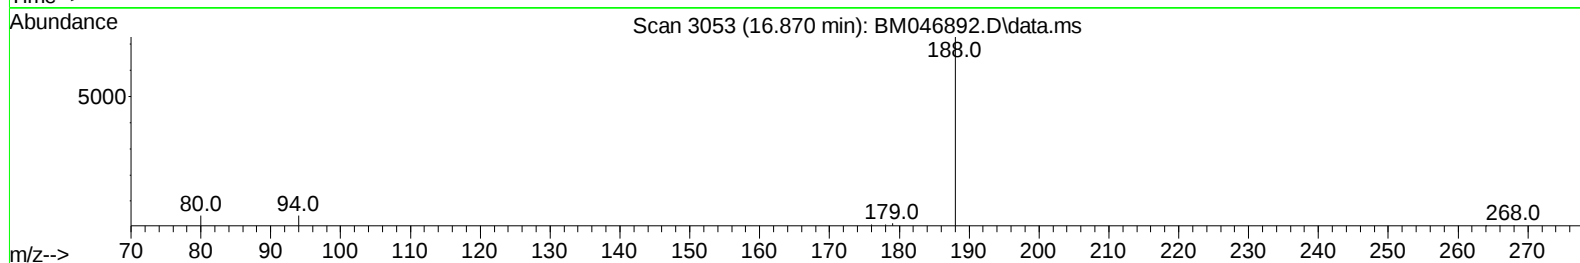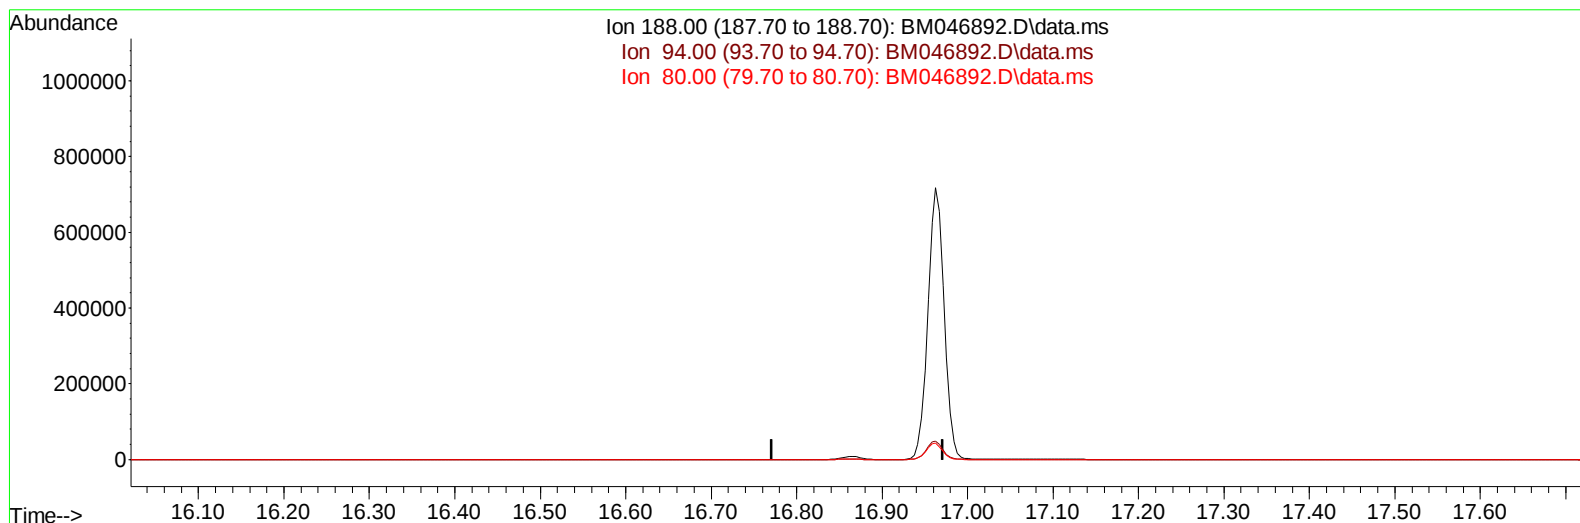

TIC: BM046892.D\data.ms

(13) Phenanthrene-d10 (I)

16.871min (-16.871) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	6.60	0.00#
80.00	6.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
Data File : BM046892.D
Acq On : 29 Jul 2024 20:23
Operator : MA/JU
Sample : P3336-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7E87

Manual IntegrationsAPPROVED

Quant Time: Jul 30 00:02:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 24 15:10:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/30/2024
Supervised By :mohammad ahmed 08/03/2024

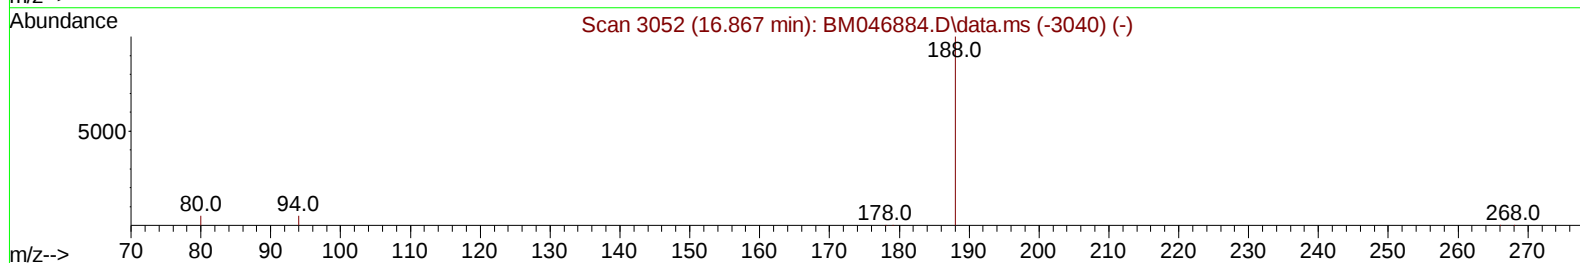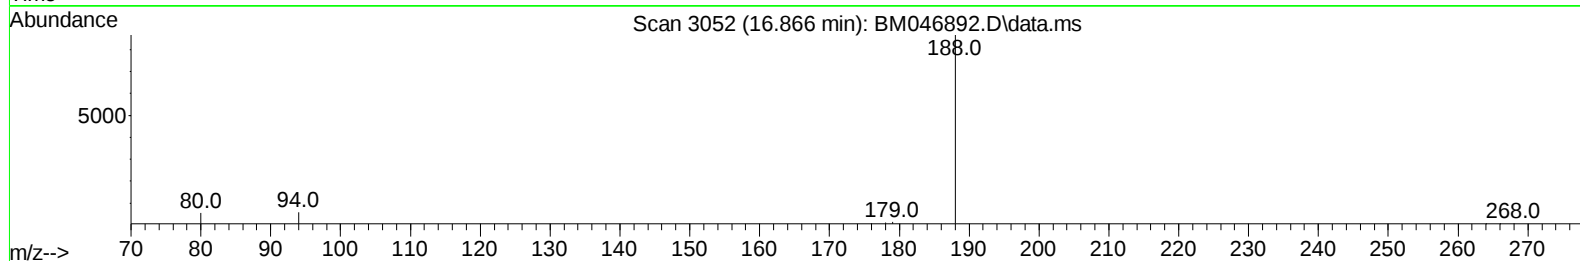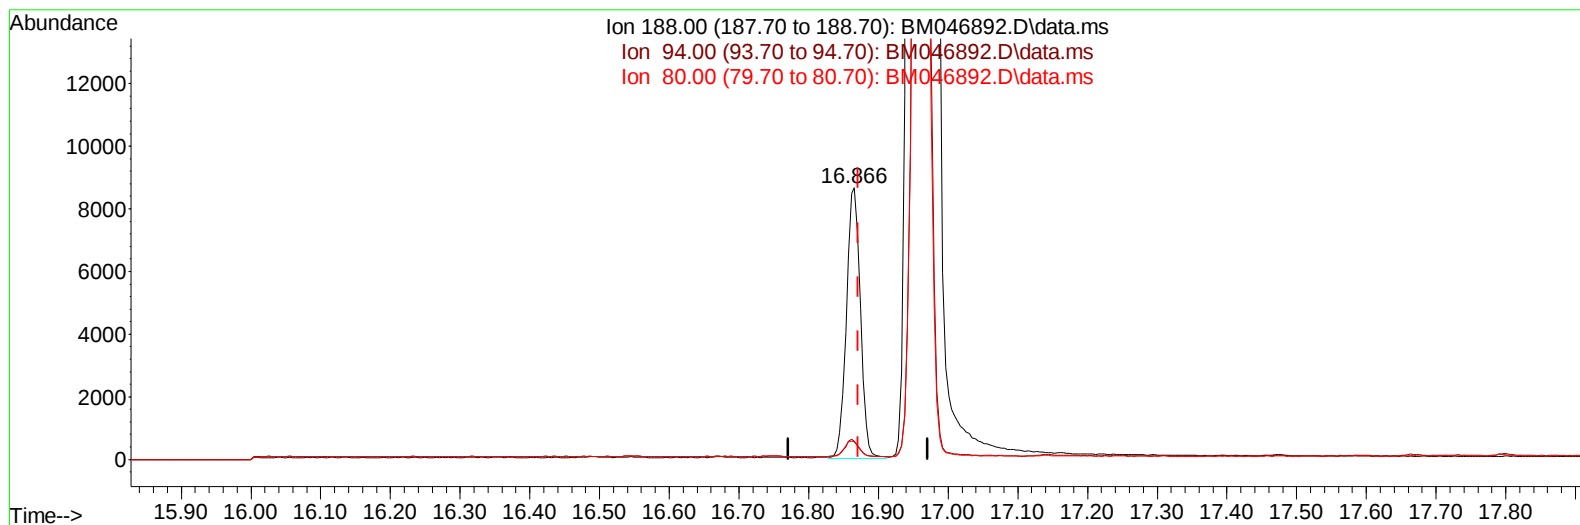

TIC: BM046892.D\data.ms

(13) Phenanthrene-d10 (I)

16.866min (-0.005) 0.40 ng/u1 m

response 11971

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	6.60	6.74
80.00	6.30	6.39
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
Data File : BM046892.D
Acq On : 29 Jul 2024 20:23
Operator : MA/JU
Sample : P3336-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7E87

Manual IntegrationsAPPROVED

Quant Time: Jul 30 00:02:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 24 15:10:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/30/2024
Supervised By :mohammad ahmed 08/03/2024

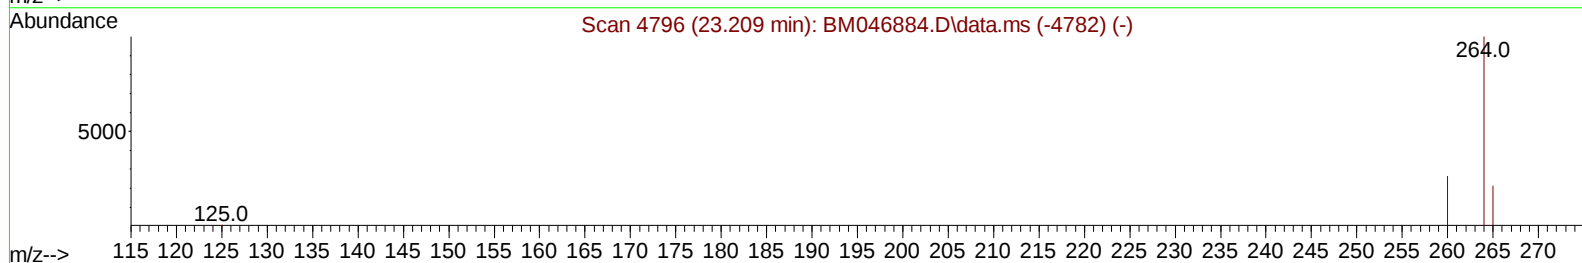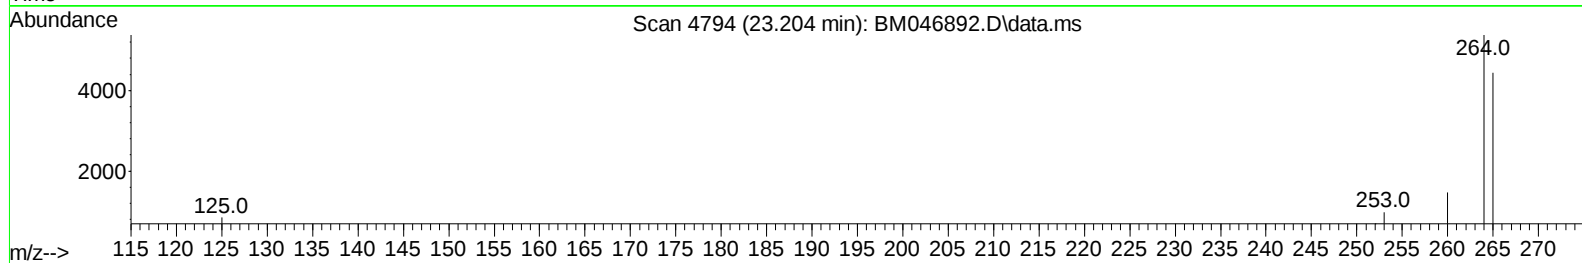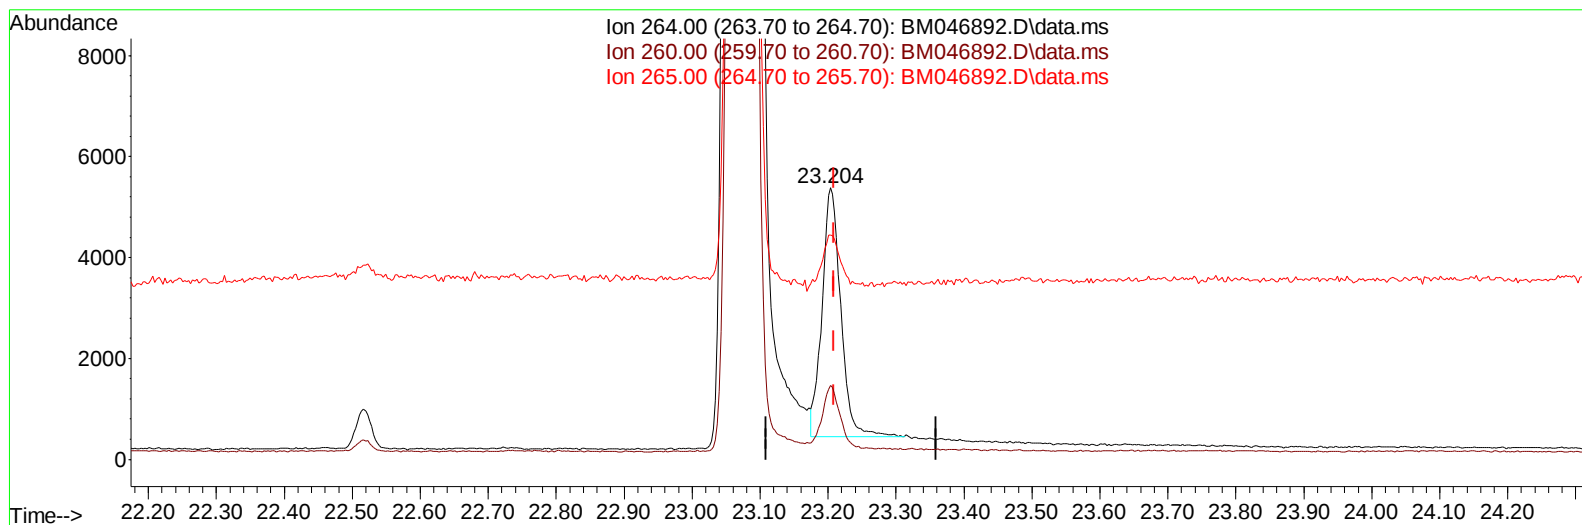

TIC: BM046892.D\data.ms

(23) Perylene-d12 (I)

23.204min (-0.005) 0.40 ng/u1

response 9507

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.10	27.18
265.00	89.90	82.65
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
Data File : BM046892.D
Acq On : 29 Jul 2024 20:23
Operator : MA/JU
Sample : P3336-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7E87

Manual IntegrationsAPPROVED

Quant Time: Jul 30 00:02:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 24 15:10:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/30/2024
Supervised By :mohammad ahmed 08/03/2024

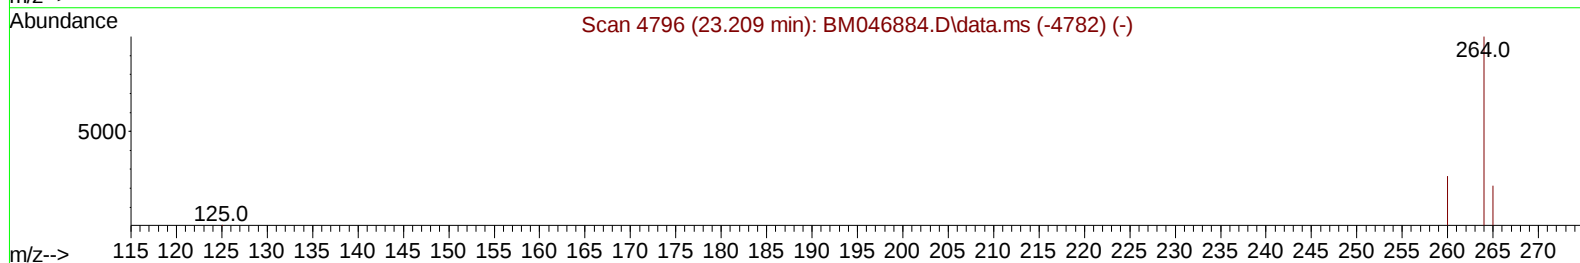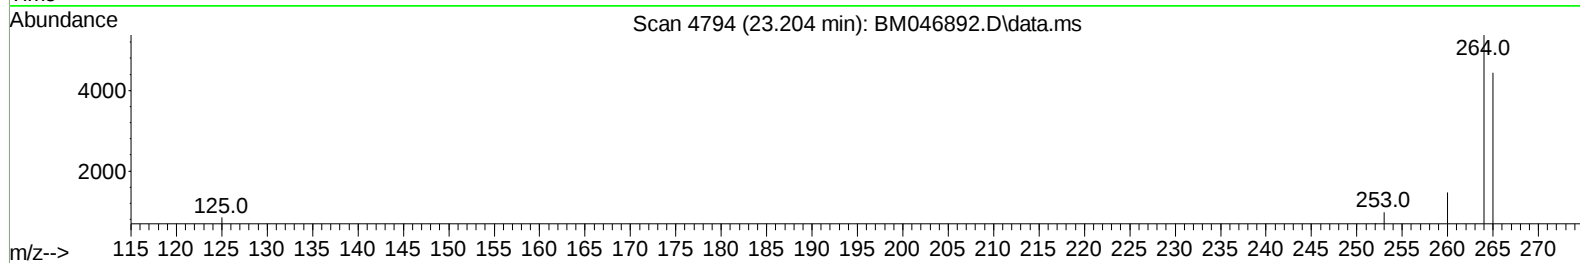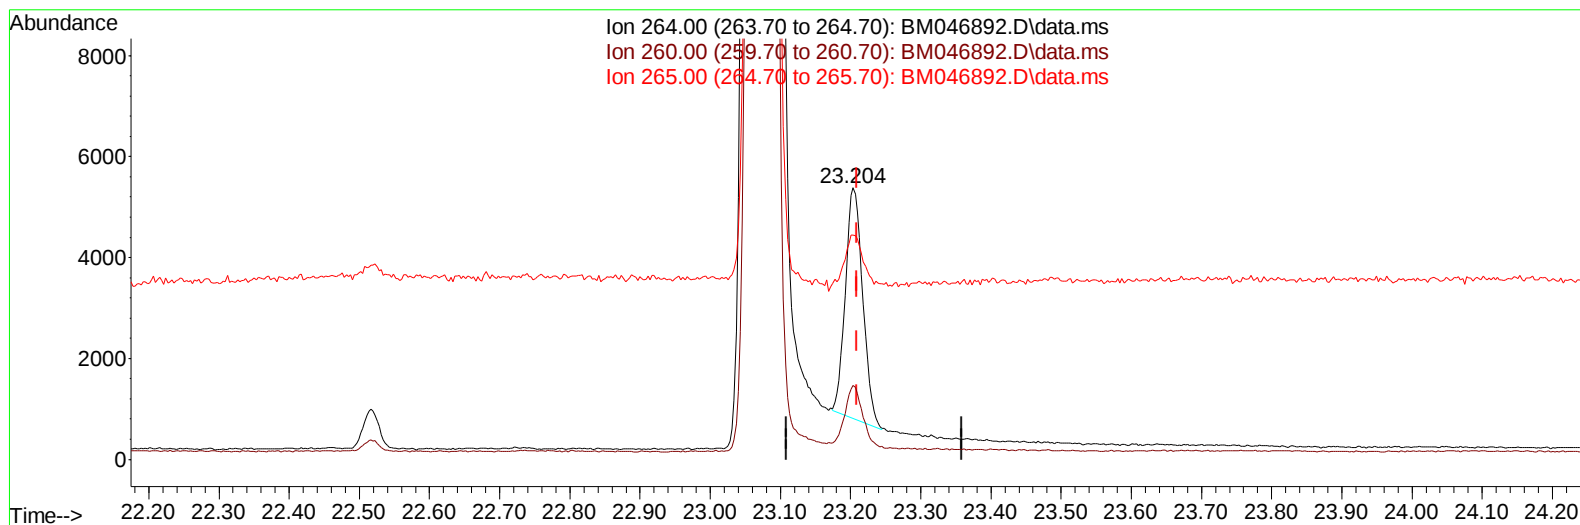

TIC: BM046892.D\data.ms

(23) Perylene-d12 (I)

23.204min (-0.005) 0.40 ng/u1 m

response 7799

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.10	27.18
265.00	89.90	82.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
 Data File : BM046892.D
 Acq On : 29 Jul 2024 20:23
 Operator : MA/JU
 Sample : P3336-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F7E87

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/30/2024
 Supervised By :mohammad ahmed 08/03/2024

Quant Time: Jul 30 00:02:21 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 24 15:10:37 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.455	152		3070	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.215	136		8985	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.108	164		5686	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.866	188		11971m	0.400	ng/ul	0.00
17) Chrysene-d12	21.079	240		8413	0.400	ng/ul	# 0.00
23) Perylene-d12	23.204	264		7799m	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.088	96		10262	4.774	ng/ul	-0.02
6) 2-Methylnaphthalene-d10	11.815	152		4482	0.314	ng/ul	-0.01
18) Fluoranthene-d10	18.908	212		10475	0.382	ng/ul	0.00
Target Compounds							Qvalue
5) Naphthalene	10.264	128		1506	0.066	ng/ul#	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
Data File : BM046892.D
Acq On : 29 Jul 2024 20:23
Operator : MA/JU
Sample : P3336-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7E87

Manual IntegrationsAPPROVED

Quant Time: Jul 30 00:02:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 24 15:10:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/30/2024
Supervised By :mohammad ahmed 08/03/2024

