




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
Data File : BM046904.D
Acq On : 30 Jul 2024 04:20
Operator : MA/JU
Sample : PB162178BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK178

Manual IntegrationsAPPROVED

Quant Time: Jul 30 04:53:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 04:18:24 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/30/2024
Supervised By :mohammad ahmed 08/03/2024

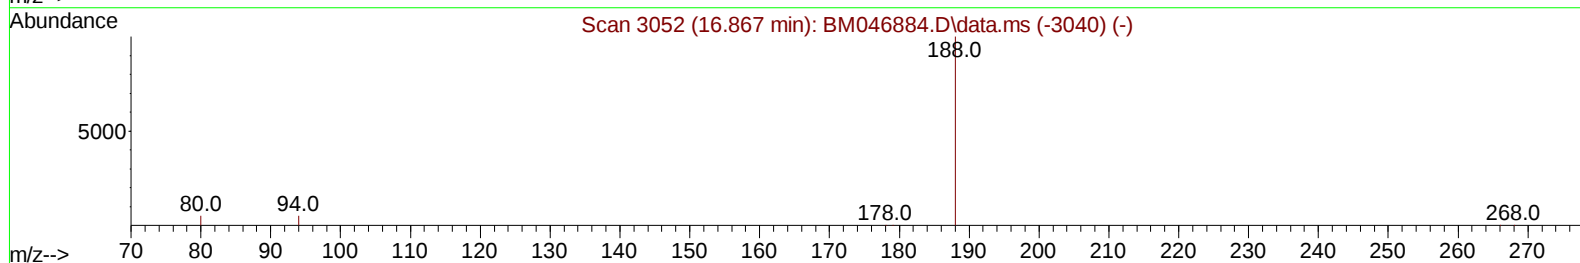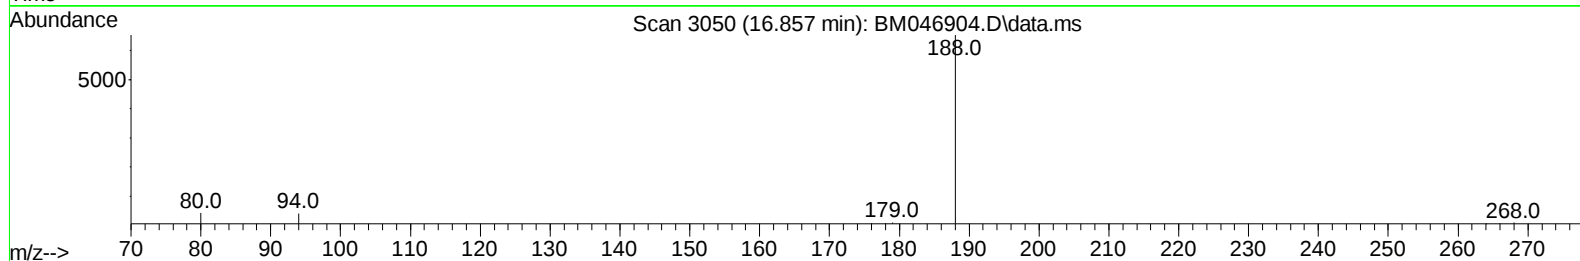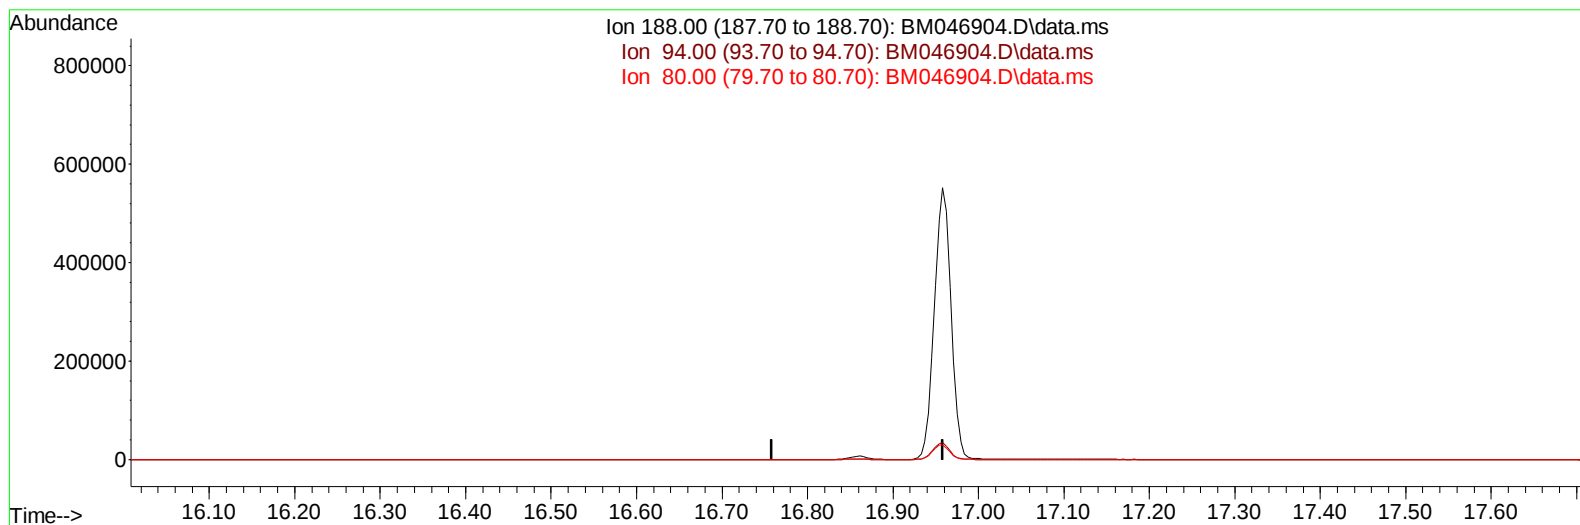

TIC: BM046904.D\data.ms

(13) Phenanthrene-d10 (I)

16.858min (-16.858) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	6.60	0.00#
80.00	6.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
Data File : BM046904.D
Acq On : 30 Jul 2024 04:20
Operator : MA/JU
Sample : PB162178BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK178

Manual IntegrationsAPPROVED

Quant Time: Jul 30 04:53:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 04:18:24 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/30/2024
Supervised By :mohammad ahmed 08/03/2024

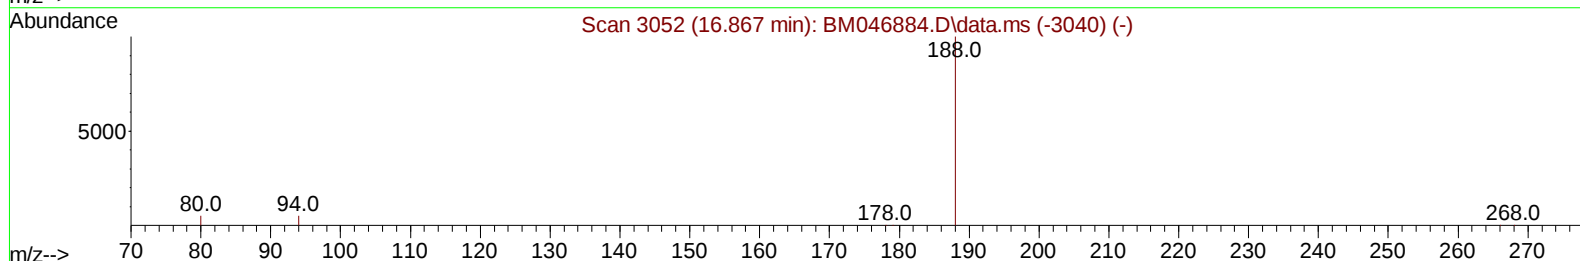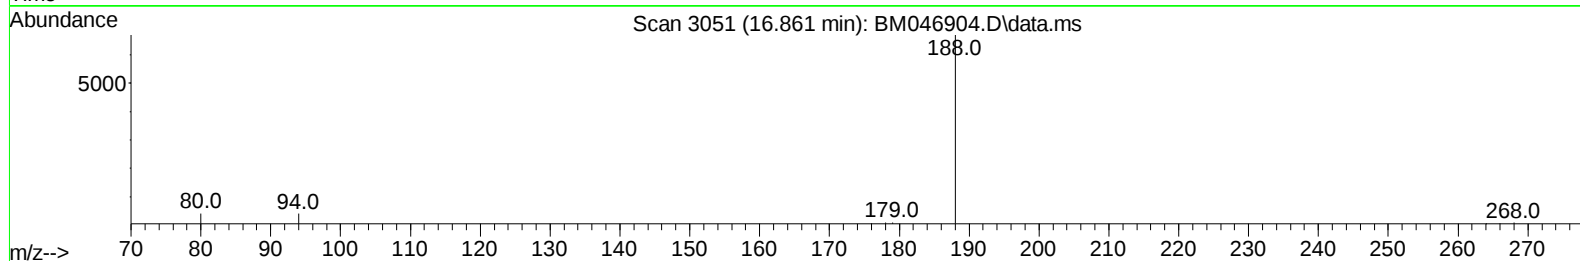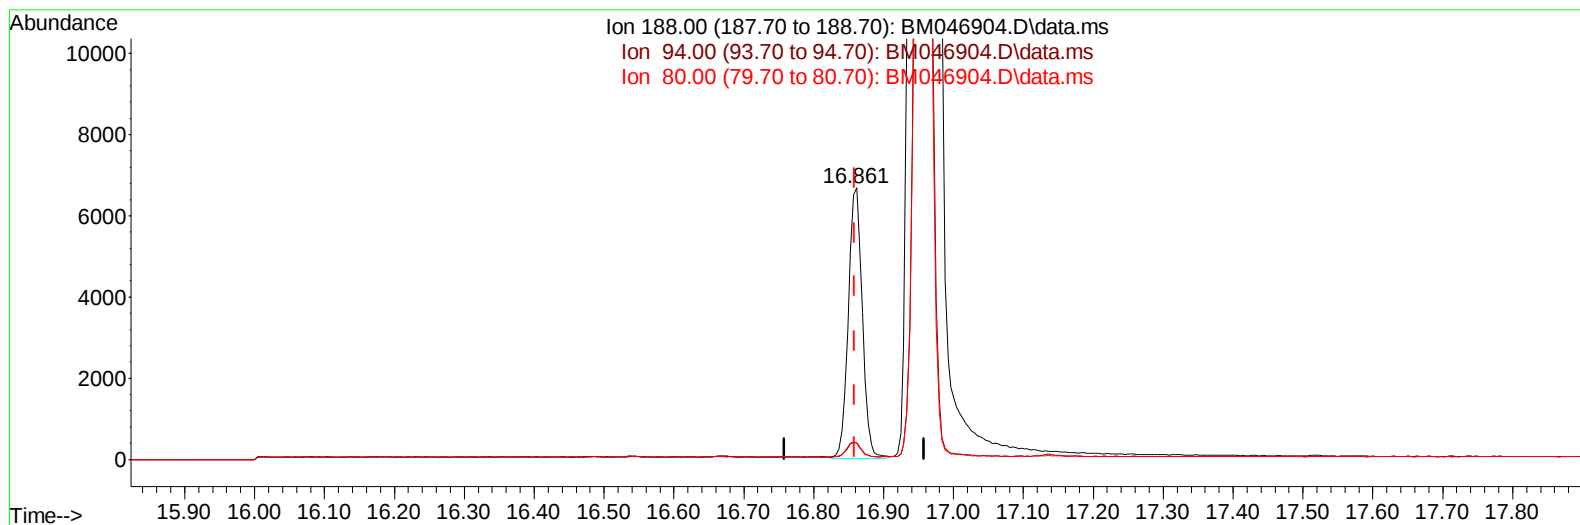

TIC: BM046904.D\data.ms

(13) Phenanthrene-d10 (I)

16.861min (+ 0.003) 0.40 ng/ul m

response 9244

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	6.60	6.15
80.00	6.30	6.25
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
Data File : BM046904.D
Acq On : 30 Jul 2024 04:20
Operator : MA/JU
Sample : PB162178BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK178

Manual IntegrationsAPPROVED

Quant Time: Jul 30 04:53:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 04:18:24 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/30/2024
Supervised By :mohammad ahmed 08/03/2024

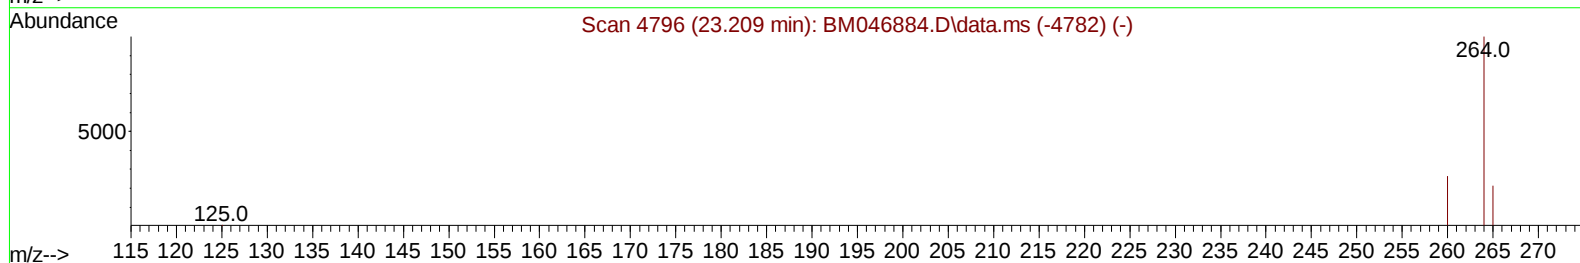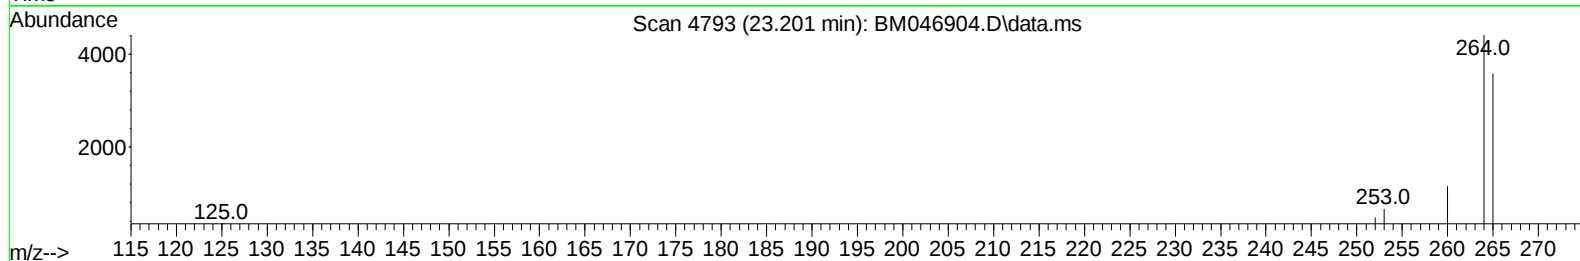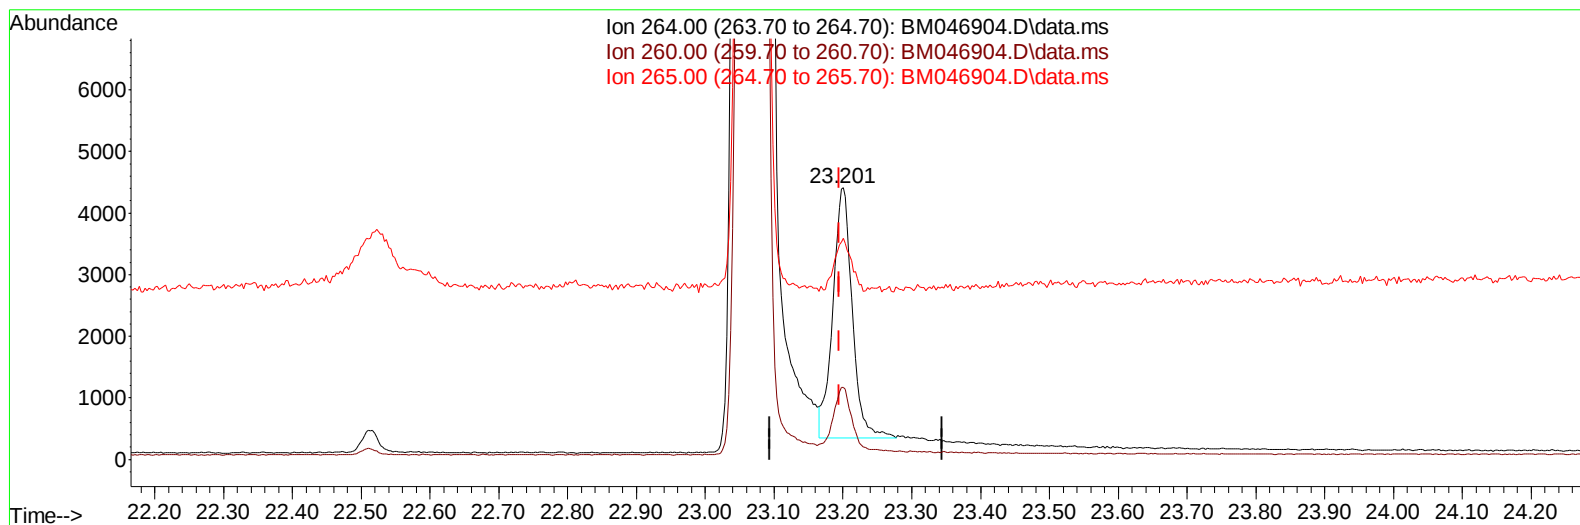

TIC: BM046904.D\data.ms

(23) Perylene-d12 (I)

23.201min (+ 0.006) 0.40 ng/ul

response 7923

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.10	26.50
265.00	89.90	81.42
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
 Data File : BM046904.D
 Acq On : 30 Jul 2024 04:20
 Operator : MA/JU
 Sample : PB162178BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK178

Manual IntegrationsAPPROVED

Quant Time: Jul 30 04:53:04 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 04:18:24 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/30/2024
 Supervised By :mohammad ahmed 08/03/2024

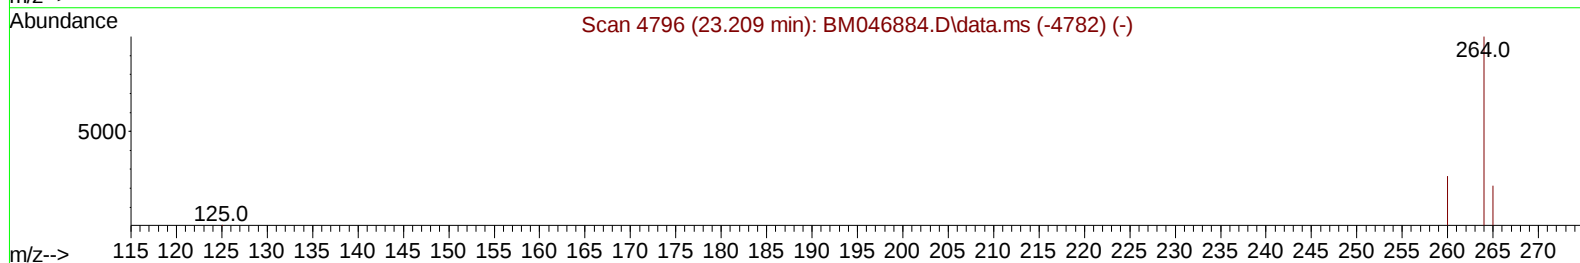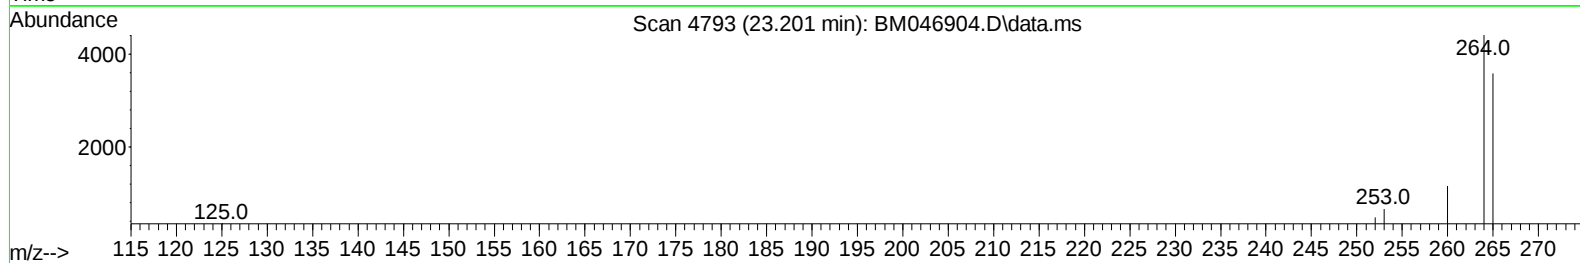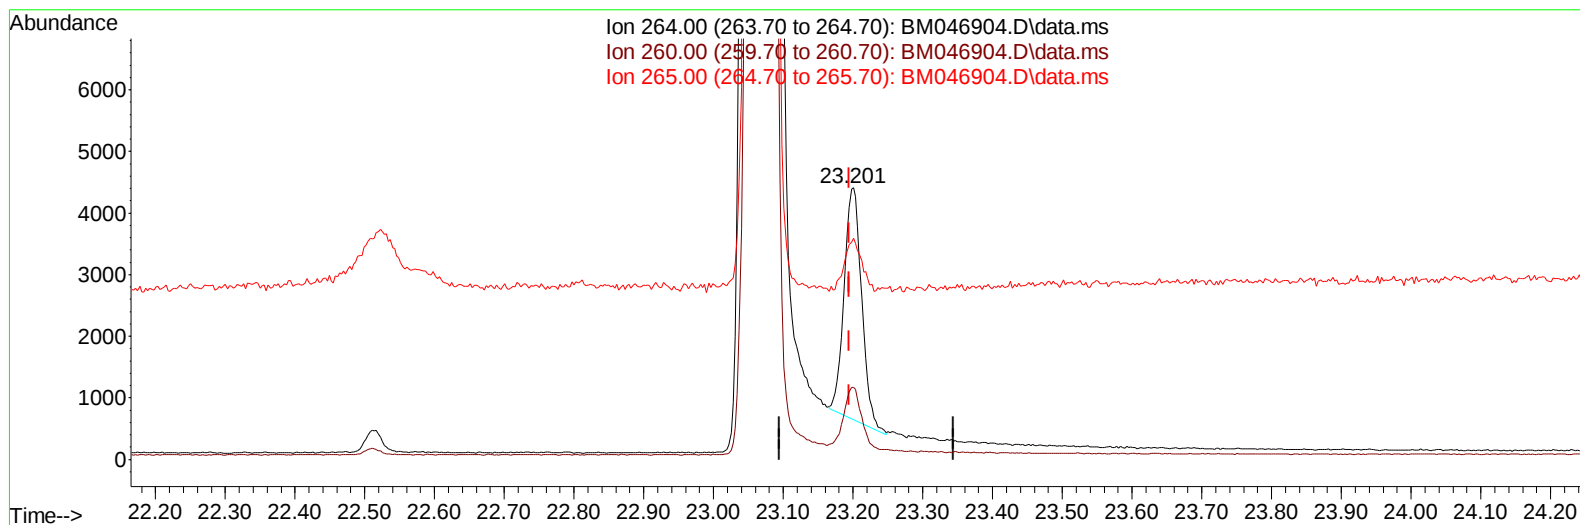

TIC: BM046904.D\data.ms

(23) Perylene-d12 (I)

23.201min (+ 0.006) 0.40 ng/ul m

response 6532

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.10	26.50
265.00	89.90	81.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
 Data File : BM046904.D
 Acq On : 30 Jul 2024 04:20
 Operator : MA/JU
 Sample : PB162178BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK178

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/30/2024
 Supervised By :mohammad ahmed 08/03/2024

Quant Time: Jul 30 04:53:04 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 04:18:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.455	152	2521	0.400	ng/ul	0.00
4) Naphthalene-d8	10.209	136	7125	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.103	164	4283	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.861	188	9244m	0.400	ng/ul	0.00
17) Chrysene-d12	21.073	240	6927	0.400	ng/ul	0.00
23) Perylene-d12	23.201	264	6532m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.084	96	10857	6.151	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.809	152	4054	0.358	ng/ul	0.00
18) Fluoranthene-d10	18.903	212	8067	0.358	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
Data File : BM046904.D
Acq On : 30 Jul 2024 04:20
Operator : MA/JU
Sample : PB162178BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK178

Manual IntegrationsAPPROVED

Quant Time: Jul 30 04:53:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 04:18:24 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/30/2024
Supervised By :mohammad ahmed 08/03/2024

