




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
Data File : BM046908.D
Acq On : 30 Jul 2024 06:46
Operator : MA/JU
Sample : P3300-04
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1GE7

Manual IntegrationsAPPROVED

Quant Time: Jul 30 07:14:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 04:18:24 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/30/2024
Supervised By :mohammad ahmed 08/03/2024

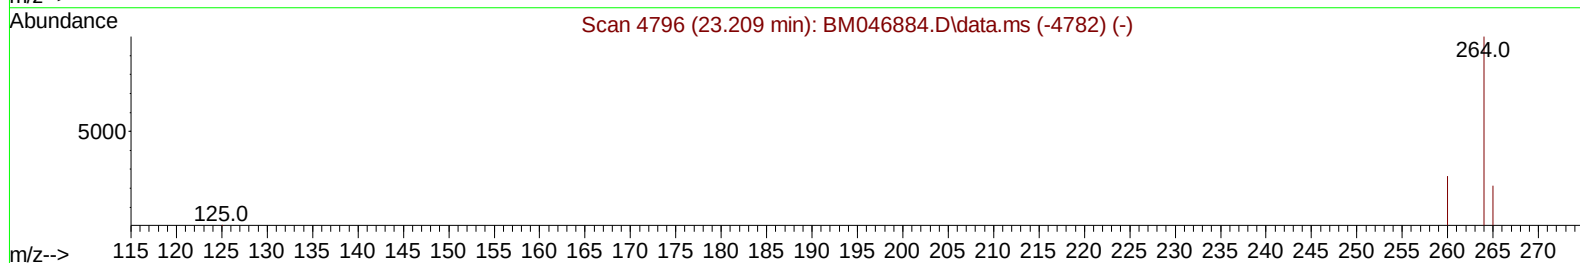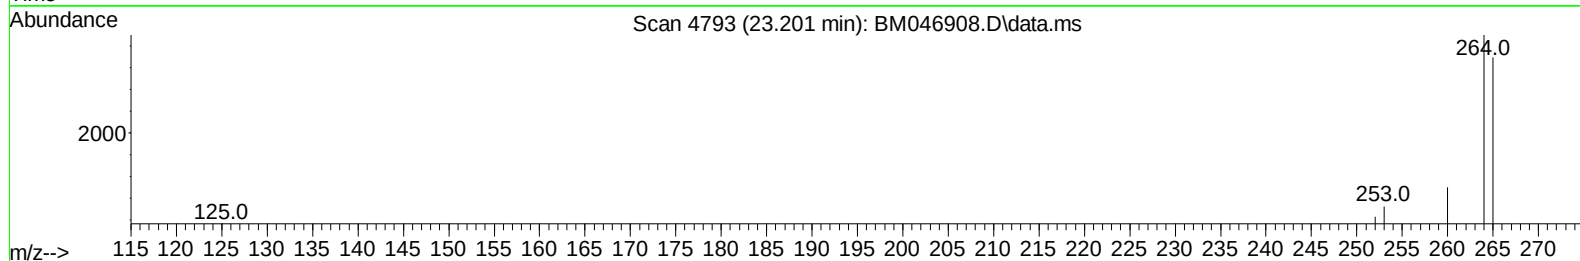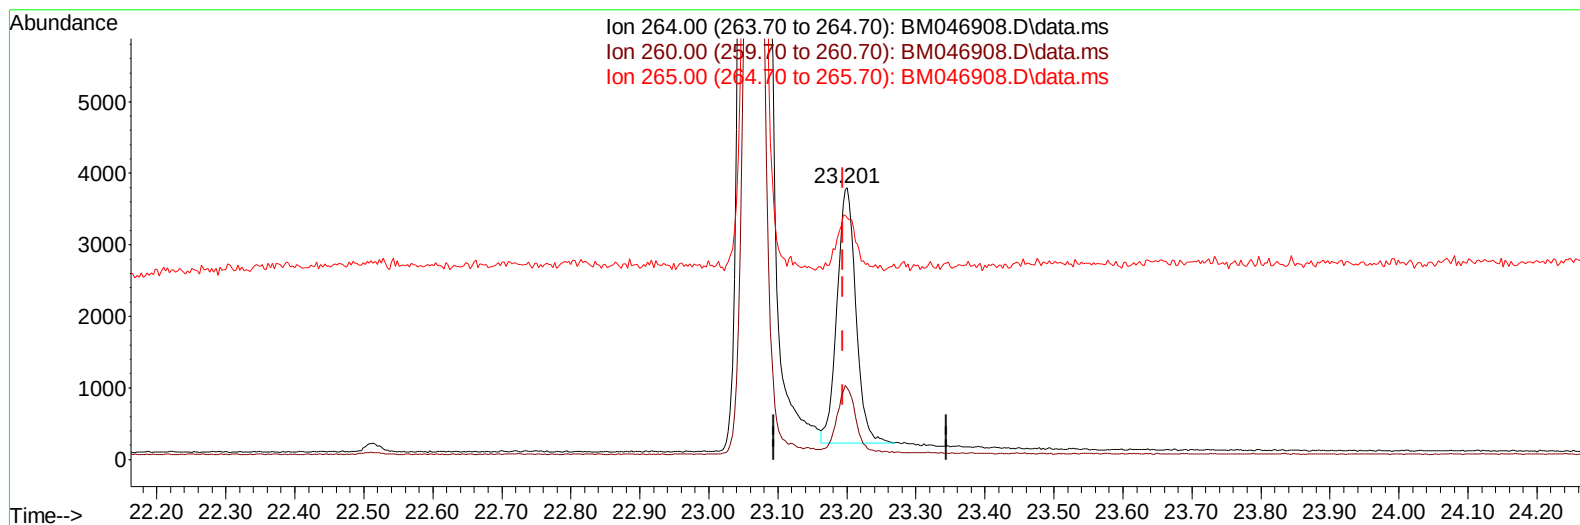

TIC: BM046908.D\data.ms

(23) Perylene-d12 (I)

23.201min (+ 0.006) 0.40 ng/ul

response 6760

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.10	26.36
265.00	89.90	89.11
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
Data File : BM046908.D
Acq On : 30 Jul 2024 06:46
Operator : MA/JU
Sample : P3300-04
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1GE7

Manual IntegrationsAPPROVED

Quant Time: Jul 30 07:14:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 04:18:24 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/30/2024
Supervised By :mohammad ahmed 08/03/2024

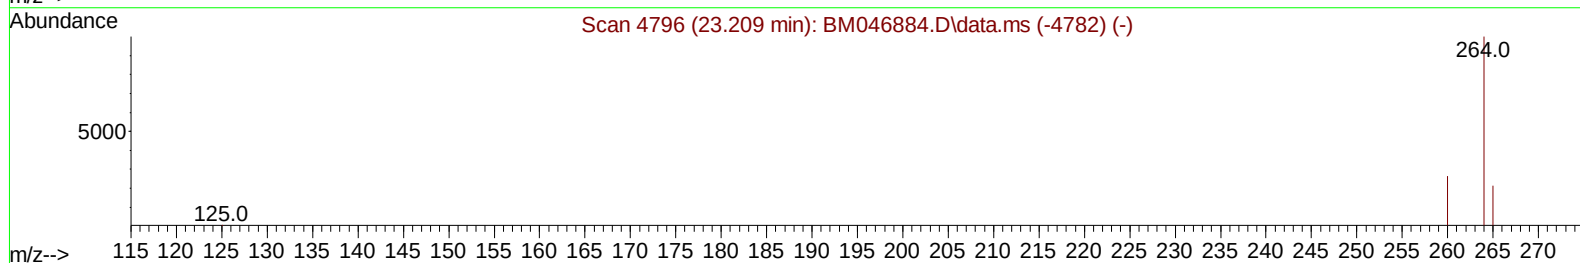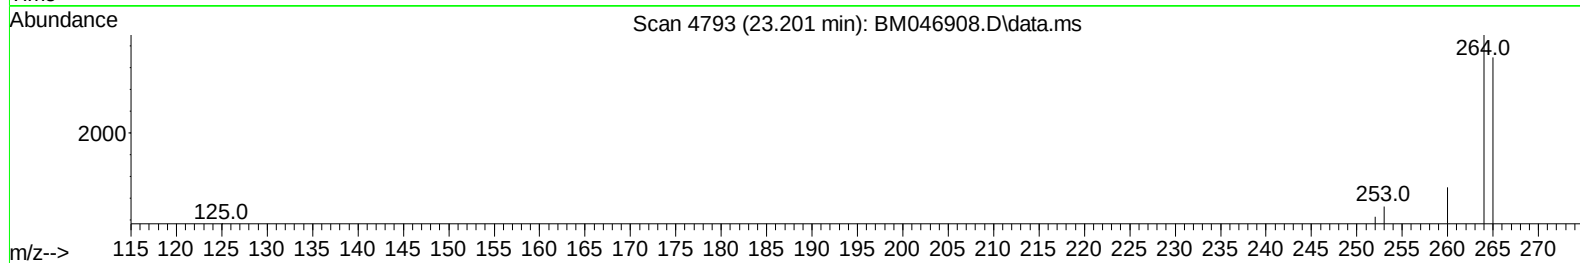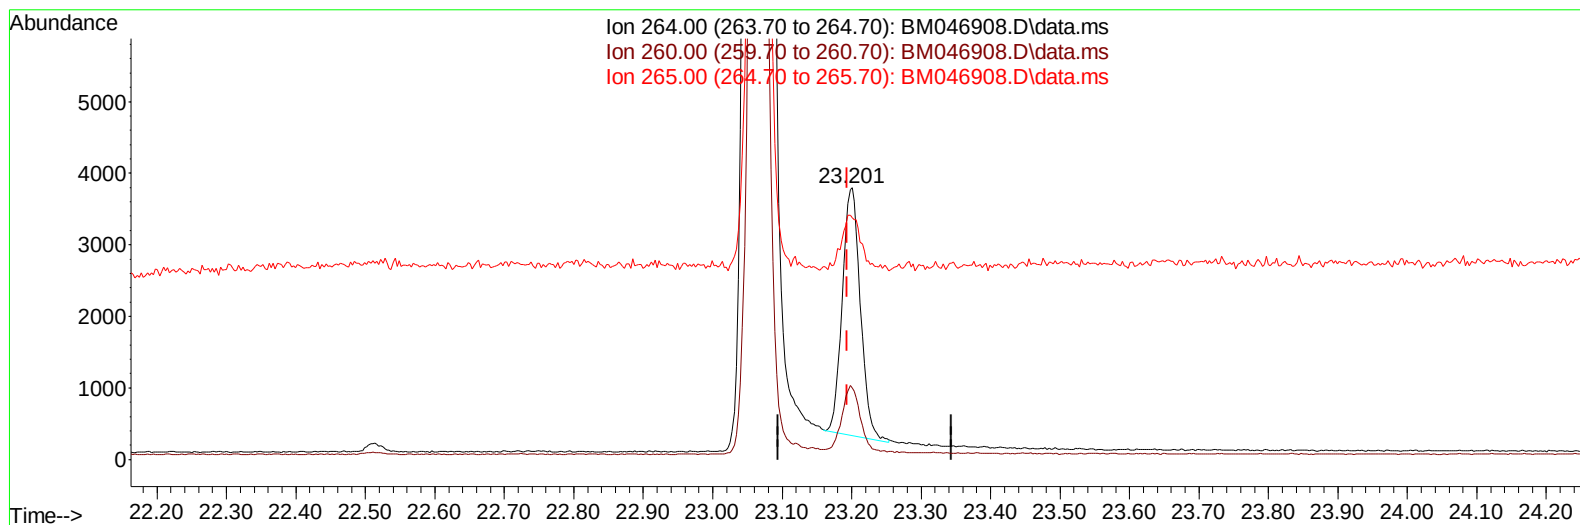

TIC: BM046908.D\data.ms

(23) Perylene-d12 (I)

23.201min (+ 0.006) 0.40 ng/ul m

response 6241

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.10	26.36
265.00	89.90	89.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
 Data File : BM046908.D
 Acq On : 30 Jul 2024 06:46
 Operator : MA/JU
 Sample : P3300-04
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1GE7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/30/2024
 Supervised By :mohammad ahmed 08/03/2024

Quant Time: Jul 30 07:14:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 04:18:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.451	152	3712	0.400	ng/ul	0.00
4) Naphthalene-d8	10.209	136	8065	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.103	164	5101	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.857	188	9424	0.400	ng/ul	0.00
17) Chrysene-d12	21.076	240	6100	0.400	ng/ul	0.00
23) Perylene-d12	23.201	264	6241m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.084	96	6170	2.374	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.810	152	876	0.068	ng/ul	0.00
18) Fluoranthene-d10	18.899	212	2141	0.108	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
Data File : BM046908.D
Acq On : 30 Jul 2024 06:46
Operator : MA/JU
Sample : P3300-04
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1GE7

Manual IntegrationsAPPROVED

Quant Time: Jul 30 07:14:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 04:18:24 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/30/2024
Supervised By :mohammad ahmed 08/03/2024

