




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
Data File : BM046911.D
Acq On : 30 Jul 2024 08:35
Operator : MA/JU
Sample : P3300-07MS
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1G93MS

Manual IntegrationsAPPROVED

Quant Time: Jul 30 09:13:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 04:18:24 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/30/2024
Supervised By :mohammad ahmed 08/03/2024

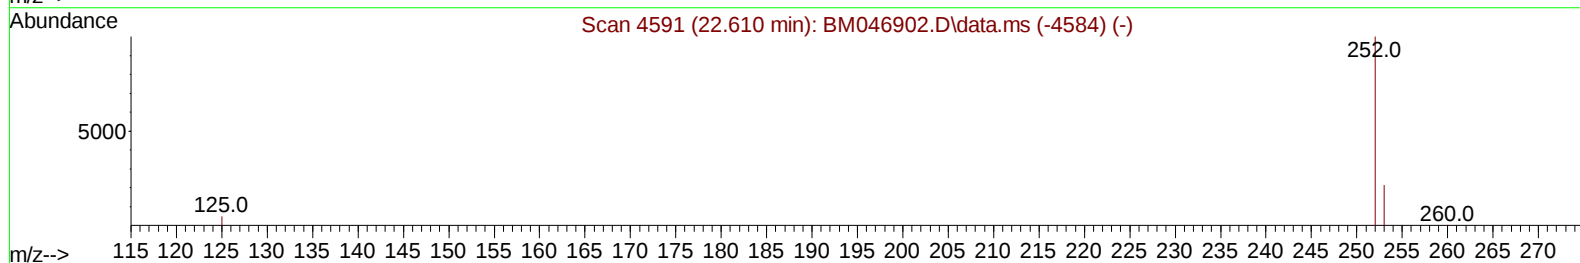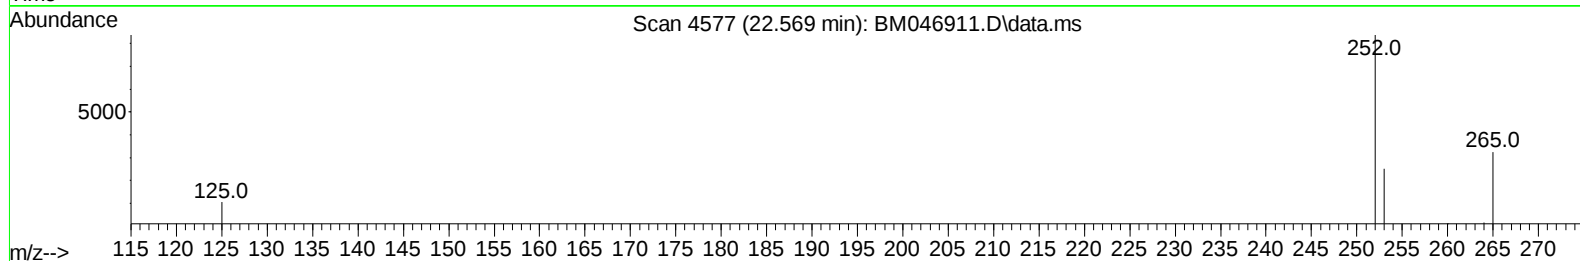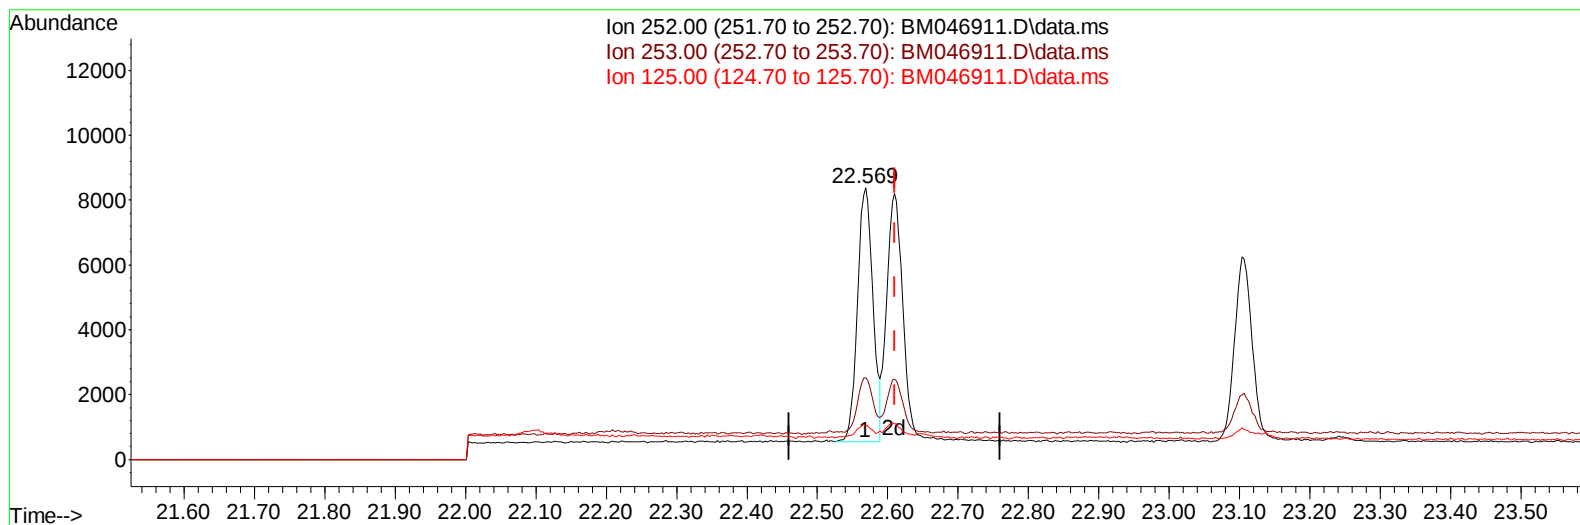

TIC: BM046911.D\data.ms

(25) Benzo(k)fluoranthene

22.569min (-0.041) 0.34 ng/u1

response 12011

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	29.40	29.98
125.00	10.80	12.42
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
 Data File : BM046911.D
 Acq On : 30 Jul 2024 08:35
 Operator : MA/JU
 Sample : P3300-07MS
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1G93MS

Manual IntegrationsAPPROVED

Quant Time: Jul 30 09:13:10 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 04:18:24 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/30/2024
 Supervised By :mohammad ahmed 08/03/2024

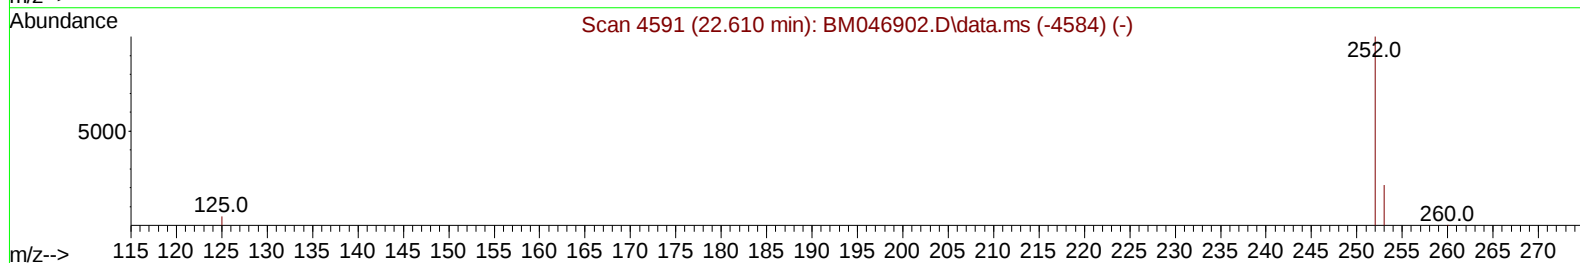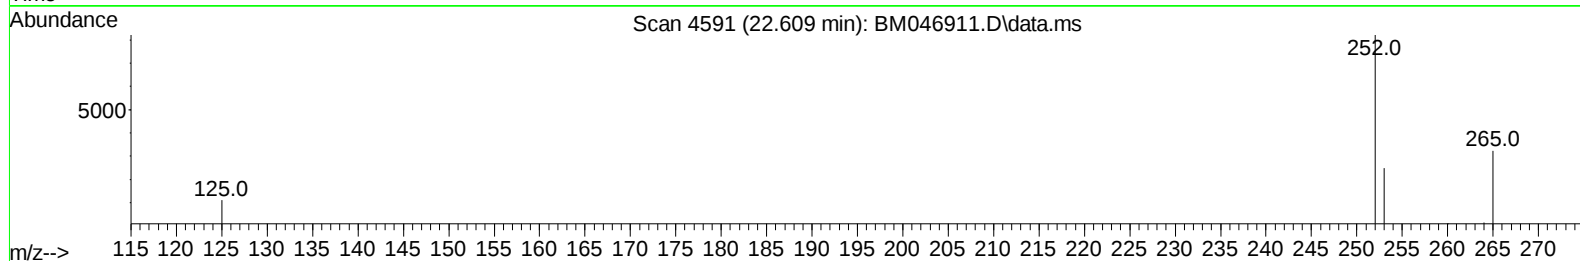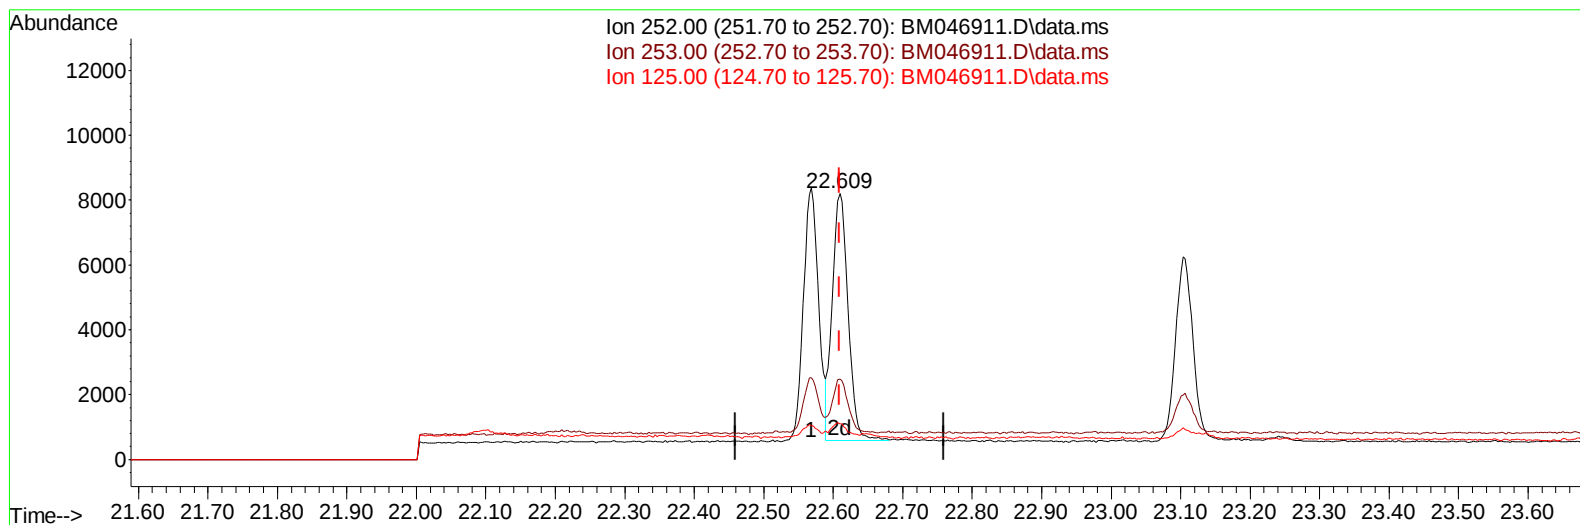

TIC: BM046911.D\data.ms

(25) Benzo(k)fluoranthene

22.609min (-0.000) 0.35 ng/u1 m

response 12069

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	29.40	30.29
125.00	10.80	13.39#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
 Data File : BM046911.D
 Acq On : 30 Jul 2024 08:35
 Operator : MA/JU
 Sample : P3300-07MS
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1G93MS

Manual IntegrationsAPPROVED

Quant Time: Jul 30 09:13:10 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 04:18:24 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/30/2024
 Supervised By :mohammad ahmed 08/03/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.451	152		2854	0.400	ng/ul	0.00
4) Naphthalene-d8	10.205	136		7874	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.099	164		4879	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.858	188		9340	0.400	ng/ul	0.00
17) Chrysene-d12	21.073	240		7162	0.400	ng/ul	# 0.00
23) Perylene-d12	23.197	264		7883	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.088	96		497	0.249	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.805	152		5805	0.464	ng/ul	0.00
18) Fluoranthene-d10	18.900	212		9435	0.404	ng/ul	0.00
Target Compounds							
							Qvalue
2) 1,4-Dioxane	3.117	88		1485	0.649	ng/ul	89
5) Naphthalene	10.254	128		6662	0.335	ng/ul	99
7) 2-Methylnaphthalene	11.882	142		6563	0.479	ng/ul	100
8) 1-Methylnaphthalene	12.108	142		4892	0.346	ng/ul	100
10) Acenaphthylene	13.813	152		7673	0.343	ng/ul	99
11) Acenaphthene	14.164	153		5541	0.365	ng/ul	99
12) Fluorene	15.159	166		6710	0.354	ng/ul	97
14) Pentachlorophenol	16.516	266		3456	0.817	ng/ul	98
15) Phenanthrene	16.896	178		10834	0.404	ng/ul	99
16) Anthracene	16.989	178		9544	0.382	ng/ul	98
19) Fluoranthene	18.928	202		12063	0.384	ng/ul	98
20) Pyrene	19.295	202		12526	0.385	ng/ul	99
21) Benzo(a)anthracene	21.055	228		11494	0.385	ng/ul	99
22) Chrysene	21.108	228		11565	0.381	ng/ul	99
24) Benzo(b)fluoranthene	22.569	252		12011	0.347	ng/ul	95
25) Benzo(k)fluoranthene	22.609	252		12069m	0.346	ng/ul	
26) Benzo(a)pyrene	23.104	252		10066	0.405	ng/ul#	95
27) Indeno(1,2,3-cd)pyrene	25.292	276		12990	0.340	ng/ul#	99
28) Dibenzo(a,h)anthracene	25.309	278		10394	0.371	ng/ul	98
29) Benzo(g,h,i)perylene	25.930	276		9753	0.290	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
Data File : BM046911.D
Acq On : 30 Jul 2024 08:35
Operator : MA/JU
Sample : P3300-07MS
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1G93MS

Manual IntegrationsAPPROVED

Quant Time: Jul 30 09:13:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 04:18:24 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/30/2024
Supervised By :mohammad ahmed 08/03/2024

