




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
Data File : BM046932.D
Acq On : 30 Jul 2024 23:04
Operator : MA/JU
Sample : P3300-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1GE7

Manual IntegrationsAPPROVED

Quant Time: Jul 31 00:01:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 04:18:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/31/2024
Supervised By :mohammad ahmed 08/03/2024

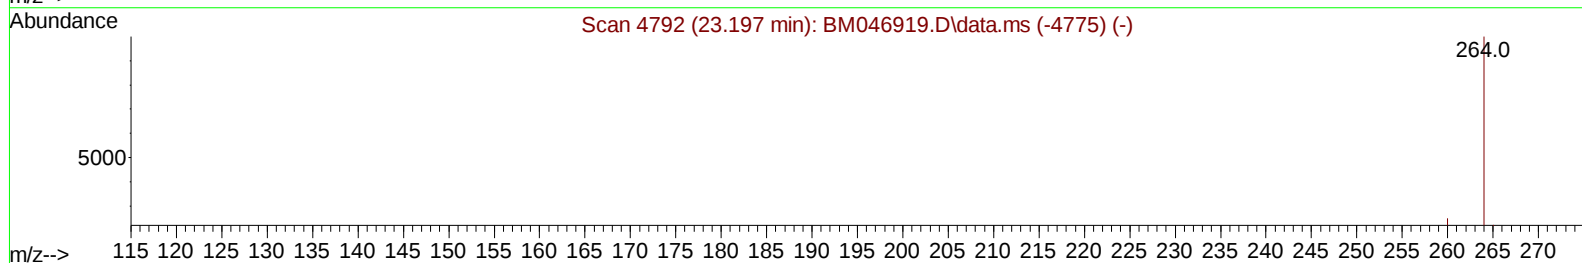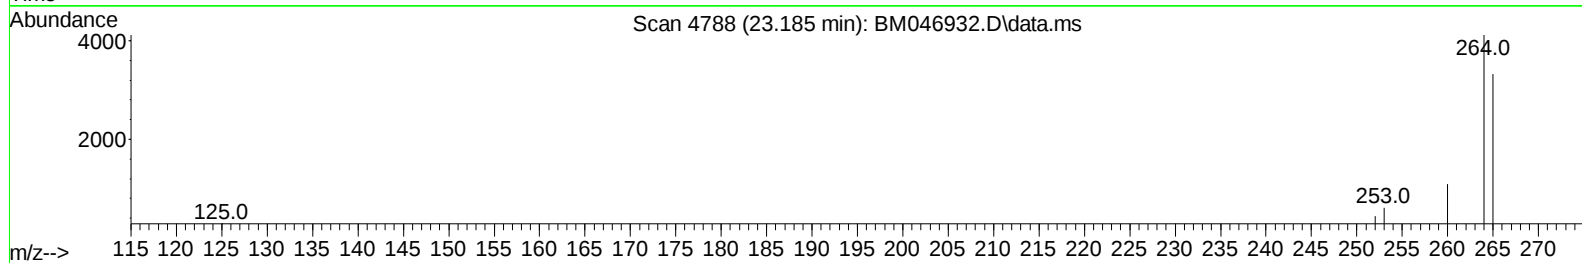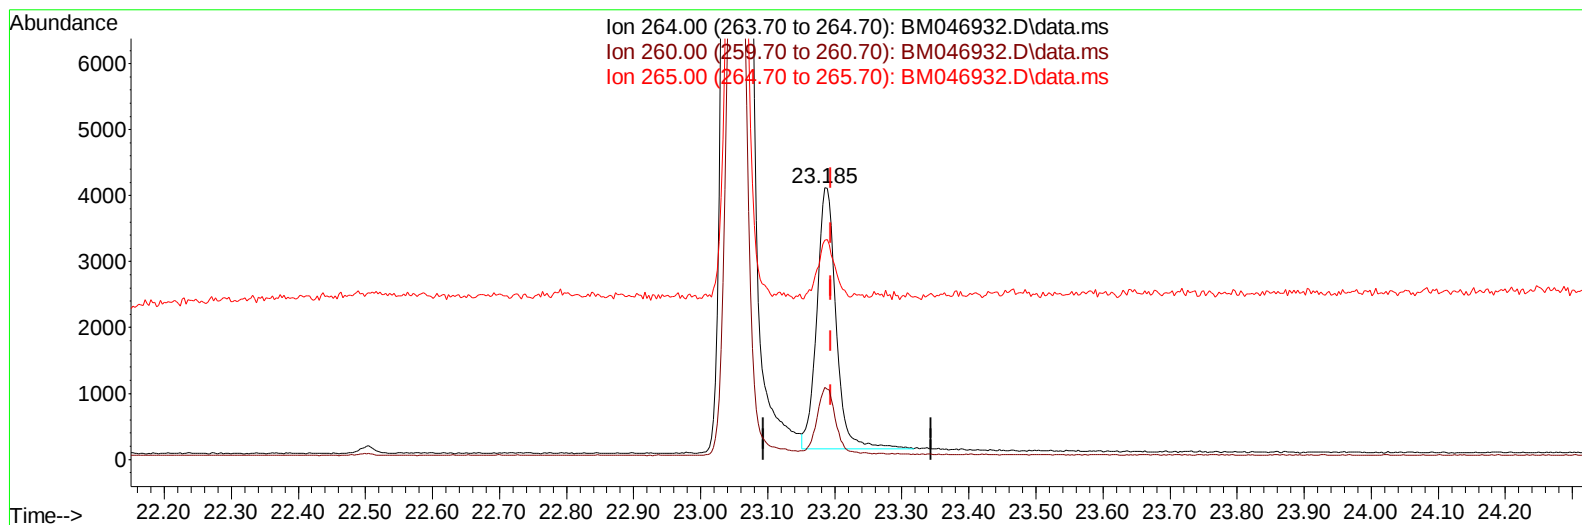

TIC: BM046932.D\data.ms

(23) Perylene-d12 (I)

23.185min (-0.009) 0.40 ng/u1

response 7826

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.10	26.55
265.00	89.90	80.69
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
Data File : BM046932.D
Acq On : 30 Jul 2024 23:04
Operator : MA/JU
Sample : P3300-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1GE7

Manual IntegrationsAPPROVED

Quant Time: Jul 31 00:01:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 04:18:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/31/2024
Supervised By :mohammad ahmed 08/03/2024

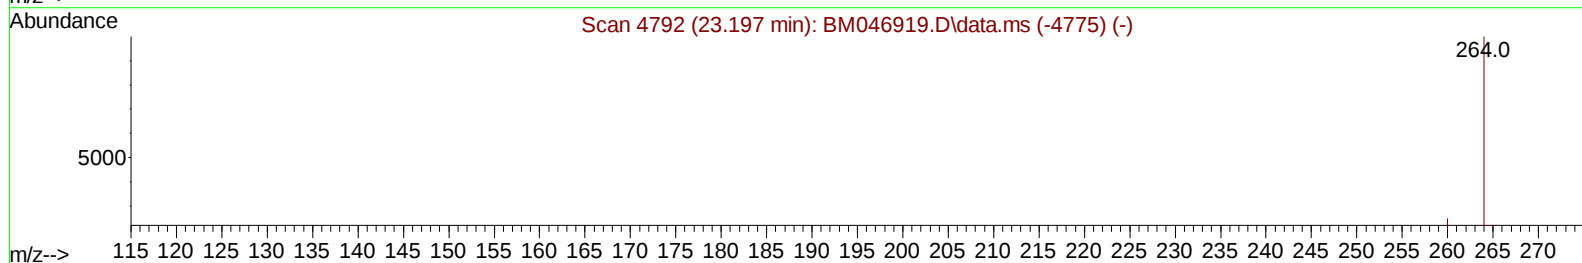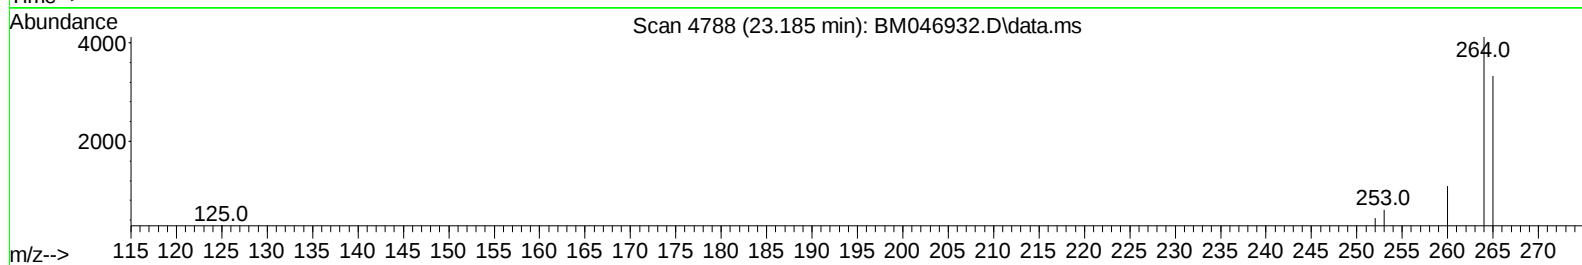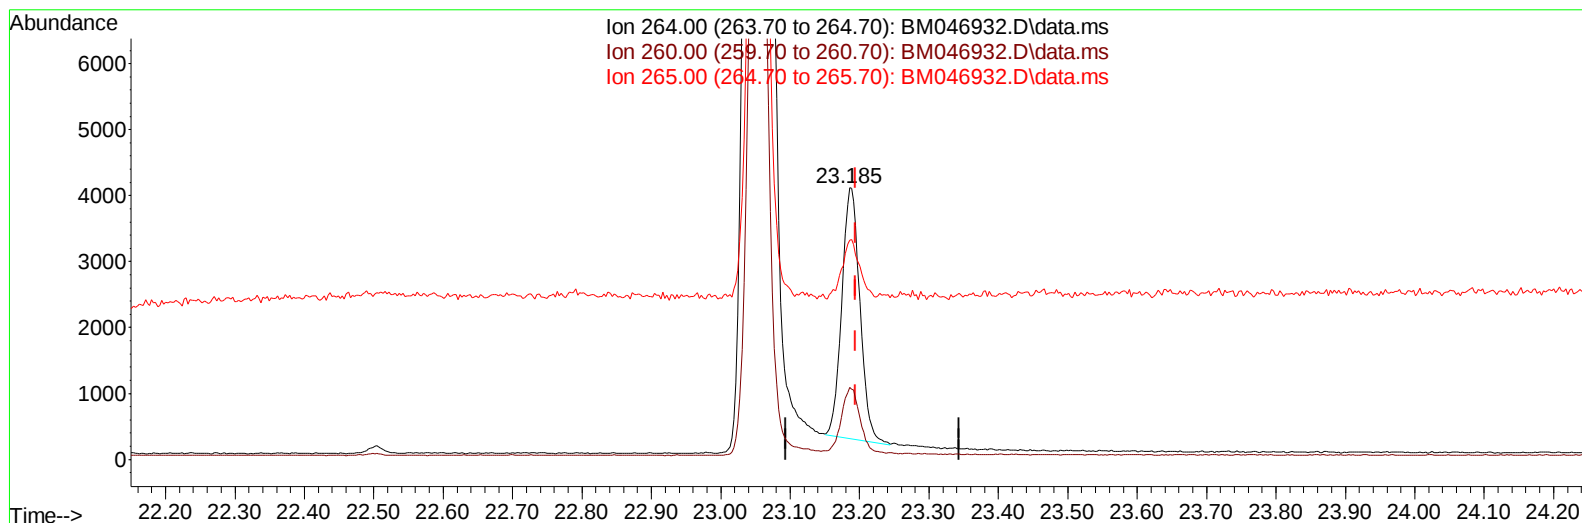

TIC: BM046932.D\data.ms

(23) Perylene-d12 (I)

23.185min (-0.009) 0.40 ng/ul m

response 6897

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.10	26.55
265.00	89.90	80.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
 Data File : BM046932.D
 Acq On : 30 Jul 2024 23:04
 Operator : MA/JU
 Sample : P3300-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1GE7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/31/2024
 Supervised By :mohammad ahmed 08/03/2024

Quant Time: Jul 31 00:01:51 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 04:18:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.447	152	4536	0.400	ng/ul	0.00
4) Naphthalene-d8	10.200	136	6802	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.095	164	4619	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.850	188	9846	0.400	ng/ul	0.00
17) Chrysene-d12	21.067	240	6637	0.400	ng/ul	0.00
23) Perylene-d12	23.185	264	6897m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.084	96	6426	2.023	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.805	152	2042	0.189	ng/ul	0.00
18) Fluoranthene-d10	18.895	212	4330	0.200	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
Data File : BM046932.D
Acq On : 30 Jul 2024 23:04
Operator : MA/JU
Sample : P3300-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1GE7

Manual IntegrationsAPPROVED

Quant Time: Jul 31 00:01:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 04:18:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/31/2024
Supervised By :mohammad ahmed 08/03/2024

