




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
Data File : BM046935.D
Acq On : 31 Jul 2024 09:53
Operator : MA/JU
Sample : P3336-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7E42

Manual IntegrationsAPPROVED

Quant Time: Jul 31 11:09:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 04:18:24 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/31/2024
Supervised By :mohammad ahmed 08/03/2024

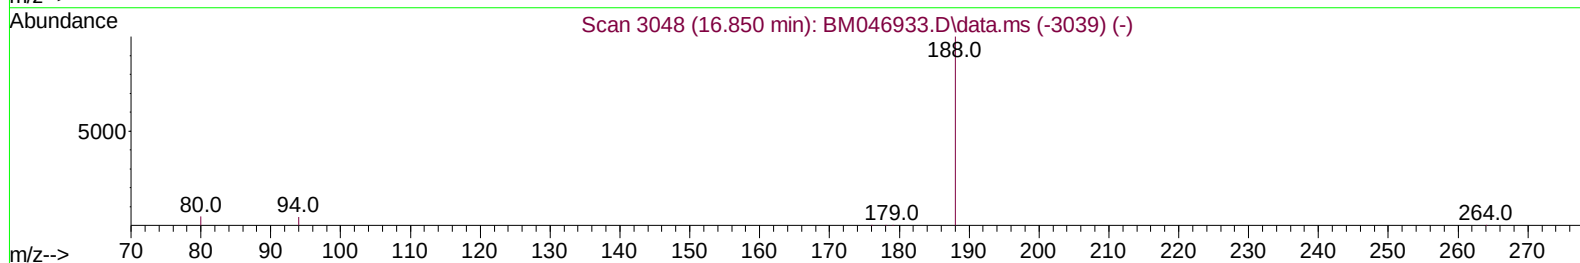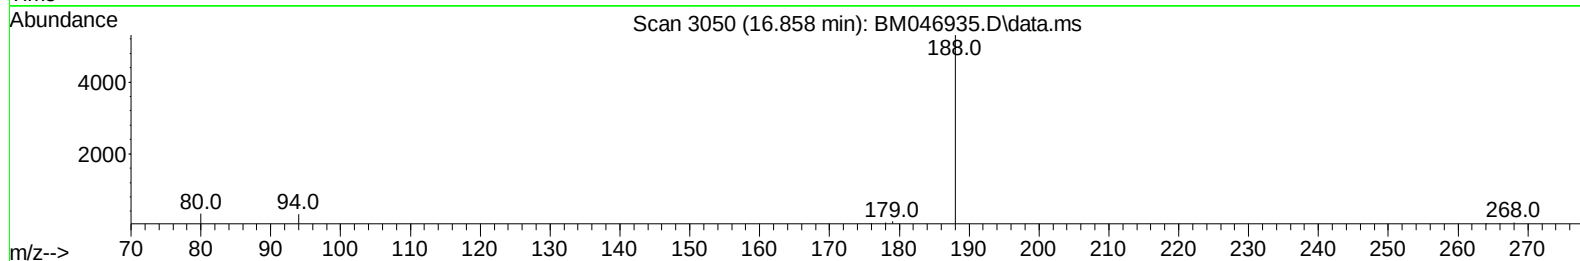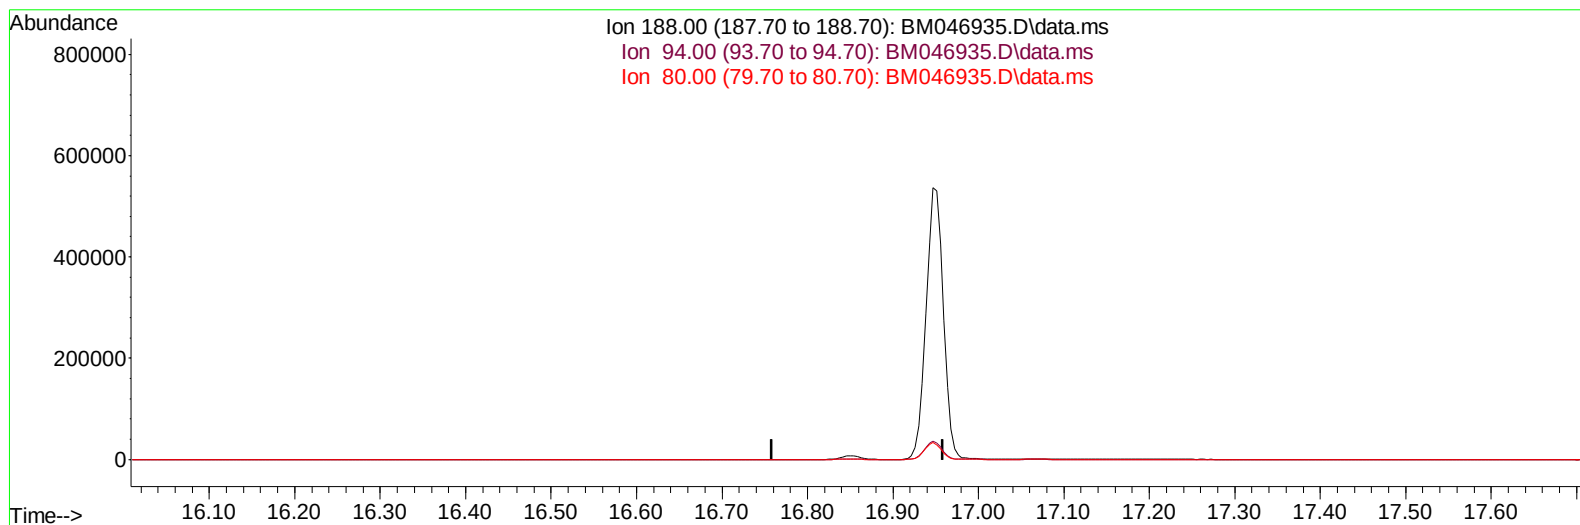

TIC: BM046935.D\data.ms

(13) Phenanthrene-d10 (I)

16.858min (-16.858) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	6.60	0.00#
80.00	6.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
Data File : BM046935.D
Acq On : 31 Jul 2024 09:53
Operator : MA/JU
Sample : P3336-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7E42

Manual IntegrationsAPPROVED

Quant Time: Jul 31 11:09:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 04:18:24 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/31/2024
Supervised By :mohammad ahmed 08/03/2024

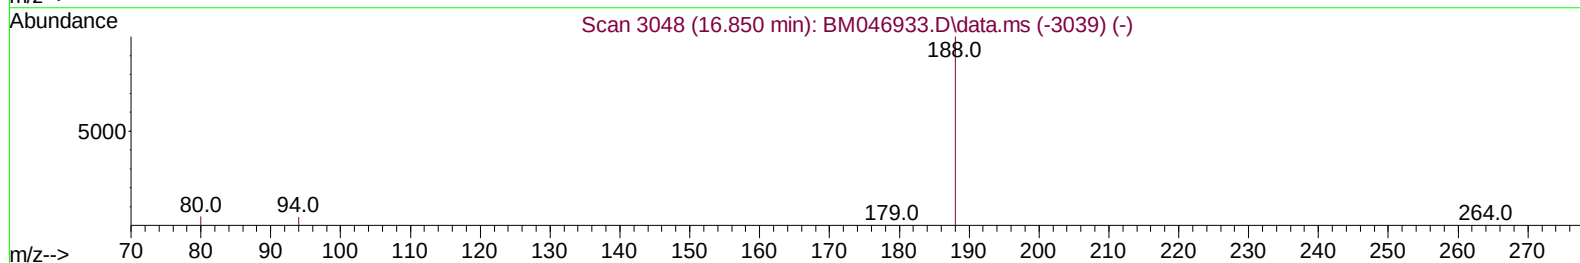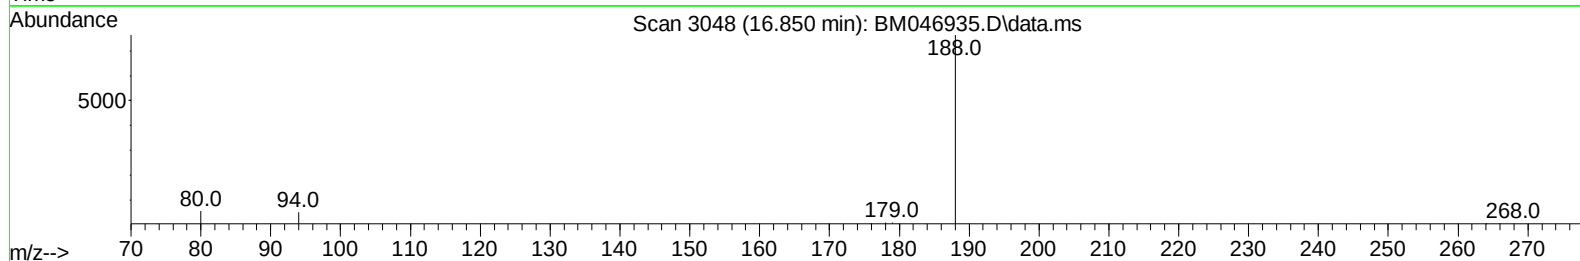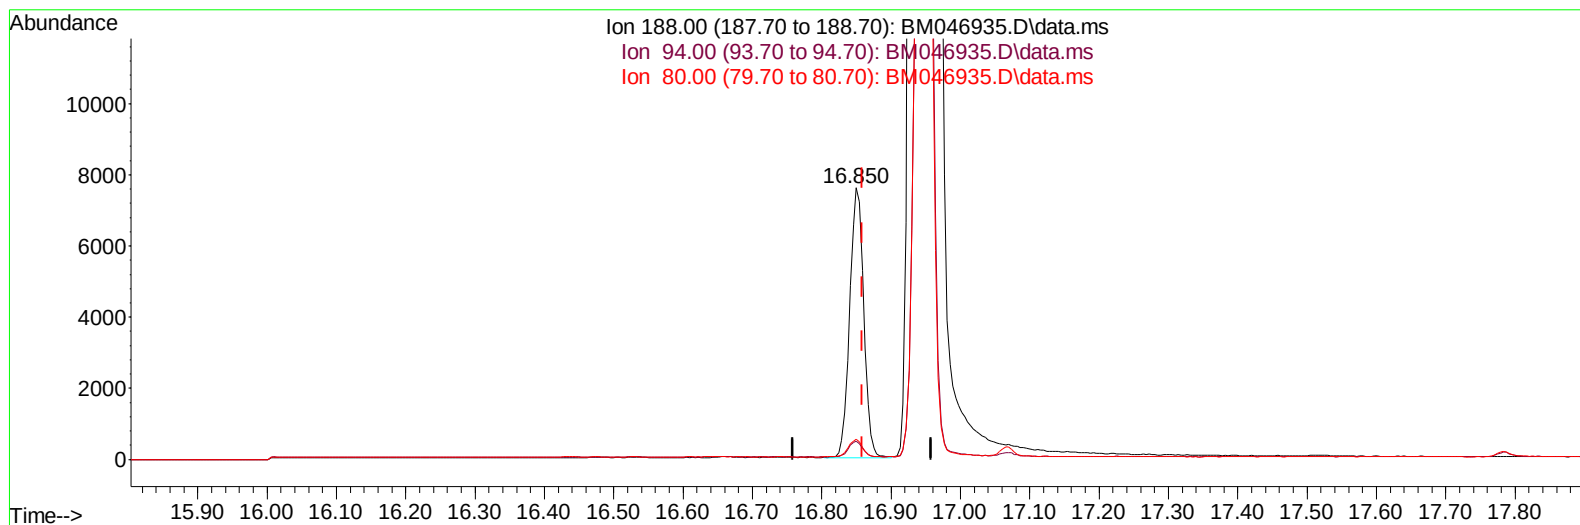

TIC: BM046935.D\data.ms

(13) Phenanthrene-d10 (I)

16.850min (-0.009) 0.40 ng/ul m

response 10605

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	6.60	6.77
80.00	6.30	7.48
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
 Data File : BM046935.D
 Acq On : 31 Jul 2024 09:53
 Operator : MA/JU
 Sample : P3336-14
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F7E42

Manual IntegrationsAPPROVED

Quant Time: Jul 31 11:09:17 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 04:18:24 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/31/2024
 Supervised By :mohammad ahmed 08/03/2024

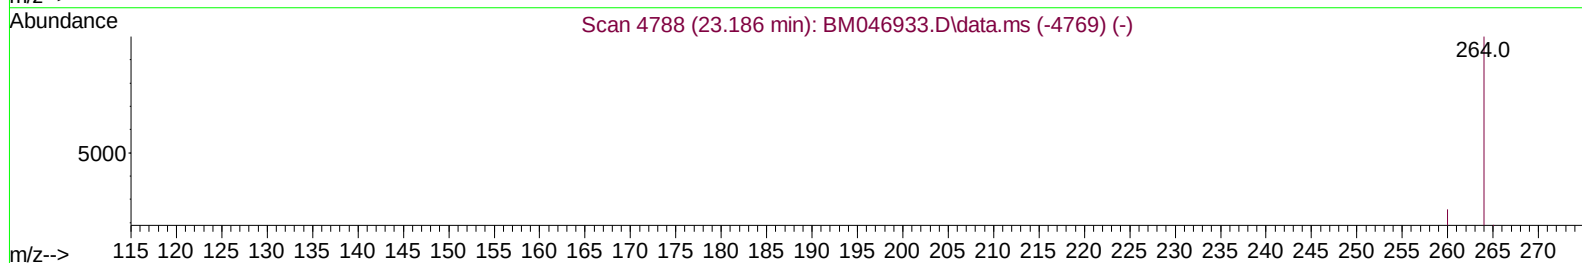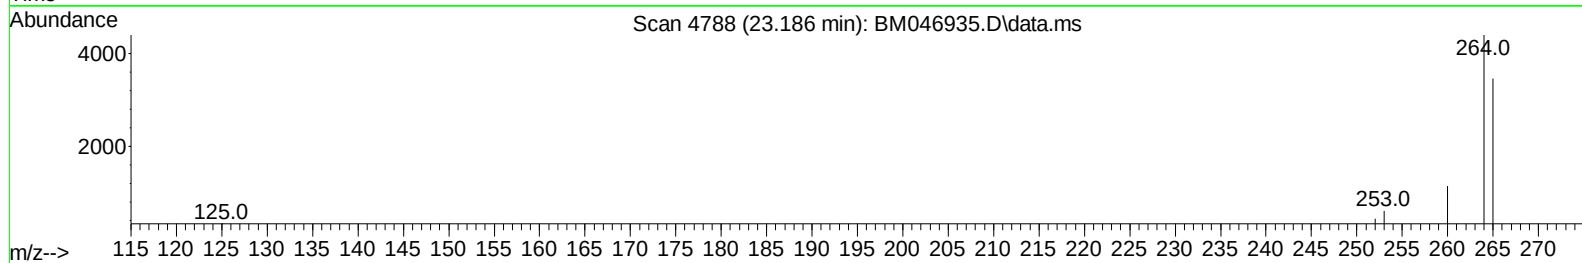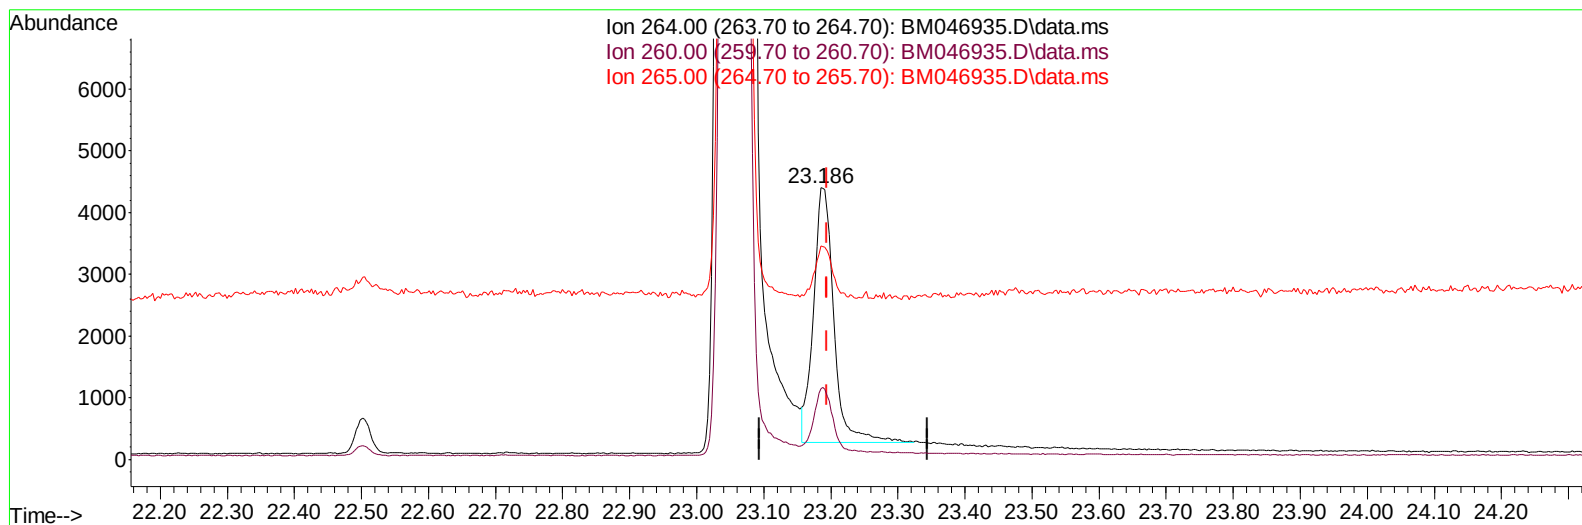

TIC: BM046935.D\data.ms

(23) Perylene-d12 (I)

23.186min (-0.009) 0.40 ng/u1

response 8662

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.10	25.98
265.00	89.90	78.70
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
Data File : BM046935.D
Acq On : 31 Jul 2024 09:53
Operator : MA/JU
Sample : P3336-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7E42

Manual IntegrationsAPPROVED

Quant Time: Jul 31 11:09:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 04:18:24 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/31/2024
Supervised By :mohammad ahmed 08/03/2024

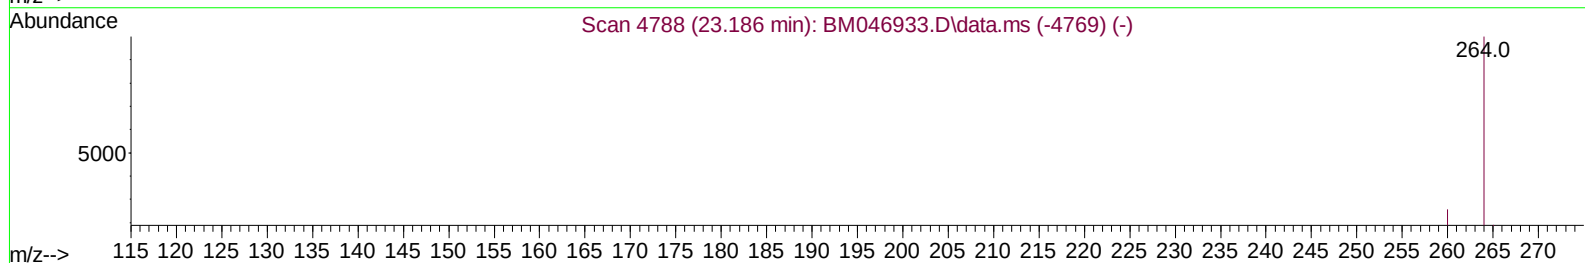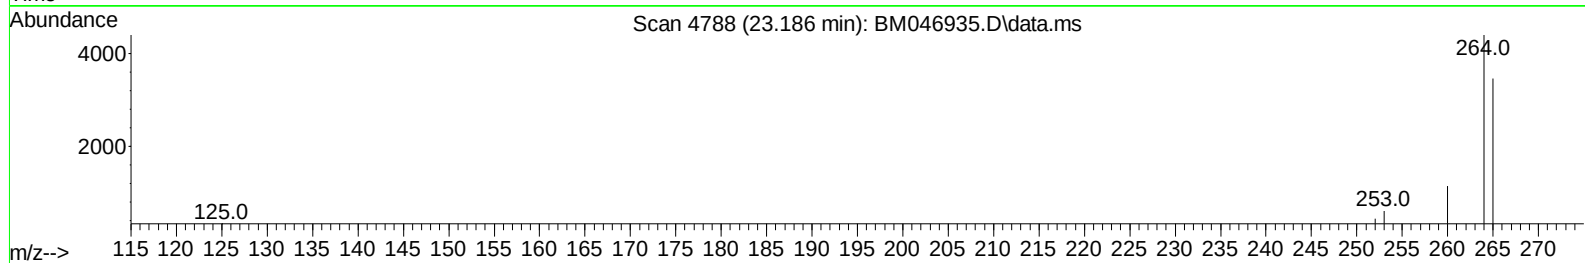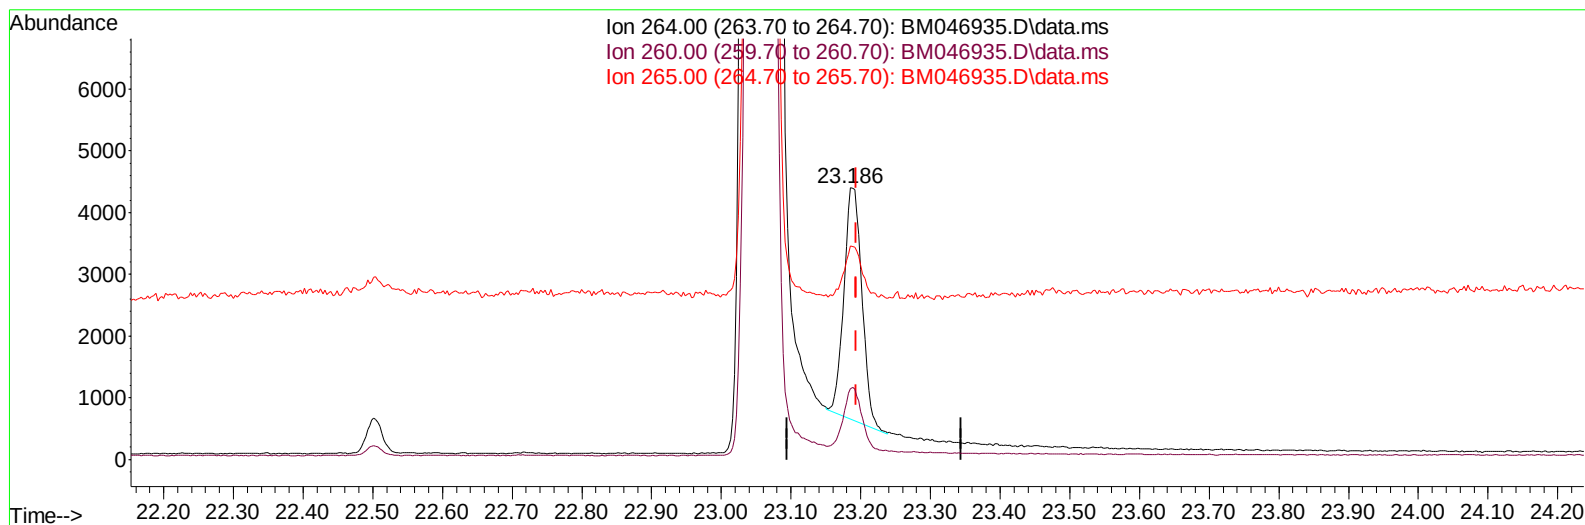

TIC: BM046935.D\data.ms

(23) Perylene-d12 (I)

23.186min (-0.009) 0.40 ng/ul m

response 6738

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.10	25.98
265.00	89.90	78.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
 Data File : BM046935.D
 Acq On : 31 Jul 2024 09:53
 Operator : MA/JU
 Sample : P3336-14
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F7E42

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/31/2024
 Supervised By :mohammad ahmed 08/03/2024

Quant Time: Jul 31 11:09:17 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 04:18:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.442	152	1939	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.200	136	5105	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.090	164	3407	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.850	188	10605m	0.400	ng/ul	0.00
17) Chrysene-d12	21.067	240	6982	0.400	ng/ul	0.00
23) Perylene-d12	23.186	264	6738m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.080	96	7378	5.434	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.800	152	2766	0.341	ng/ul	-0.01
18) Fluoranthene-d10	18.895	212	6627	0.291	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
Data File : BM046935.D
Acq On : 31 Jul 2024 09:53
Operator : MA/JU
Sample : P3336-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7E42

Manual IntegrationsAPPROVED

Quant Time: Jul 31 11:09:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 04:18:24 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/31/2024
Supervised By :mohammad ahmed 08/03/2024

