

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
 Data File : BM046882.D
 Acq On : 29 Jul 2024 14:13
 Operator : MA/JU
 Sample : P3329-19
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F7E85

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/30/2024
 Supervised By :mohammad ahmed 08/03/2024

Quant Time: Jul 29 14:54:02 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 24 15:10:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.459	152	3660	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.216	136	11467	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.109	164	7382	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.867	188	14013m	0.400	ng/ul	0.00
17) Chrysene-d12	21.082	240	8469	0.400	ng/ul	0.00
23) Perylene-d12	23.209	264	7404m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.088	96	9418	3.675	ng/ul	-0.02
6) 2-Methylnaphthalene-d10	11.816	152	4833	0.265	ng/ul	-0.01
18) Fluoranthene-d10	18.909	212	8746	0.317	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.266	128	1460	0.050	ng/ul#	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
Data File : BM046882.D
Acq On : 29 Jul 2024 14:13
Operator : MA/JU
Sample : P3329-19
Misc :
ALS Vial : 4 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
F7E85

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/30/2024
Supervised By :mohammad ahmed 08/03/2024


Quant Time: Jul 29 14:54:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 24 15:10:37 2024
Response via : Initial Calibration

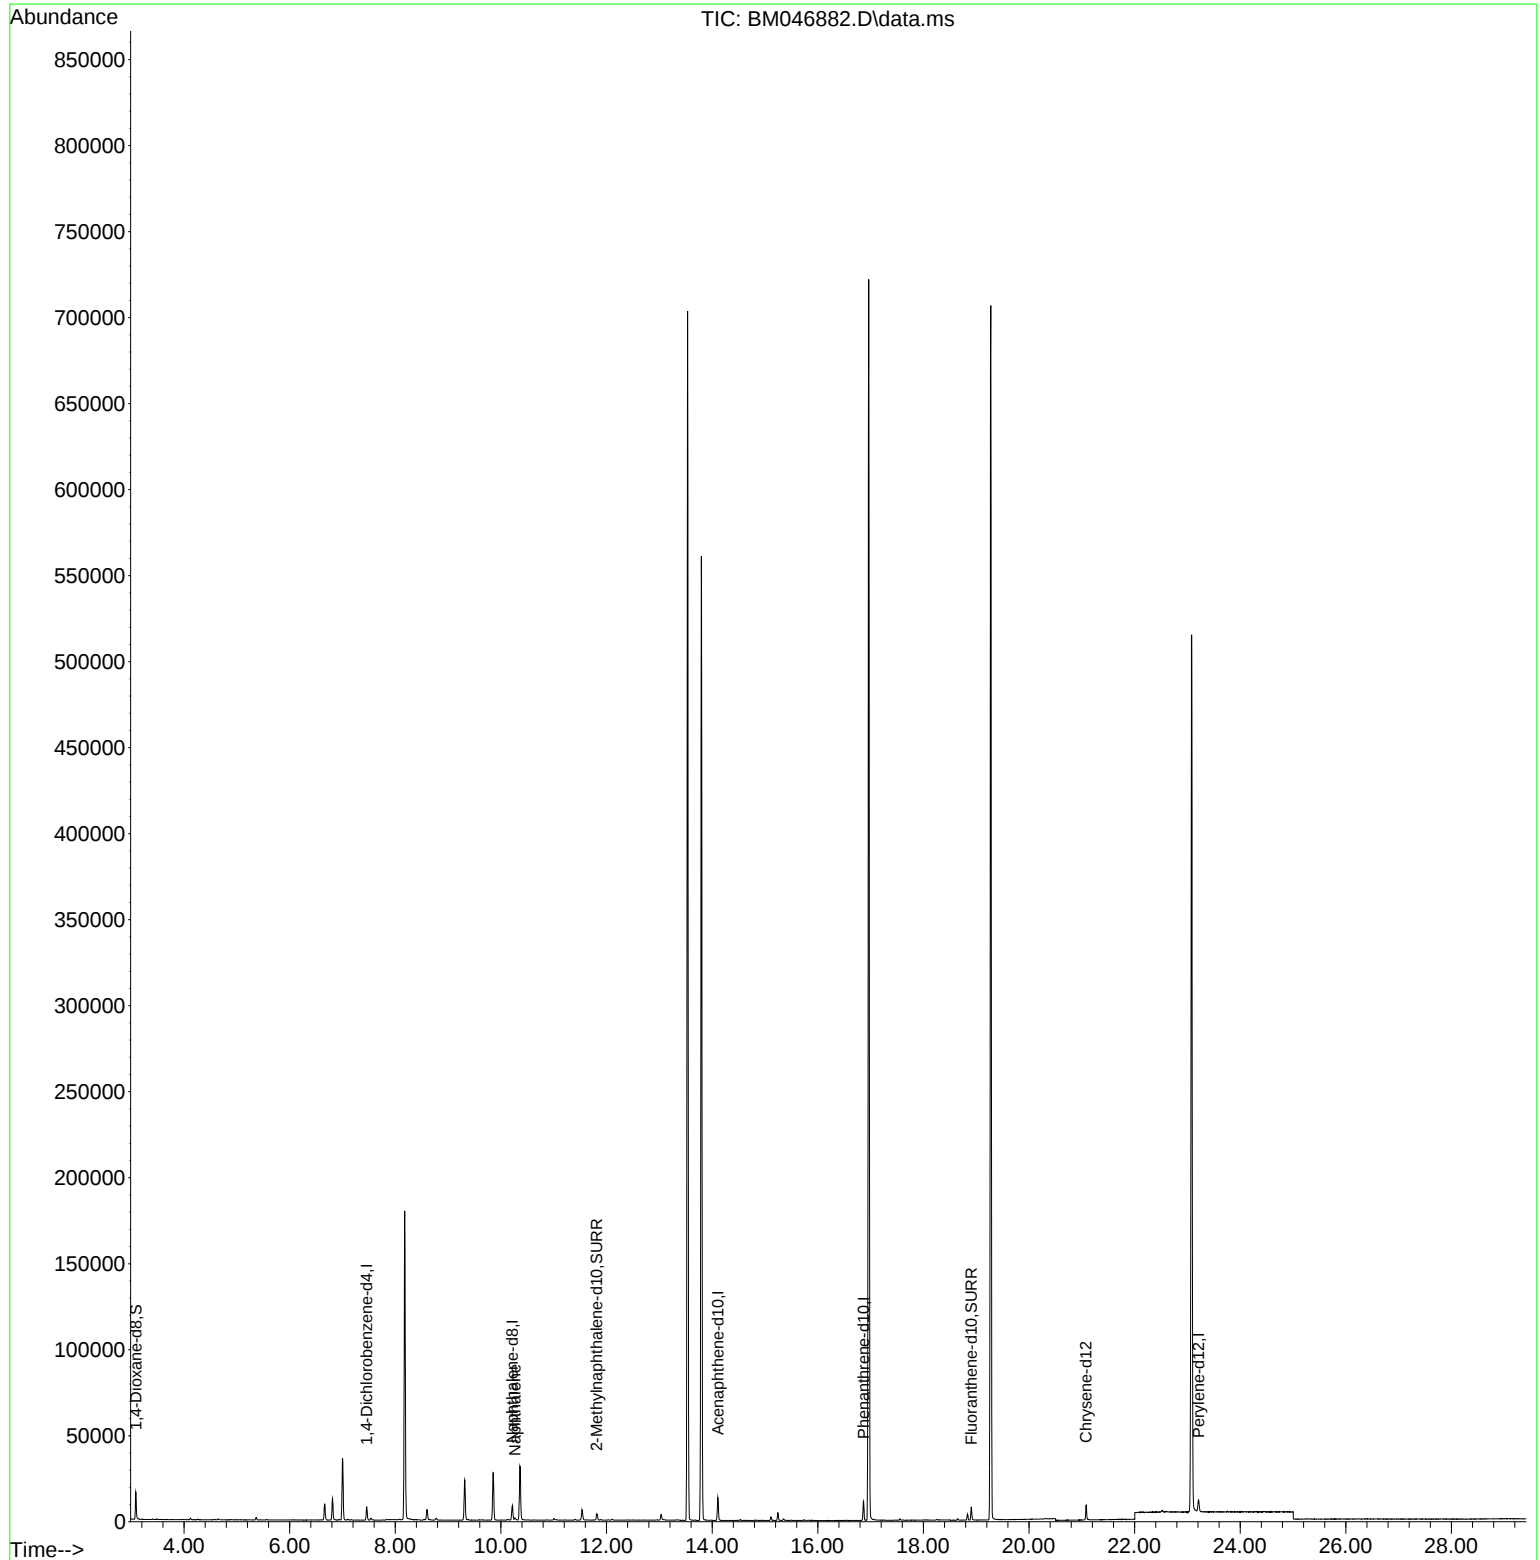

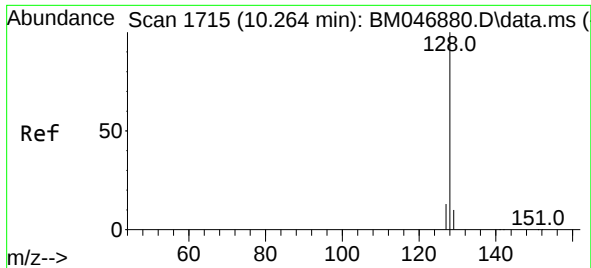

#5
Naphthalene
Concen: 0.050 ng/ul
RT: 10.266 min Scan# 11
Delta R.T. -0.011 min
Lab File: BM046882.D
Acq: 29 Jul 2024 14:13

Instrument :
BNA_M
ClientSampleId :
F7E85

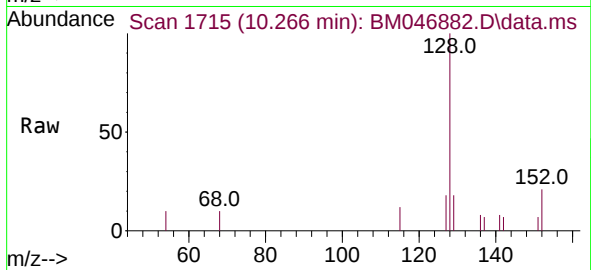

Tgt Ion:128 Resp: 1460
Ion Ratio Lower Upper
128 100
129 18.1 10.1 15.1
127 18.2 11.5 17.3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/30/2024
Supervised By :mohammad ahmed 08/03/2024

