

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
 Data File : BM046905.D
 Acq On : 30 Jul 2024 04:56
 Operator : MA/JU
 Sample : P3300-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 E1G91

Manual Integrations
APPROVED
 Reviewed By :Jagrut Upadhyay 07/30/2024
 Supervised By :mohammad ahmed 08/03/2024

Quant Time: Jul 30 05:30:20 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 04:18:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.451	152	3082	0.400	ng/ul	0.00
4) Naphthalene-d8	10.211	136	14980	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.100	164	5866	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.858	188	12030m	0.400	ng/ul	0.00
17) Chrysene-d12	21.073	240	7700	0.400	ng/ul	0.00
23) Perylene-d12	23.200	264	7292m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.084	96	7750	3.591	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.811	152	5051	0.212	ng/ul	0.00
18) Fluoranthene-d10	18.900	212	9679	0.386	ng/ul	0.00
Target Compounds						Qvalue
19) Fluoranthene	18.932	202	838	0.025	ng/ul#	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
 Data File : BM046905.D
 Acq On : 30 Jul 2024 04:56
 Operator : MA/JU
 Sample : P3300-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 E1G91

Quant Time: Jul 30 05:30:20 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 04:18:24 2024
 Response via : Initial Calibration


Manual Integrations
APPROVED
 Reviewed By :Jagrut Upadhyay 07/30/2024
 Supervised By :mohammad ahmed 08/03/2024

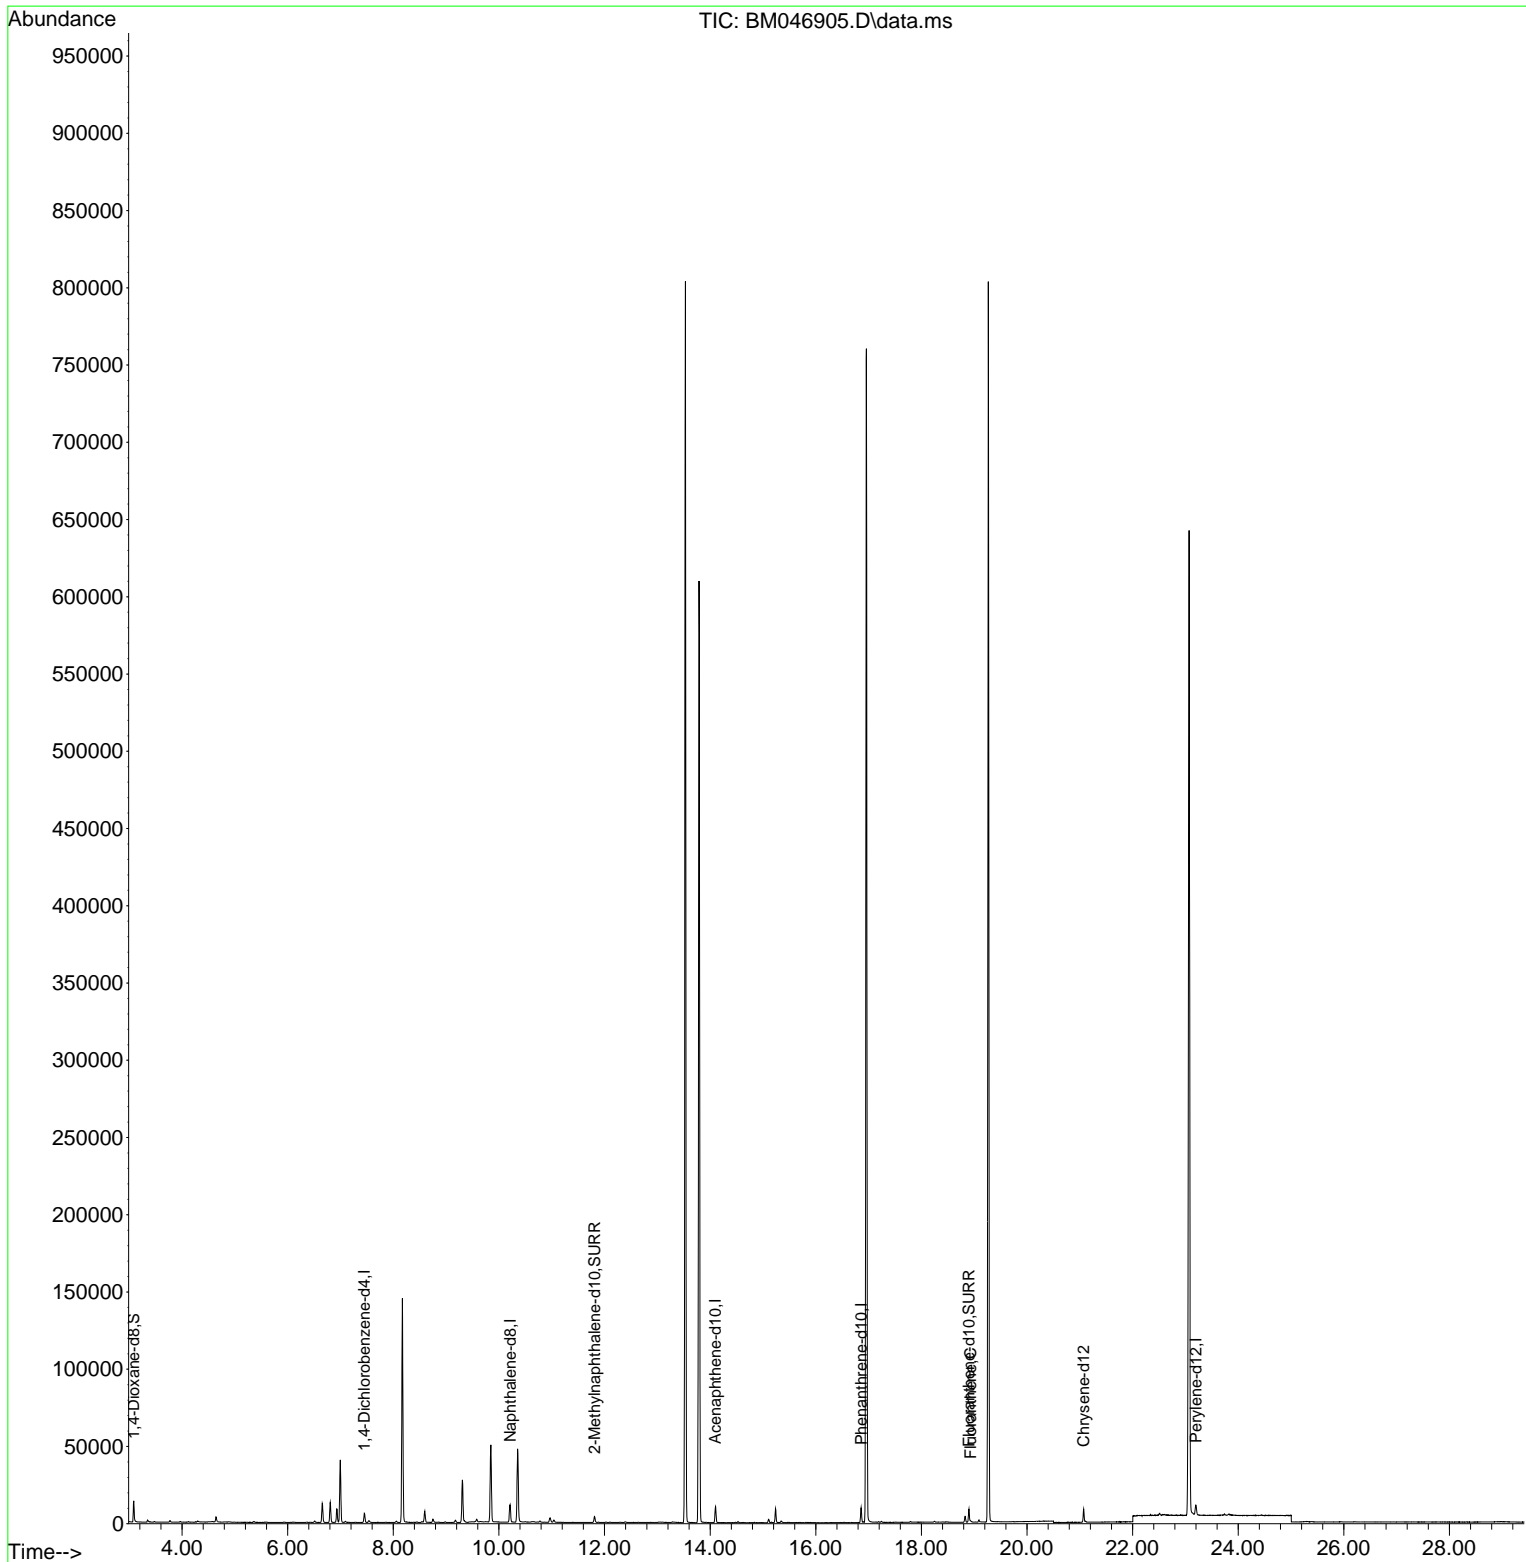

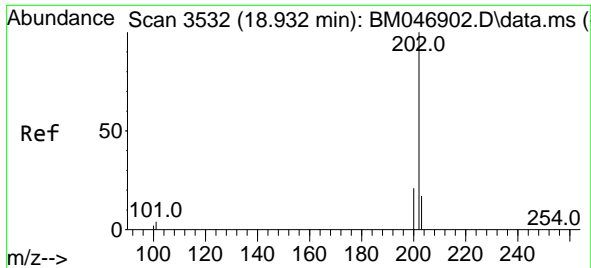

#19
 Fluoranthene
 Concen: 0.025 ng/ul
 RT: 18.932 min Scan# 3532
 Delta R.T. -0.000 min
 Lab File: BM046905.D
 Acq: 30 Jul 2024 04:56

Instrument :
 BNA_M
 ClientSampleId :
 E1G91

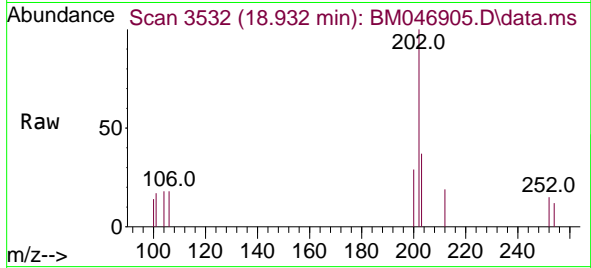

Tgt Ion: 202 Resp: 838

Ion	Ratio	Lower	Upper
202	100		
101	17.1	4.7	7.1
100	14.2	3.4	5.2

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 07/30/2024
 Supervised By :mohammad ahmed 08/03/2024

