

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
 Data File : BM046907.D
 Acq On : 30 Jul 2024 06:09
 Operator : MA/JU
 Sample : P3300-03
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1GD3

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 07/30/2024
 Supervised By :mohammad ahmed 08/03/2024

Quant Time: Jul 30 06:41:05 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 04:18:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.451	152	3100	0.400	ng/ul	0.00
4) Naphthalene-d8	10.209	136	9270	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.103	164	6159	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.857	188	11901m	0.400	ng/ul	0.00
17) Chrysene-d12	21.073	240	7048	0.400	ng/ul	0.00
23) Perylene-d12	23.201	264	6421m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.084	96	9587	4.417	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.810	152	5185	0.352	ng/ul	0.00
18) Fluoranthene-d10	18.898	212	8628	0.376	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.259	128	813	0.035	ng/ul#	79

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
Data File : BM046907.D
Acq On : 30 Jul 2024 06:09
Operator : MA/JU
Sample : P3300-03
Misc :
ALS Vial : 29 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
E1GD3

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/30/2024
Supervised By :mohammad ahmed 08/03/2024


Quant Time: Jul 30 06:41:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 04:18:24 2024
Response via : Initial Calibration

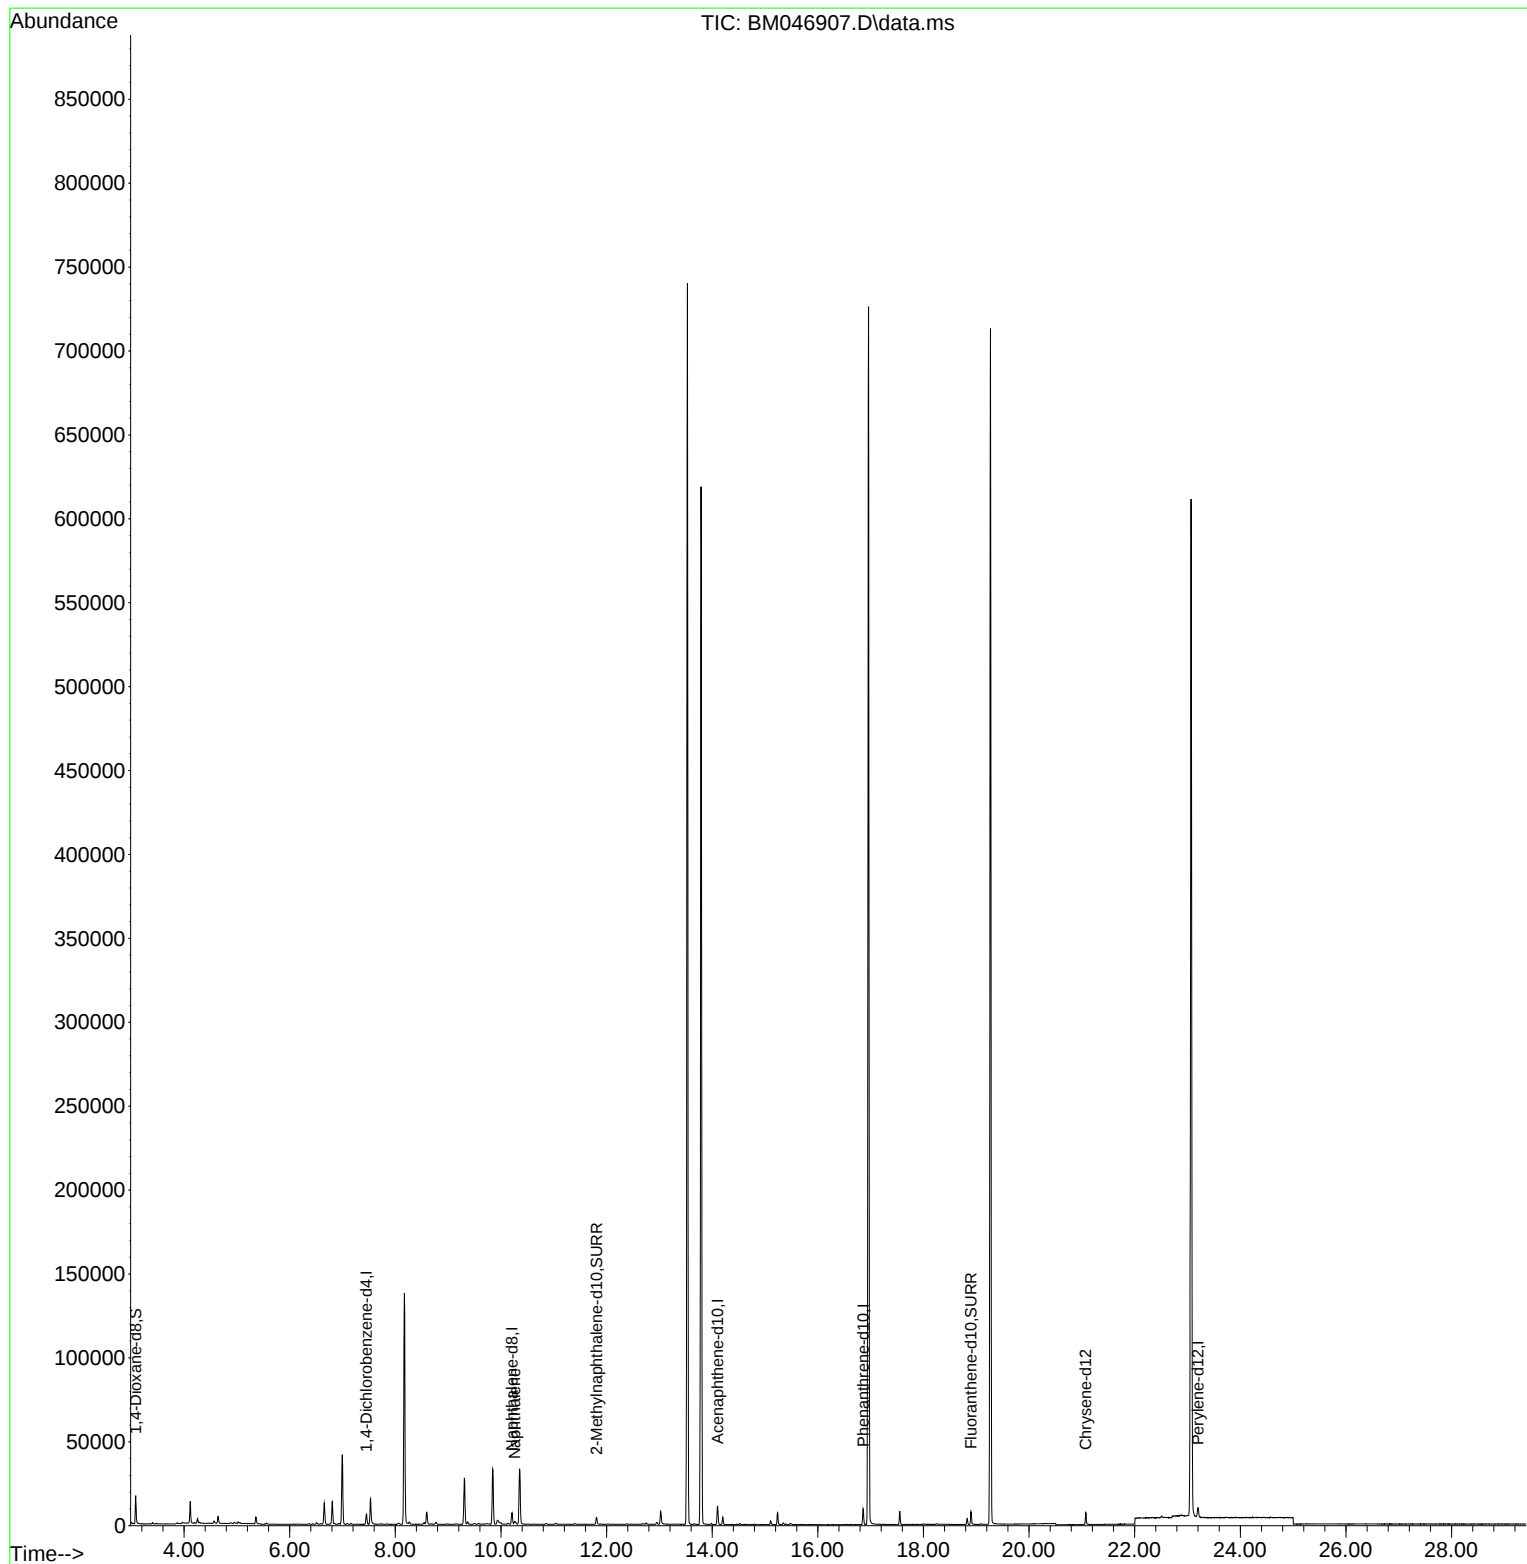

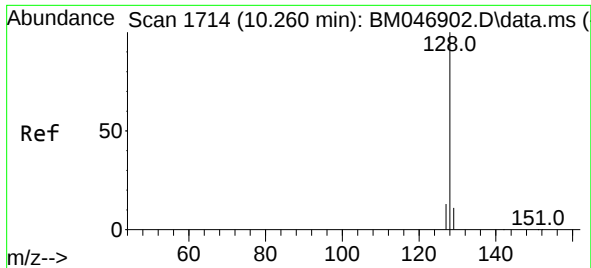

#5
Naphthalene
Concen: 0.035 ng/ul
RT: 10.259 min Scan# 11
Delta R.T. -0.001 min
Lab File: BM046907.D
Acq: 30 Jul 2024 06:09

Instrument :
BNA_M
ClientSampleId :
E1GD3

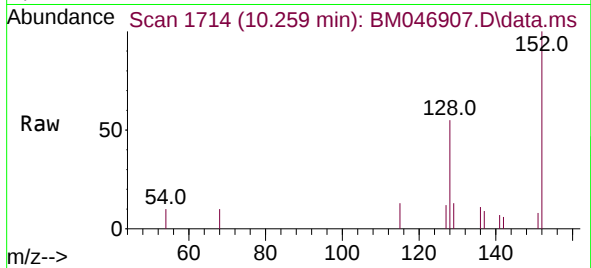

Tgt Ion:128 Resp: 811
Ion Ratio Lower Upper
128 100
129 22.8 10.1 15.1
127 21.3 11.5 17.3

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/30/2024
Supervised By :mohammad ahmed 08/03/2024

