

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
 Data File : BM046916.D
 Acq On : 30 Jul 2024 11:38
 Operator : MA/JU
 Sample : P3336-04
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F7E12

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 07/30/2024
 Supervised By :mohammad ahmed 08/03/2024

Quant Time: Jul 30 13:31:14 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 04:18:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.451	152	2309	0.400	ng/ul	0.00
4) Naphthalene-d8	10.204	136	13517	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.098	164	4542	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.857	188	8907m	0.400	ng/ul	0.00
17) Chrysene-d12	21.073	240	5463	0.400	ng/ul	0.00
23) Perylene-d12	23.195	264	5153m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.084	96	6409	3.964	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.810	152	3252	0.151	ng/ul	0.00
18) Fluoranthene-d10	18.899	212	5415	0.304	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.253	128	1387	0.041	ng/ul#	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
Data File : BM046916.D
Acq On : 30 Jul 2024 11:38
Operator : MA/JU
Sample : P3336-04
Misc :
ALS Vial : 38 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
F7E12

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/30/2024
Supervised By :mohammad ahmed 08/03/2024


Quant Time: Jul 30 13:31:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 04:18:24 2024
Response via : Initial Calibration

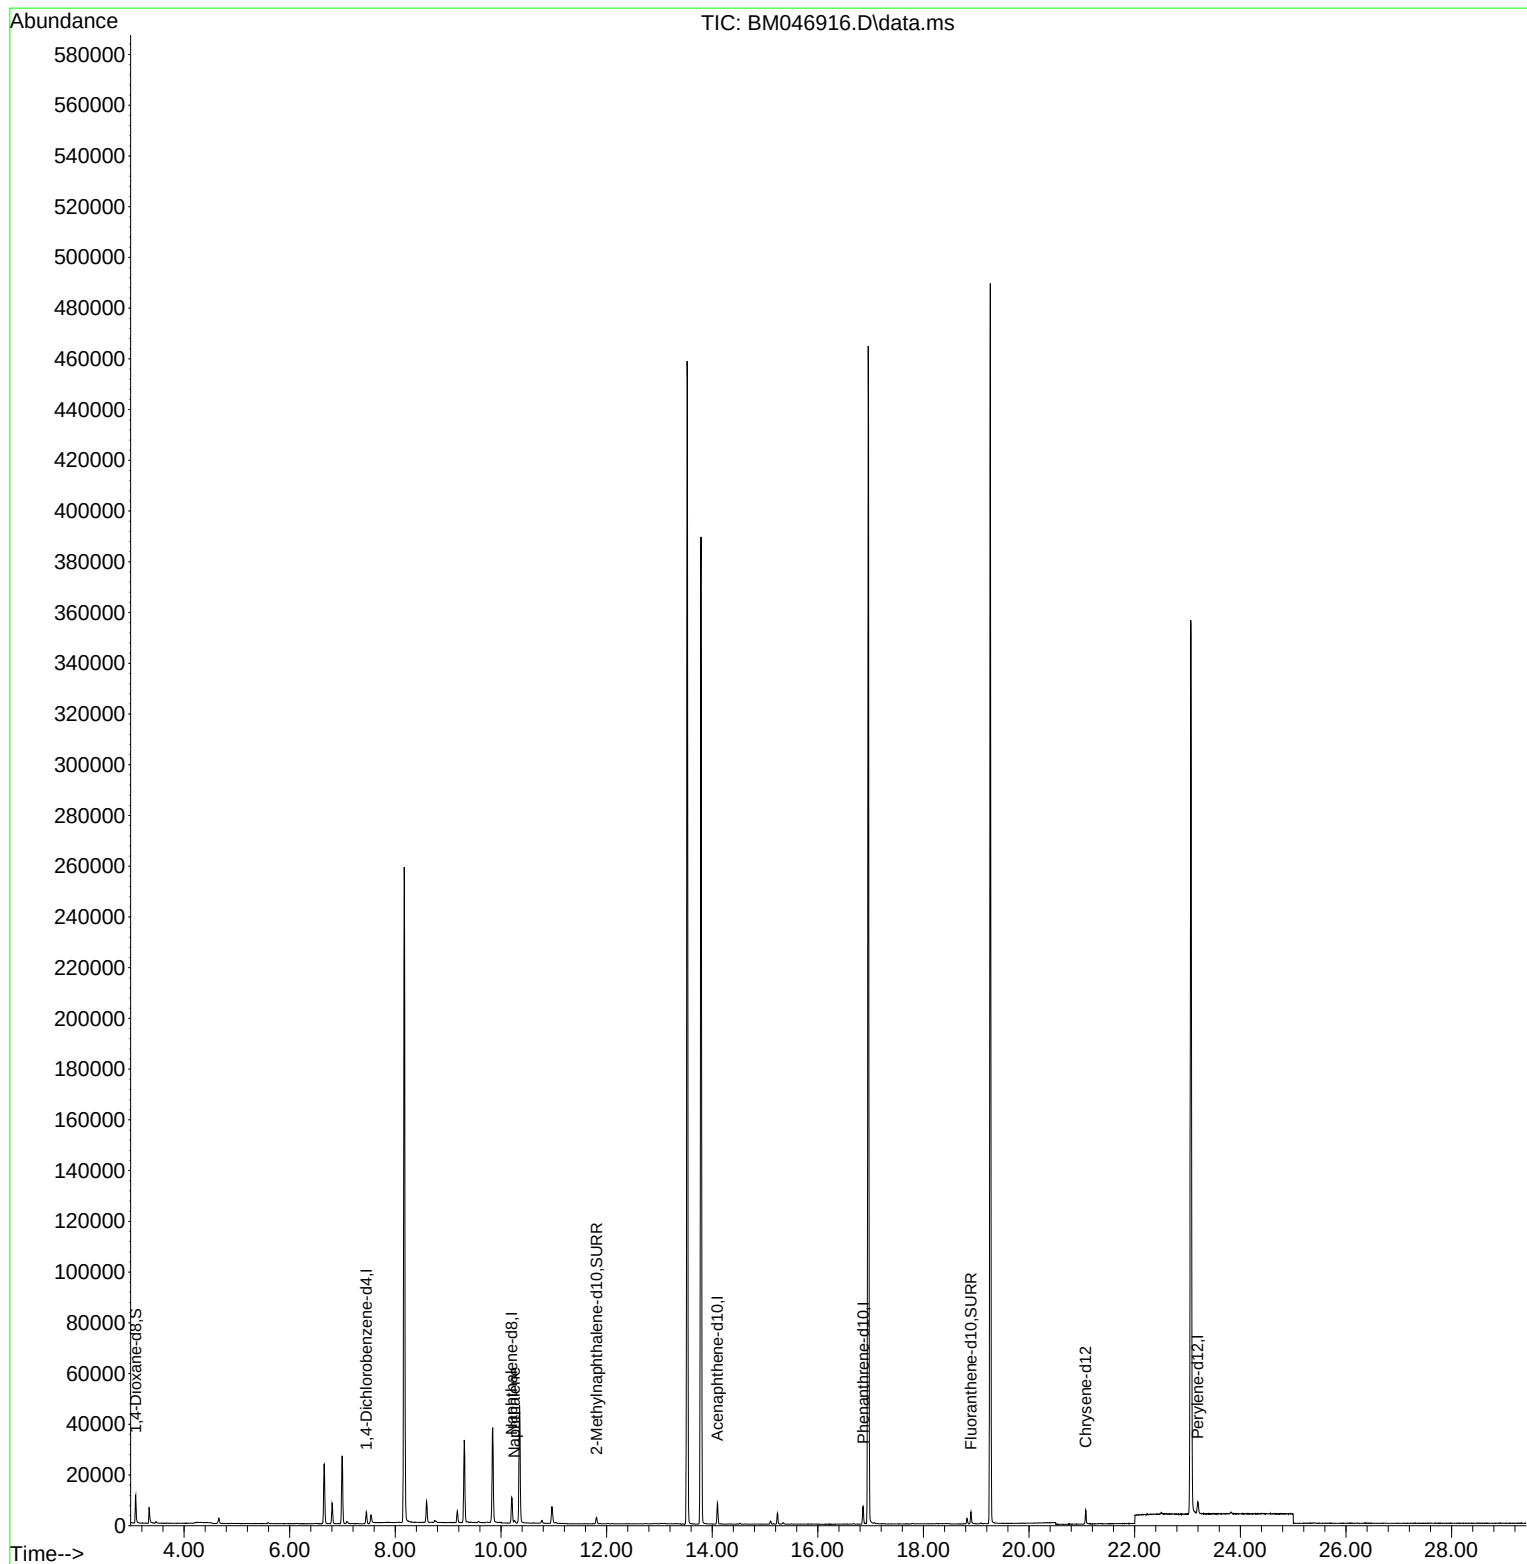

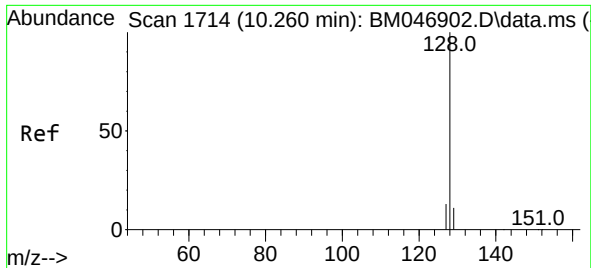

#5
Naphthalene
Concen: 0.041 ng/ul
RT: 10.253 min Scan# 11
Delta R.T. -0.007 min
Lab File: BM046916.D
Acq: 30 Jul 2024 11:38

Instrument :
BNA_M
ClientSampleId :
F7E12

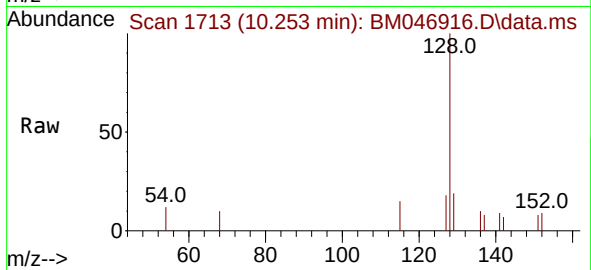

Tgt Ion:128 Resp: 138
Ion Ratio Lower Upper
128 100
129 18.6 10.1 15.1
127 17.7 11.5 17.3

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/30/2024
Supervised By :mohammad ahmed 08/03/2024

