

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
 Data File : BM046927.D
 Acq On : 30 Jul 2024 20:01
 Operator : MA/JU
 Sample : P3329-18DL 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F7E26DL

Quant Time: Jul 31 00:01:02 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 04:18:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.447	152	2714	0.400	ng/ul	0.00
4) Naphthalene-d8	10.200	136	6941	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.095	164	4502	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.854	188	9662	0.400	ng/ul	0.00
17) Chrysene-d12	21.070	240	7363	0.400	ng/ul	0.00
23) Perylene-d12	23.191	264	8911	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.084	96	1561	0.821	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.805	152	537	0.049	ng/ul	0.00
18) Fluoranthene-d10	18.895	212	1041	0.043	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.249	128	5691	0.324	ng/ul	99
7) 2-Methylnaphthalene	11.882	142	677	0.056	ng/ul	99
8) 1-Methylnaphthalene	12.102	142	281	0.023	ng/ul	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
Data File : BM046927.D
Acq On : 30 Jul 2024 20:01
Operator : MA/JU
Sample : P3329-18DL 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7E26DL


Quant Time: Jul 31 00:01:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 04:18:24 2024
Response via : Initial Calibration

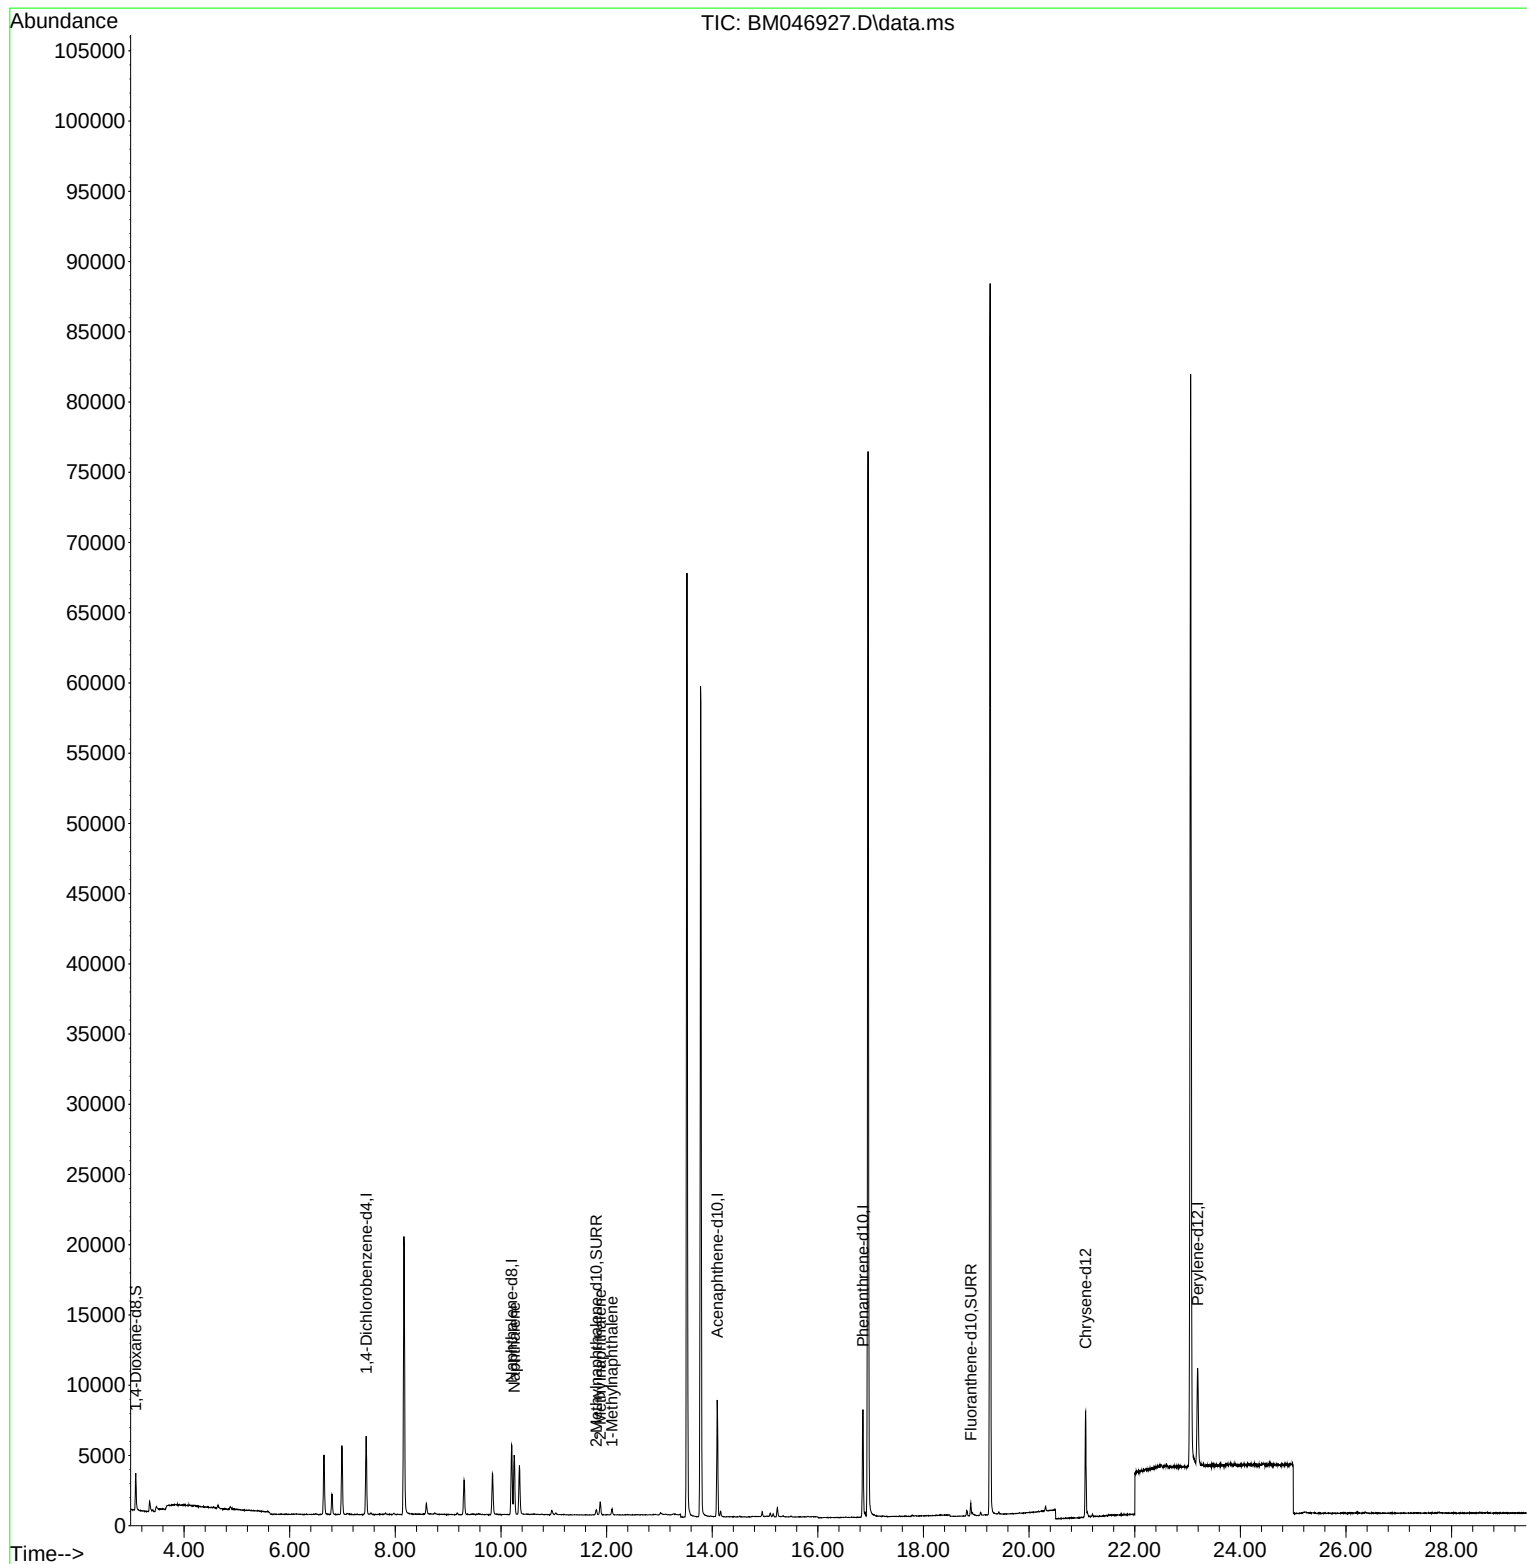



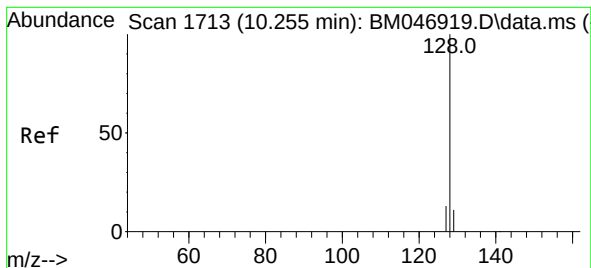


#5
Naphthalene
Concen: 0.324 ng/ul
RT: 10.249 min Scan# 1
Delta R.T. -0.011 min
Lab File: BM046927.D
Acq: 30 Jul 2024 20:01

Instrument :
BNA_M
ClientSampleId :
F7E26DL



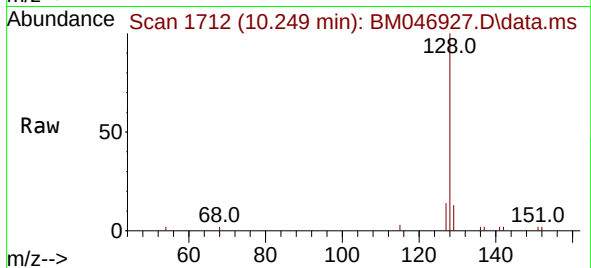



Tgt Ion:128 Resp: 5691
Ion Ratio Lower Upper
128 100
129 12.6 10.1 15.1
127 14.0 11.5 17.3

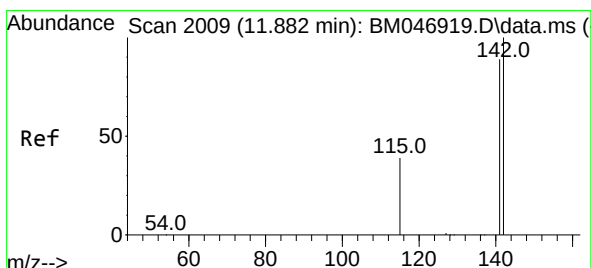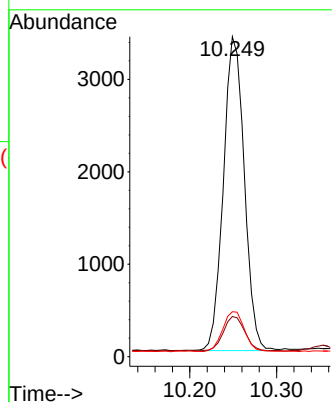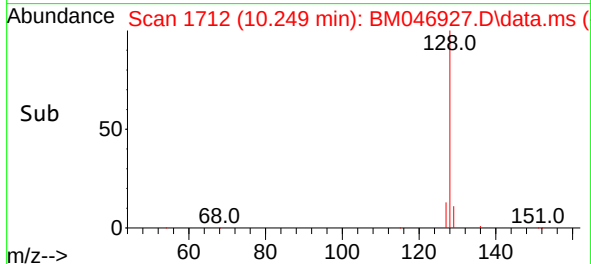

#7
2-Methylnaphthalene
Concen: 0.056 ng/ul
RT: 11.882 min Scan# 2009
Delta R.T. -0.006 min
Lab File: BM046927.D
Acq: 30 Jul 2024 20:01

Tgt Ion:142 Resp: 677
Ion Ratio Lower Upper
142 100
141 87.0 70.5 105.7

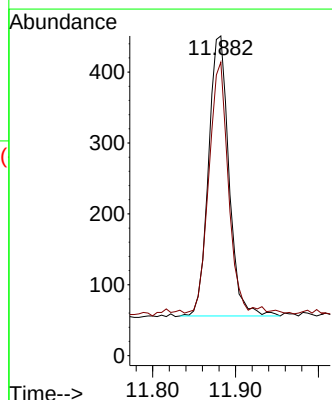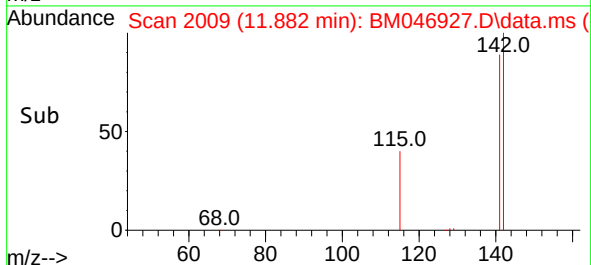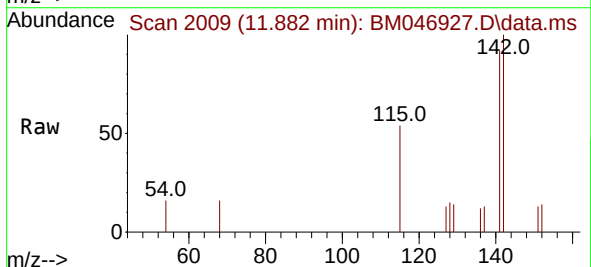

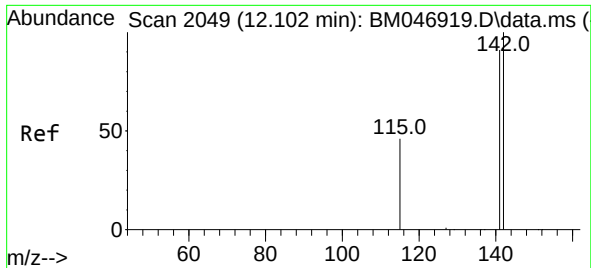

#8
 1-Methylnaphthalene
 Concen: 0.023 ng/ul
 RT: 12.102 min Scan# 2049
 Delta R.T. -0.006 min
 Lab File: BM046927.D
 Acq: 30 Jul 2024 20:01

Instrument :
 BNA_M
 ClientSampleId :
 F7E26DL

Tgt Ion:142 Resp: 281
 Ion Ratio Lower Upper
 142 100
 141 96.1 73.1 109.7

