

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM073119\
 Data File : BM021756.D
 Acq On : 31 Jul 2019 22:21
 Operator : HP/JU
 Sample : PB120381BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Aug 01 02:37:14 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM073119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 31 15:40:15 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	2091	0.40	ng/ul	0.00
2) Naphthalene-d8	10.44	136	5398	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.31	164	2085	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.17	188	1087097	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.27
20) Perylene-d12	23.35	264	1354517	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.06	152	1882	0.29	ng/ul	-0.01
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.31	166	1960	0.208	ng/ul#	Ovalue 11




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM073119\
Data File : BM021756.D
Acq On : 31 Jul 2019 22:21
Operator : HP/JU
Sample : PB120381BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Aug 01 02:37:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM073119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 31 15:40:15 2019
Response via : Initial Calibration

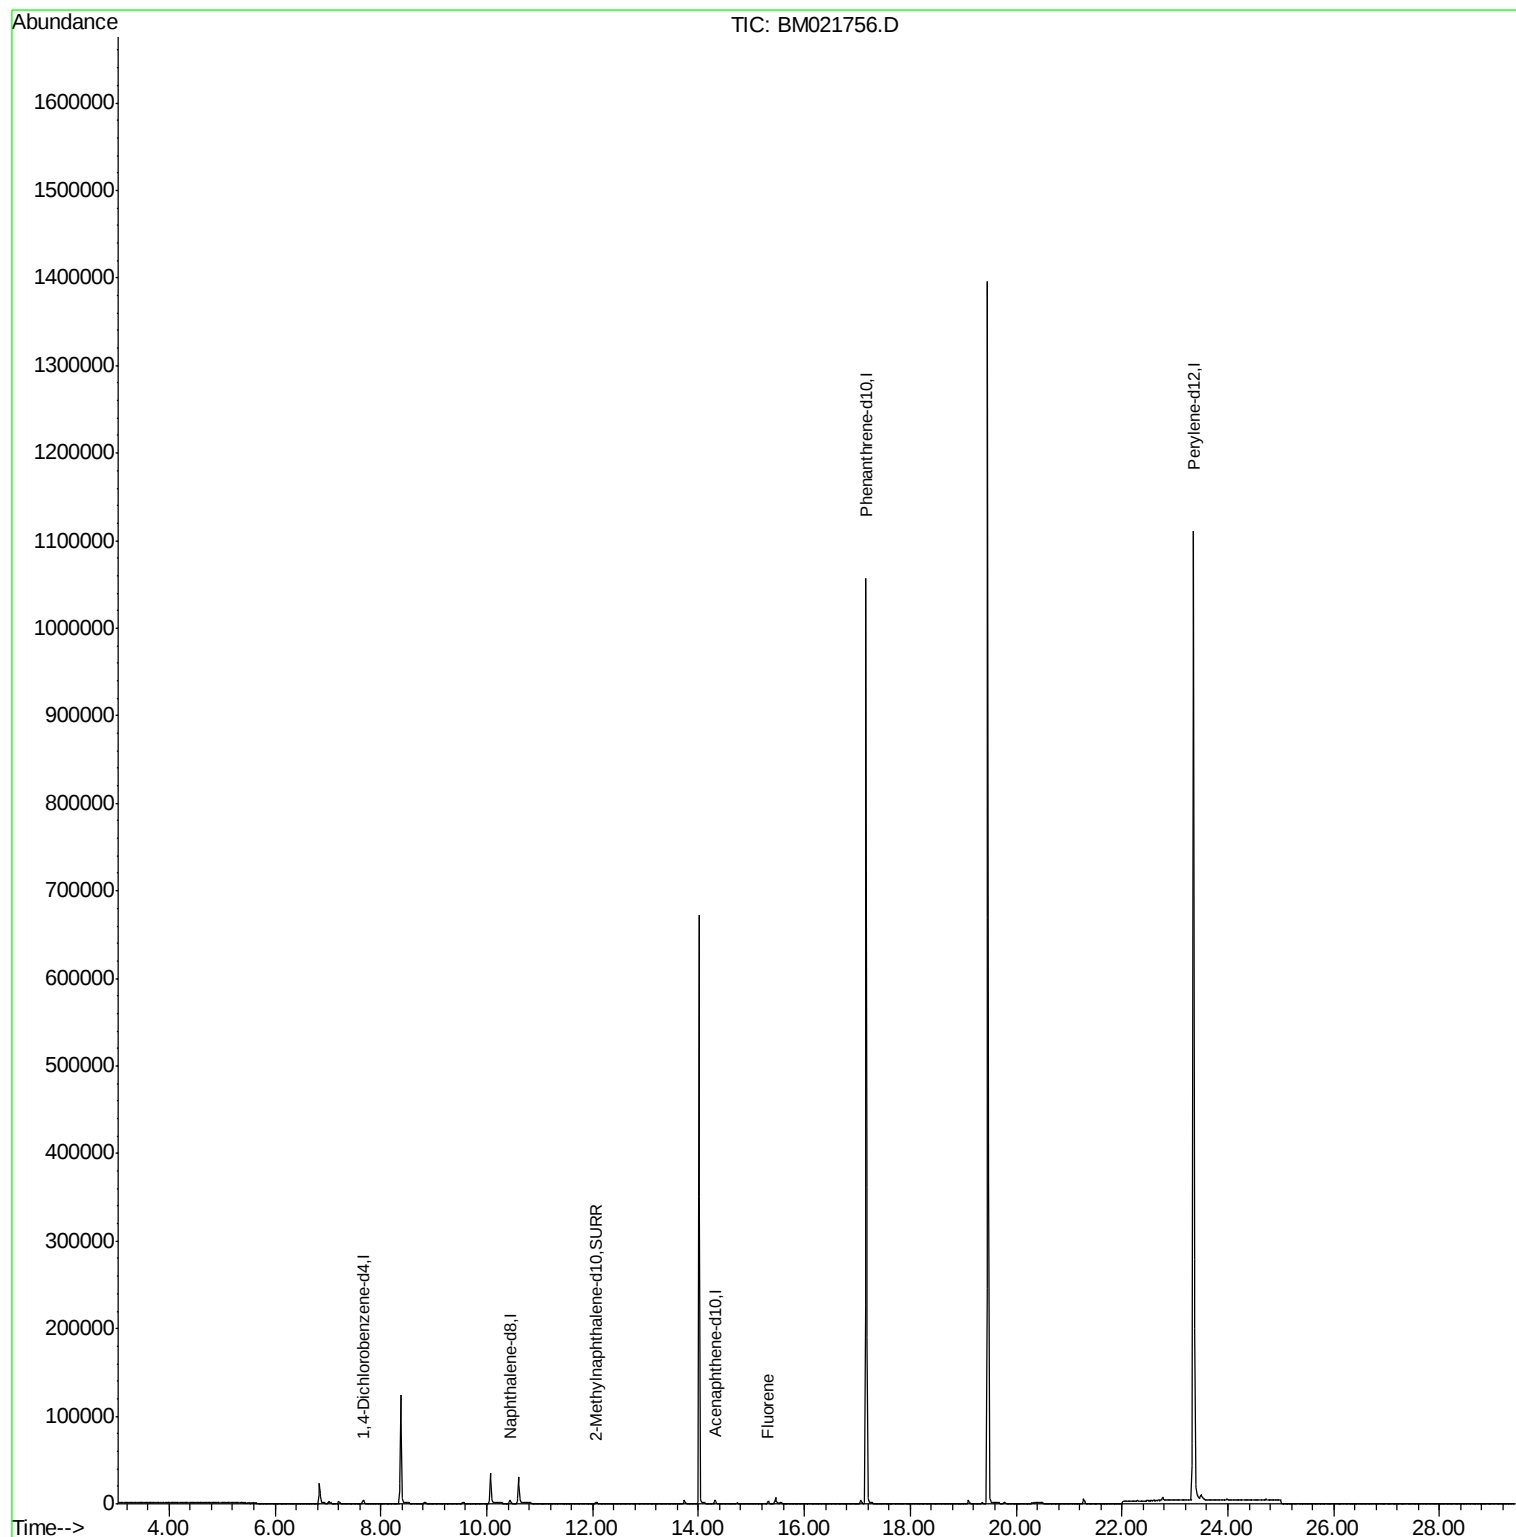

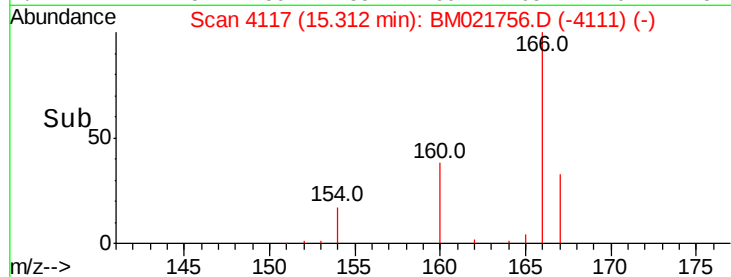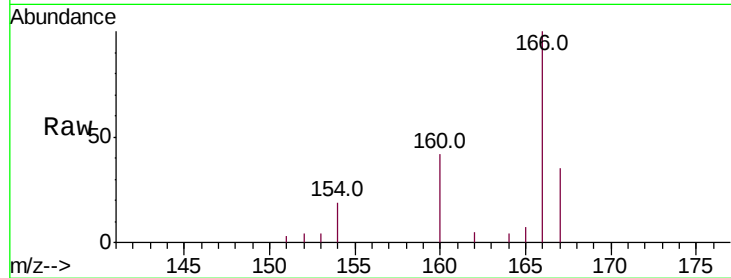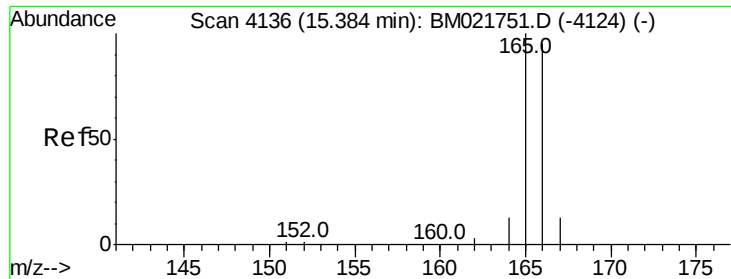

#9

Fluorene

Concen: 0.208 ng/ul

RT: 15.31 min Scan# 4117

Delta R.T. -0.08 min

Lab File: BM021756.D

Acq: 31 Jul 2019 22:21

Instrument :

BNA_M

ClientSampleId :

Tot Ion:166 Resp: 1960

Ion Ratio Lower Upper

166 100

165 7.1 85.2 127.8#

167 34.7 13.0 19.6#

