

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM073119\
 Data File : BM021757.D
 Acq On : 31 Jul 2019 22:57
 Operator : HP/JU
 Sample : K3215-01RE
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Aug 01 02:37:18 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM073119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 31 15:40:15 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	2255	0.40	ng/ul	0.00
2) Naphthalene-d8	10.44	136	5844	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.31	164	2268	0.40	ng/ul	-0.01
10) Phenanthrene-d10	17.17	188	1209495	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.27
20) Perylene-d12	23.35	264	1352163	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.06	152	1824	0.26	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.31	166	2145	0.209	ng/ul#	11


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM073119\
Data File : BM021757.D
Acq On : 31 Jul 2019 22:57
Operator : HP/JU
Sample : K3215-01RE
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Aug 01 02:37:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM073119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 31 15:40:15 2019
Response via : Initial Calibration

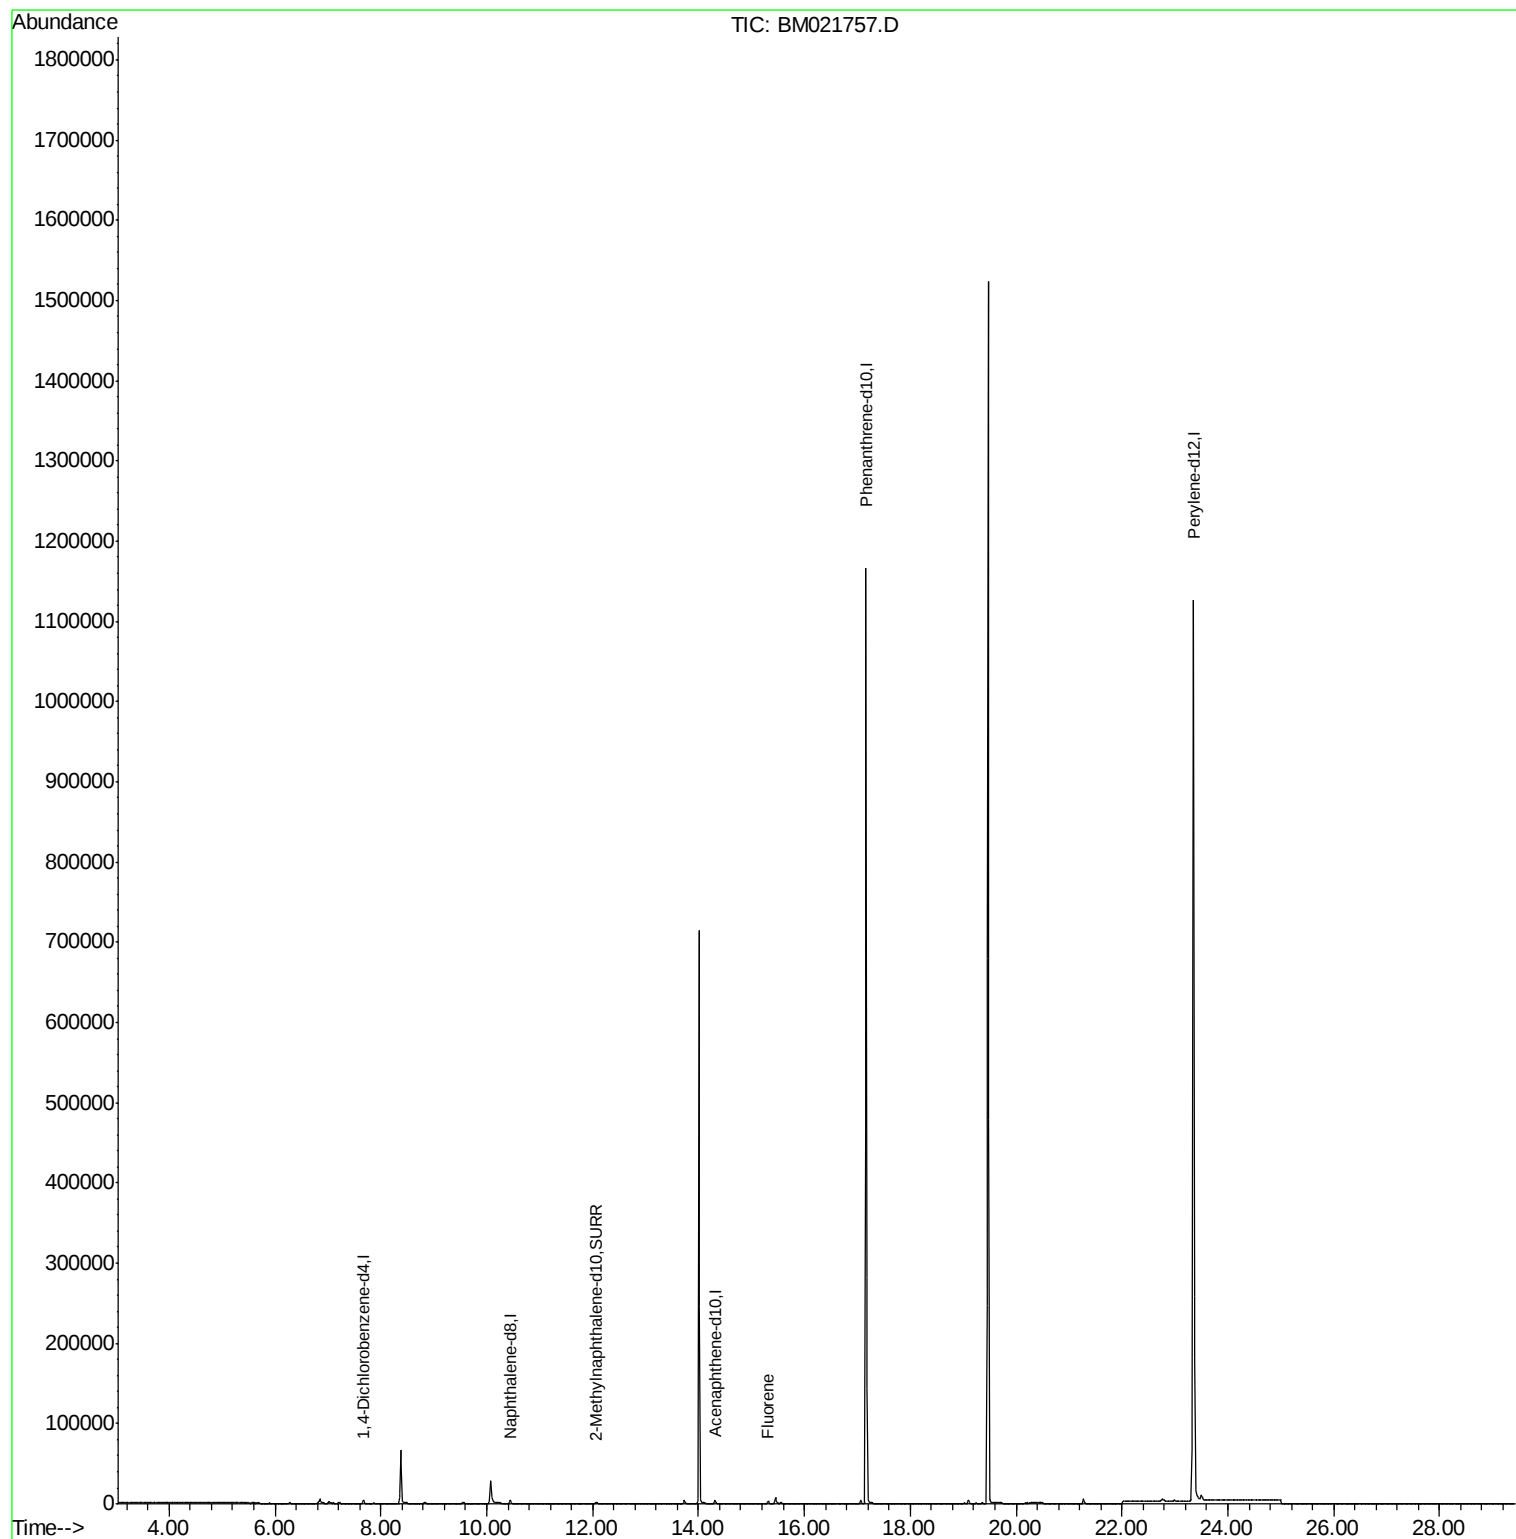

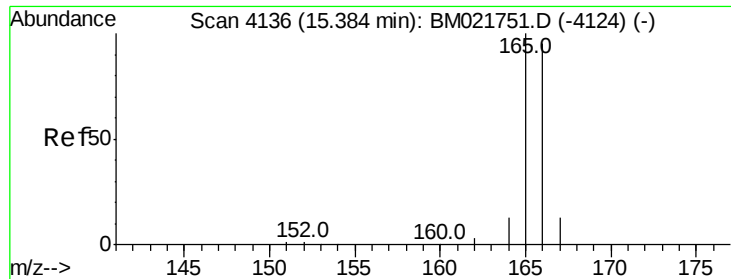

#9

Fluorene

Concen: 0.209 ng/ul

RT: 15.31 min Scan# 4117

Delta R.T. -0.08 min

Lab File: BM021757.D

Acq: 31 Jul 2019 22:57

Instrument :

BNA_M

ClientSampleId :


Tot Ion:166 Resp: 2145

Ion Ratio Lower Upper

166 100

165 7.3 85.2 127.8#

167 36.3 13.0 19.6#

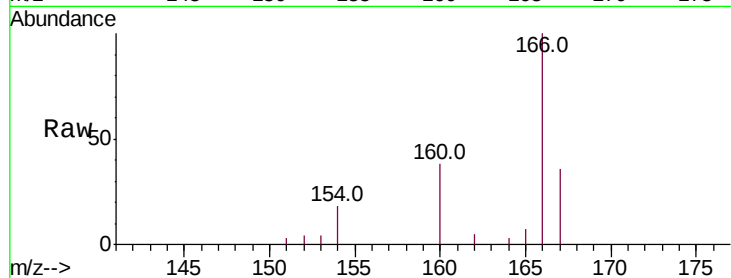

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

