

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM073123\
 Data File : BM041193.D
 Acq On : 31 Jul 2023 17:26
 Operator : MA/JU
 Sample : 03788-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CHRT-20430

Quant Time: Jul 31 17:56:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 31 16:29:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.798	152	123067	20.000	ng	0.00
21) Naphthalene-d8	10.604	136	483167	20.000	ng	0.00
39) Acenaphthene-d10	14.463	164	285785	20.000	ng	0.00
64) Phenanthrene-d10	17.227	188	540705	20.000	ng	# 0.00
76) Chrysene-d12	21.427	240	512705	20.000	ng	0.00
86) Perylene-d12	23.797	264	601989	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.369	112	756088	91.823	ng	0.00
7) Phenol-d6	6.975	99	965852	90.491	ng	0.00
23) Nitrobenzene-d5	8.975	82	581303	55.950	ng	0.00
42) 2,4,6-Tribromophenol	15.968	330	313968	77.671	ng	0.00
45) 2-Fluorobiphenyl	13.080	172	957252	42.313	ng	0.00
79) Terphenyl-d14	19.862	244	1188316	41.906	ng	0.00
Target Compounds						
						Qvalue
32) Benzoic acid	9.975	122	54	7.164	ng	# 1
49) Acenaphthylene	14.186	152	63024	2.257	ng	# 85
50) Dimethylphthalate	14.016	163	72951	3.394	ng	# 92
53) 3-Nitroaniline	14.410	138	3920	3.297	ng	# 21
54) 2,4-Dinitrophenol	14.857	184	407	5.960	ng	# 1
57) 2,4-Dinitrotoluene	14.874	165	2971	3.112	ng	# 45
58) Fluorene	15.521	166	44663	2.063	ng	# 85
62) 4-Nitroaniline	15.339	138	18971	7.796	ng	80
71) Phenanthrene	17.268	178	712169	23.706	ng	# 96
72) Anthracene	17.268	178	712169	23.969	ng	96
73) Carbazole	17.645	167	89435	3.326	ng	# 65
75) Fluoranthene	19.298	202	1454047	43.081	ng	98
78) Pyrene	19.662	202	1398963	39.018	ng	99
81) Benzo(a)anthracene	21.409	228	789492	22.714	ng	99
83) Chrysene	21.462	228	1076656	32.026	ng	98
84) Bis(2-ethylhexyl)phtha...	21.333	149	193177	11.338	ng	# 96
87) Indeno(1,2,3-cd)pyrene	26.238	276	450217	10.172	ng	# 93
88) Benzo(b)fluoranthene	23.080	252	1274030	35.625	ng	98
89) Benzo(k)fluoranthene	23.080	252	1274030	34.828	ng	98
90) Benzo(a)pyrene	23.692	252	692559	20.155	ng	98
92) Benzo(g,h,i)perylene	26.991	276	401686	11.120	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM073123\
Data File : BM041193.D
Acq On : 31 Jul 2023 17:26
Operator : MA/JU
Sample : 03788-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CHRT-20430

Quant Time: Jul 31 17:56:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 31 16:29:28 2023
Response via : Initial Calibration

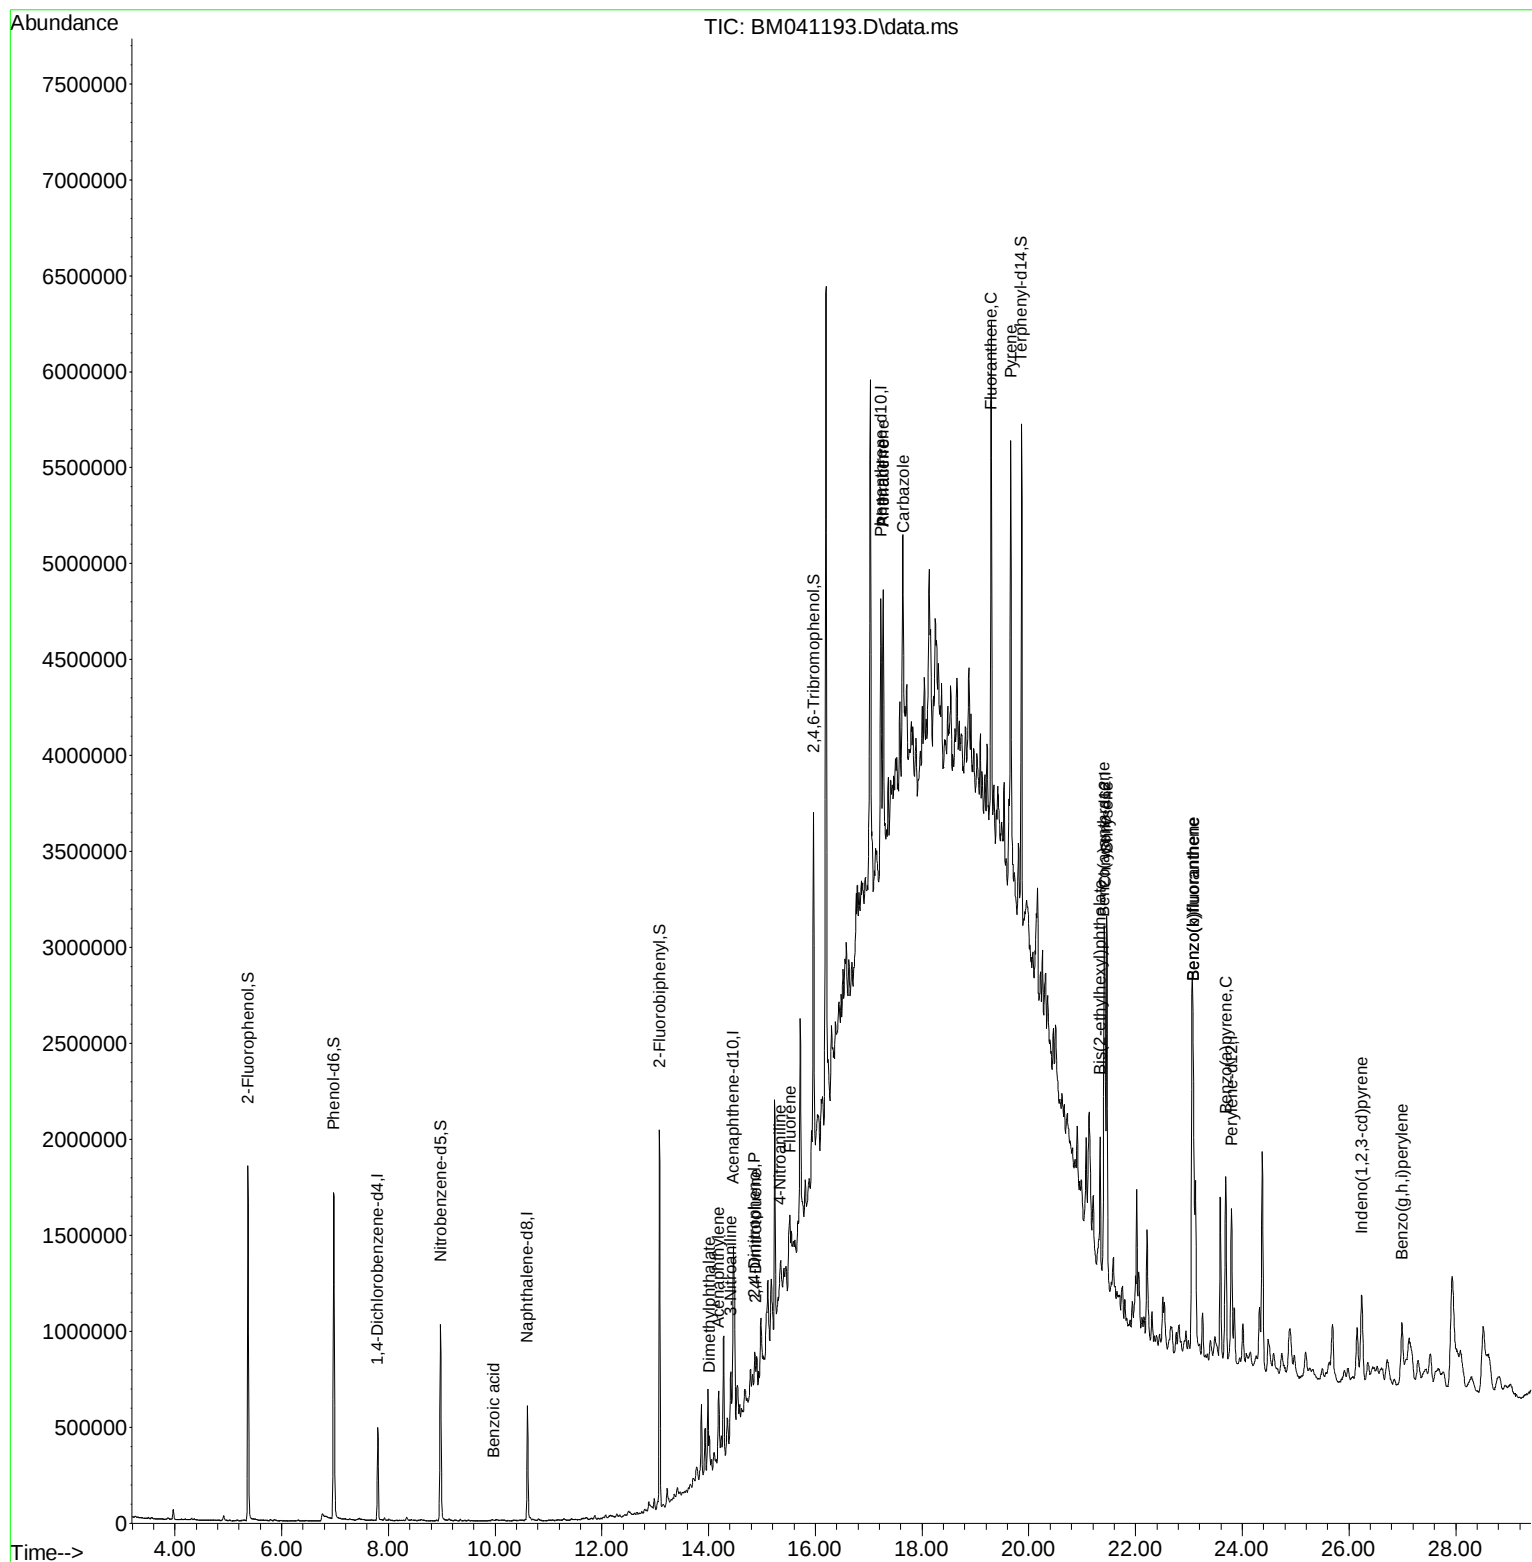

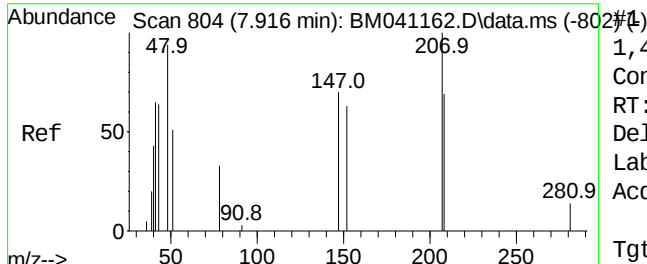

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 7.798 min Scan#

Delta R.T. 0.000 min

Lab File: BM041193.D

Acq: 31 Jul 2023 17:26

Instrument :

BNA_M

ClientSampleId :

CHRT-20430





Tgt Ion:152 Resp: 123067

Ion Ratio Lower Upper

152 100

150 155.7 125.5 188.3

115 58.8 48.0 72.0

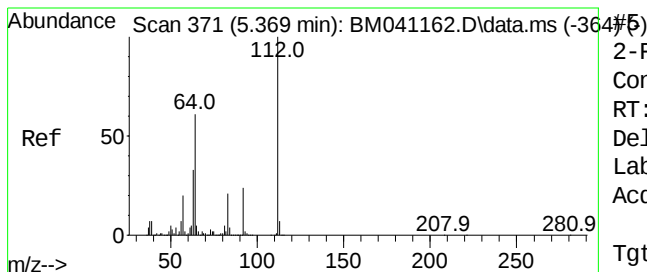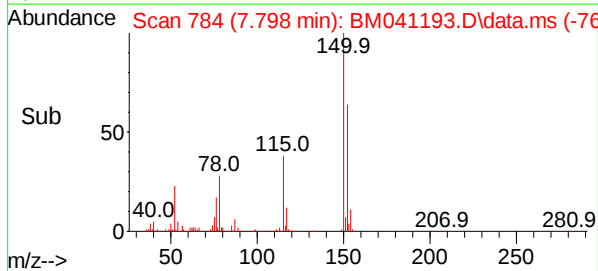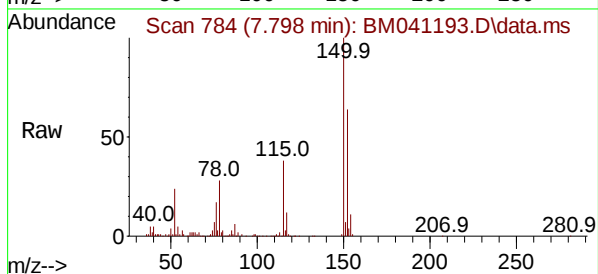

2-Fluorophenol

Concen: 91.823 ng

RT: 5.369 min Scan# 371

Delta R.T. 0.006 min

Lab File: BM041193.D

Acq: 31 Jul 2023 17:26




Tgt Ion:112 Resp: 756088


Ion Ratio Lower Upper

112 100

64 59.0 48.5 72.7

63 32.1 26.5 39.7

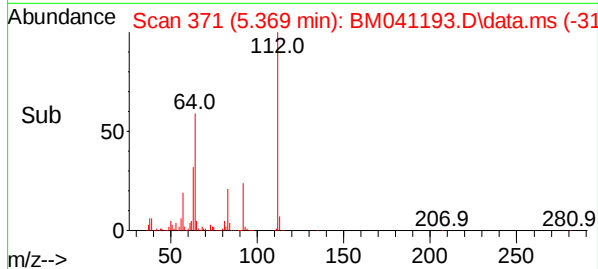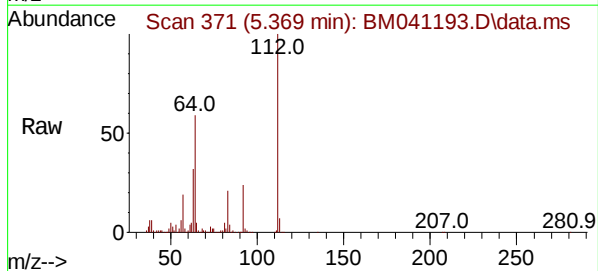

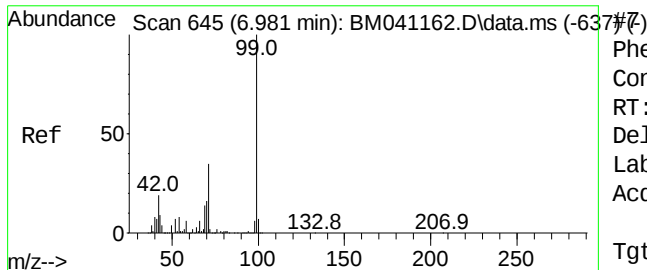

Phenol-d6

Concen: 90.491 ng

RT: 6.975 min Scan#

Delta R.T. 0.000 min

Lab File: BM041193.D

Acq: 31 Jul 2023 17:26

Instrument :

BNA_M

ClientSampleId :

CHRT-20430





Tgt Ion: 99 Resp: 965852

Ion Ratio Lower Upper

99 100

42 19.0 15.4 23.0

71 35.6 28.2 42.4

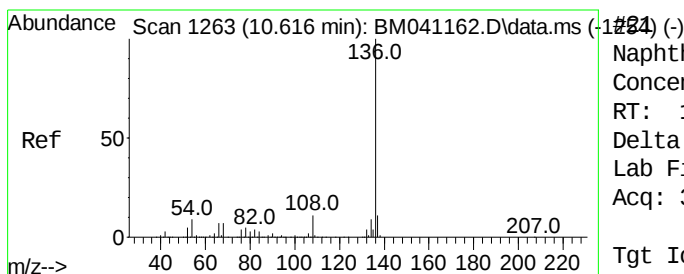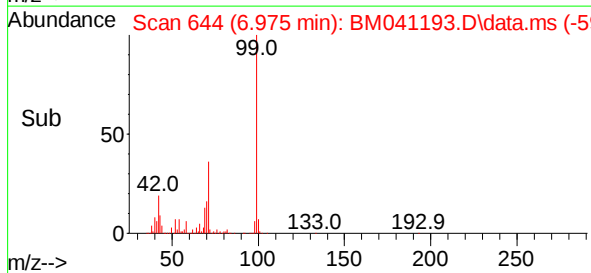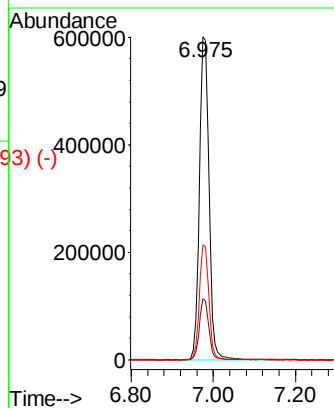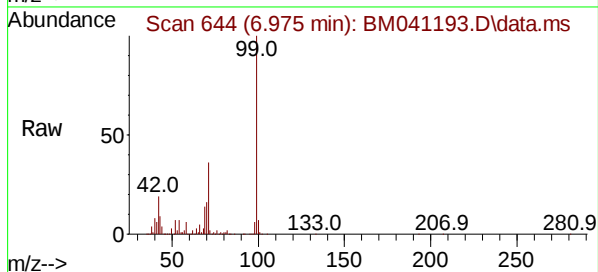

Naphthalene-d8

Concen: 20.000 ng

RT: 10.604 min Scan# 1261

Delta R.T. 0.000 min

Lab File: BM041193.D

Acq: 31 Jul 2023 17:26

Tgt Ion: 136 Resp: 483167




Ion Ratio Lower Upper


136 100

137 10.9 8.8 13.2

54 8.2 6.9 10.3

68 6.3 5.4 8.2


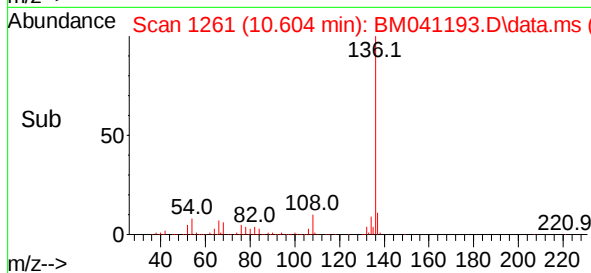

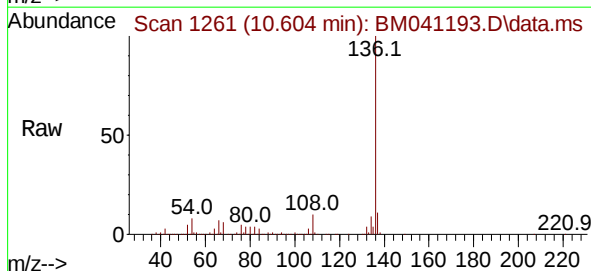


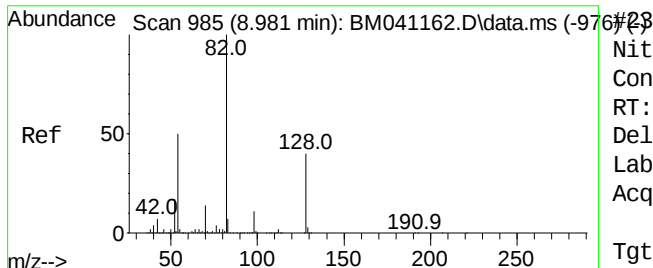

Nitrobenzene-d5
Concen: 55.950 ng
RT: 8.975 min Scan# 985
Delta R.T. 0.000 min
Lab File: BM041193.D
Acq: 31 Jul 2023 17:26




Instrument :
BNA_M
ClientSampleId :
CHRT-20430


Tgt Ion:	82	Resp:	581303
Ion	Ratio	Lower	Upper
82	100		
128	41.1	31.8	47.6
54	48.5	40.1	60.1

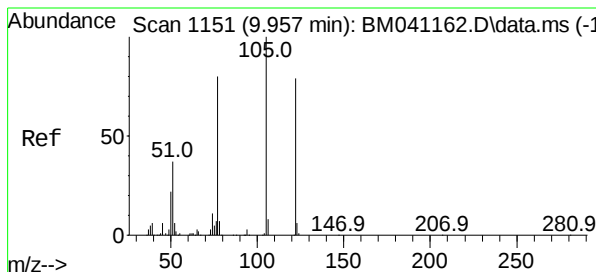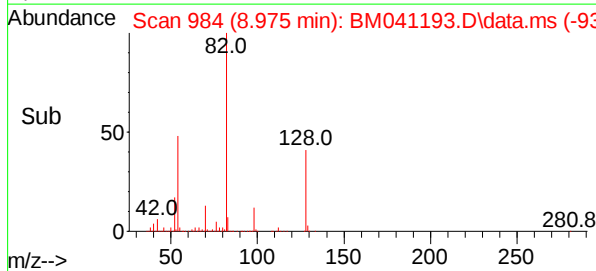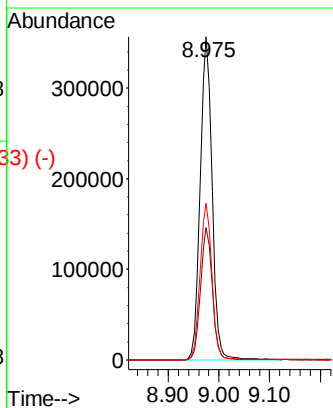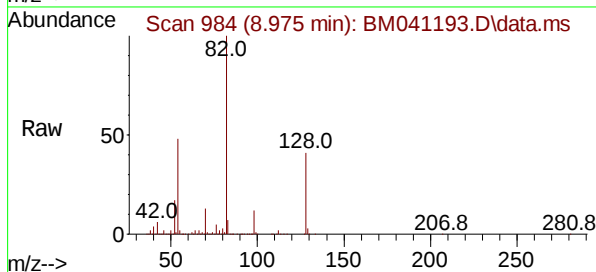

Benzoic acid
Concen: 7.164 ng
RT: 9.975 min Scan# 1154
Delta R.T. 0.029 min
Lab File: BM041193.D
Acq: 31 Jul 2023 17:26

Tgt Ion:	122	Resp:	54
Ion	Ratio	Lower	Upper
122	100		
105	190.9	104.0	144.0#
77	449.4	79.9	119.9#

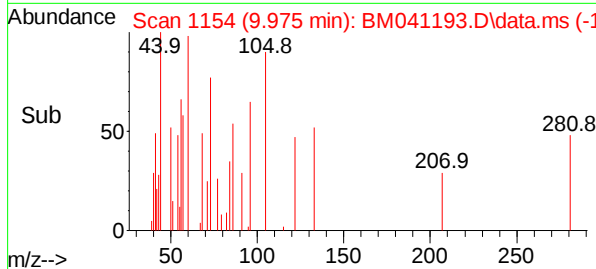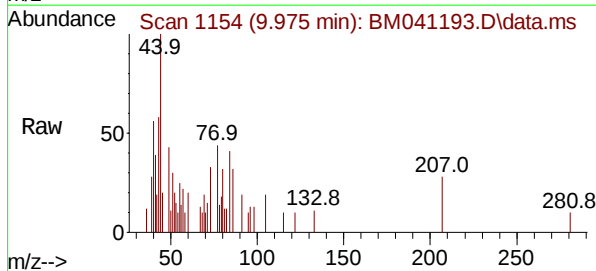

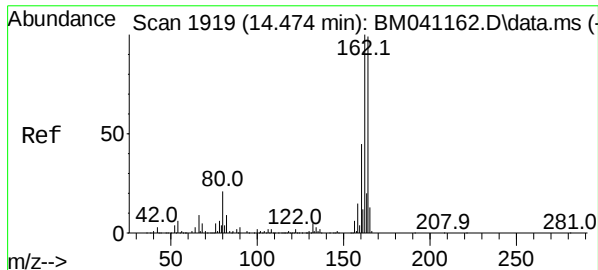

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.463 min Scan# 1919

Delta R.T. 0.000 min

Lab File: BM041193.D

Acq: 31 Jul 2023 17:26

Instrument :

BNA_M

ClientSampleId :

CHRT-20430





Tgt Ion:164 Resp: 285785

Ion Ratio Lower Upper

164 100

162 99.6 80.4 120.6

160 44.9 36.2 54.2

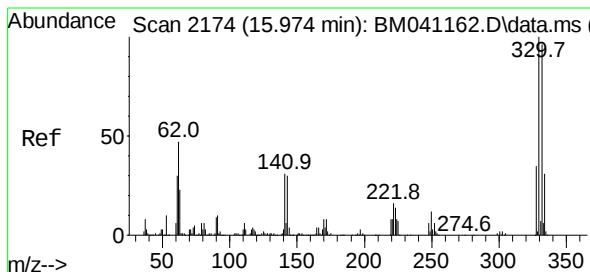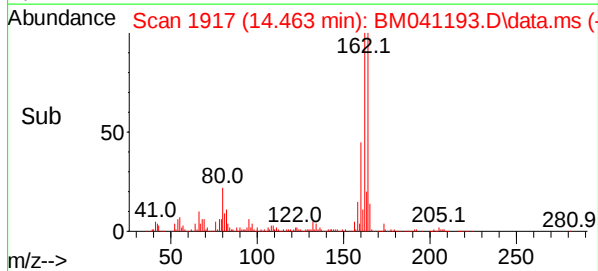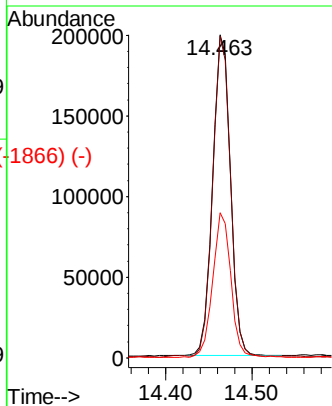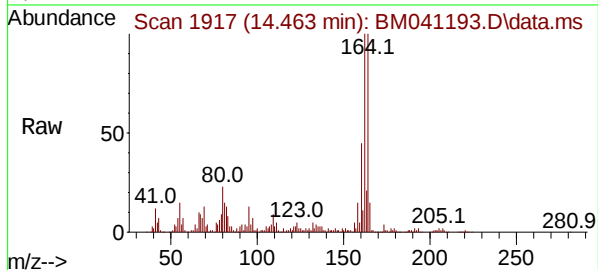

2,4,6-Tribromophenol

Concen: 77.671 ng

RT: 15.968 min Scan# 2173

Delta R.T. 0.006 min

Lab File: BM041193.D

Acq: 31 Jul 2023 17:26




Tgt Ion:330 Resp: 313968


Ion Ratio Lower Upper

330 100

332 98.1 77.7 116.5

141 34.7 28.3 42.5


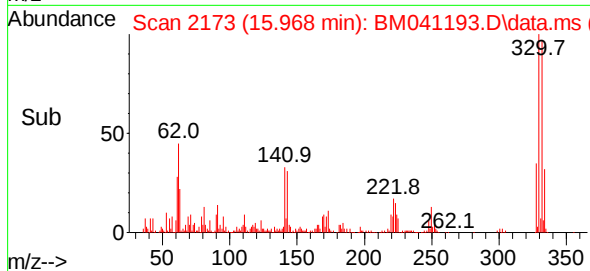
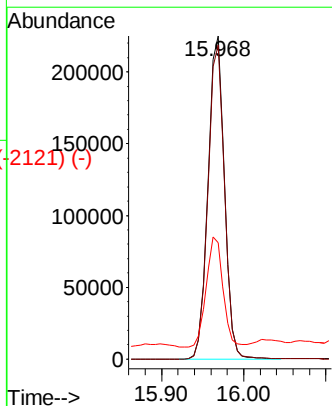
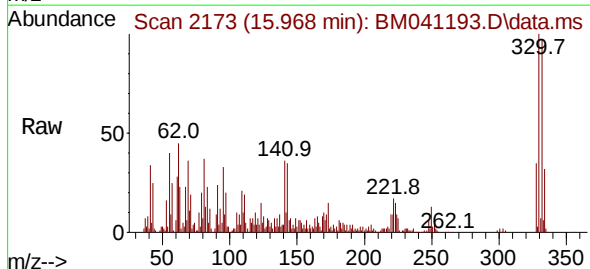


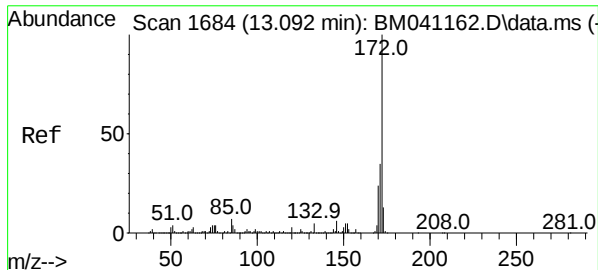

2-Fluorobiphenyl
Concen: 42.313 ng
RT: 13.080 min Scan# 1645
Delta R.T. -0.006 min
Lab File: BM041193.D
Acq: 31 Jul 2023 17:26




Instrument :
BNA_M
ClientSampleId :
CHRT-20430


Tgt Ion:	172	Resp:	957252
Ion	Ratio	Lower	Upper
172	100		
171	35.3	28.1	42.1
170	23.9	18.9	28.3

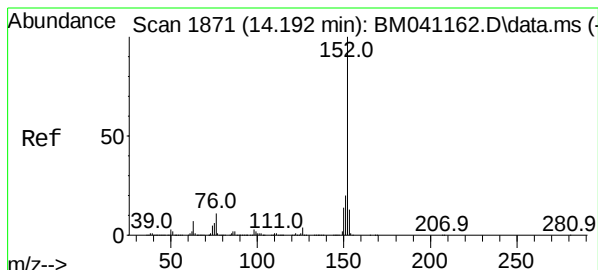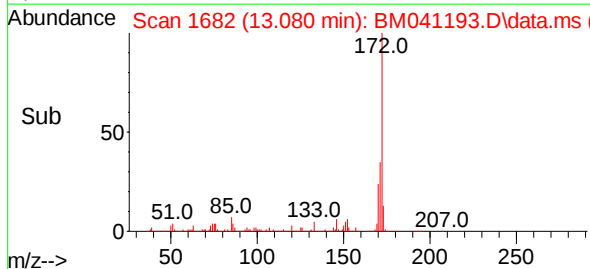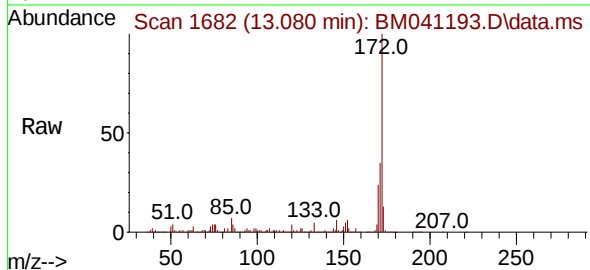

Acenaphthylene
Concen: 2.257 ng
RT: 14.186 min Scan# 1870
Delta R.T. 0.000 min
Lab File: BM041193.D
Acq: 31 Jul 2023 17:26

Tgt Ion:	152	Resp:	63024
Ion	Ratio	Lower	Upper
152	100		
151	29.4	16.1	24.1#
153	15.5	10.5	15.7


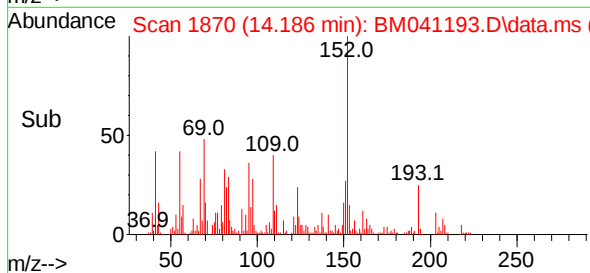

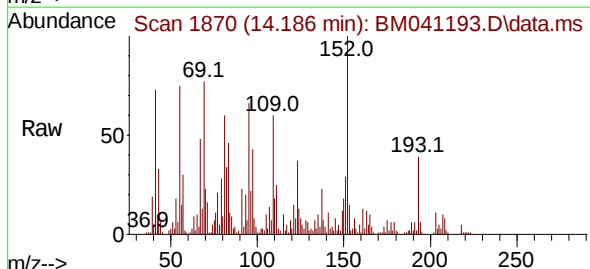


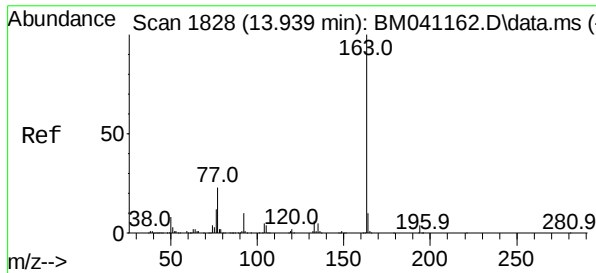

Scan 1828 (13.939 min): BM041162.D\data.ms (-1850) (-)
 Dimethylphthalate
 Concen: 3.394 ng
 RT: 14.016 min Scan# 1828
 Delta R.T. 0.082 min
 Lab File: BM041193.D
 Acq: 31 Jul 2023 17:26




Instrument :
 BNA_M
 ClientSampleId :
 CHRT-20430


Tgt Ion:	163	Resp:	72951
Ion	Ratio	Lower	Upper
163	100		
194	1.4	3.3	4.9#
164	13.3	8.3	12.5#

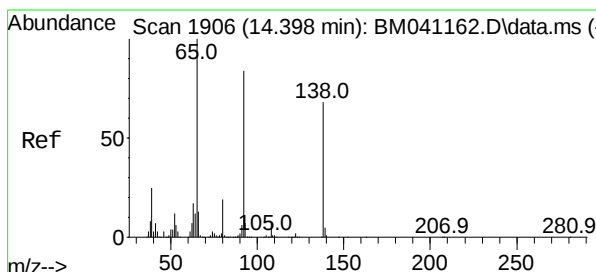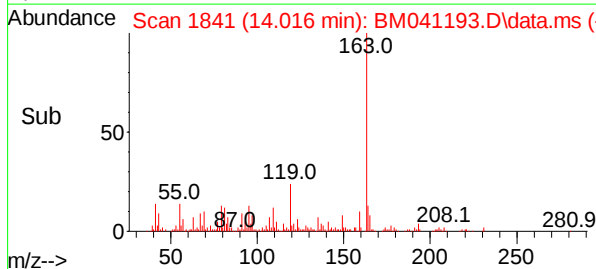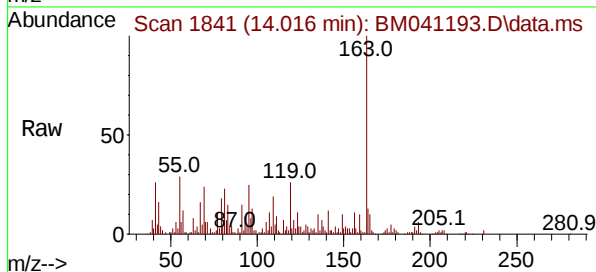

Scan 1906 (14.398 min): BM041162.D\data.ms (-1859) (-)
 3-Nitroaniline
 Concen: 3.297 ng
 RT: 14.410 min Scan# 1908
 Delta R.T. 0.018 min
 Lab File: BM041193.D
 Acq: 31 Jul 2023 17:26

Tgt Ion:	138	Resp:	3920
Ion	Ratio	Lower	Upper
138	100		
108	86.0	7.6	11.4#
92	45.6	98.9	148.3#


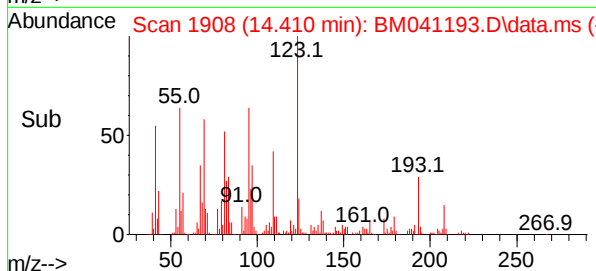

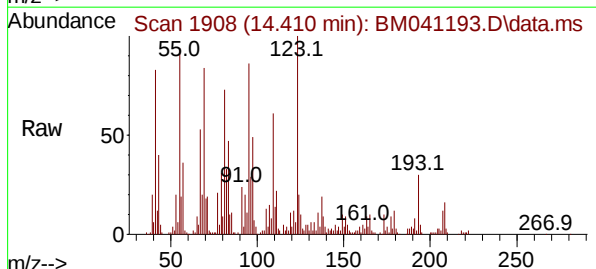


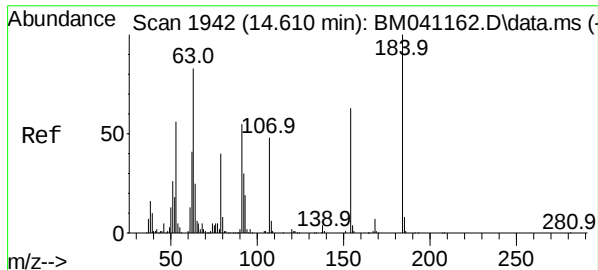

2,4-Dinitrophenol
Concen: 5.960 ng
RT: 14.857 min Scan# 1884
Delta R.T. 0.253 min
Lab File: BM041193.D
Acq: 31 Jul 2023 17:26




Instrument :
BNA_M
ClientSampleId :
CHRT-20430

Tgt Ion:184 Resp: 407
Ion Ratio Lower Upper
184 100
63 816.1 66.5 99.7#
154 808.5 52.8 79.2#

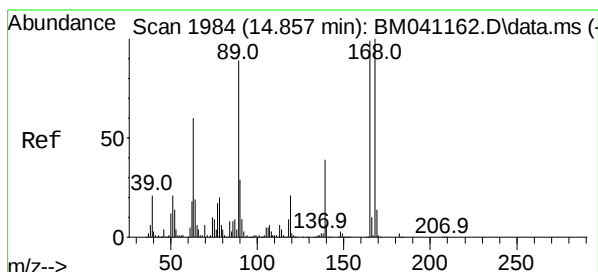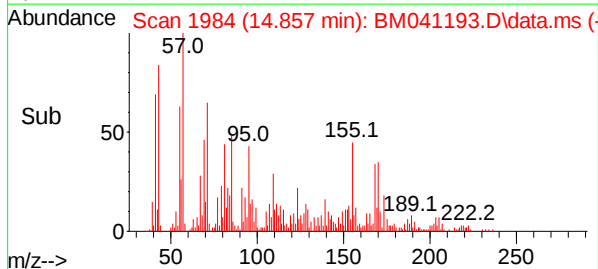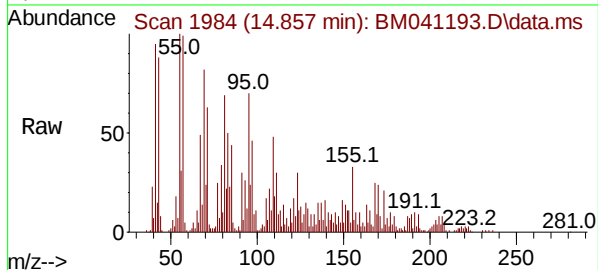


2,4-Dinitrotoluene
Concen: 3.112 ng
RT: 14.874 min Scan# 1987
Delta R.T. 0.024 min
Lab File: BM041193.D
Acq: 31 Jul 2023 17:26

Tgt Ion:165 Resp: 2971
Ion Ratio Lower Upper
165 100
63 36.3 48.3 72.5#
89 22.4 71.8 107.8#
182 12.5 2.0 3.0#

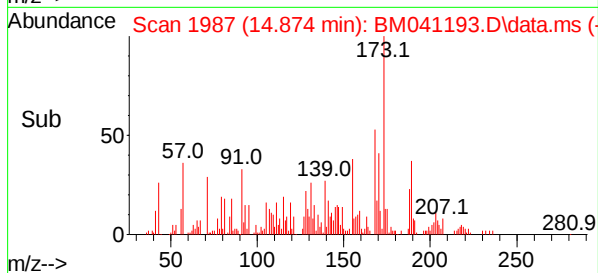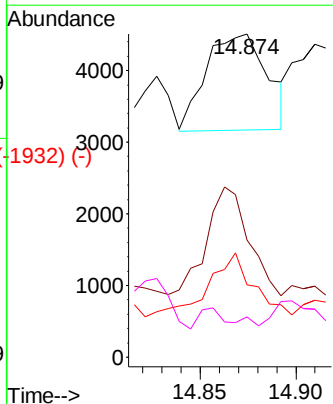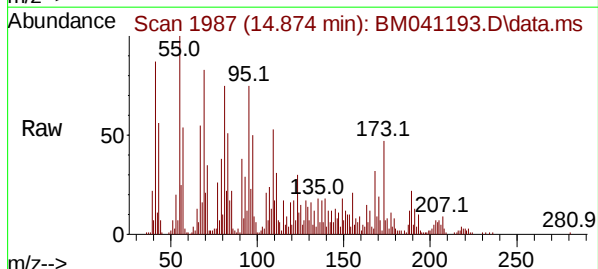

Abundance Scan 2098 (15.527 min): BM041162.D\data.ms (-2050) (-)

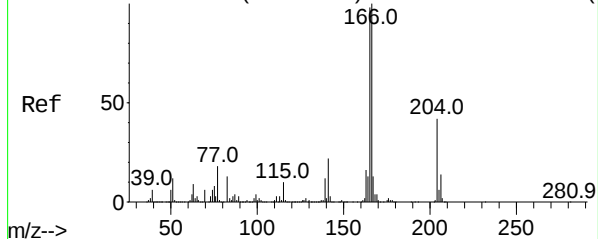

Fluorene

Concen: 2.063 ng

RT: 15.521 min Scan# 2098

Delta R.T. 0.006 min

Lab File: BM041193.D

Acq: 31 Jul 2023 17:26

Instrument :

BNA_M

ClientSampleId :

CHRT-20430

Tgt Ion:166 Resp: 44663


Ion Ratio Lower Upper

166 100


165 112.3 78.2 117.4

167 21.5 10.6 16.0#


Abundance Scan 2097 (15.521 min): BM041193.D\data.ms

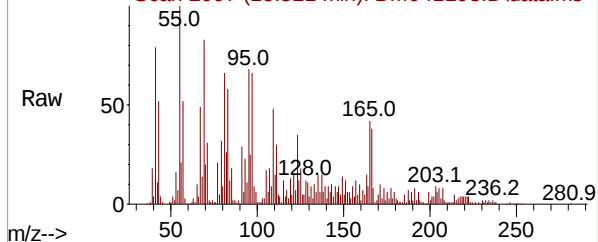


Abundance

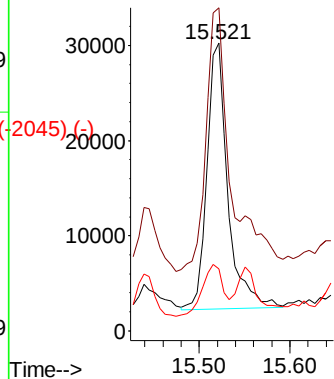

Abundance Scan 2097 (15.521 min): BM041193.D\data.ms (-2045) (-)

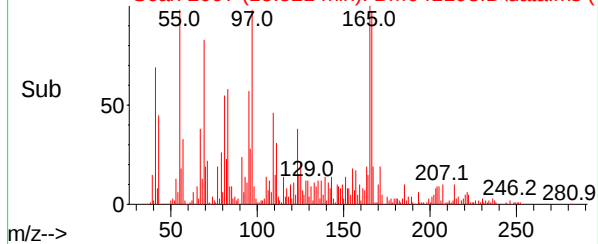

Abundance Scan 2105 (15.568 min): BM041162.D\data.ms (-2060) (-)

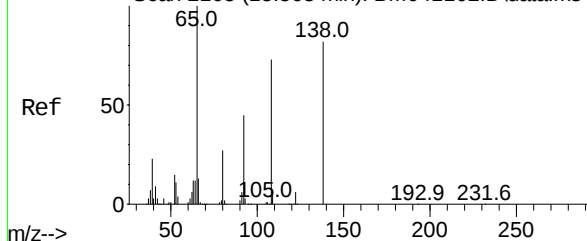

4-Nitroaniline

Concen: 7.796 ng

RT: 15.339 min Scan# 2066

Delta R.T. -0.223 min

Lab File: BM041193.D

Acq: 31 Jul 2023 17:26

Tgt Ion:138 Resp: 18971


Ion Ratio Lower Upper

138 100


92 40.1 35.1 75.1

108 69.6 67.8 107.8


Abundance Scan 2066 (15.339 min): BM041193.D\data.ms

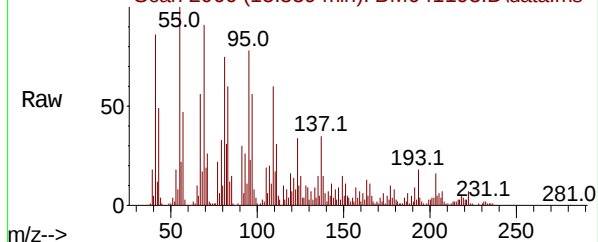


Abundance

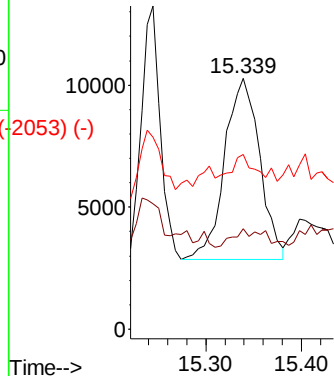

Abundance Scan 2066 (15.339 min): BM041193.D\data.ms (-2053) (-)




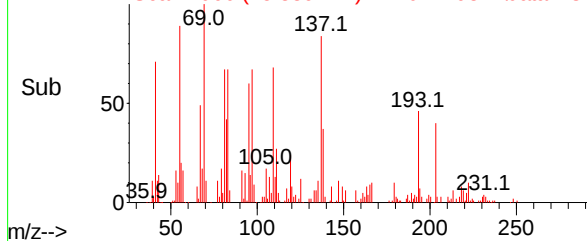


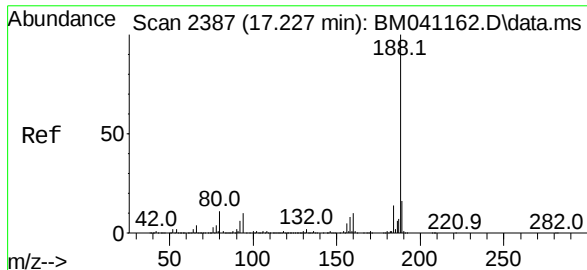

Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.227 min Scan# 2387
 Delta R.T. 0.006 min
 Lab File: BM041193.D
 Acq: 31 Jul 2023 17:26




Instrument :
 BNA_M
 ClientSampleId :
 CHRT-20430


Tgt Ion:	188	Resp:	540705
Ion	Ratio	Lower	Upper
188	100		
94	13.3	8.2	12.2#
80	13.6	8.6	13.0#

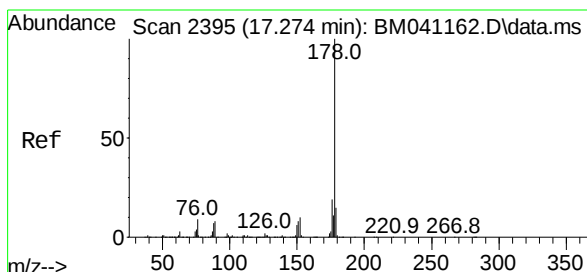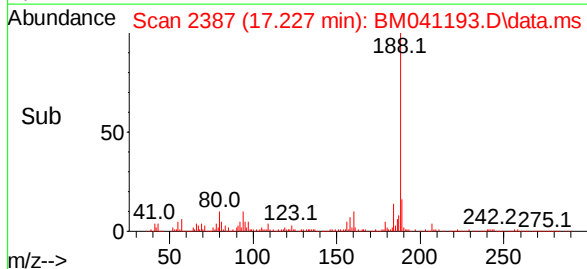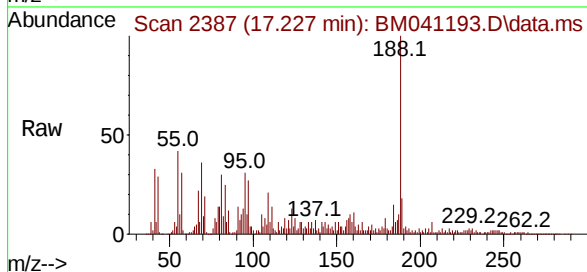

Phenanthrene
 Concen: 23.706 ng
 RT: 17.268 min Scan# 2394
 Delta R.T. 0.000 min
 Lab File: BM041193.D
 Acq: 31 Jul 2023 17:26

Tgt Ion:	178	Resp:	712169
Ion	Ratio	Lower	Upper
178	100		
176	20.0	15.6	23.4
179	18.1	12.1	18.1#


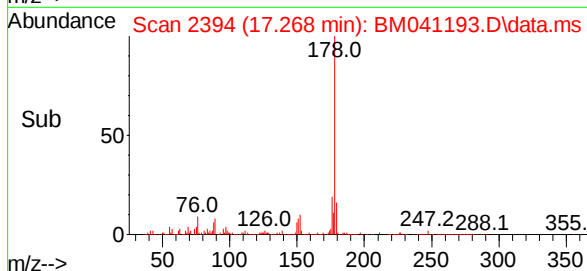

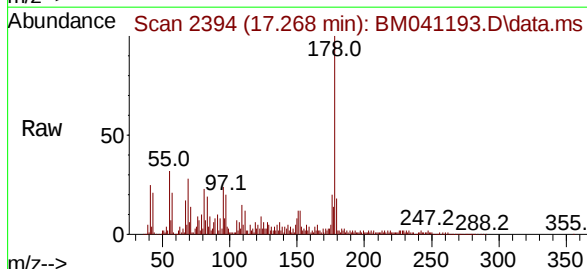


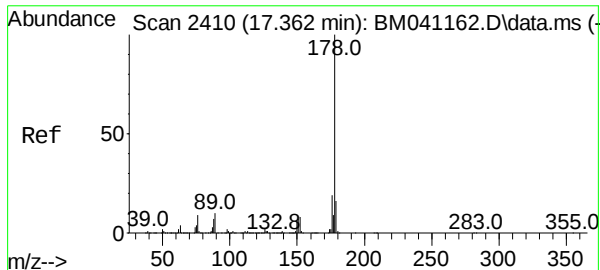

Scan 2410 (17.362 min): BM041162.D\data.ms (-2472) (-)
 Anthracene
 Concen: 23.969 ng
 RT: 17.268 min Scan# 2410
 Delta R.T. -0.088 min
 Lab File: BM041193.D
 Acq: 31 Jul 2023 17:26




Instrument :
 BNA_M
 ClientSampleId :
 CHRT-20430

Tgt Ion:	178	Resp:	712169
Ion	Ratio	Lower	Upper
178	100		
176	20.0	15.2	22.8
179	18.1	12.4	18.6

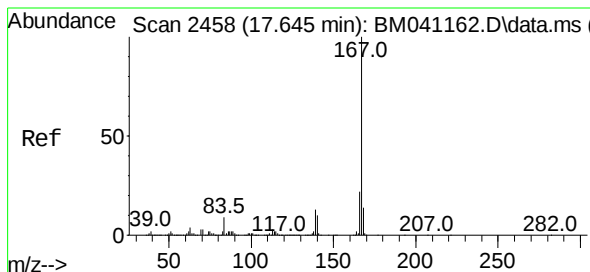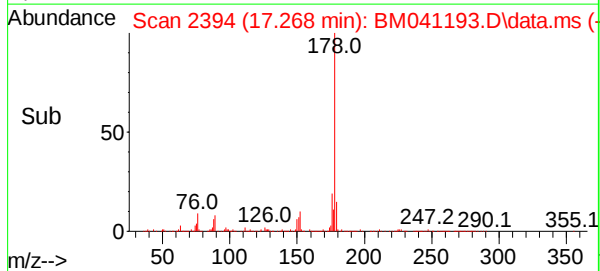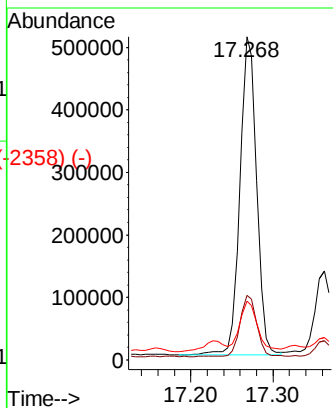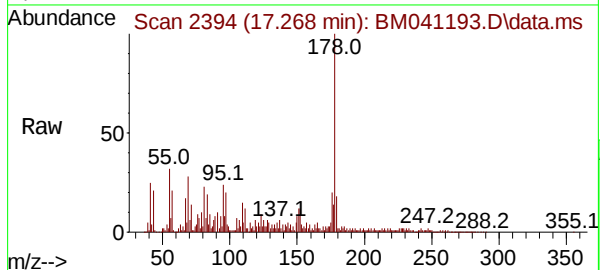

Scan 2458 (17.645 min): BM041162.D\data.ms (-2472) (-)
 Carbazole
 Concen: 3.326 ng
 RT: 17.645 min Scan# 2458
 Delta R.T. 0.006 min
 Lab File: BM041193.D
 Acq: 31 Jul 2023 17:26

Tgt Ion:	167	Resp:	89435
Ion	Ratio	Lower	Upper
167	100		
166	33.8	17.3	25.9#
139	32.8	10.3	15.5#

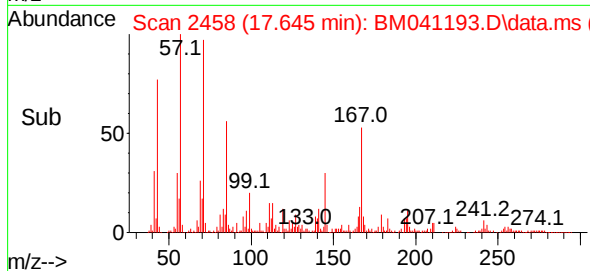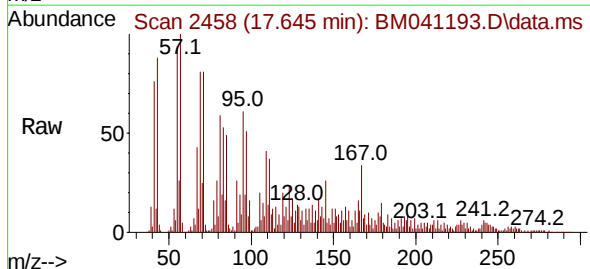

Abundance Scan 2739 (19.298 min): BM041162.D\data.ms (-2735) (-)

Fluoranthene

Concen: 43.081 ng

RT: 19.298 min Scan# 2739

Delta R.T. 0.006 min

Lab File: BM041193.D


Acq: 31 Jul 2023 17:26

Instrument :

BNA_M

ClientSampleId :

CHRT-20430

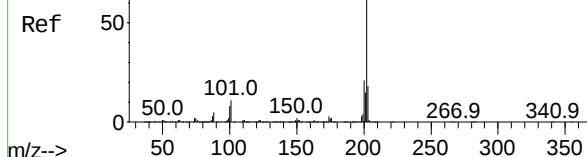




Tgt Ion:202 Resp: 1454047

Ion Ratio Lower Upper

202 100

101 10.0 0.0 30.8

203 18.3 0.0 37.6

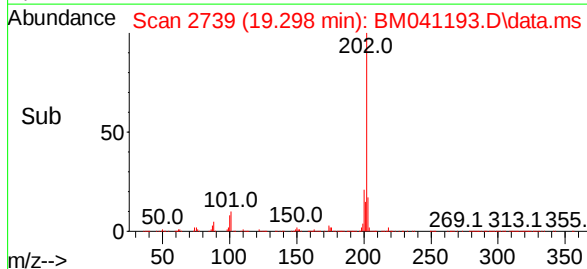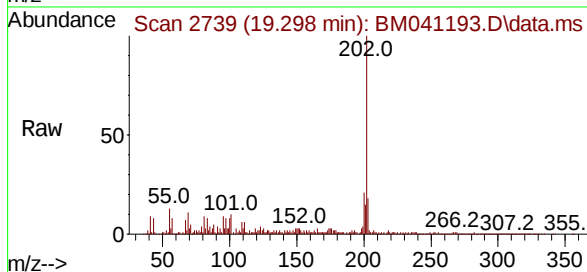

Abundance Scan 3102 (21.433 min): BM041162.D\data.ms (-3075) (-)

Chrysene-d12

Concen: 20.000 ng

RT: 21.427 min Scan# 3101

Delta R.T. 0.000 min

Lab File: BM041193.D

Acq: 31 Jul 2023 17:26




Tgt Ion:240 Resp: 512705


Ion Ratio Lower Upper

240 100

120 10.3 8.3 12.5

236 26.0 20.6 30.8


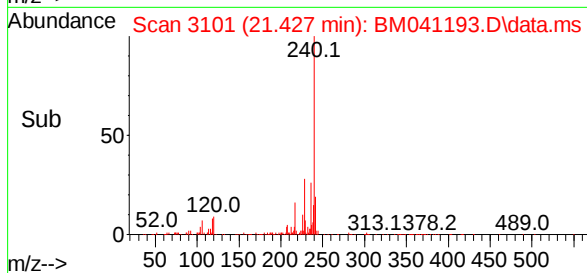

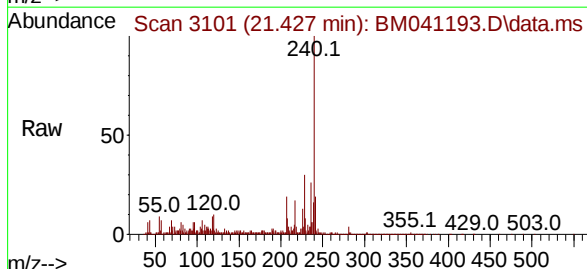


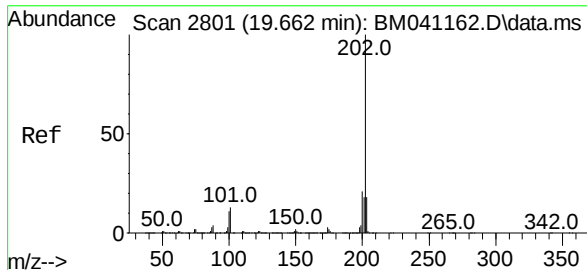

Pyrene
 Concen: 39.018 ng
 RT: 19.662 min Scan# 2801
 Delta R.T. 0.006 min
 Lab File: BM041193.D
 Acq: 31 Jul 2023 17:26




Instrument :
 BNA_M
 ClientSampleId :
 CHRT-20430


Tgt Ion:	202	Resp:	1398963
Ion	Ratio	Lower	Upper
202	100		
200	21.0	16.9	25.3
203	18.4	14.1	21.1

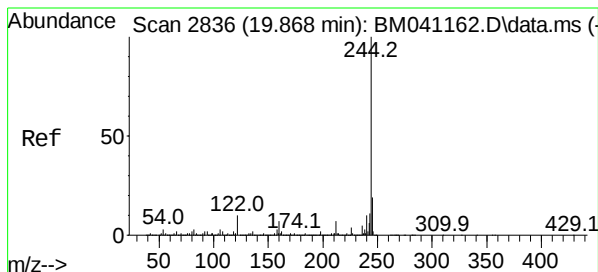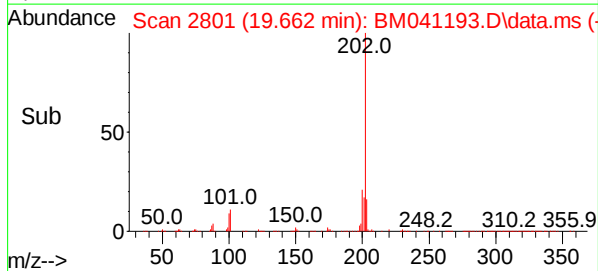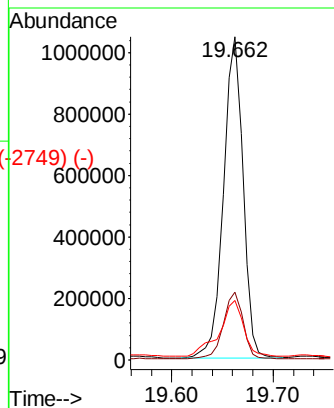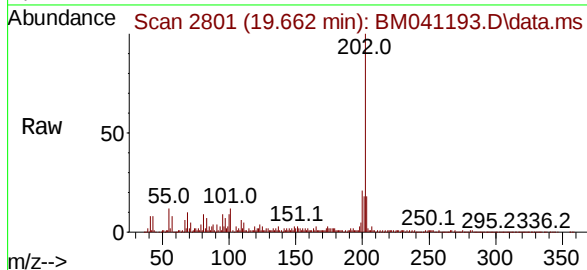

Terphenyl-d14
 Concen: 41.906 ng
 RT: 19.862 min Scan# 2835
 Delta R.T. 0.000 min
 Lab File: BM041193.D
 Acq: 31 Jul 2023 17:26

Tgt Ion:	244	Resp:	1188316
Ion	Ratio	Lower	Upper
244	100		
212	6.9	5.4	8.2
122	10.1	7.8	11.6


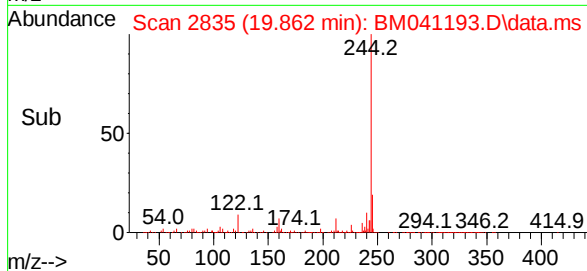

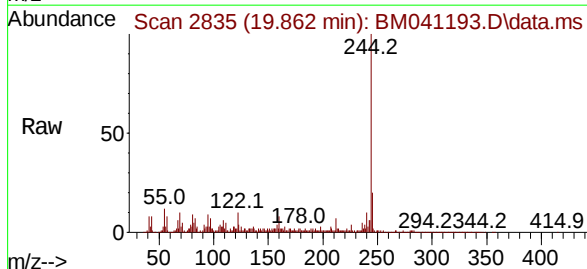


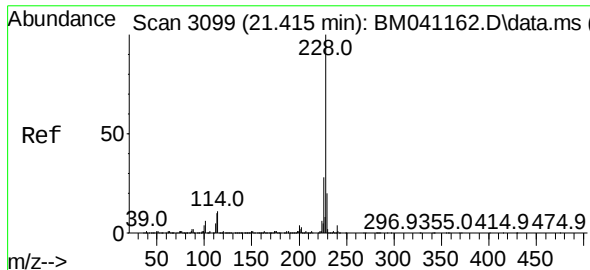

Benzo(a)anthracene
Concen: 22.714 ng
RT: 21.409 min Scan# 3103
Delta R.T. 0.000 min
Lab File: BM041193.D
Acq: 31 Jul 2023 17:26




Instrument :
BNA_M
ClientSampleId :
CHRT-20430

Tgt Ion:	228	Resp:	789492
Ion	Ratio	Lower	Upper
228	100		
226	28.2	22.4	33.6
229	21.2	15.8	23.8

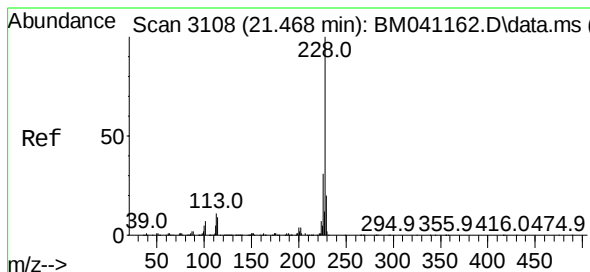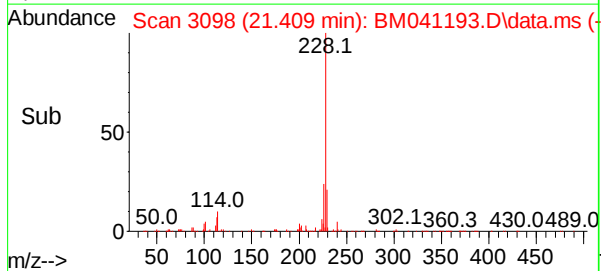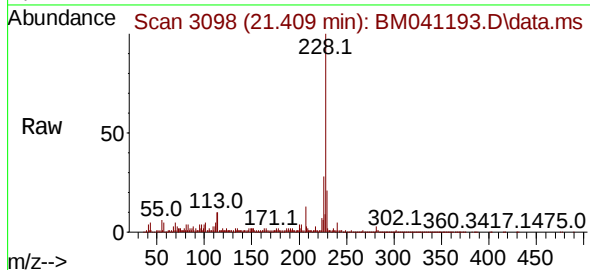

Chrysene
Concen: 32.026 ng
RT: 21.462 min Scan# 3107
Delta R.T. 0.000 min
Lab File: BM041193.D
Acq: 31 Jul 2023 17:26

Tgt Ion:	228	Resp:	1076656
Ion	Ratio	Lower	Upper
228	100		
226	30.2	24.5	36.7
229	22.0	15.8	23.8

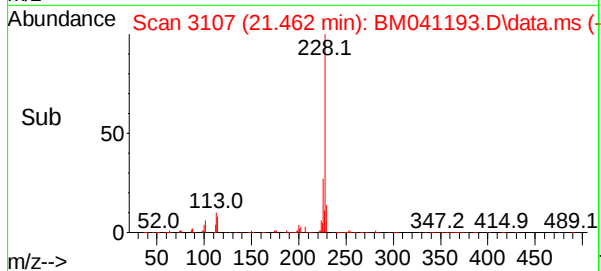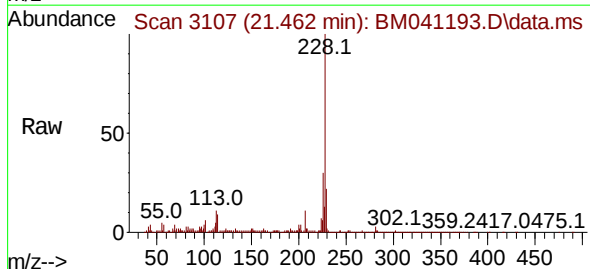

Abundance Scan 3086 (21.339 min): BM041162.D\data.ms (-3086) (-)

Bis(2-ethylhexyl)phthalate

Concen: 11.338 ng

RT: 21.333 min Scan# 3086

Delta R.T. -0.006 min

Lab File: BM041193.D

Acq: 31 Jul 2023 17:26

Instrument :

BNA_M

ClientSampleId :

CHRT-20430

Tgt Ion:149 Resp: 193177

Ion Ratio Lower Upper

149 100

167 28.5 21.0 31.6

279 4.7 3.1 4.7#

Abundance Scan 3085 (21.333 min): BM041193.D\data.ms

Ref 50

57.0 148.9 279.1 344.0 415.0

m/z--> 50 100 150 200 250 300 350 400 450 500

Abundance Scan 3085 (21.333 min): BM041193.D\data.ms

Raw 50

57.0 149.0 215.1 281.0 356.1 429.0 549.2

m/z--> 50 100 150 200 250 300 350 400 450 500

Abundance Scan 3085 (21.333 min): BM041193.D\data.ms (-3035) (-)

Sub 50

57.0 149.0 234.0 302.1 368.3 475.1 549.2

m/z--> 50 100 150 200 250 300 350 400 450 500

Abundance

21.333

150000

100000

50000

0

Time--> 21.30 21.35

Abundance Scan 3505 (23.803 min): BM041162.D\data.ms (-3486) (-)

Perylene-d12

Concen: 20.000 ng

RT: 23.797 min Scan# 3504

Delta R.T. 0.000 min

Lab File: BM041193.D

Acq: 31 Jul 2023 17:26

Tgt Ion:264 Resp: 601989

Ion Ratio Lower Upper

264 100

260 23.8 18.5 27.7

265 23.2 17.4 26.0

Abundance Scan 3504 (23.797 min): BM041193.D\data.ms

Ref 50

66.0 131.9 197.9 264.1 338.9 415.9 491.0

m/z--> 50 100 150 200 250 300 350 400 450 500

Abundance Scan 3504 (23.797 min): BM041193.D\data.ms

Raw 50

43.0 132.1 197.0 264.1 355.1 430.0 502.9

m/z--> 50 100 150 200 250 300 350 400 450 500

Abundance Scan 3504 (23.797 min): BM041193.D\data.ms (-3453) (-)

Sub 50

66.0 132.0 197.9 264.1 335.1 401.0 475.1

m/z--> 50 100 150 200 250 300 350 400 450 500

Abundance

23.797

300000


200000

100000

0

Time--> 23.70 23.80 23.90




Abundance Scan 3922 (26.256 min): BM041162.D\data.ms (-3922) (-)

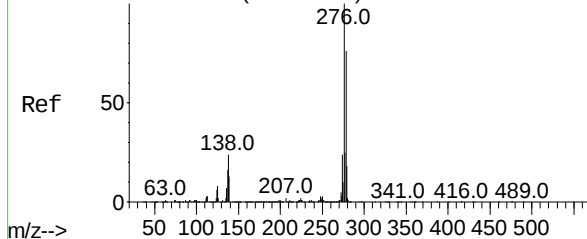


Indeno(1,2,3-cd)pyrene
Concen: 10.172 ng
RT: 26.238 min Scan# 3919
Delta R.T. -0.006 min
Lab File: BM041193.D
Acq: 31 Jul 2023 17:26

Instrument :
BNA_M
ClientSampleId :
CHRT-20430

Tgt Ion:	276	Resp:	450217
Ion Ratio	Lower	Upper	
276	100		
138	19.2	20.0	30.0#
277	24.3	20.1	30.1

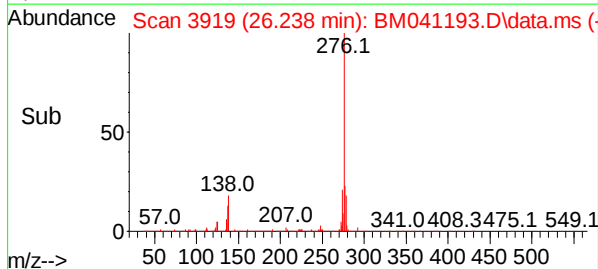

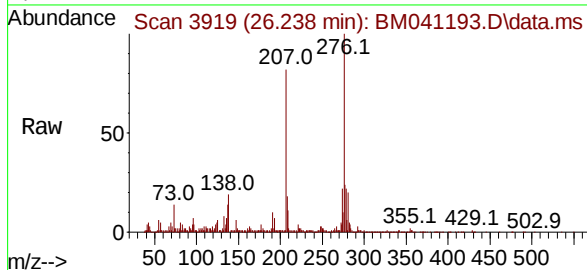



Abundance Scan 3382 (23.080 min): BM041162.D\data.ms (-3382) (-)

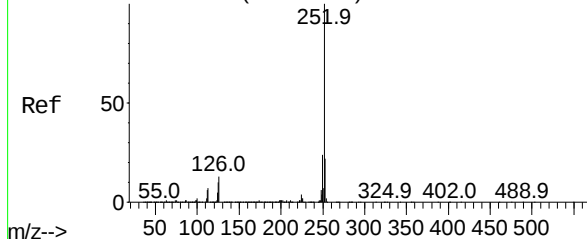

Benzo(b)fluoranthene
Concen: 35.625 ng
RT: 23.080 min Scan# 3382
Delta R.T. 0.006 min
Lab File: BM041193.D
Acq: 31 Jul 2023 17:26

Tgt Ion:	252	Resp:	1274030
Ion Ratio	Lower	Upper	
252	100		
253	23.0	17.7	26.5
125	9.9	8.2	12.4


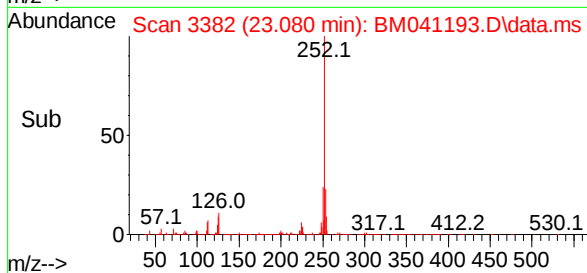

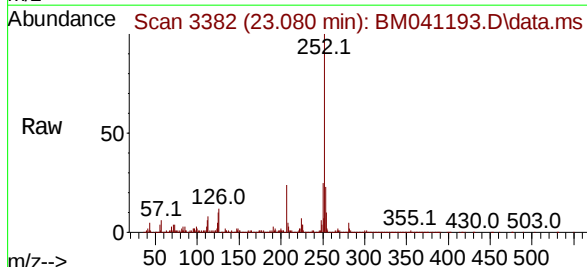


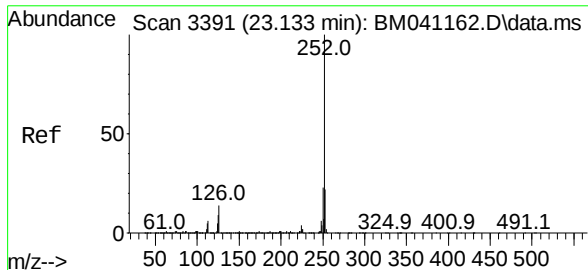

Benzo(k)fluoranthene
 Concen: 34.828 ng
 RT: 23.080 min Scan# 3389
 Delta R.T. -0.041 min
 Lab File: BM041193.D
 Acq: 31 Jul 2023 17:26




Instrument :
 BNA_M
 ClientSampleId :
 CHRT-20430

Tgt Ion:252 Resp: 1274030
 Ion Ratio Lower Upper
 252 100
 253 23.0 17.4 26.0
 125 9.9 7.6 11.4

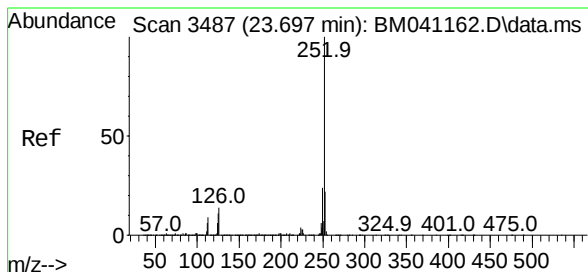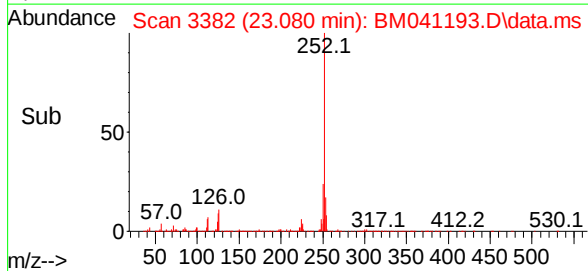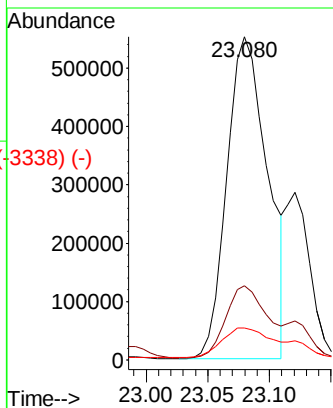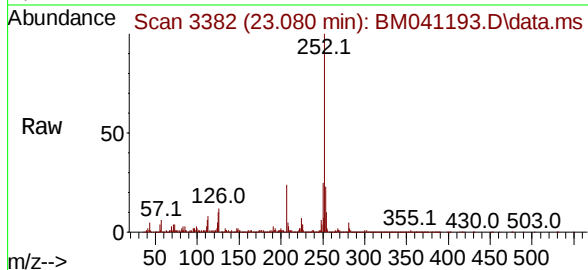


Benzo(a)pyrene
 Concen: 20.155 ng
 RT: 23.692 min Scan# 3486
 Delta R.T. 0.000 min
 Lab File: BM041193.D
 Acq: 31 Jul 2023 17:26

Tgt Ion:252 Resp: 692559
 Ion Ratio Lower Upper
 252 100
 253 22.7 17.3 25.9
 125 10.6 9.0 13.4

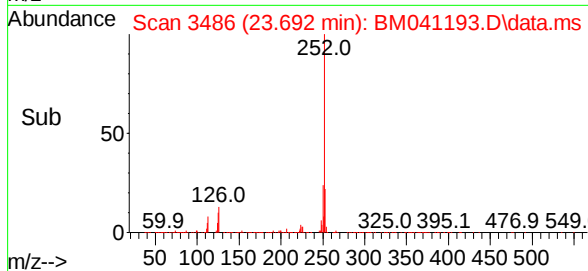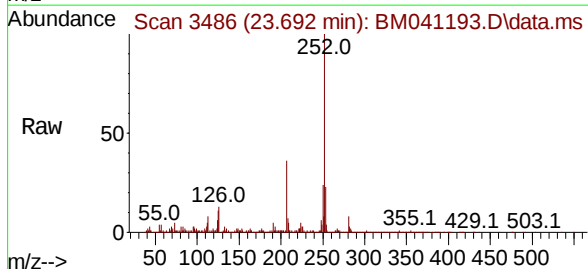

Abundance Scan 4050 (27.009 min): BM041162.D\data.ms (-4050) (-)


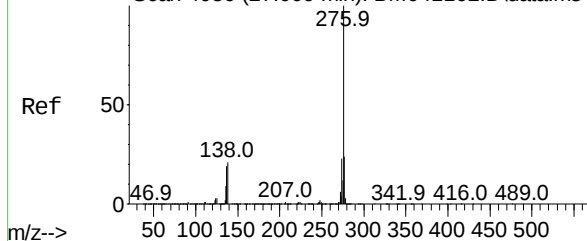


Benzo(g,h,i)perylene
 Concen: 11.120 ng
 RT: 26.991 min Scan# 4050
 Delta R.T. -0.006 min
 Lab File: BM041193.D
 Acq: 31 Jul 2023 17:26

Instrument :
 BNA_M
 ClientSampleId :
 CHRT-20430

Tgt Ion:	276	Resp:	401686
Ion	Ratio	Lower	Upper
276	100		
277	24.2	19.1	28.7
138	20.7	17.1	25.7

Abundance Scan 4047 (26.991 min): BM041193.D\data.ms

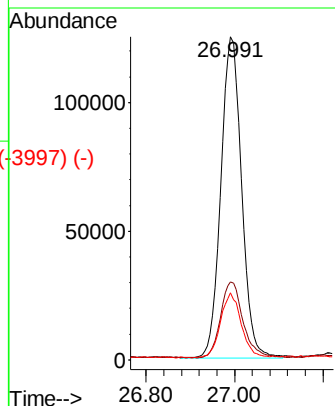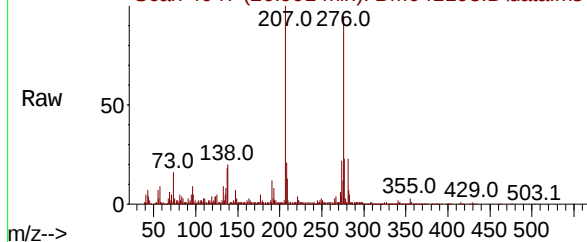

Abundance Scan 4047 (26.991 min): BM041193.D\data.ms (-3997) (-)

