
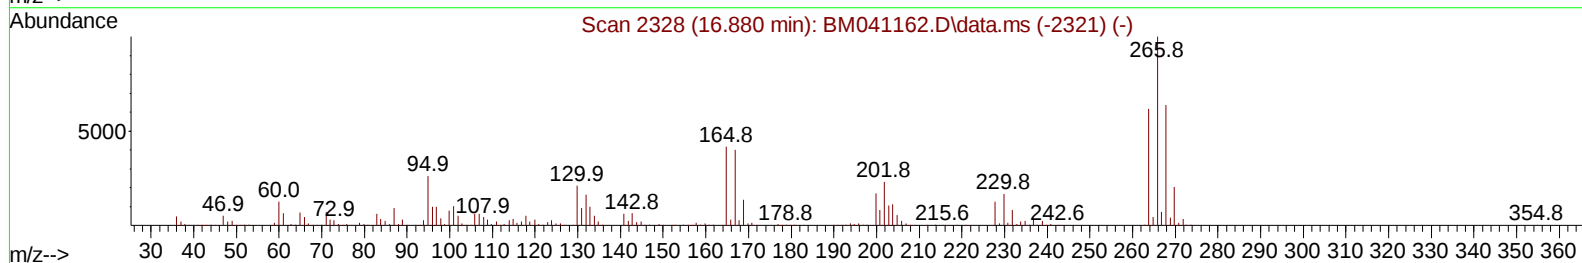
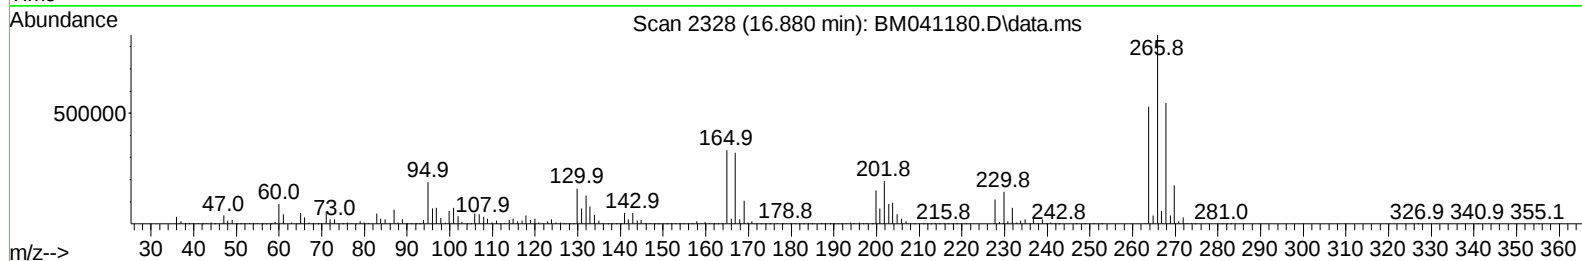


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM073123\  
Data File : BM041180.D  
Acq On : 31 Jul 2023 08:47  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 10:55:25 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM072823.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Jul 29 00:19:24 2023  
Response via : Initial Calibration



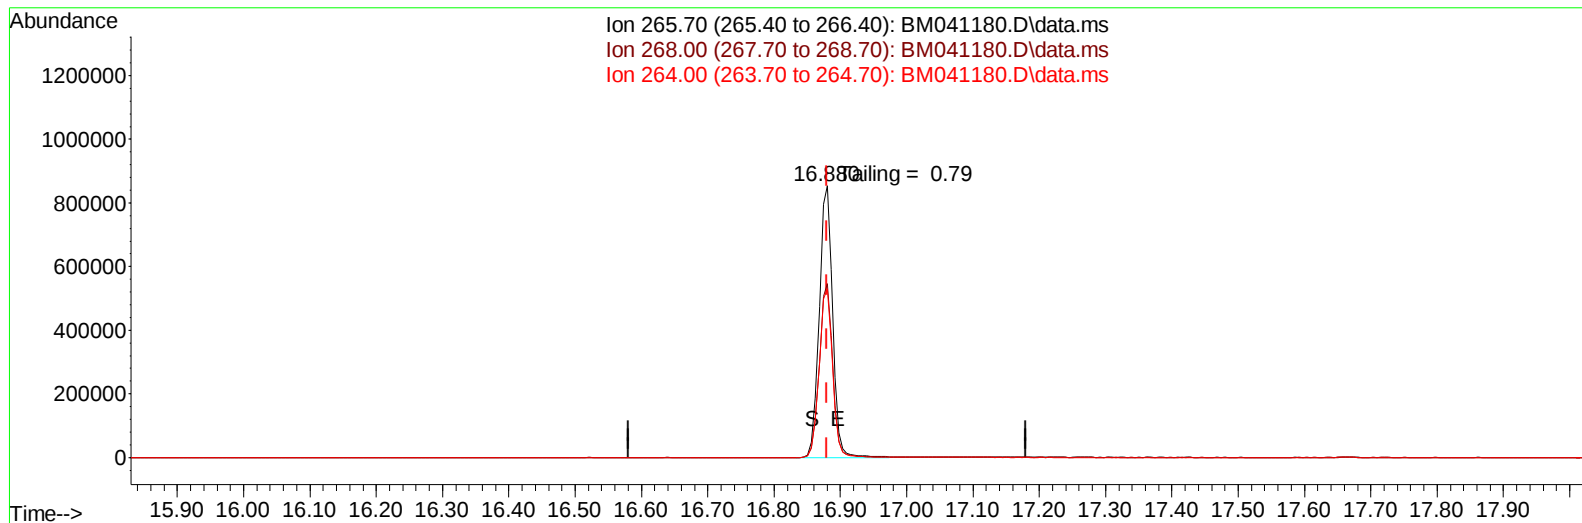


TIC: BM041180.D\data.ms

**(70) Pentachlorophenol (C)****16.880min (-0.000) 2437789.09 ng****response 1193666**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.80  | 63.92  |
| 264.00 | 61.80  | 62.17  |
| 0.00   | 0.00   | 0.00   |

Quant Time: Jul 31 10:55:25 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM072823.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Jul 29 00:19:24 2023  
Response via : Initial Calibration

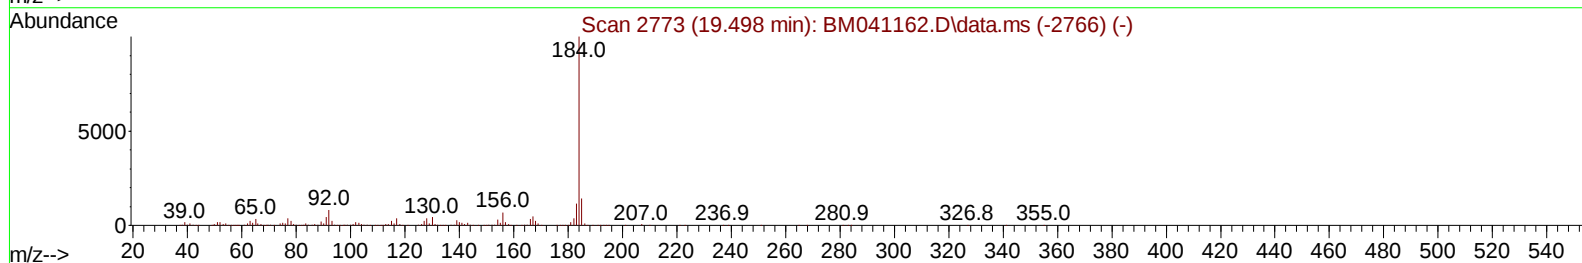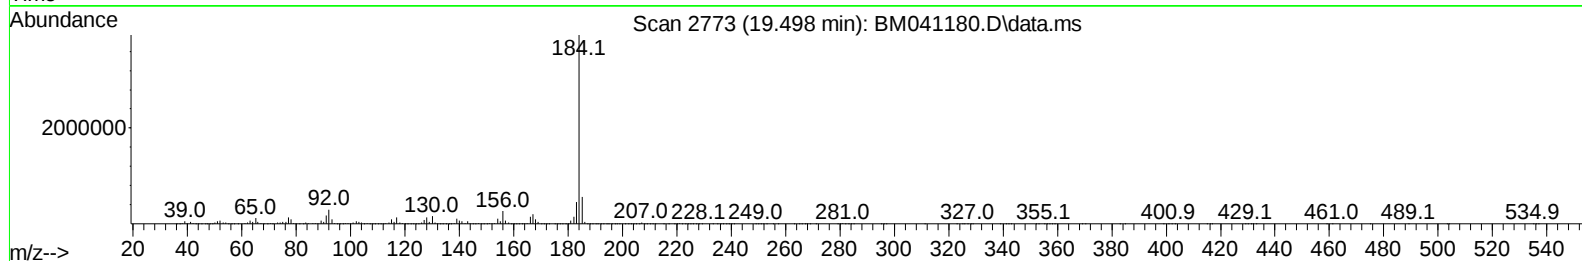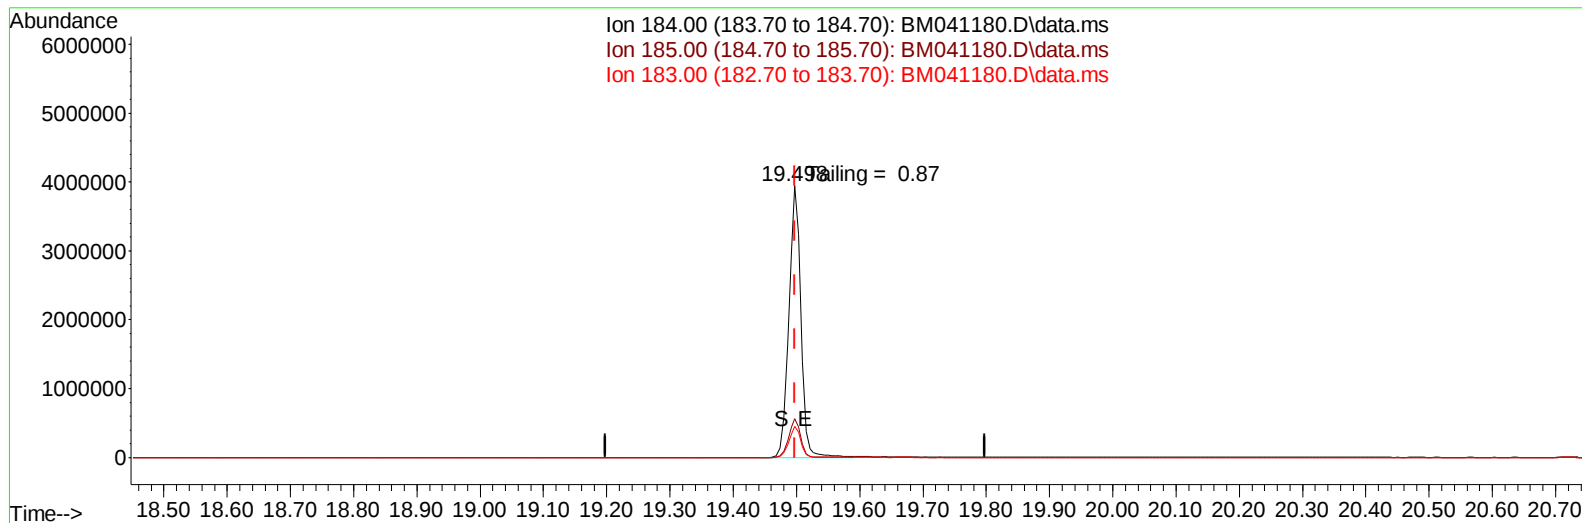

TIC: BM041180.D\data.ms

(77) Benzidine

**19.498min (-0.000) 13088.10 ng**

**response**      **5290497**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.20  | 14.31  |
| 183.00 | 11.50  | 11.40  |
| 0.00   | 0.00   | 0.00   |