
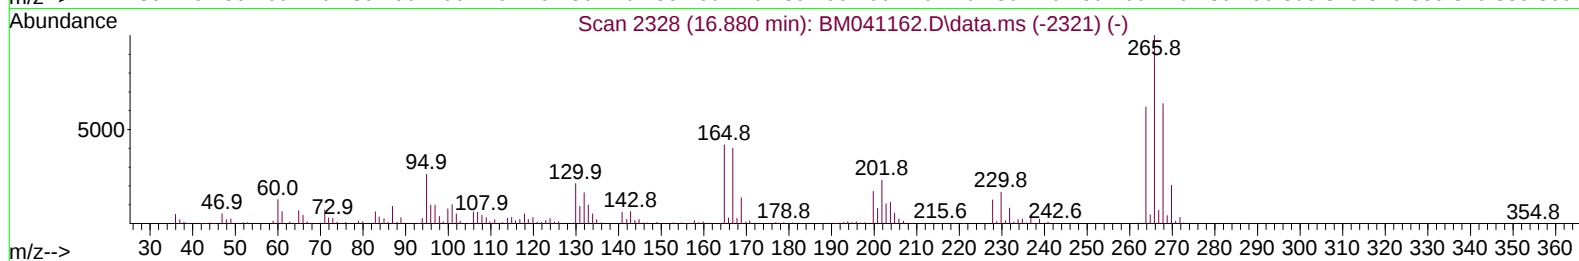
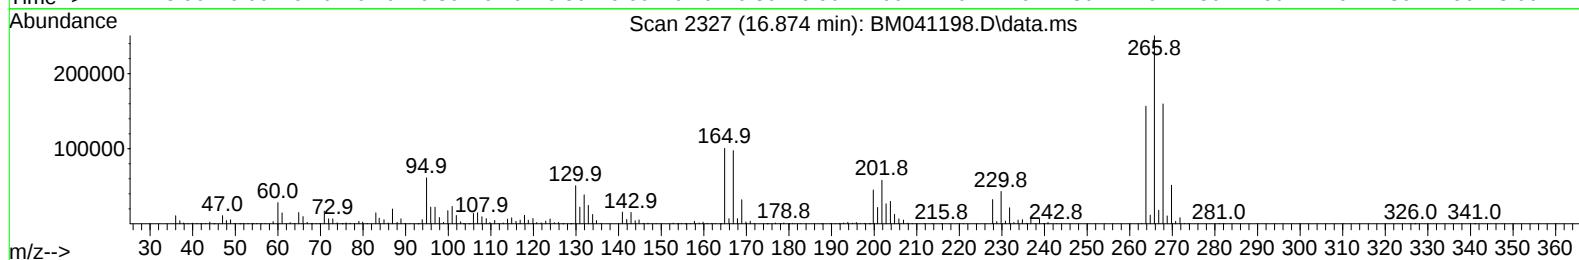


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM073123\
 Data File : BM041198.D
 Acq On : 31 Jul 2023 20:32
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 02:24:53 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 31 16:29:28 2023
 Response via : Initial Calibration

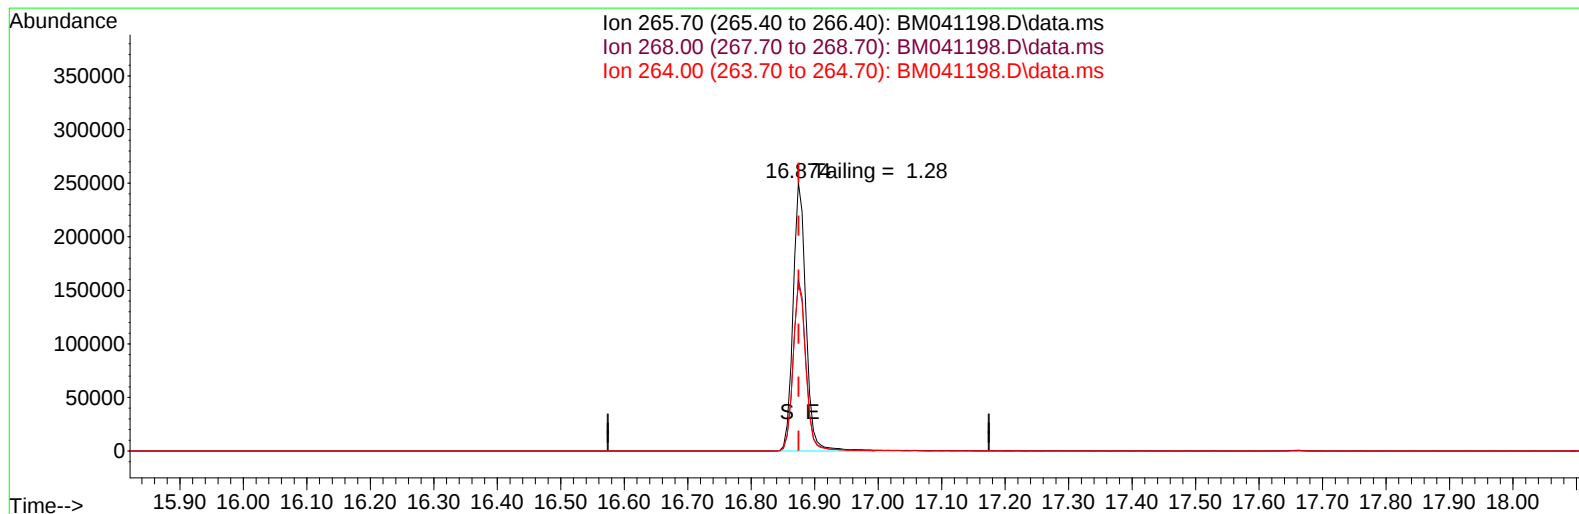

TIC: BM041198.D\data.ms

(70) Pentachlorophenol (C)




16.874min (+ 0.000) 345212.55 ng

response 358468

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.80
264.00	61.80	62.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM073123\
Data File : BM041198.D
Acq On : 31 Jul 2023 20:32
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 02:24:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 31 16:29:28 2023
Response via : Initial Calibration

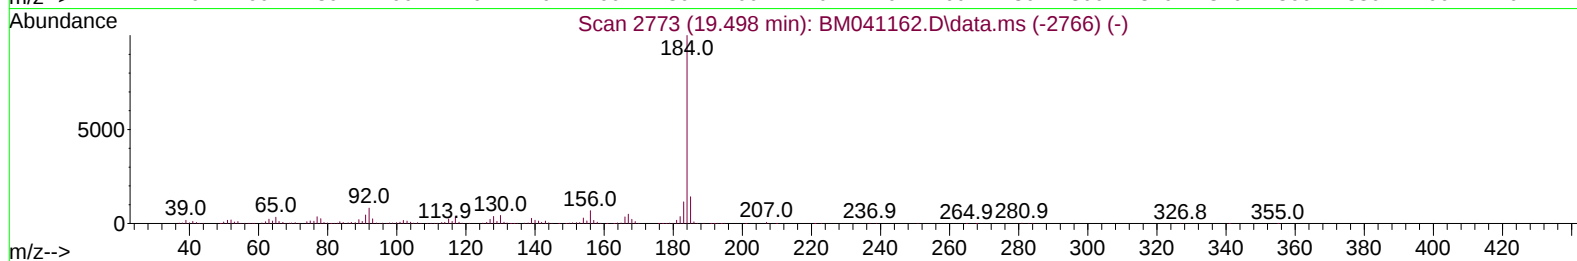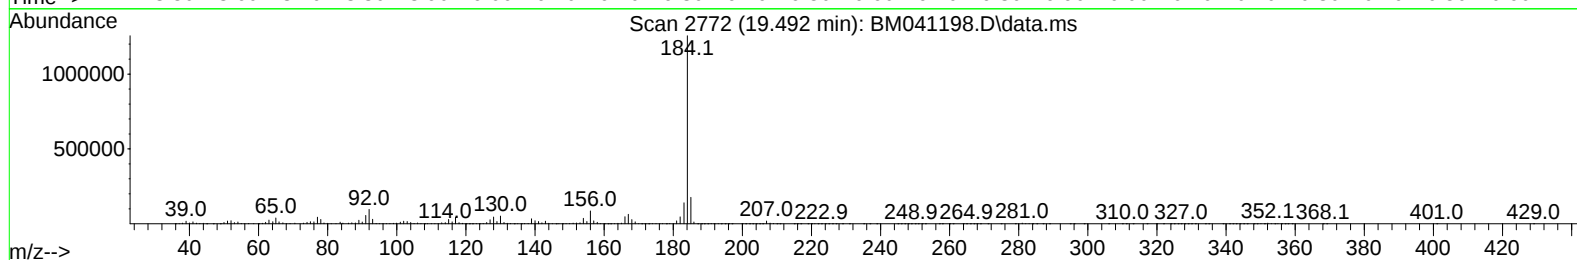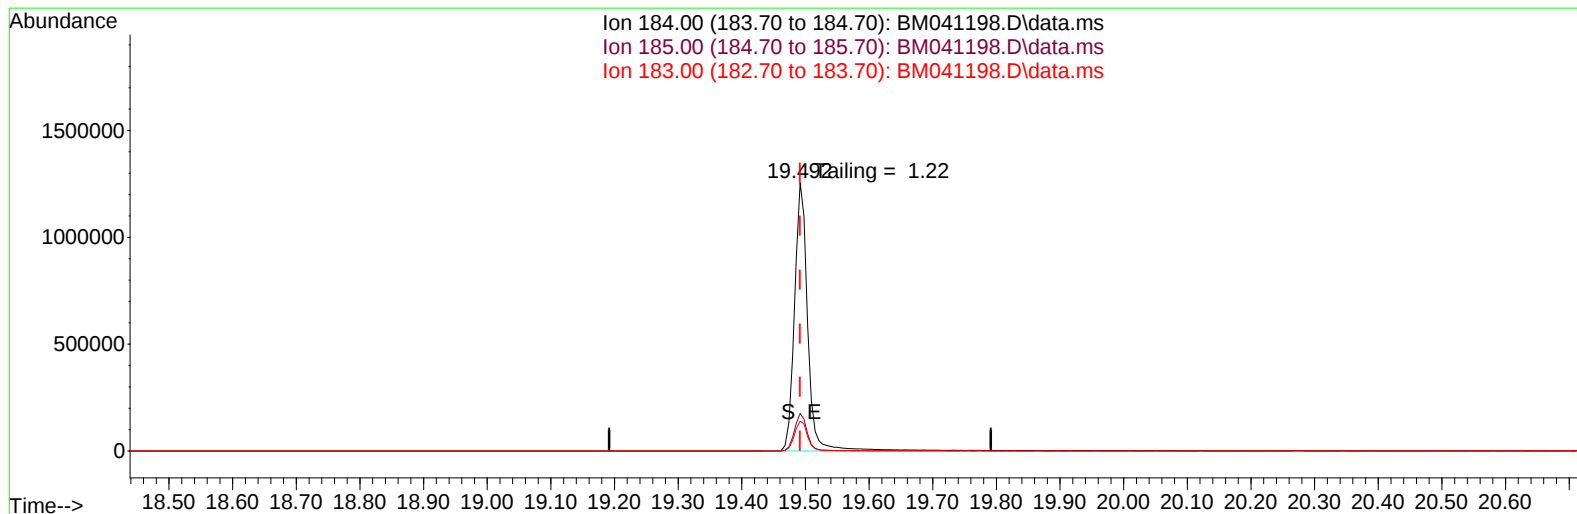

TIC: BM041198.D\data.ms

(77) Benzidine**19.492min (+ 0.000) 76496.35 ng****response 1813146**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.03
183.00	11.50	11.19
0.00	0.00	0.00