

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM073123\
Data File : BM041200.D
Acq On : 31 Jul 2023 23:00
Operator : MA/JU
Sample : PB154429BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB154429BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM041200.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.369	365	371	389	rBV	3591092	5256174	64.17%	12.426%
2	6.981	637	645	664	rBV	3300465	5133374	62.67%	12.136%
3	7.798	777	784	795	rBV	706332	1077944	13.16%	2.548%
4	8.975	976	984	999	rBV	1999887	3282728	40.07%	7.761%
5	10.604	1254	1261	1275	rBV	806919	1340585	16.37%	3.169%
6	13.080	1675	1682	1698	rBV	4561856	6614070	80.74%	15.636%
7	14.463	1911	1917	1930	rBV	1036957	1454009	17.75%	3.437%
8	15.963	2165	2172	2188	rBV	3313987	4500769	54.94%	10.640%
9	17.221	2380	2386	2395	rBV	1094986	1510539	18.44%	3.571%
10	19.856	2829	2834	2844	rBV	6987701	8191482	100.00%	19.366%
11	21.421	3095	3100	3105	rBV	1542675	1823227	22.26%	4.310%
12	23.786	3497	3502	3512	rVB	1103271	2114086	25.81%	4.998%




Sum of corrected areas: 42298987

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM073123\
Data File : BM041200.D
Acq On : 31 Jul 2023 23:00
Operator : MA/JU
Sample : PB154429BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB154429BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

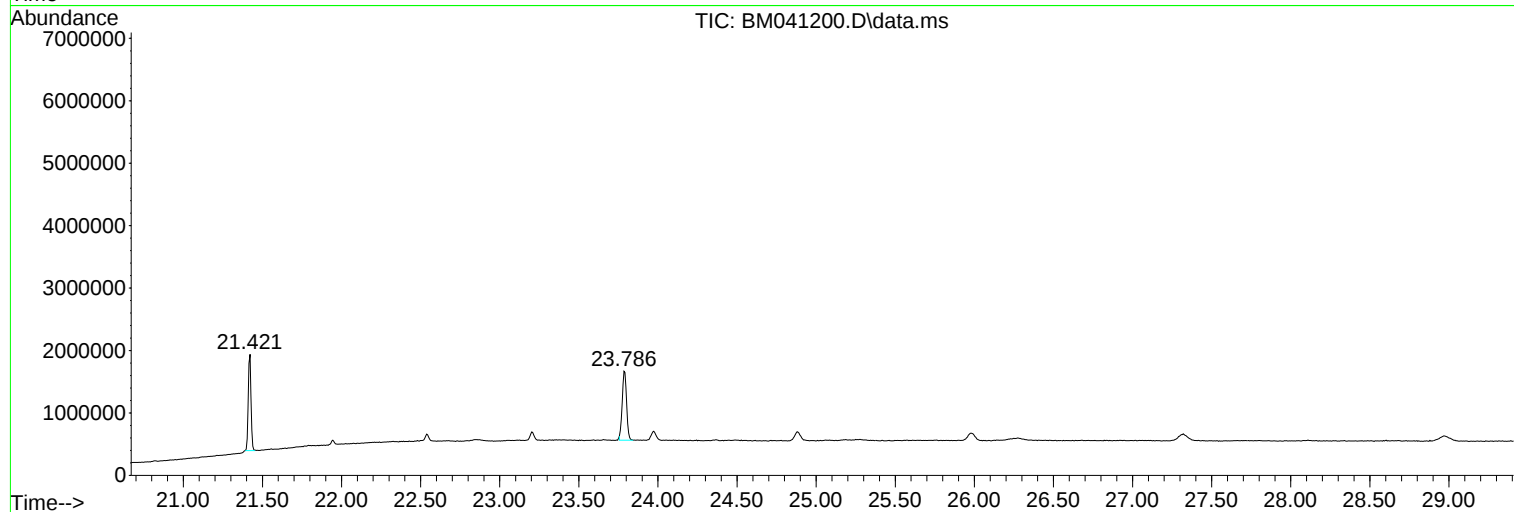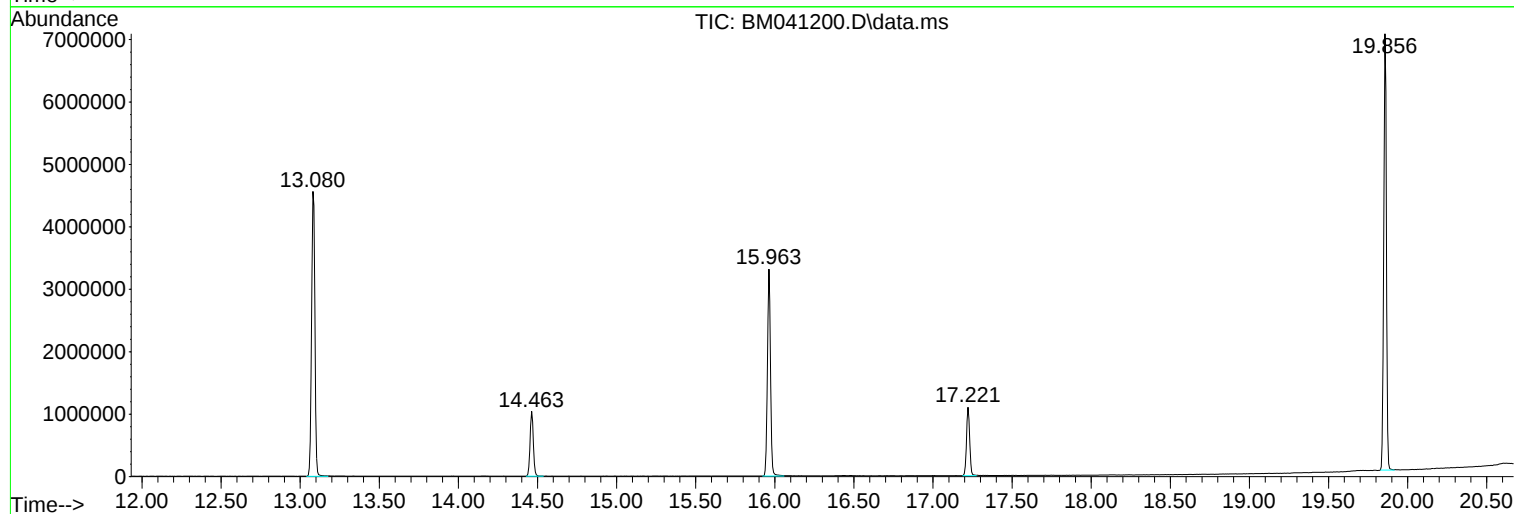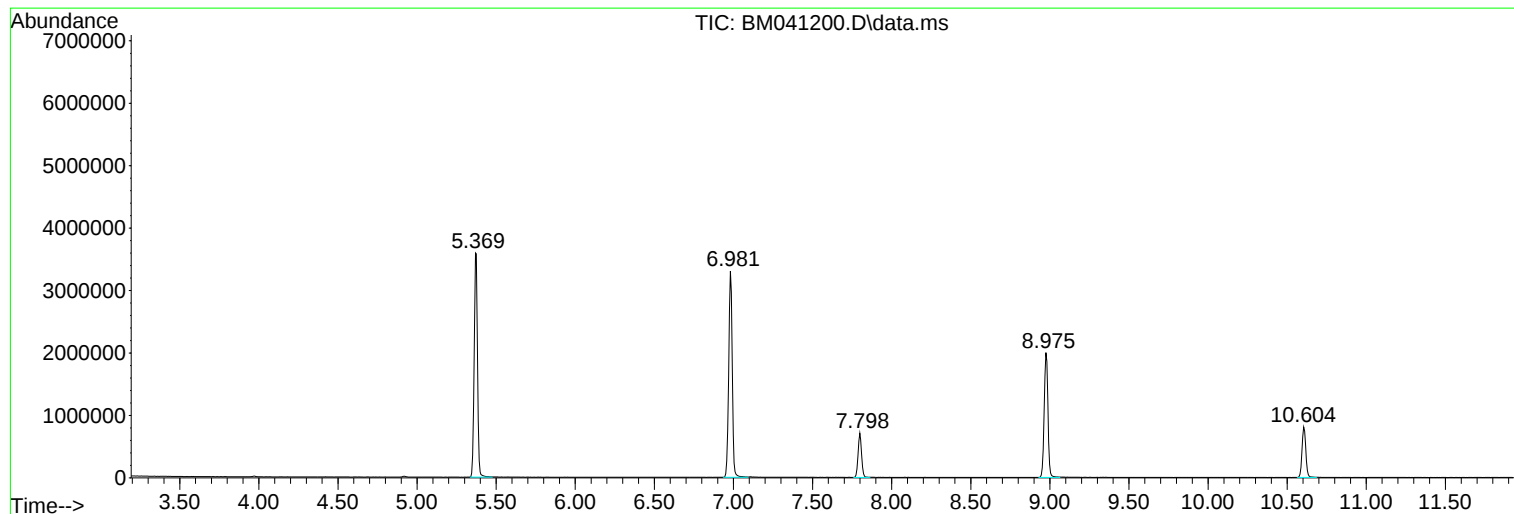

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM073123\
Data File : BM041200.D
Acq On : 31 Jul 2023 23:00
Operator : MA/JU
Sample : PB154429BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB154429BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM073123\
Data File : BM041200.D
Acq On : 31 Jul 2023 23:00
Operator : MA/JU
Sample : PB154429BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB154429BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------