
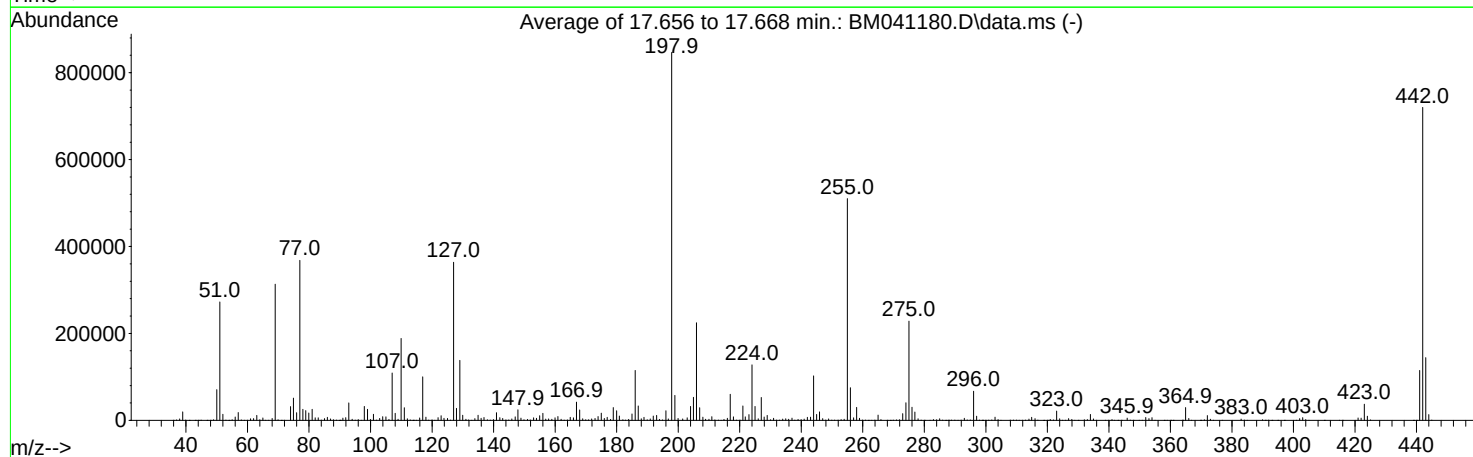


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM073123\
 Data File : BM041180.D
 Acq On : 31 Jul 2023 08:47
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 31 16:29:28 2023

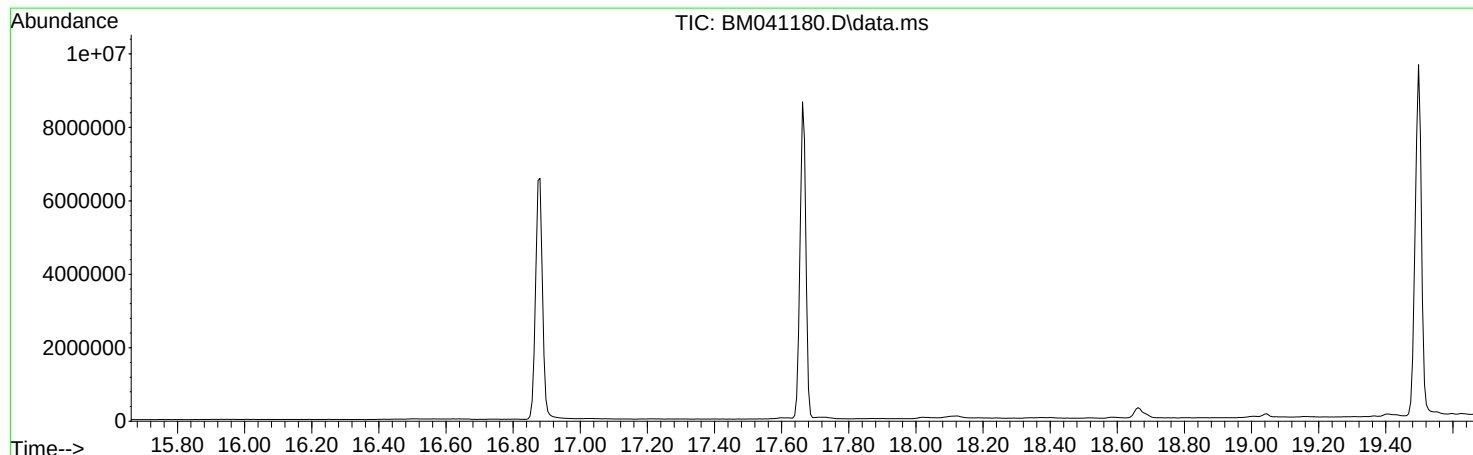




AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	272406	PASS
68	69	0.00	2	1.5	4581	PASS
69	198	0.00	100	37.0	313474	PASS
70	69	0.00	2	0.5	1614	PASS
127	198	10	80	43.0	363641	PASS
197	198	0.00	2	0.4	3487	PASS
198	198	100	100	100.0	846383	PASS
199	198	5	9	6.8	57557	PASS
275	198	10	60	27.0	228352	PASS
365	198	1	100	3.5	29331	PASS
441	198	0.01	100	13.6	114712	PASS
442	442	50	100	100.0	720085	PASS
443	442	15	24	20.0	144269	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM073123\
Data File : BM041180.D
Acq On : 31 Jul 2023 08:47
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 31 10:55:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 29 00:19:24 2023
Response via : Initial Calibration

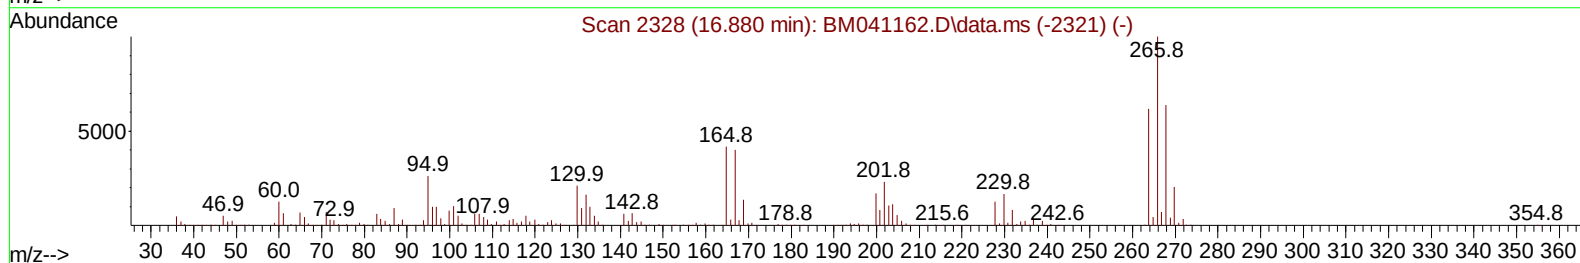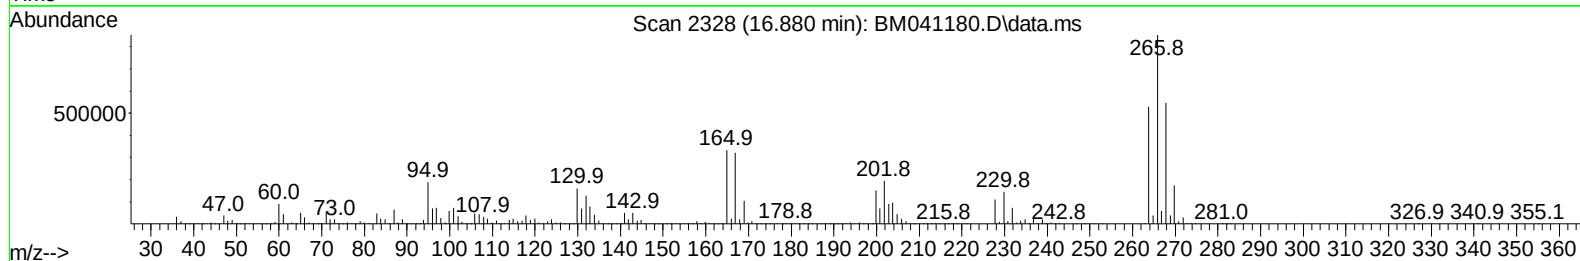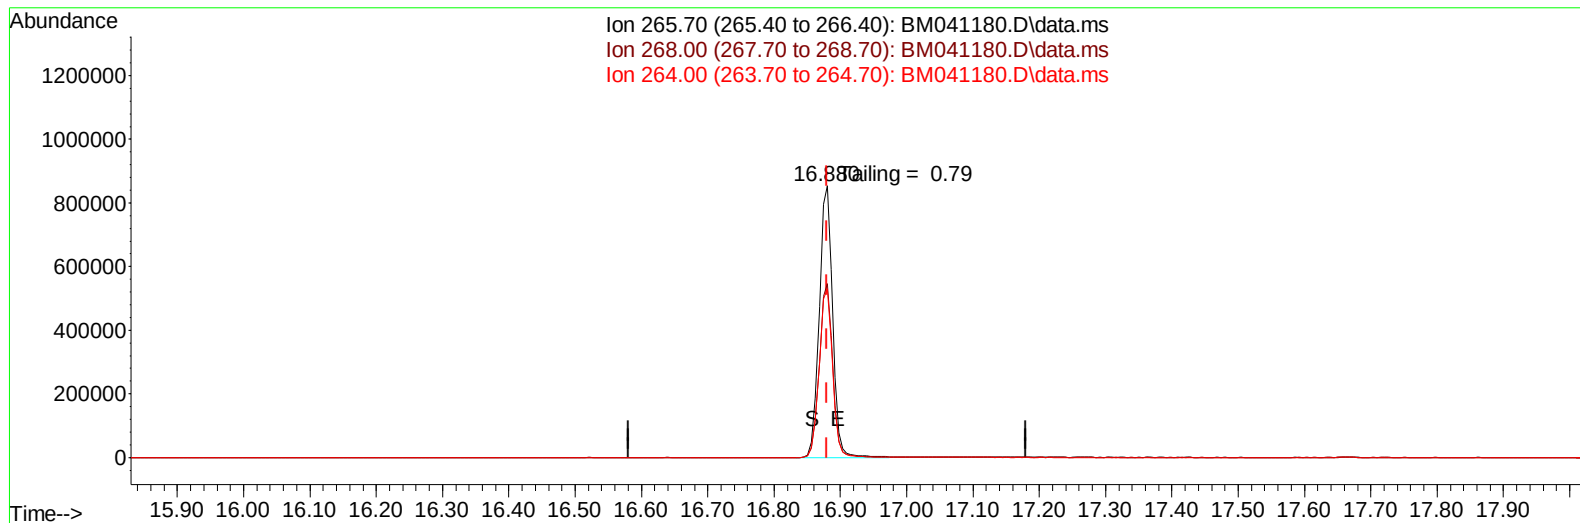

TIC: BM041180.D\data.ms

(70) Pentachlorophenol (C)

16.880min (-0.000) 2437789.09 ng




response 1193666

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.92
264.00	61.80	62.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM073123\
Data File : BM041180.D
Acq On : 31 Jul 2023 08:47
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 31 10:55:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 29 00:19:24 2023
Response via : Initial Calibration

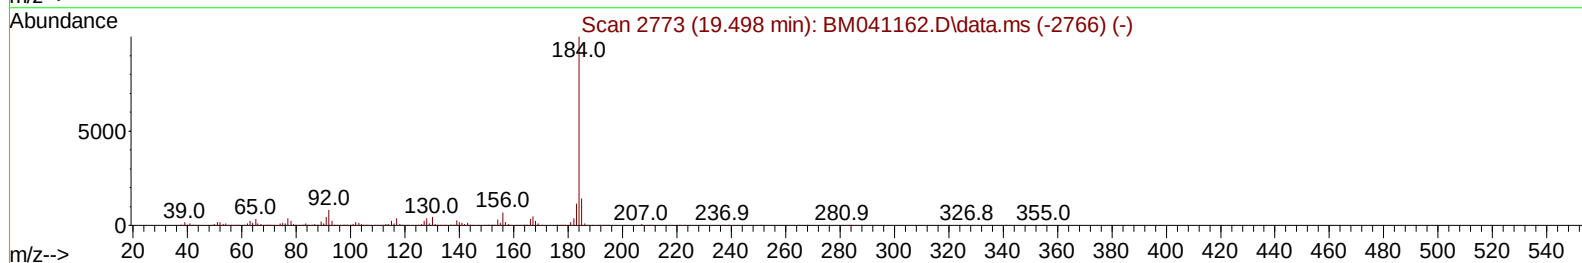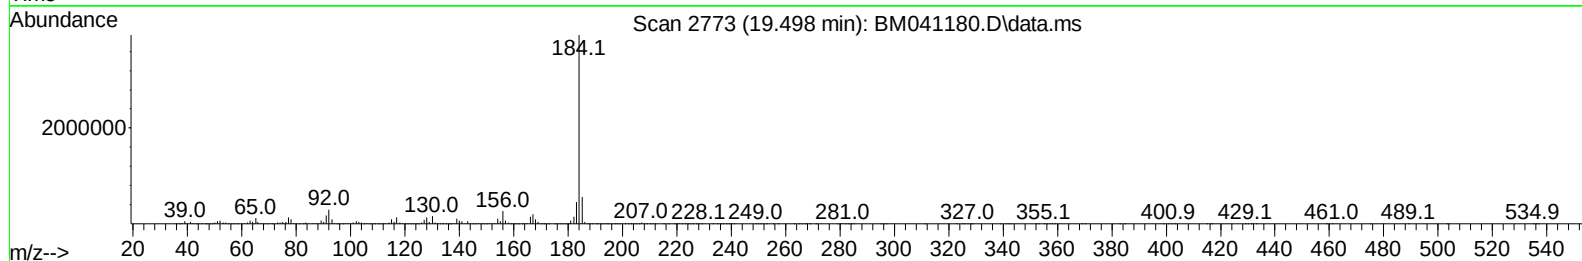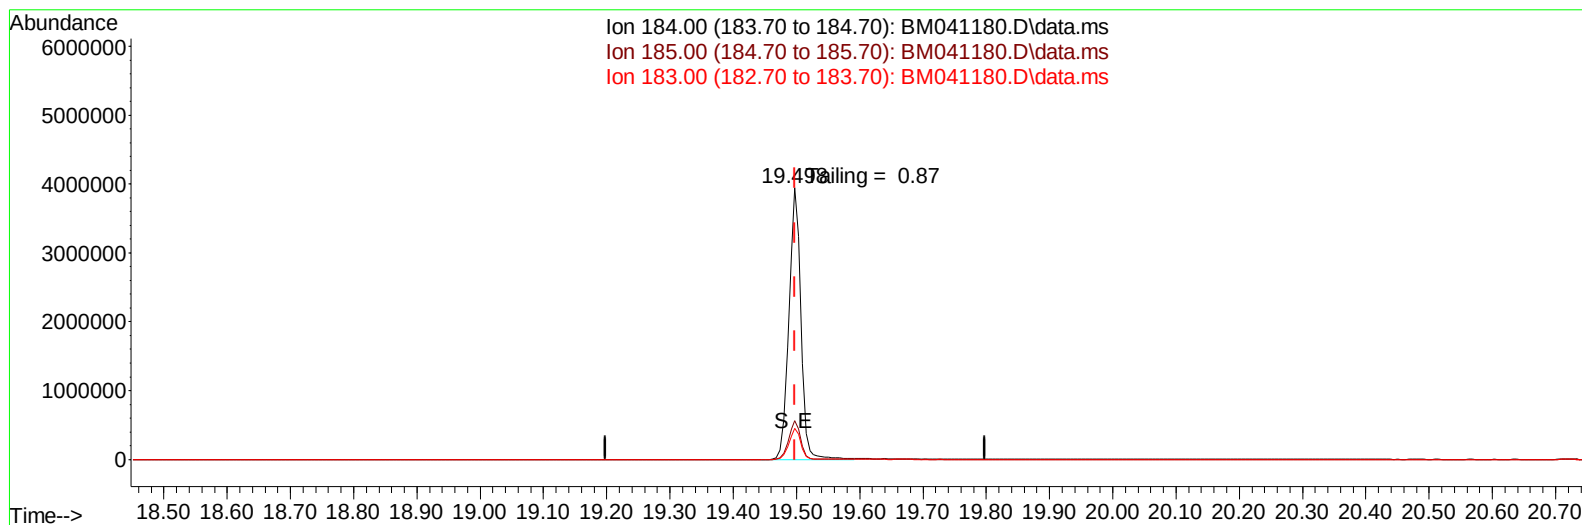

TIC: BM041180.D\data.ms

(77) Benzidine

19.498min (-0.000) 13088.10 ng

response 5290497

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.31
183.00	11.50	11.40
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/31/2023	BNA_M	<u>BM041180.D</u>
Compound Name	Response	Retention Time
DDT	2268488	20.721
DDD	273647	20.28
DDE	0	19.768
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
273647	2542135	10.76

Instrument :
BNA_M
ClientSampleId :
DFTPP