
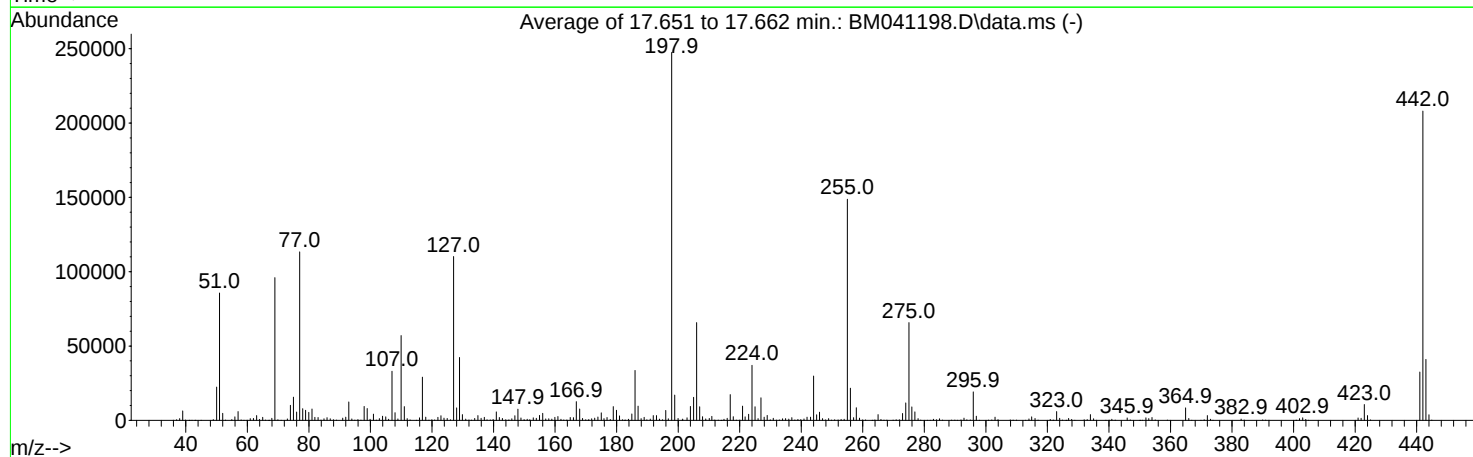


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM073123\
Data File : BM041198.D
Acq On : 31 Jul 2023 20:32
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jul 31 16:29:28 2023

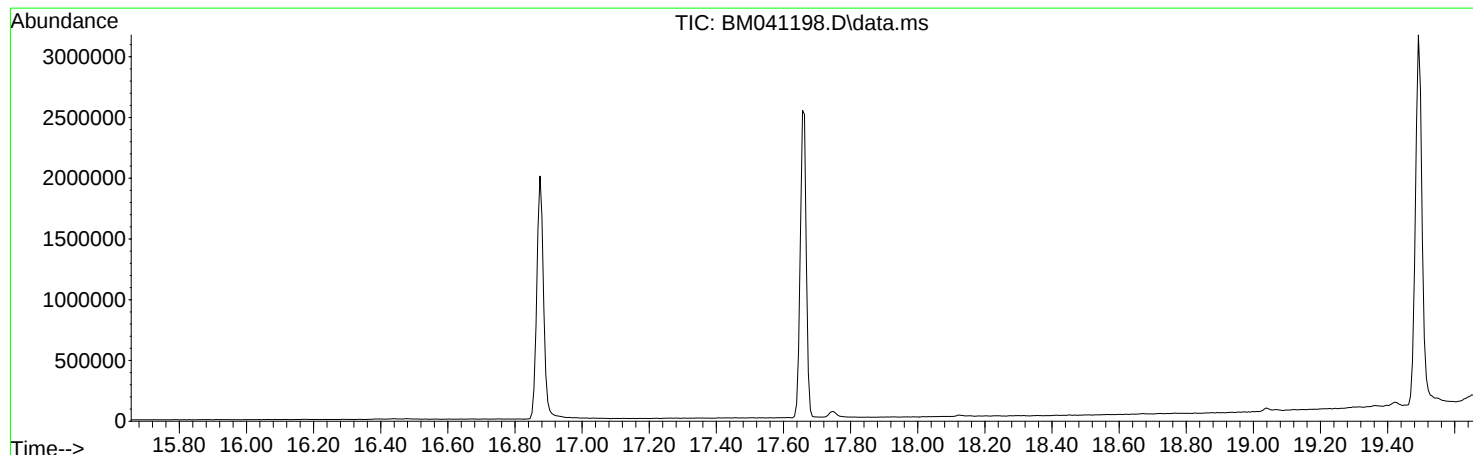




AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	85694	PASS
68	69	0.00	2	1.4	1362	PASS
69	198	0.00	100	38.8	95971	PASS
70	69	0.00	2	0.5	483	PASS
127	198	10	80	44.6	110275	PASS
197	198	0.00	2	0.4	1102	PASS
198	198	100	100	100.0	247467	PASS
199	198	5	9	6.9	17029	PASS
275	198	10	60	26.6	65720	PASS
365	198	1	100	3.4	8423	PASS
441	198	0.01	100	13.1	32496	PASS
442	442	50	100	100.0	208019	PASS
443	442	15	24	19.7	41016	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM073123\
Data File : BM041198.D
Acq On : 31 Jul 2023 20:32
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 01 02:24:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 31 16:29:28 2023
Response via : Initial Calibration

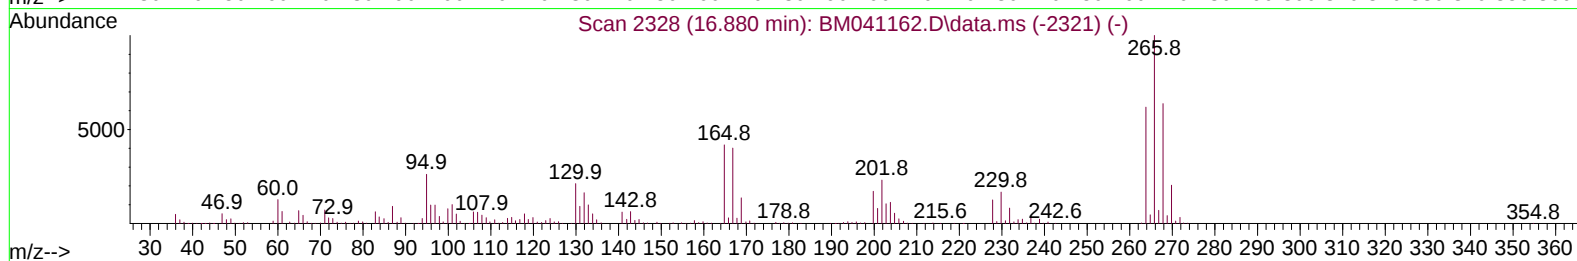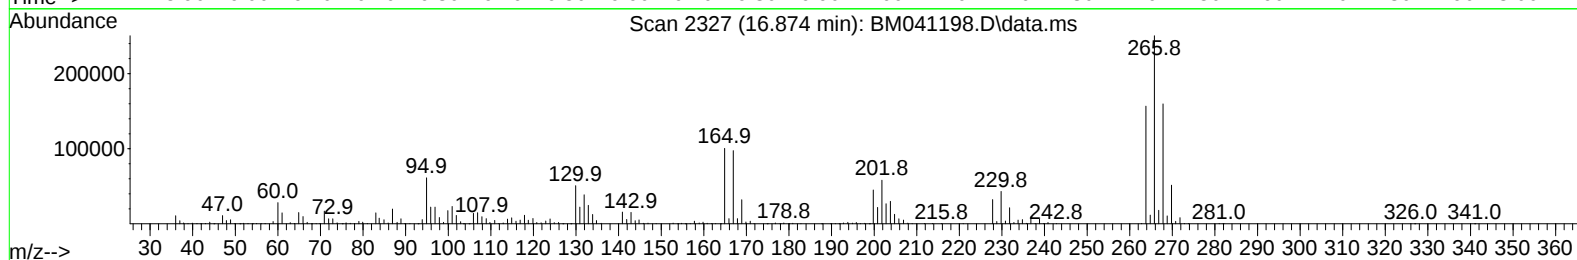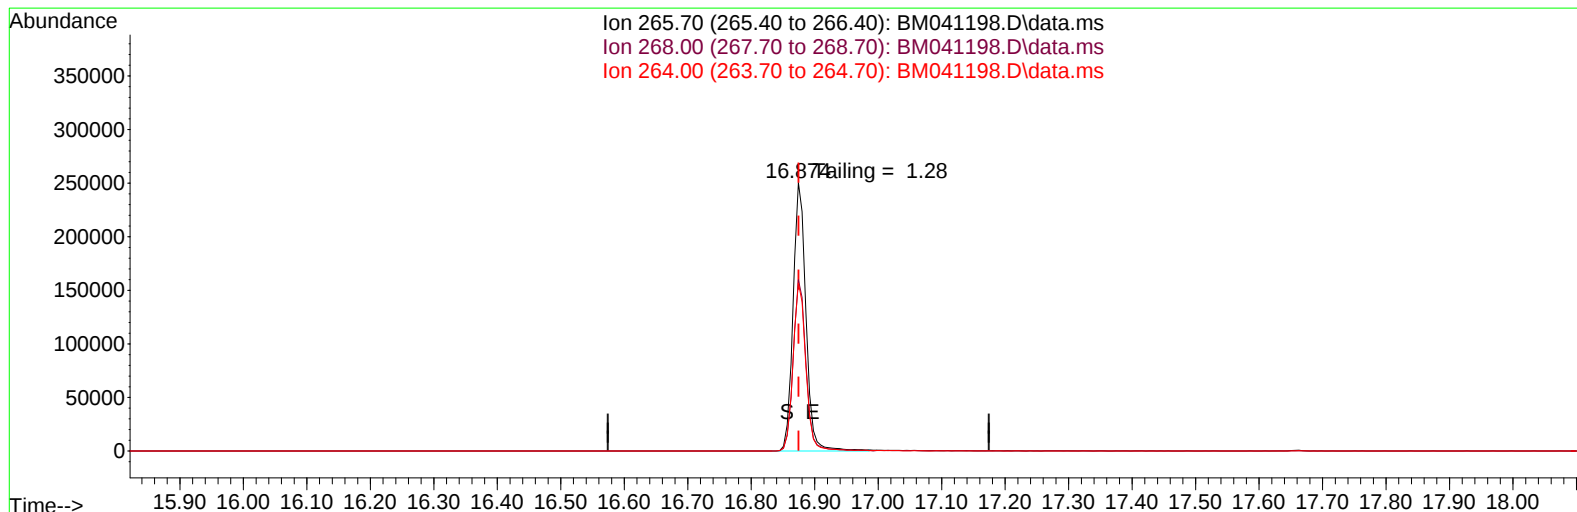

TIC: BM041198.D\data.ms

(70) Pentachlorophenol (C)

16.874min (+ 0.000) 345212.55 ng

response 358468

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.80
264.00	61.80	62.62
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/31/2023	BNA_M	<u>BM041198.D</u>
Compound Name	Response	Retention Time
DDT	226804	20.715
DDD	428448	20.28
DDE	1719	19.762
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
430167	656971	65.48

Instrument :
BNA_M
ClientSampleId :
DFTPP